

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 19:30
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:10:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 04:54:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.628	69845344	162.8E6	52.417	52.022
28)	SA Decachlor...	8.901	7.728	57366231	121.9E6	51.398	51.986
Target Compounds							
23)	Chlordane-1	4.575	3.606	27361019	47242624	541.554	535.601
24)	Chlordane-2	5.108	4.176	28635353	53912011	464.979	526.404
25)	Chlordane-3	5.820	4.800	107.5E6	158.4E6	526.569	526.338
26)	Chlordane-4	5.897	4.861	130.3E6	164.6E6	526.730	537.887
27)	Chlordane-5	6.756	5.525	21383611	44024331	514.196	571.733



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 19:30
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:10:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 04:54:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

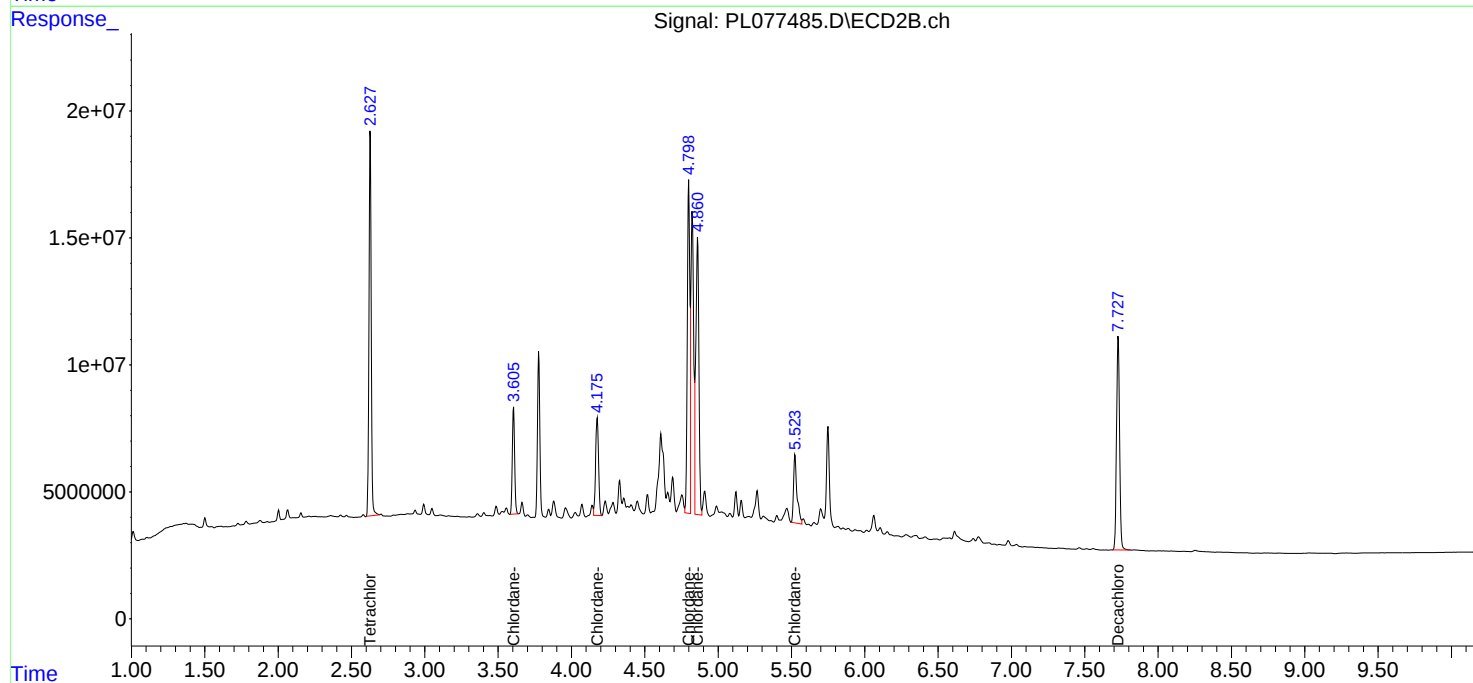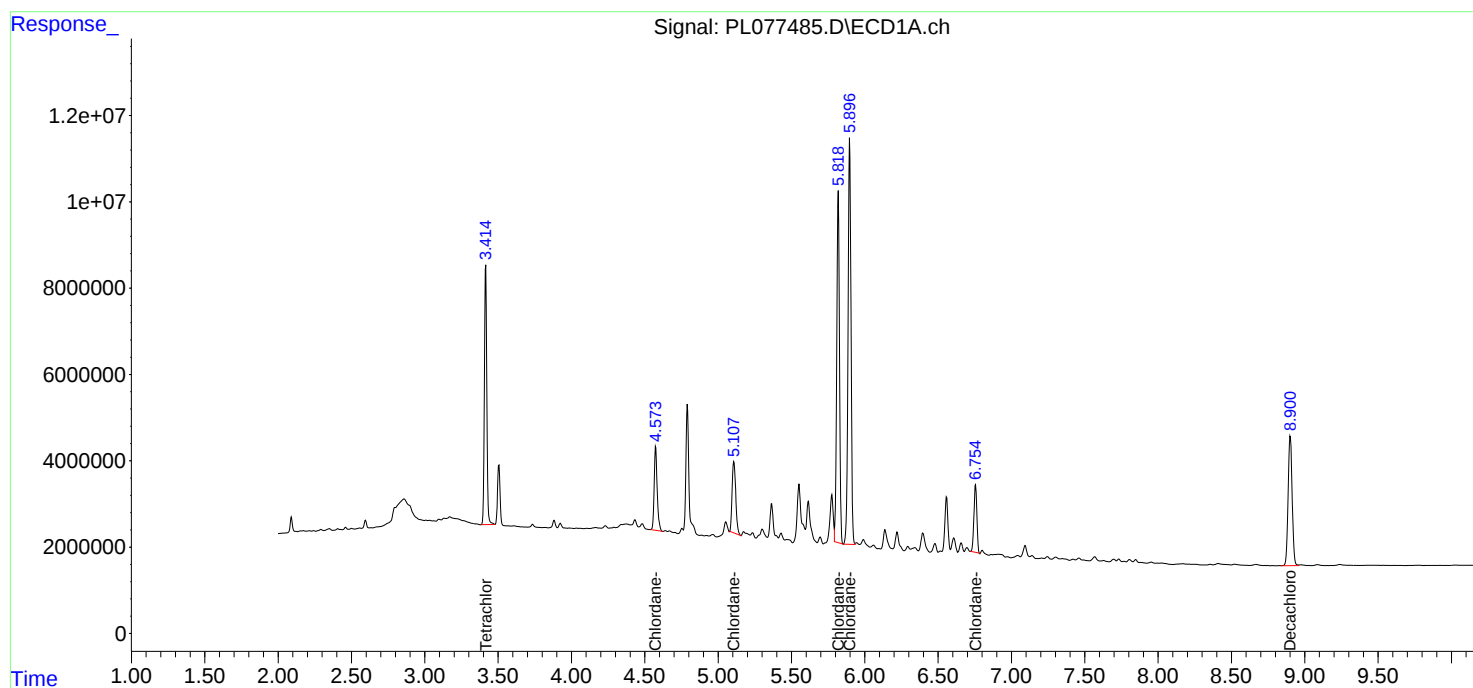


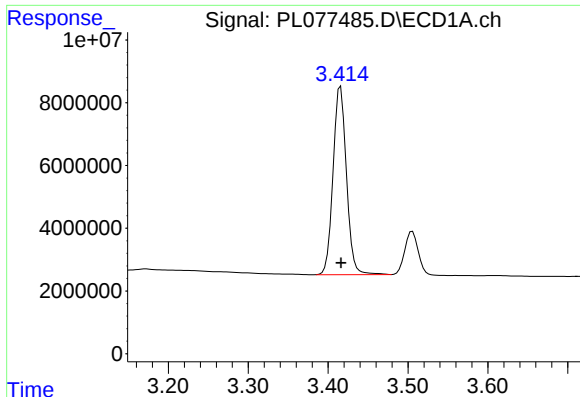

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 69845344
Conc: 52.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

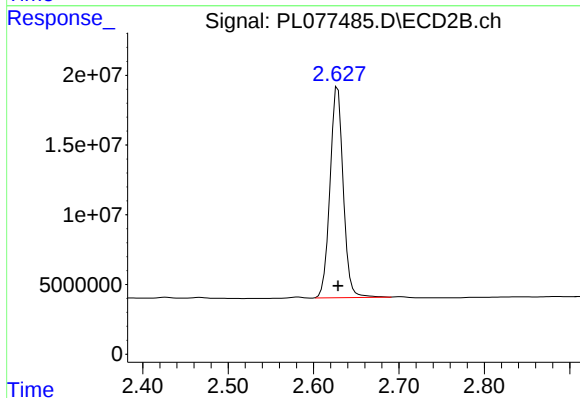


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 162766101
Conc: 52.02 ng/ml

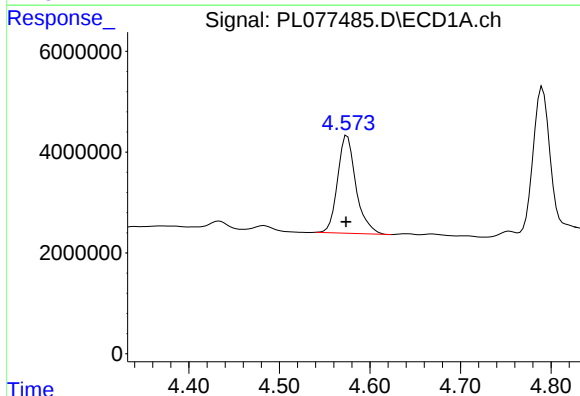


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.001 min
Response: 27361019
Conc: 541.55 ng/ml

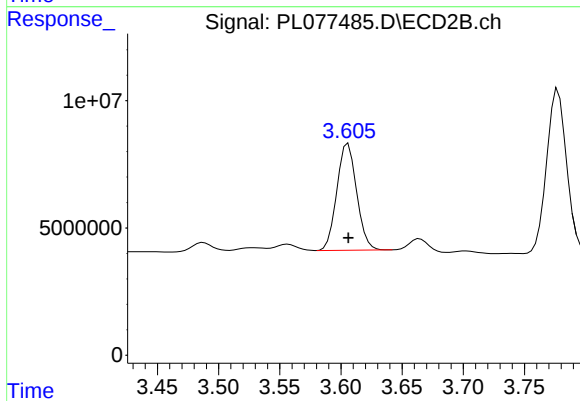

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 47242624
Conc: 535.60 ng/ml

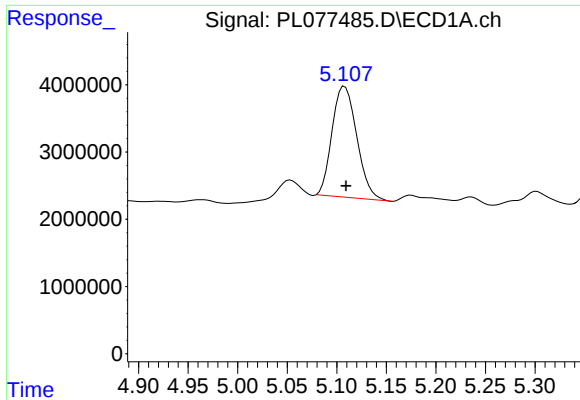

#24 Chlordane-2


R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 28635353
Conc: 464.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

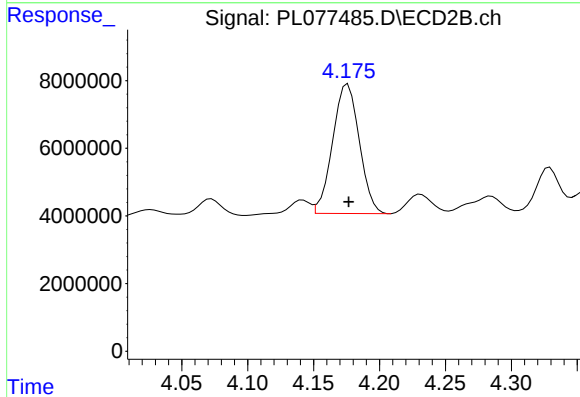


#24 Chlordane-2

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 53912011
Conc: 526.40 ng/ml

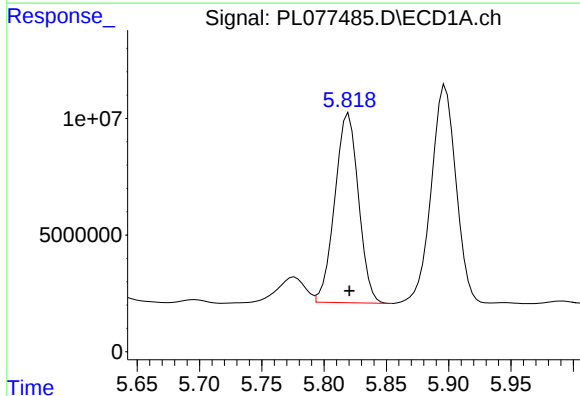


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 107469668
Conc: 526.57 ng/ml

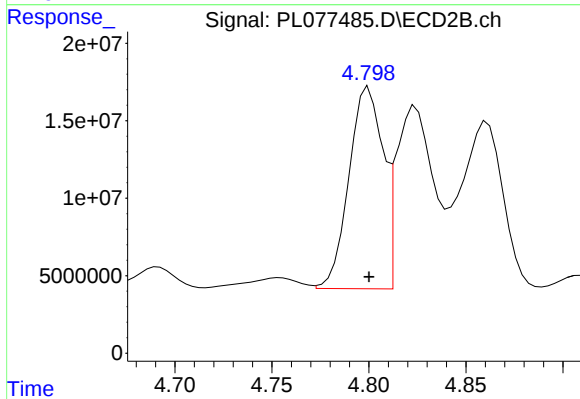

#25 Chlordane-3


R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 158382600
Conc: 526.34 ng/ml

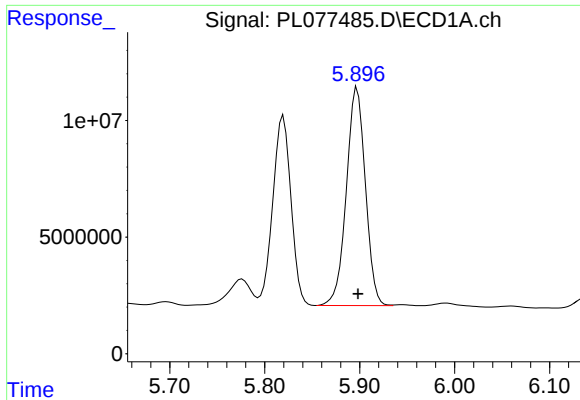

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: -0.001 min
Response: 130316341
Conc: 526.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

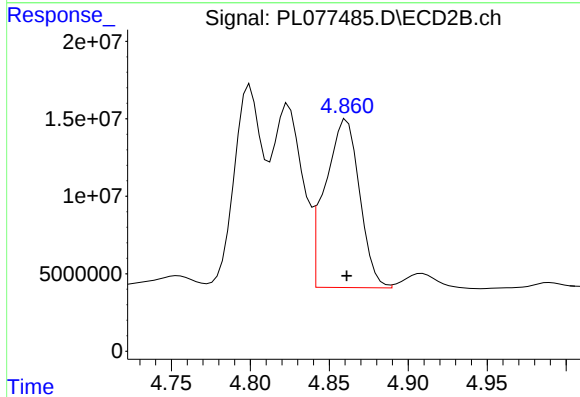


#26 Chlordane-4

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 164647334
Conc: 537.89 ng/ml

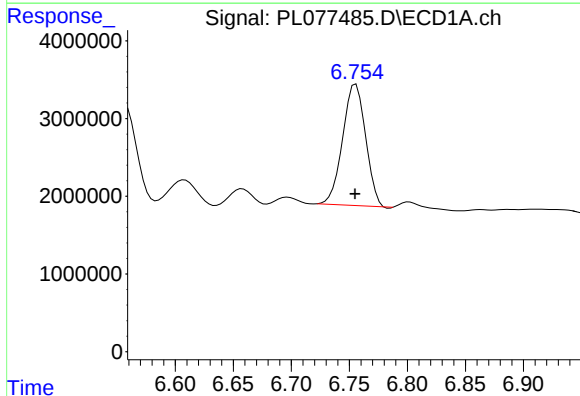


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 21383611
Conc: 514.20 ng/ml

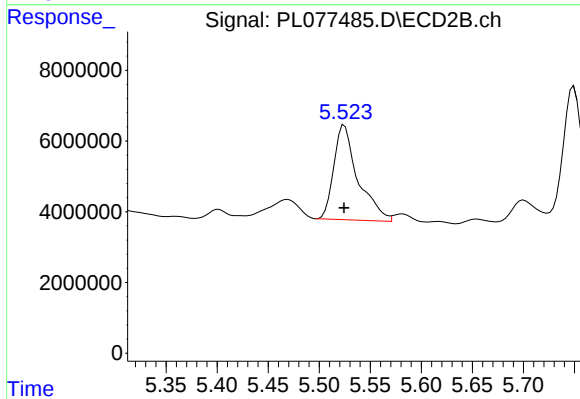

#27 Chlordane-5


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 44024331
Conc: 571.73 ng/ml

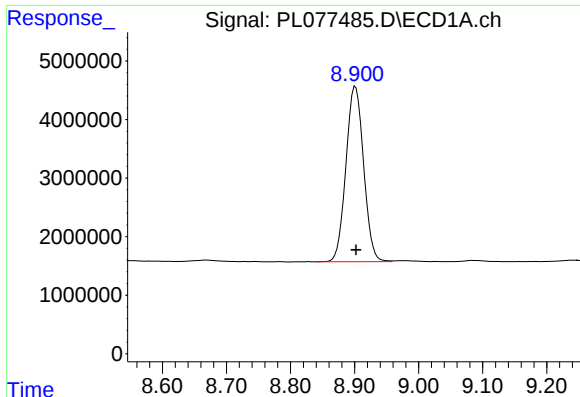

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 57366231
Conc: 51.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

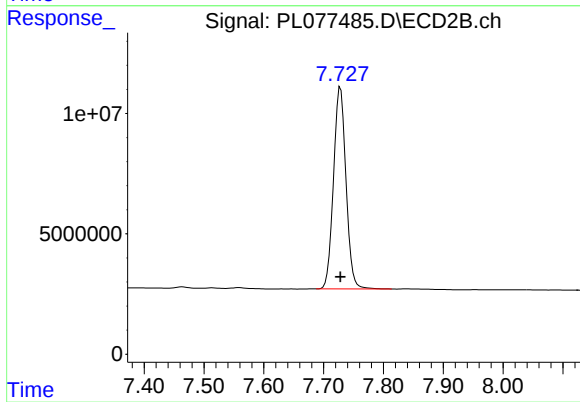

#28 Decachlorobiphenyl

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 121921764
Conc: 51.99 ng/ml