

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 20:25
 Operator : AR\AJ
 Sample : PB147431BS
 Misc : CHLOR BS
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:12:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 04:54:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.628	28206112	65139725	21.168	20.819
28)	SA Decachlor...	8.902	7.728	25152022	51127639	22.535	21.800
Target Compounds							
23)	Chlordane-1	4.575	3.606	10822157	19231301	214.202	218.030
24)	Chlordane-2	5.108	4.176	12112877	22505369	196.688	219.745
25)	Chlordane-3	5.819	4.800	42716999	62472007	209.300	207.607
26)	Chlordane-4	5.898	4.861	52696561	66251993	212.996	216.439
27)	Chlordane-5	6.755	5.524	9053070	17560757	217.693	228.057



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 20:25
Operator : AR\AJ
Sample : PB147431BS
Misc : CHLOR BS
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:12:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 04:54:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

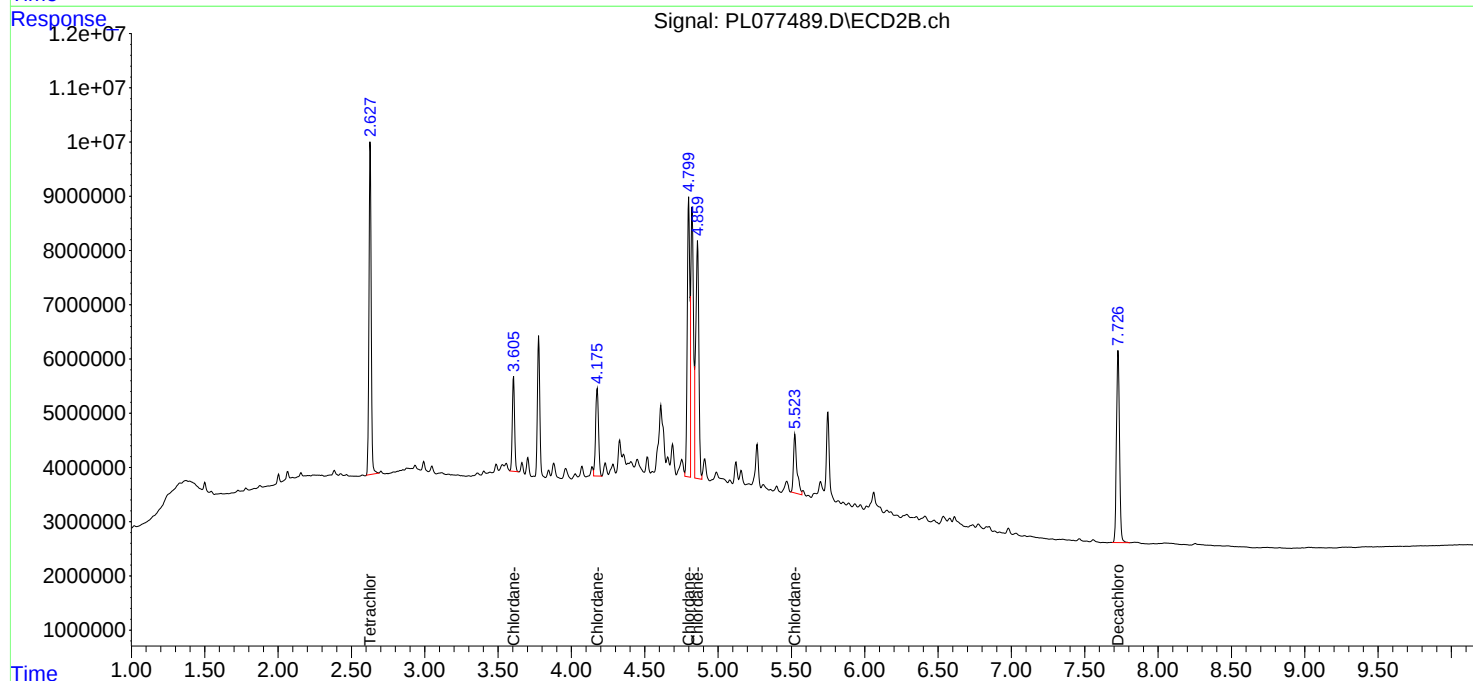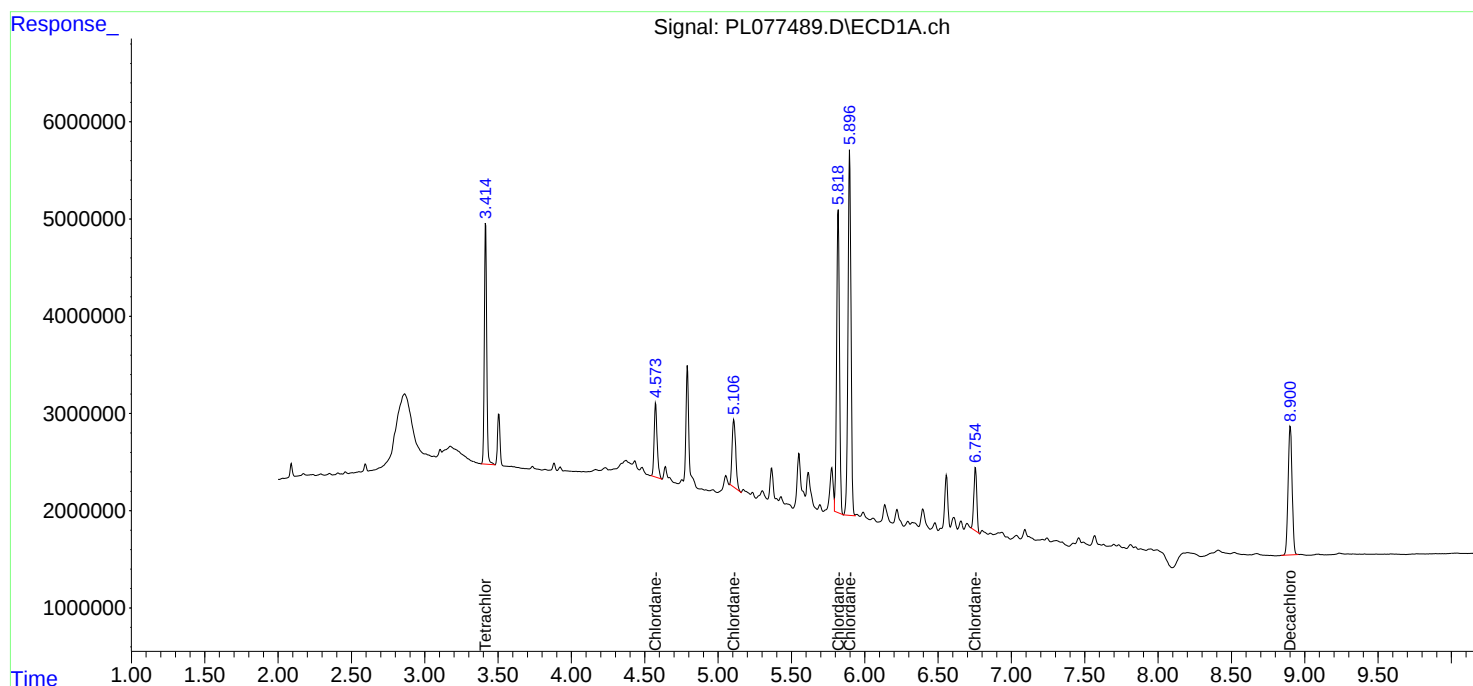


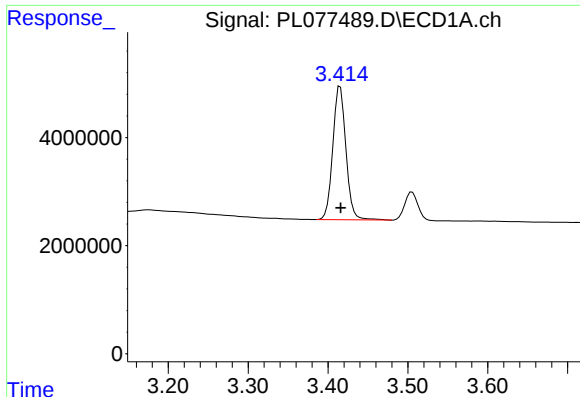

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 28206112
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

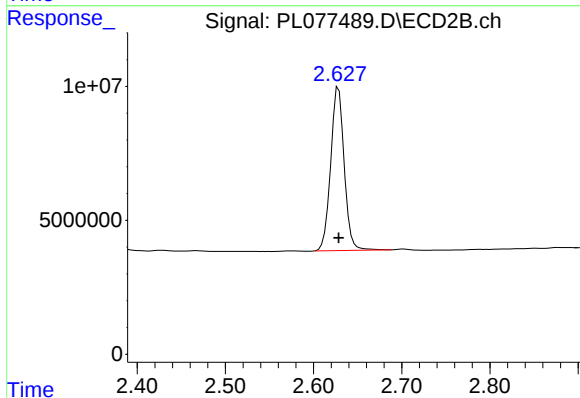


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 65139725
Conc: 20.82 ng/ml

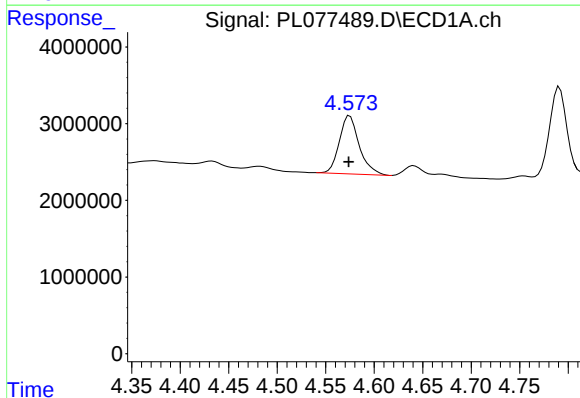


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.001 min
Response: 10822157
Conc: 214.20 ng/ml

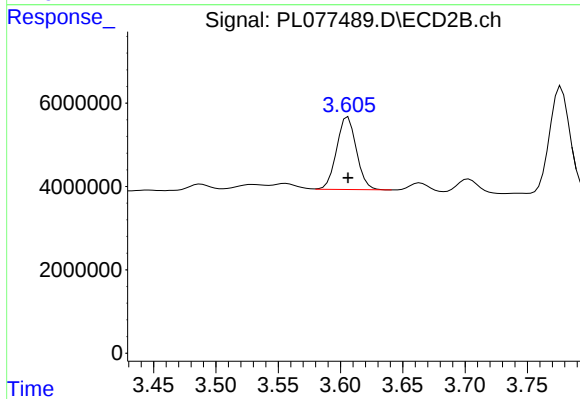

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 19231301
Conc: 218.03 ng/ml

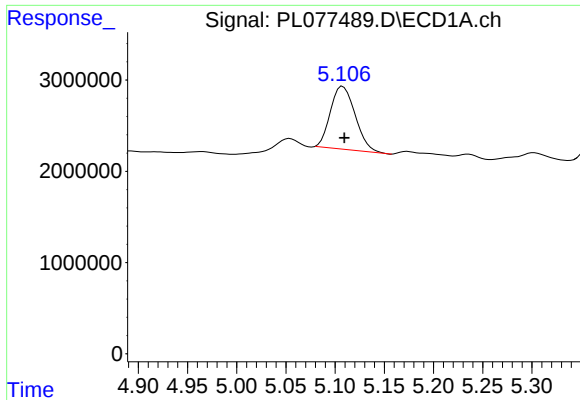

#24 Chlordane-2


R.T.: 5.108 min
Delta R.T.: -0.002 min
Response: 12112877
Conc: 196.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

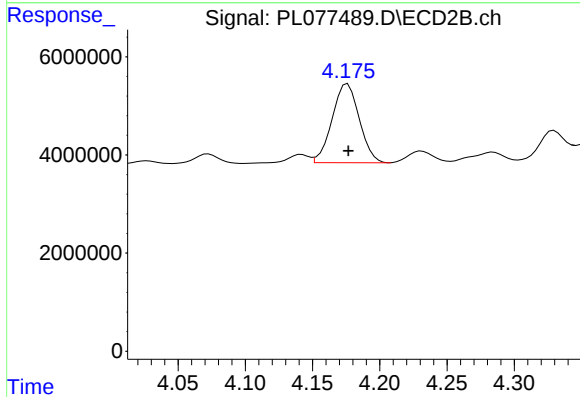


#24 Chlordane-2

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 22505369
Conc: 219.75 ng/ml

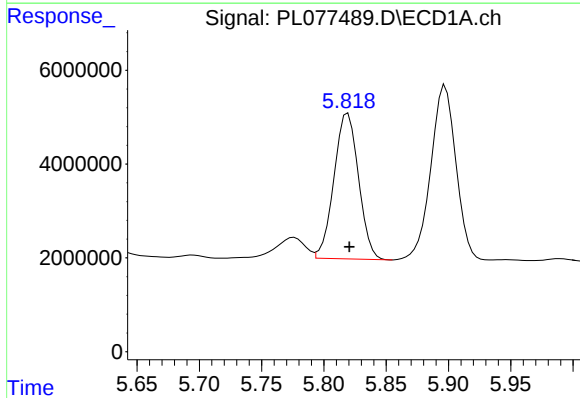


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: -0.001 min
Response: 42716999
Conc: 209.30 ng/ml

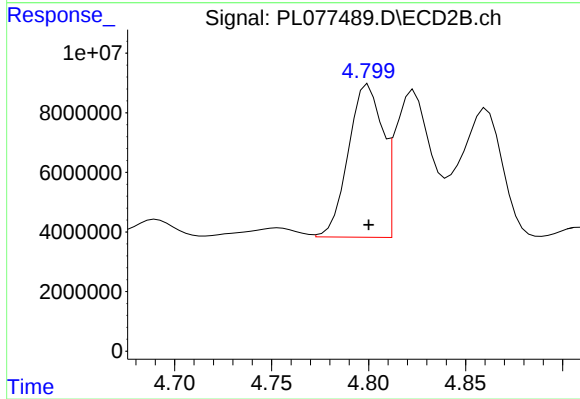

#25 Chlordane-3


R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 62472007
Conc: 207.61 ng/ml

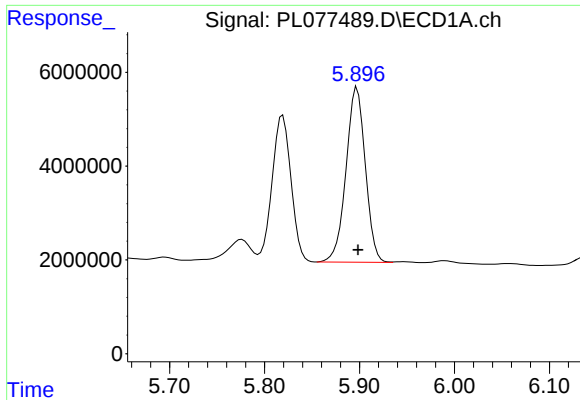

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: -0.001 min
Response: 52696561
Conc: 213.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

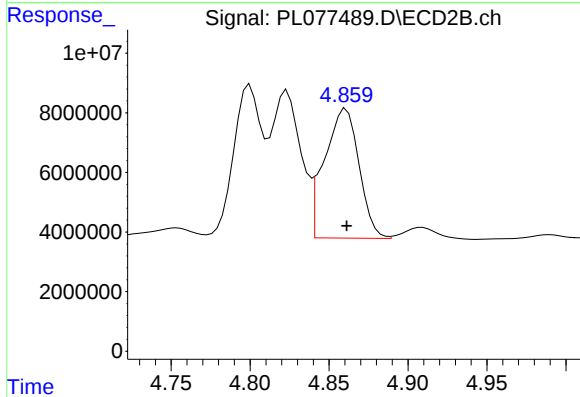


#26 Chlordane-4

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 66251993
Conc: 216.44 ng/ml

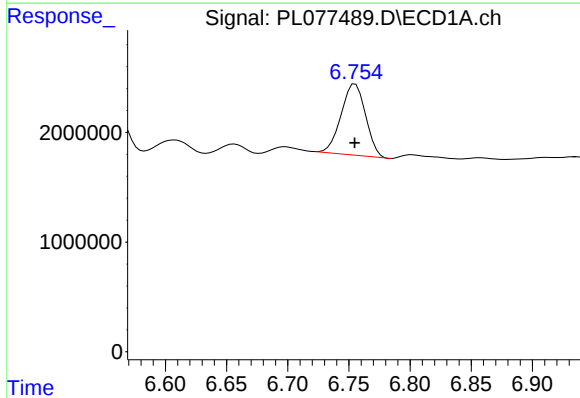


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 9053070
Conc: 217.69 ng/ml

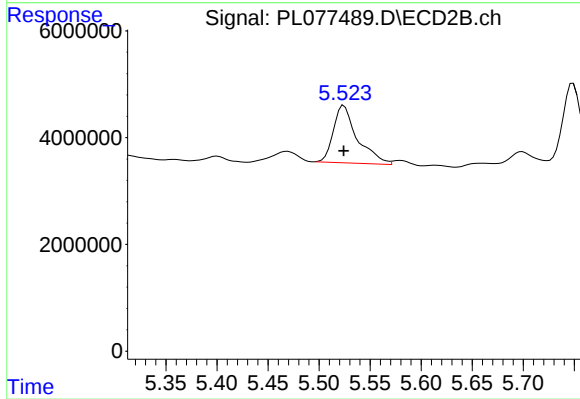

#27 Chlordane-5


R.T.: 5.524 min
Delta R.T.: 0.000 min
Response: 17560757
Conc: 228.06 ng/ml

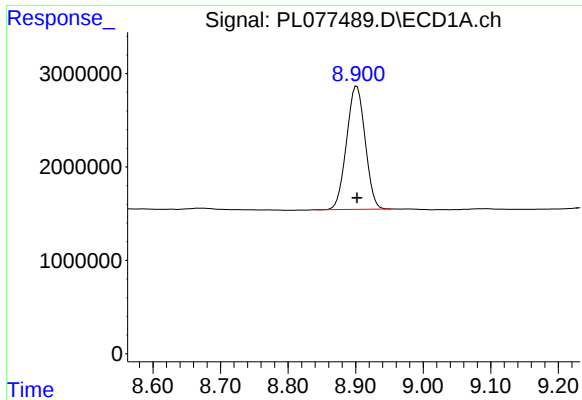

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 25152022
Conc: 22.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

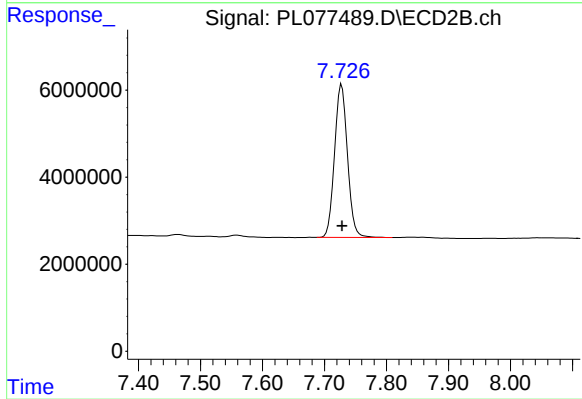

#28 Decachlorobiphenyl

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 51127639
Conc: 21.80 ng/ml