

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2022 00:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 06:29:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 05:19:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.630	29675399	52237778	21.559	19.635
28)	SA Decachlor...	8.902	7.728	23233779	37957318	20.300	16.084
Target Compounds							
5)	MB Aldrin	0.000	4.068	0	1071310	N.D.	0.325 #
6)	B beta-BHC	0.000	3.750	0	22674	N.D.	0.015 #
8)	B Heptachlo...	5.571	0.000	37661	0	0.028	N.D. #
9)	A Endosulfan I	0.000	4.933	0	173147	N.D.	0.064 #
13)	MA Dieldrin	0.000	5.172	0	5690381	N.D.	1.980 #
14)	MA Endrin	0.000	5.475f	0	20138393	N.D.	8.867 #
15)	B Endosulfa...	6.708f	0.000	277600	0	0.247	N.D. #
16)	A 4,4'-DDD	6.625f	0.000	169283	0	0.164	N.D. #
21)	B Endrin ke...	7.569f	0.000	1069827	0	0.863	N.D. #
22)	Mirex	8.003	0.000	3694977	0	3.839	N.D. #
23)	Chlordane-1	0.000	3.608	0	543910	N.D.	6.166 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2022 00:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 06:29:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 05:19:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

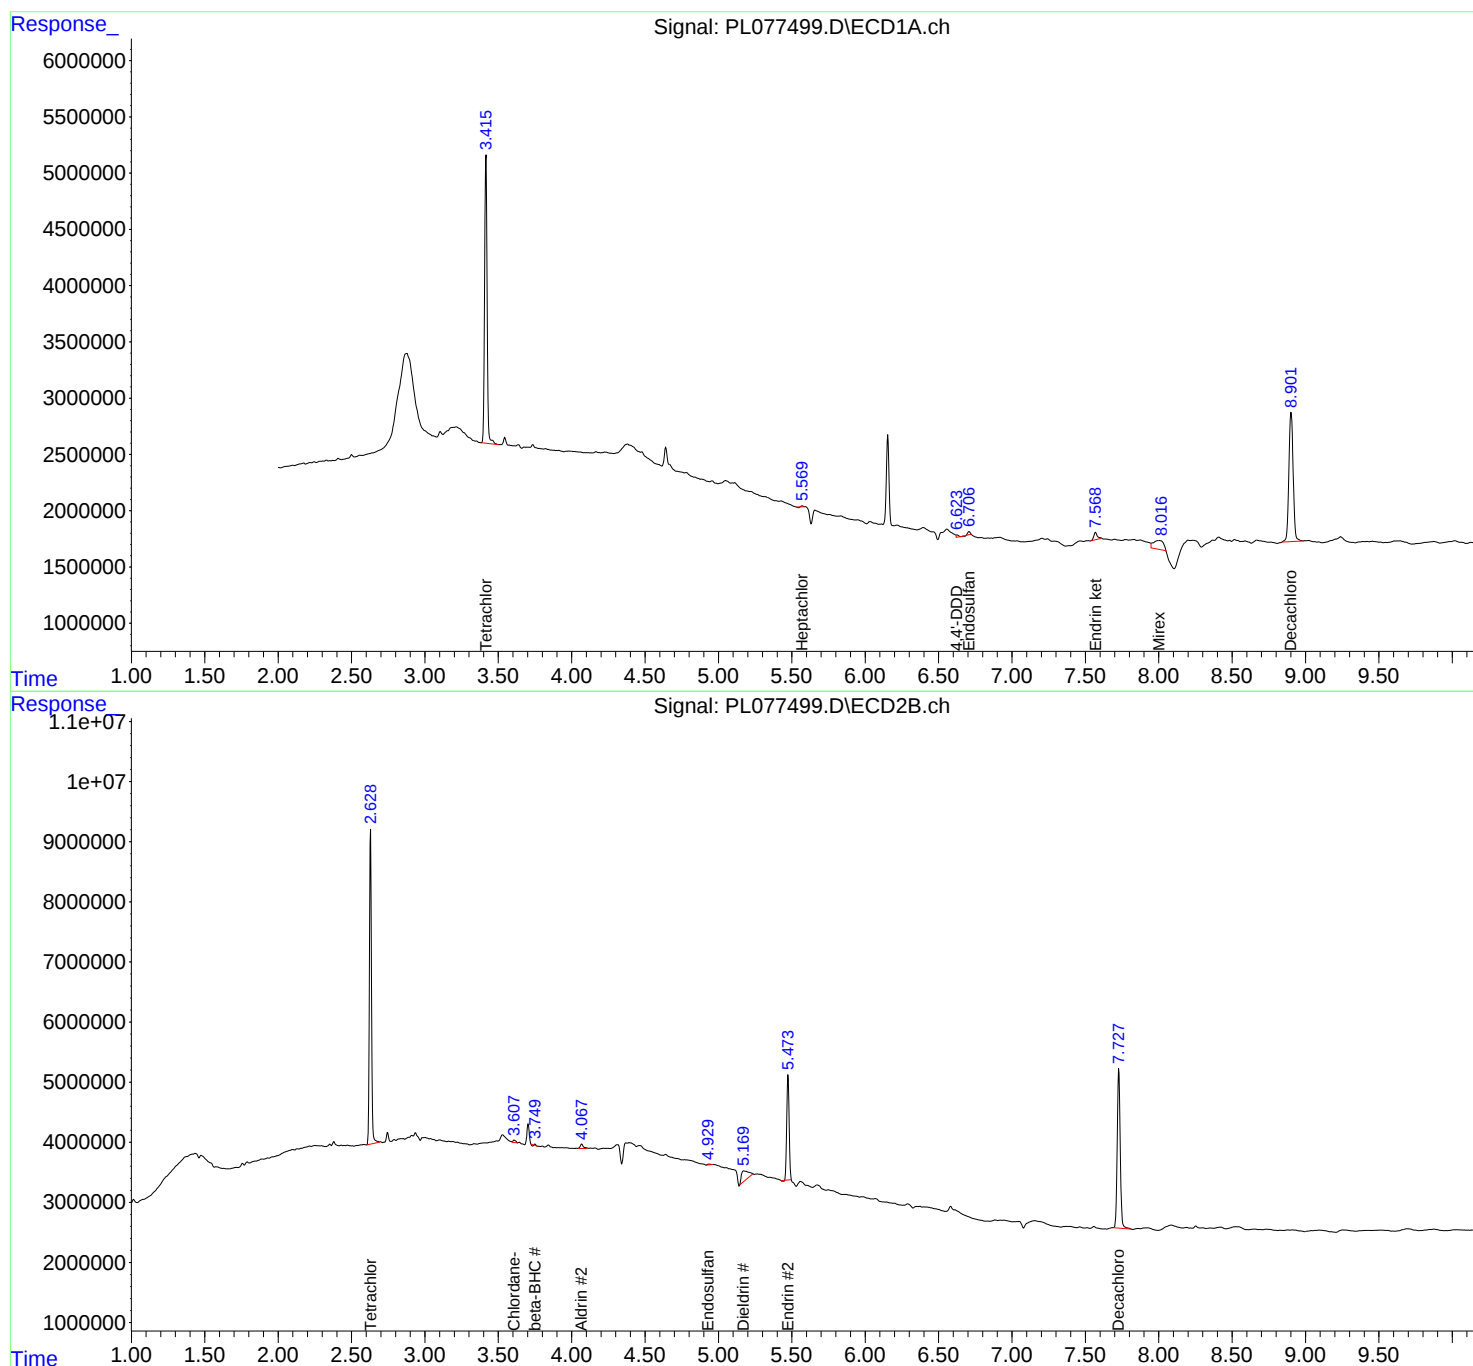


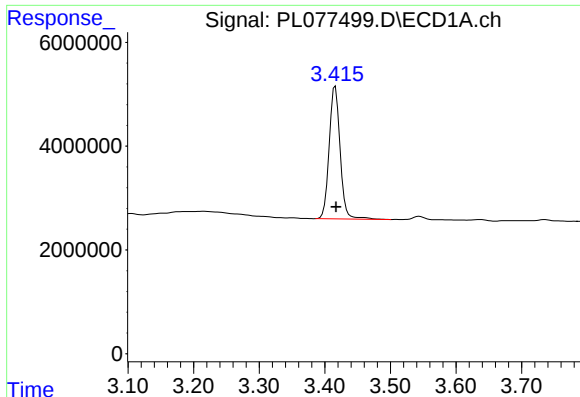

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: -0.001 min
Response: 29675399
Conc: 21.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

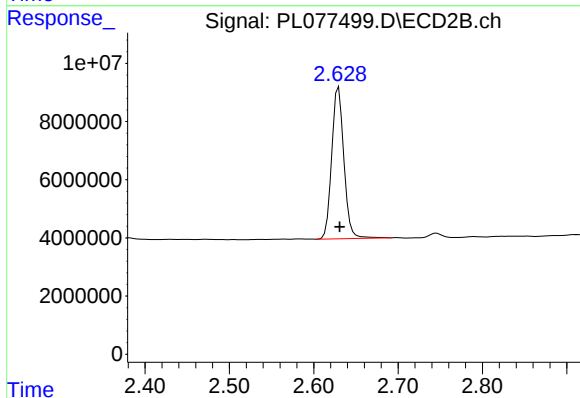


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: -0.001 min
Response: 52237778
Conc: 19.64 ng/ml

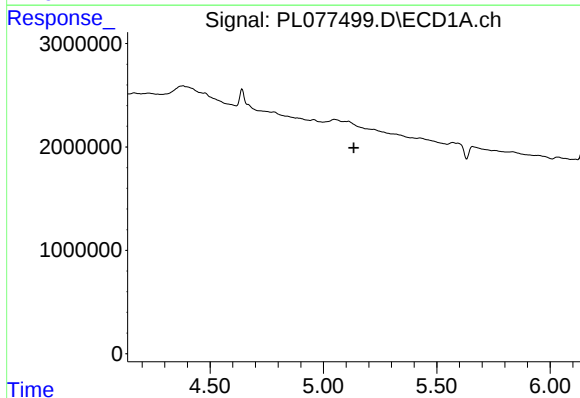


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.134 min
Response: 0
Conc: N.D.

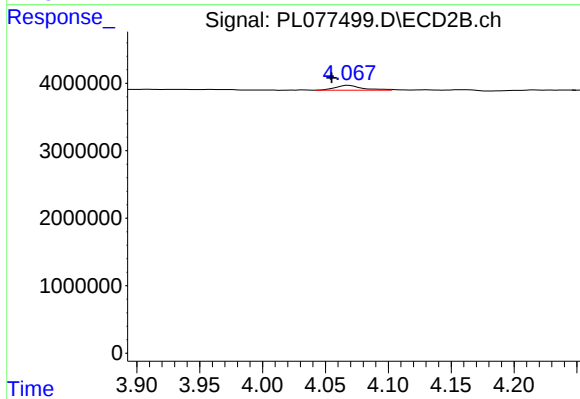

#5 Aldrin


R.T.: 4.068 min
Delta R.T.: 0.014 min
Response: 1071310
Conc: 0.33 ng/ml

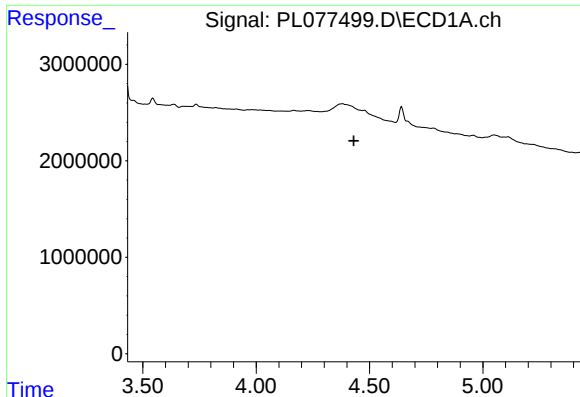

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

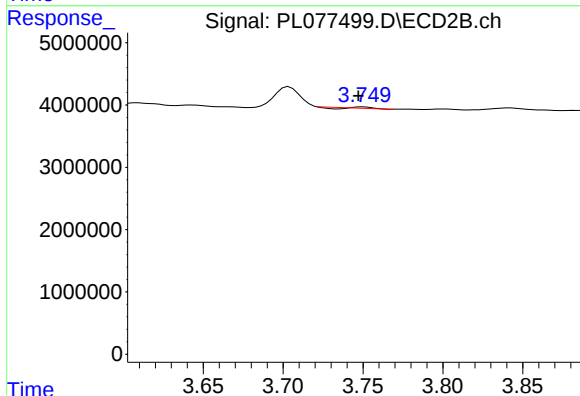


#6 beta-BHC

R.T.: 3.750 min
Delta R.T.: 0.003 min
Response: 22674
Conc: 0.02 ng/ml

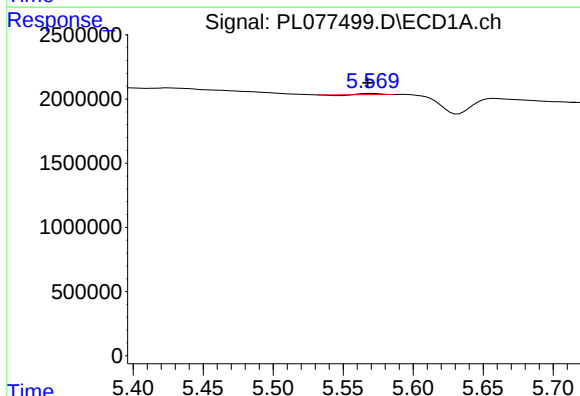


#8 Heptachlor epoxide

R.T.: 5.571 min
Delta R.T.: 0.003 min
Response: 37661
Conc: 0.03 ng/ml

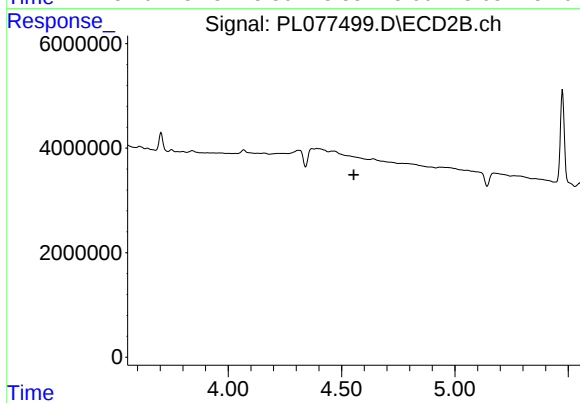

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.554 min
Response: 0
Conc: N.D.

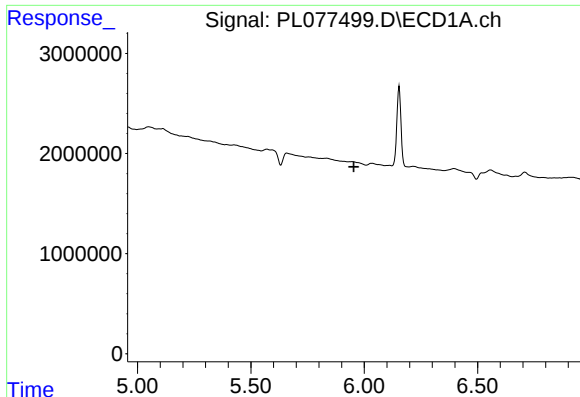

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

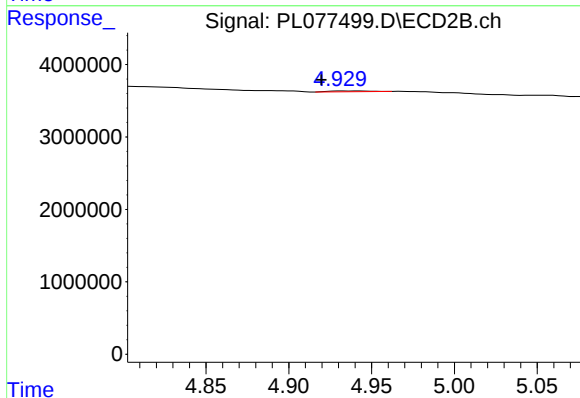


#9 Endosulfan I

R.T.: 4.933 min
Delta R.T.: 0.013 min
Response: 173147
Conc: 0.06 ng/ml

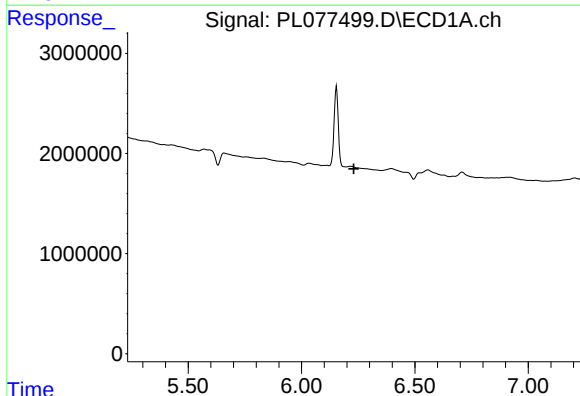


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

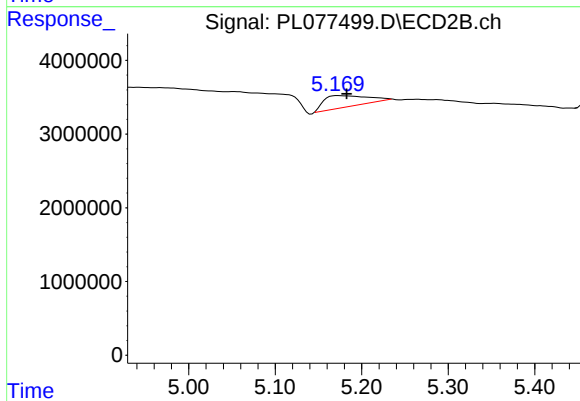

#13 Dieldrin


R.T.: 5.172 min
Delta R.T.: -0.011 min
Response: 5690381
Conc: 1.98 ng/ml

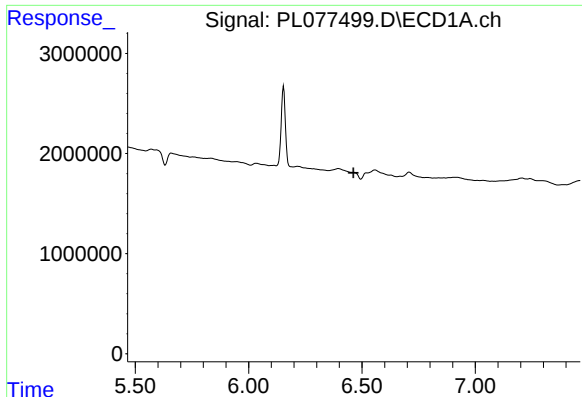

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

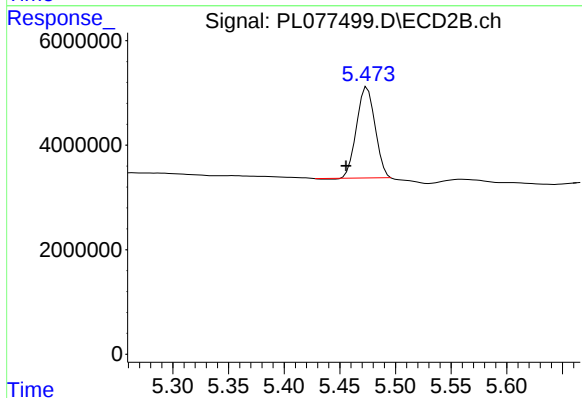


#14 Endrin

R.T.: 5.475 min
Delta R.T.: 0.019 min
Response: 20138393
Conc: 8.87 ng/ml

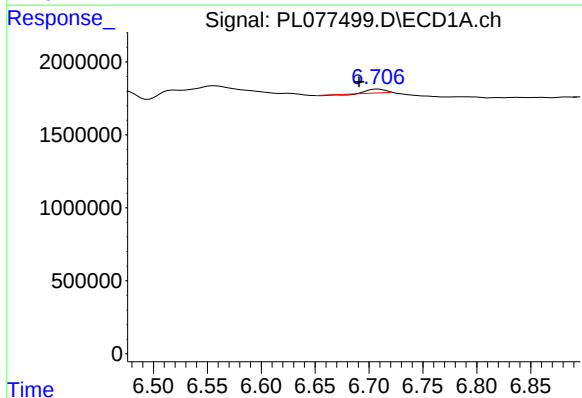


#15 Endosulfan II

R.T.: 6.708 min
Delta R.T.: 0.017 min
Response: 277600
Conc: 0.25 ng/ml

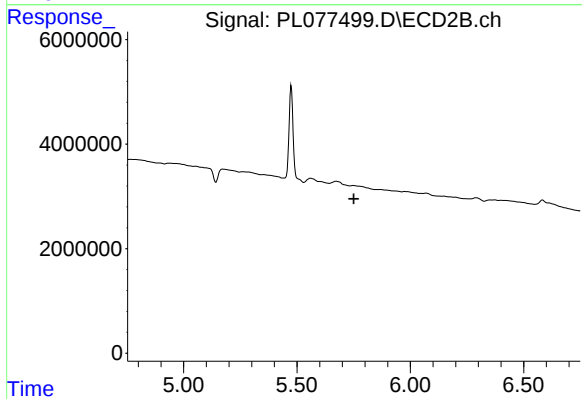

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.751 min
Response: 0
Conc: N.D.

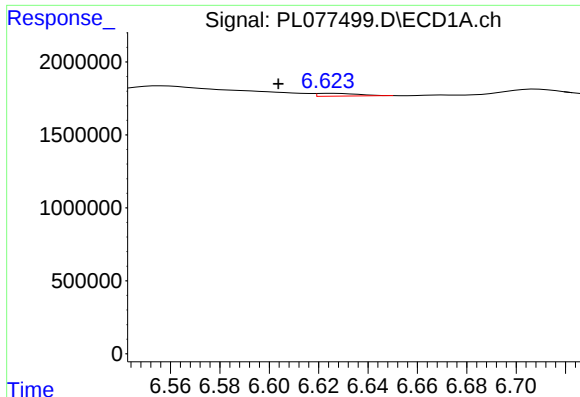

#16 4,4'-DDD


R.T.: 6.625 min
Delta R.T.: 0.021 min
Response: 169283
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

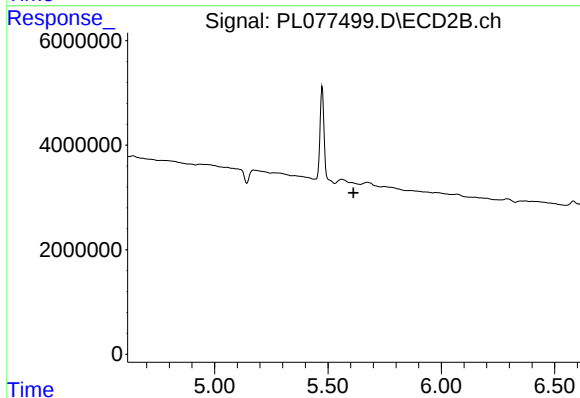


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.613 min
Response: 0
Conc: N.D.

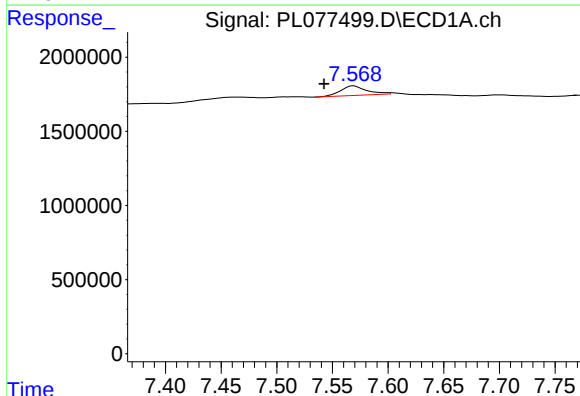


#21 Endrin ketone

R.T.: 7.569 min
Delta R.T.: 0.027 min
Response: 1069827
Conc: 0.86 ng/ml

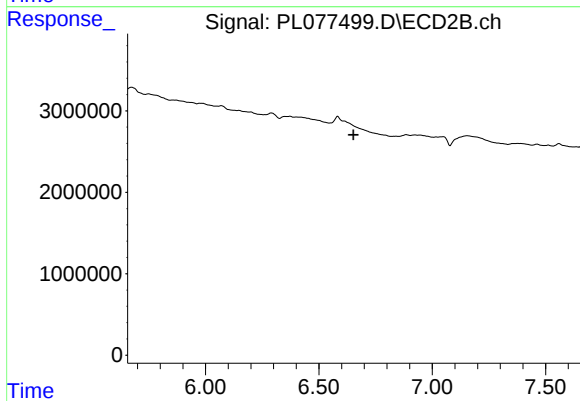

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.653 min
Response: 0
Conc: N.D.

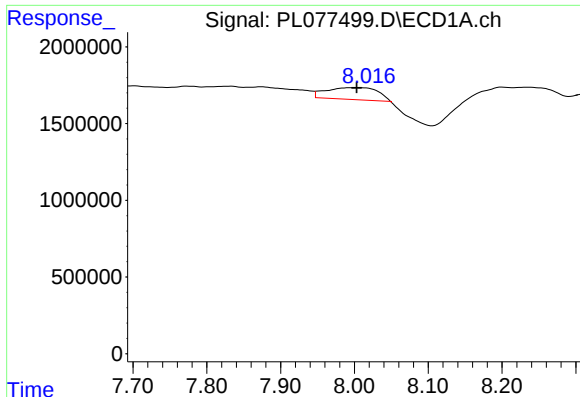

#22 Mirex


R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 3694977
Conc: 3.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

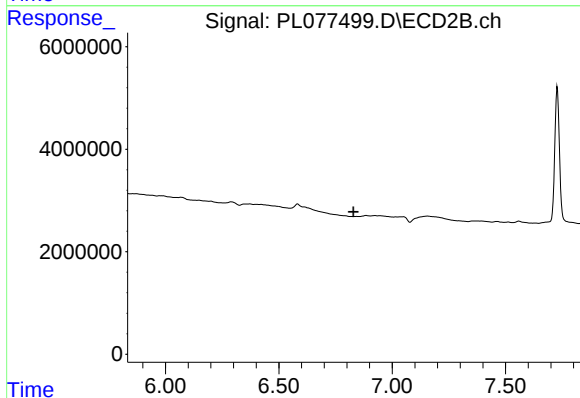


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 6.829 min
Response: 0
Conc: N.D.

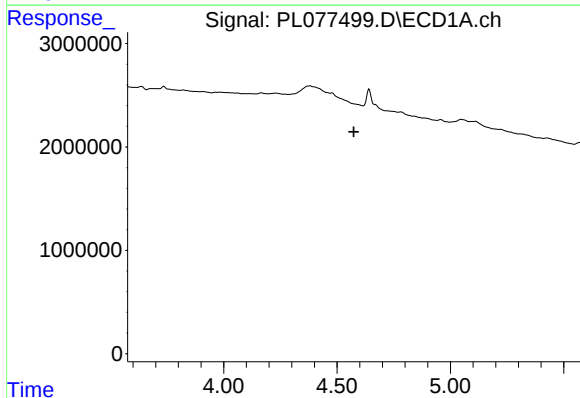


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.574 min
Response: 0
Conc: N.D.

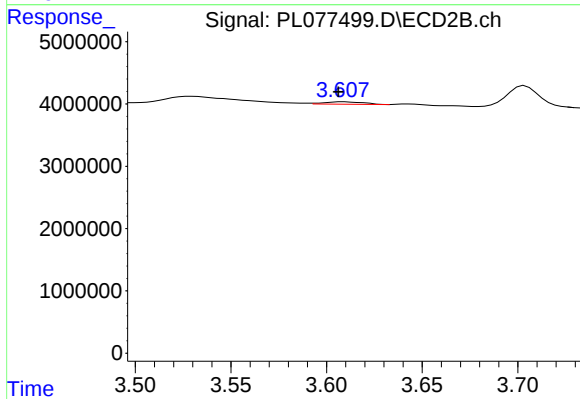

#23 Chlordane-1


R.T.: 3.608 min
Delta R.T.: 0.002 min
Response: 543910
Conc: 6.17 ng/ml

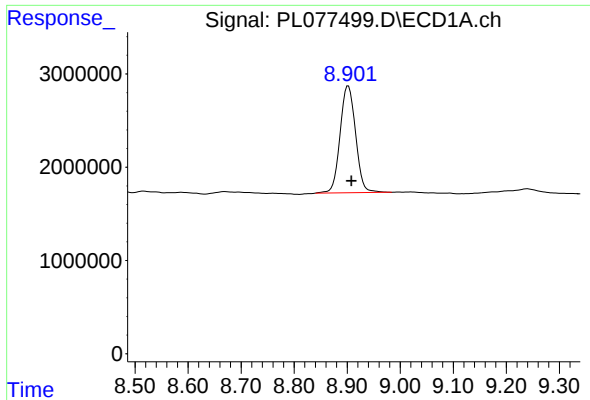

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: -0.006 min
Response: 23233779
Conc: 20.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

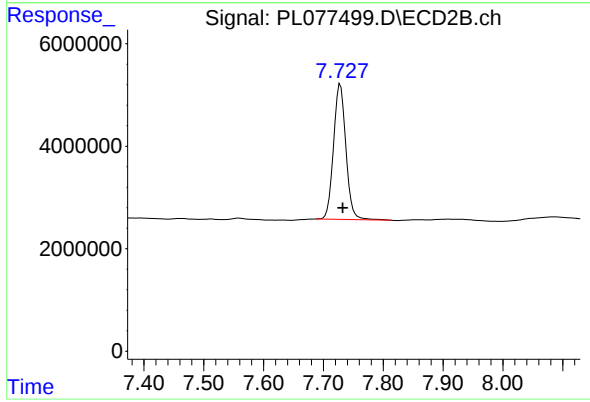

#28 Decachlorobiphenyl

R.T.: 7.728 min
Delta R.T.: -0.004 min
Response: 37957318
Conc: 16.08 ng/ml