

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2022 00:35
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:16:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 04:54:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.629	84723917	162.4E6	63.583	51.907
28)	SA Decachlor...	8.902	7.729	60247884	102.0E6	53.980	43.487
Target Compounds							
23)	Chlordane-1	4.575	3.607	32721643	50789285	647.657	575.810
24)	Chlordane-2	5.108	4.177	32168316	57840016	522.347	564.758
25)	Chlordane-3	5.820	4.801	122.3E6	169.3E6	599.031	562.469
26)	Chlordane-4	5.898	4.862	146.8E6	171.6E6	593.341	560.603
27)	Chlordane-5	6.756	5.526	19758517	42815098	475.119	556.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2022 00:35
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:16:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 04:54:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

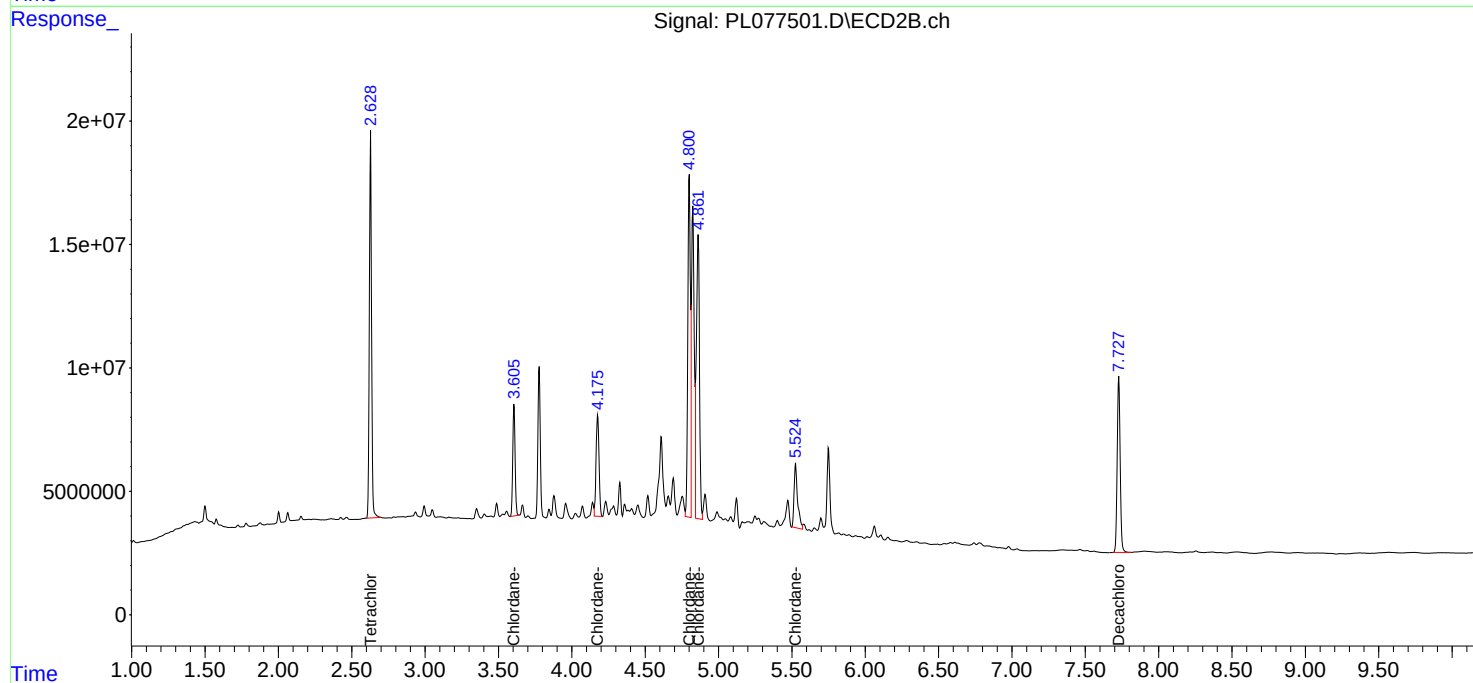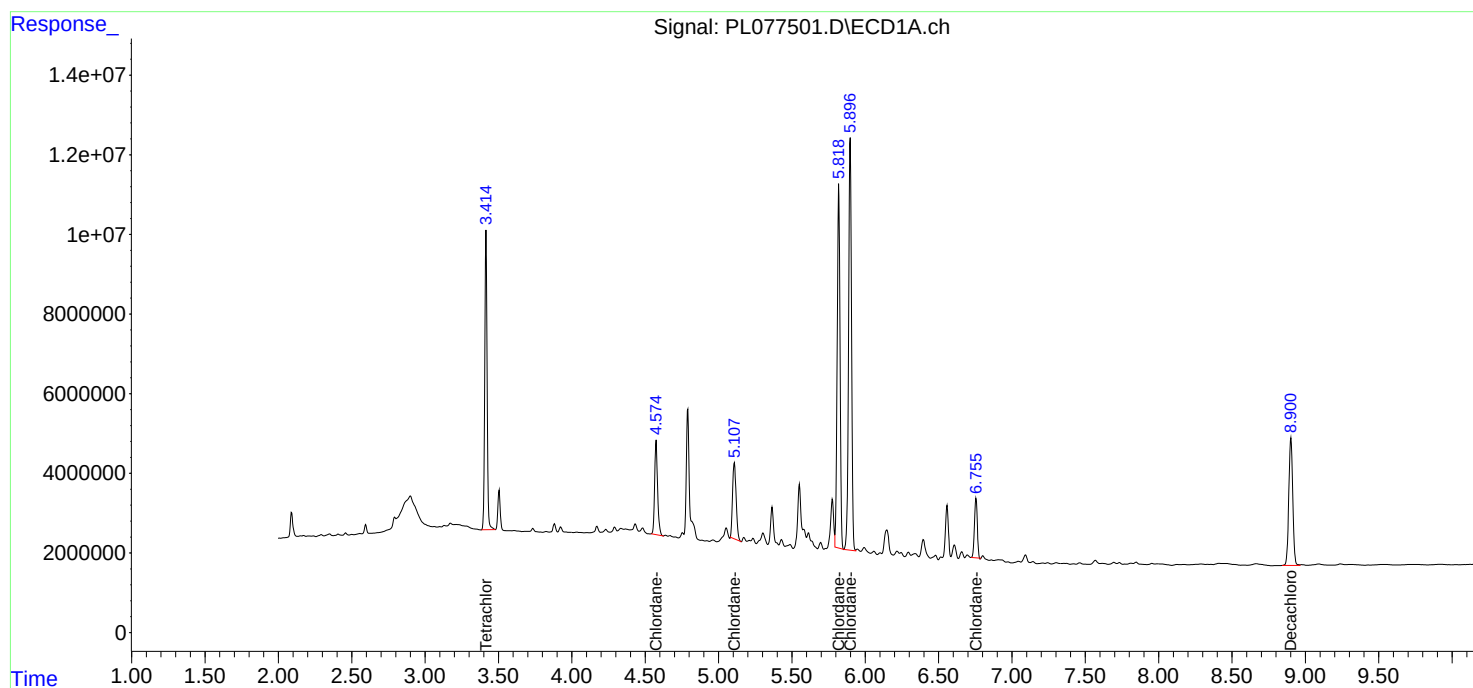


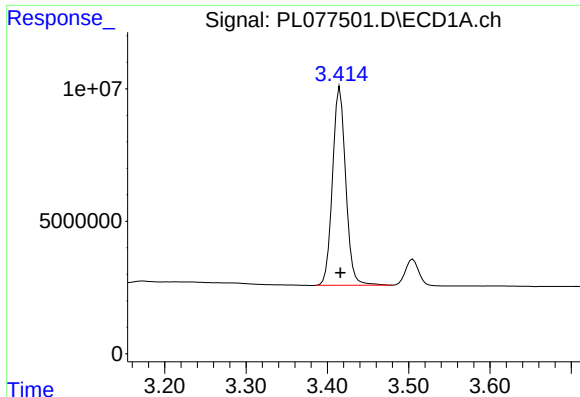

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 84723917
Conc: 63.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

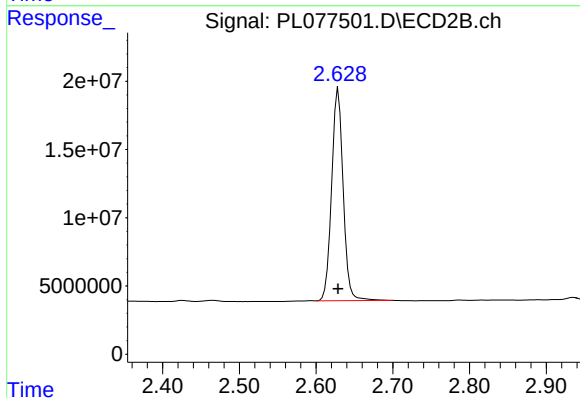


#1 Tetrachloro-m-xylene

R.T.: 2.629 min
Delta R.T.: 0.000 min
Response: 162406404
Conc: 51.91 ng/ml

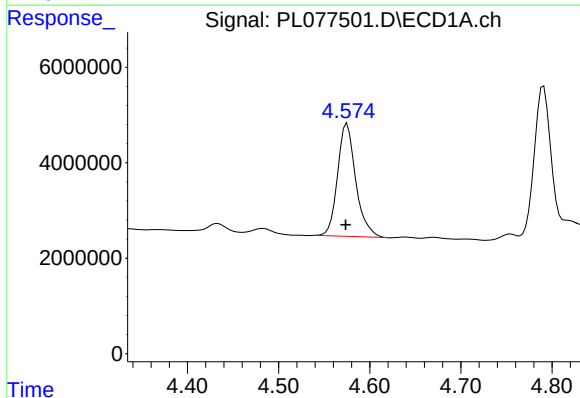


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.001 min
Response: 32721643
Conc: 647.66 ng/ml

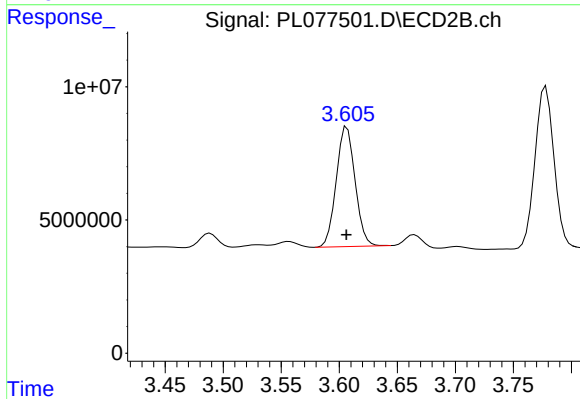

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 50789285
Conc: 575.81 ng/ml

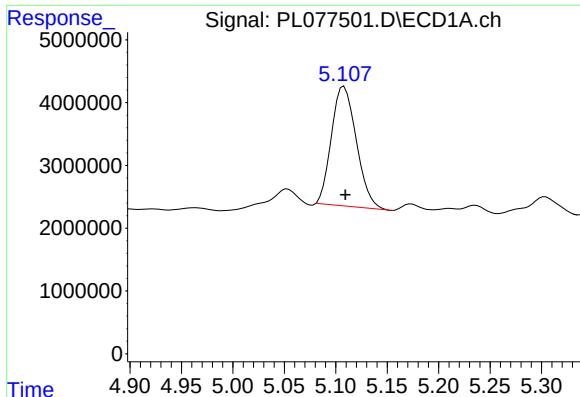

#24 Chlordane-2


R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 32168316
Conc: 522.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

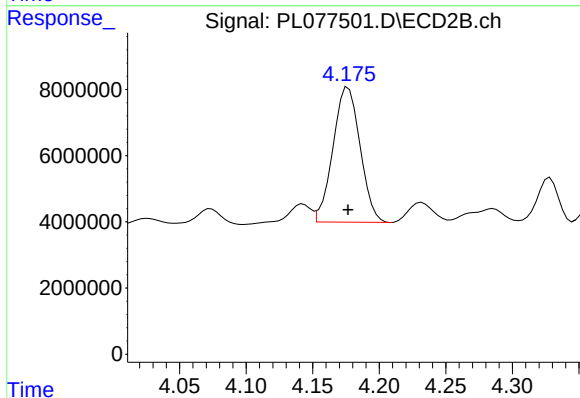


#24 Chlordane-2

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 57840016
Conc: 564.76 ng/ml

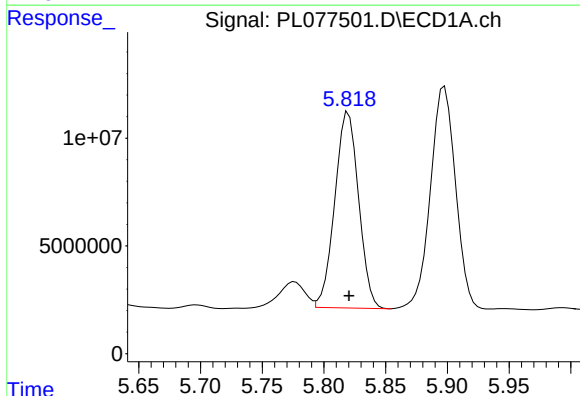


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 122258645
Conc: 599.03 ng/ml

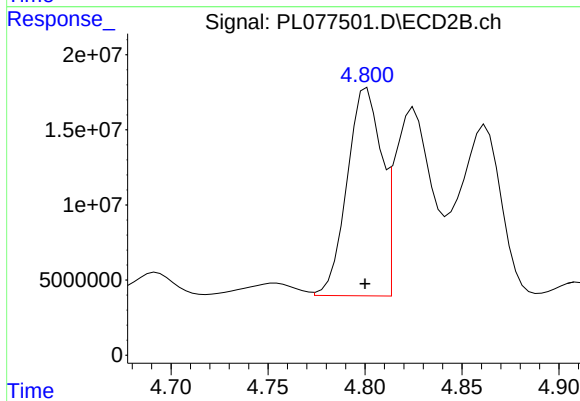

#25 Chlordane-3


R.T.: 4.801 min
Delta R.T.: 0.001 min
Response: 169255193
Conc: 562.47 ng/ml

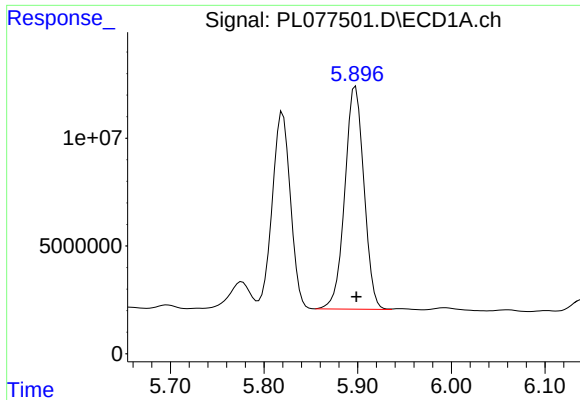

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 146796390
Conc: 593.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

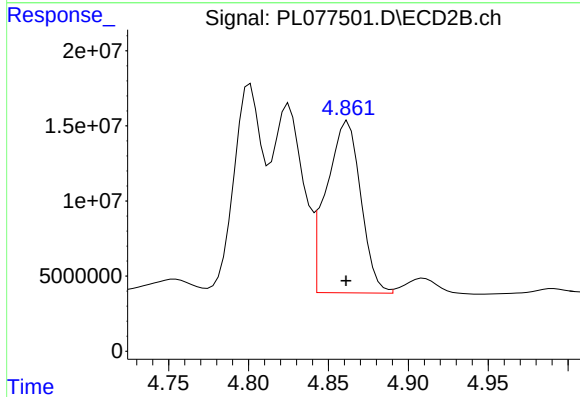


#26 Chlordane-4

R.T.: 4.862 min
Delta R.T.: 0.001 min
Response: 171600687
Conc: 560.60 ng/ml

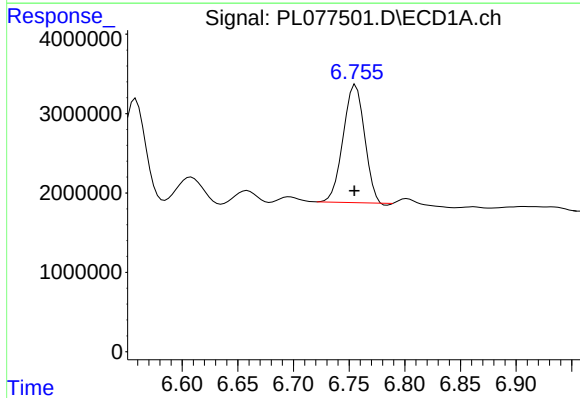


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.001 min
Response: 19758517
Conc: 475.12 ng/ml

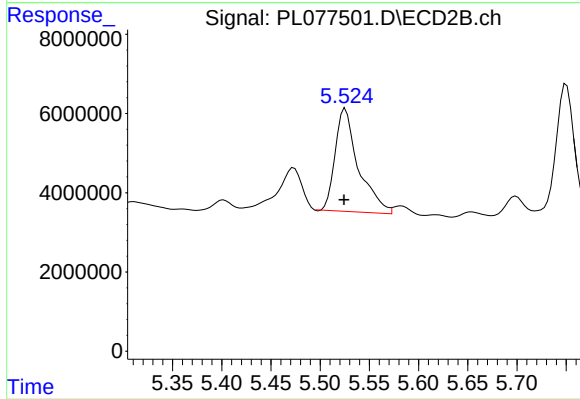

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: 0.001 min
Response: 42815098
Conc: 556.03 ng/ml

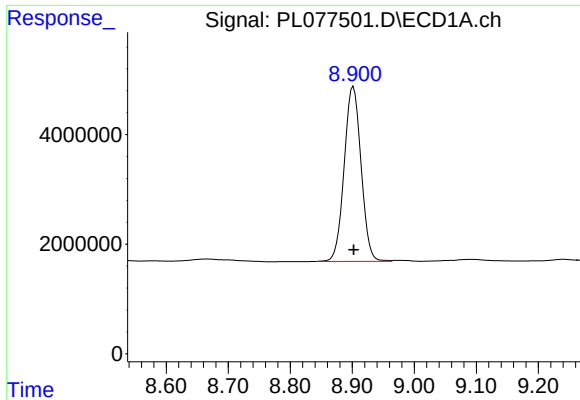

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 60247884
Conc: 53.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

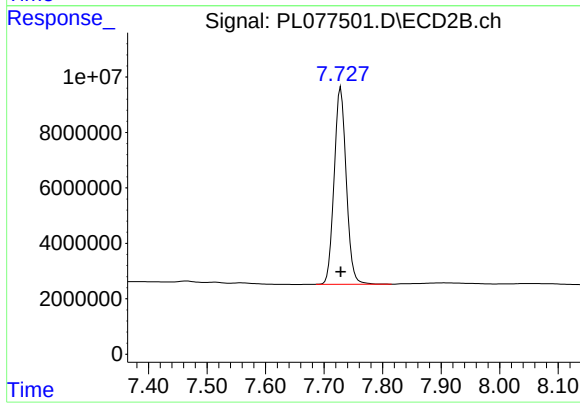

#28 Decachlorobiphenyl

R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 101988793
Conc: 43.49 ng/ml