

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 15:07
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 16:22:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 02 16:22:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.630	138.0E6	316.1E6	99.427	98.383
28)	SA Decachlor...	8.908	7.733	103.2E6	223.1E6	92.246	95.143
Target Compounds							
23)	Chlordane-1	4.578	3.609	53308173	88392263	999.855	969.584
24)	Chlordane-2	5.111	4.180	54507483	99215751	944.434	949.211
25)	Chlordane-3	5.823	4.804	212.9E6	299.1E6	1010.799	978.978
26)	Chlordane-4	5.902	4.865	255.4E6	310.7E6	996.385	988.252
27)	Chlordane-5	6.760	5.529	42003400	78473327	977.149	965.731



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 15:07
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 16:22:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Fri Sep 02 16:22:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

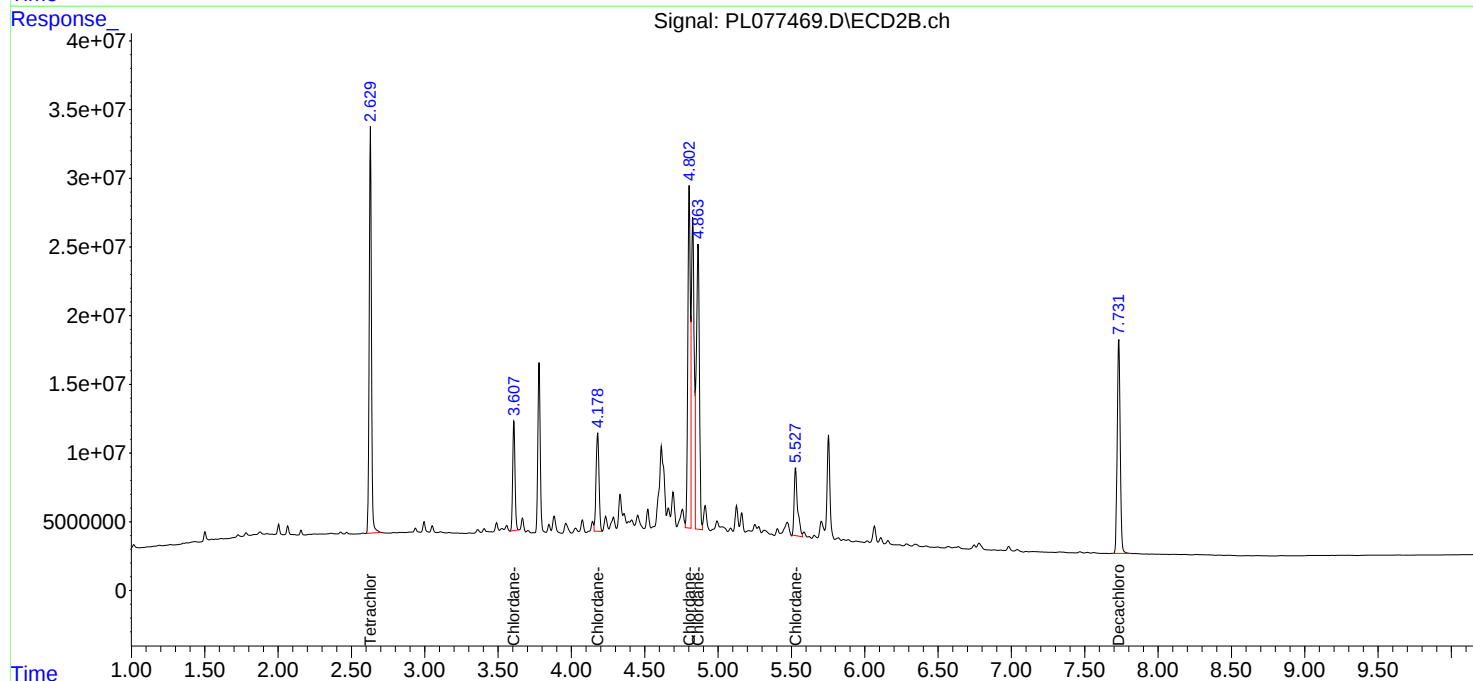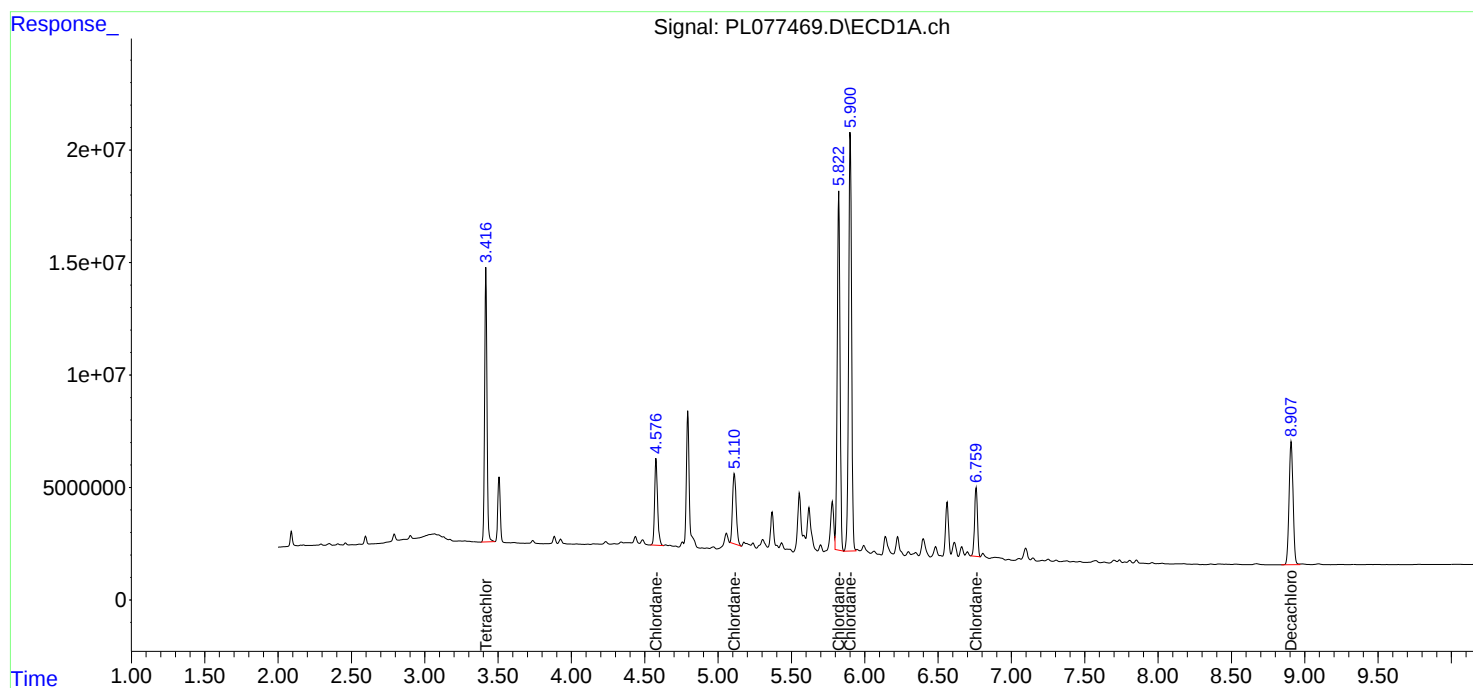


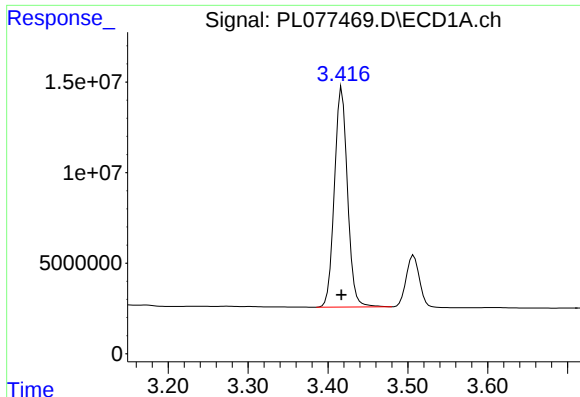

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 137966096
Conc: 99.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

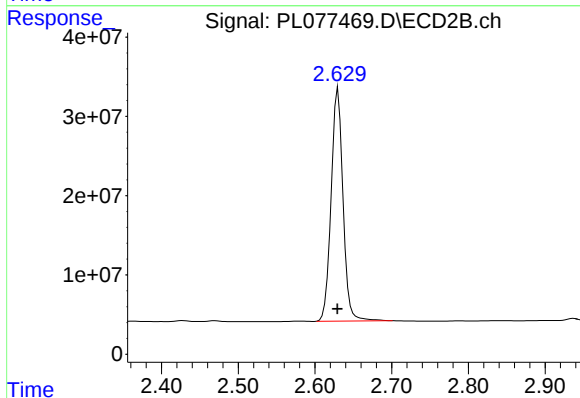


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 316121026
Conc: 98.38 ng/ml

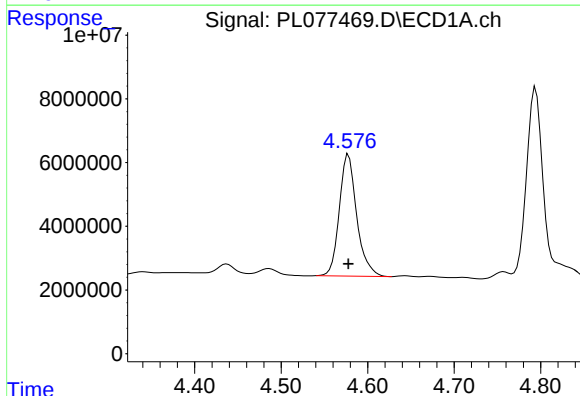


#23 Chlordane-1

R.T.: 4.578 min
Delta R.T.: 0.000 min
Response: 53308173
Conc: 999.85 ng/ml

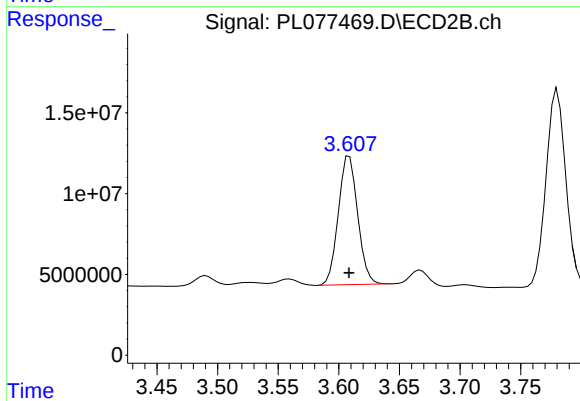

#23 Chlordane-1


R.T.: 3.609 min
Delta R.T.: 0.000 min
Response: 88392263
Conc: 969.58 ng/ml

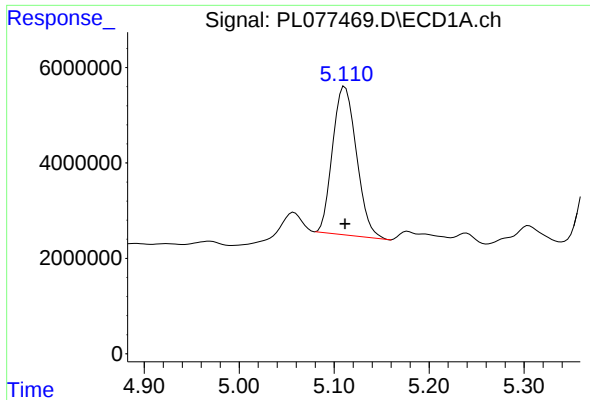

#24 Chlordane-2


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 54507483
Conc: 944.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

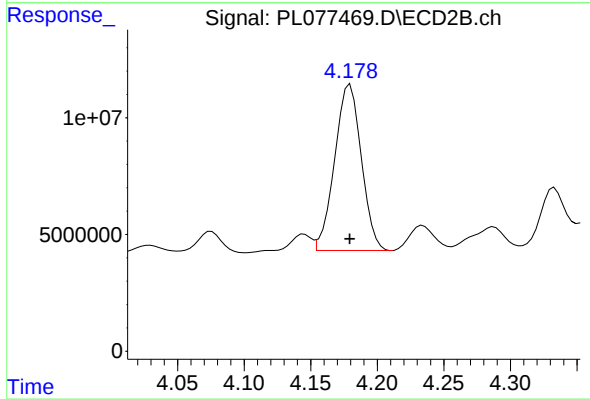


#24 Chlordane-2

R.T.: 4.180 min
Delta R.T.: 0.000 min
Response: 99215751
Conc: 949.21 ng/ml

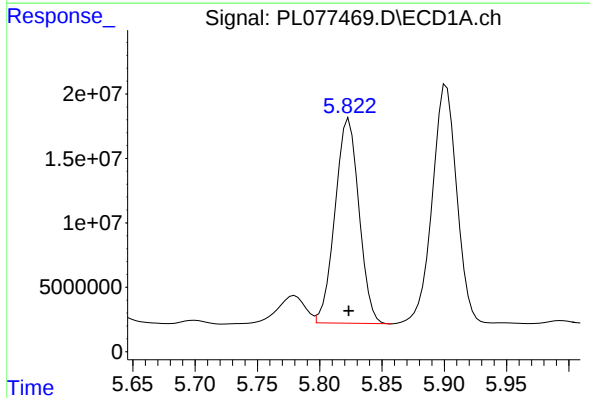


#25 Chlordane-3

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 212906607
Conc: 1010.80 ng/ml

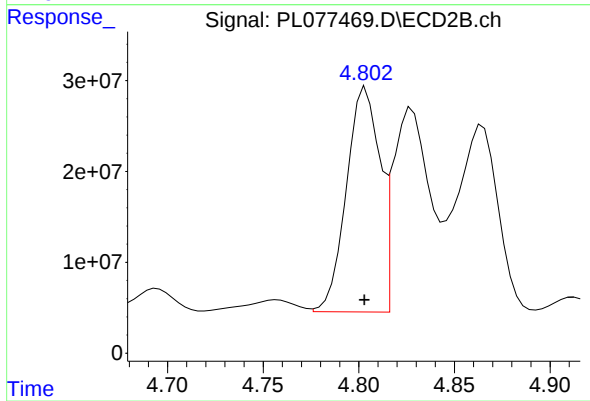

#25 Chlordane-3


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 299127458
Conc: 978.98 ng/ml

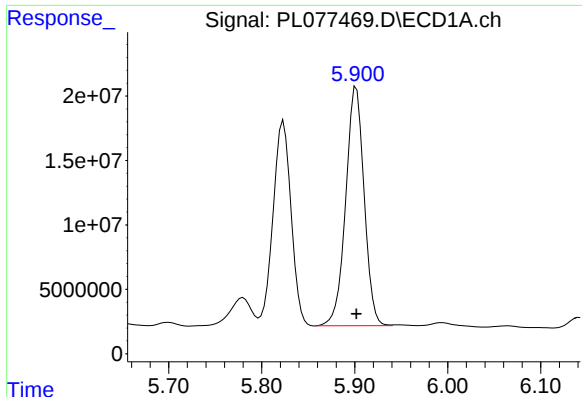

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 255367601
Conc: 996.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

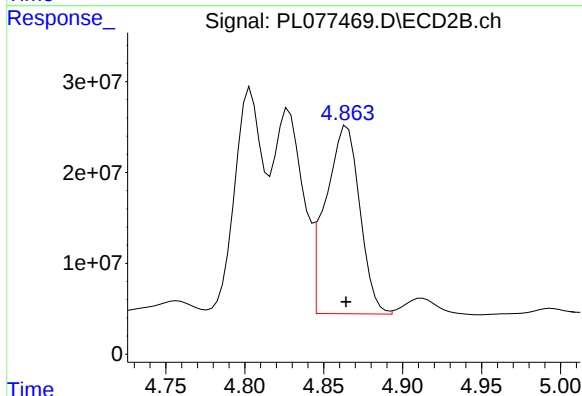


#26 Chlordane-4

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 310666017
Conc: 988.25 ng/ml

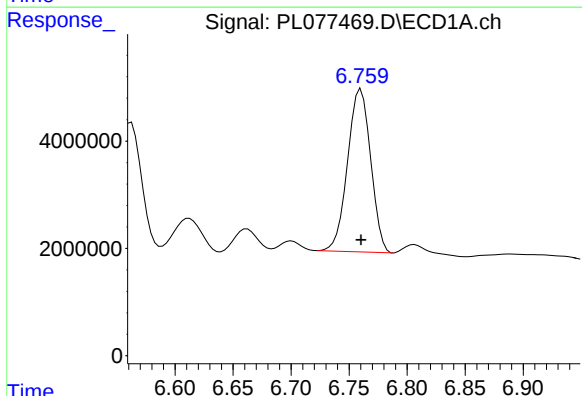


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 42003400
Conc: 977.15 ng/ml

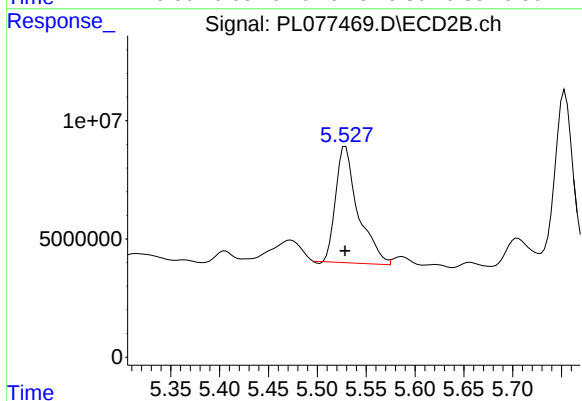

#27 Chlordane-5


R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 78473327
Conc: 965.73 ng/ml

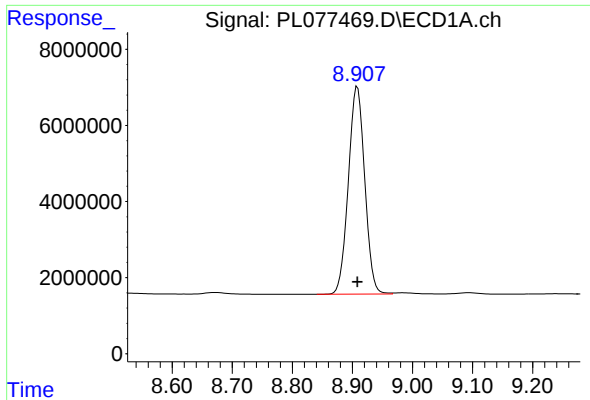

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 103156196
Conc: 92.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

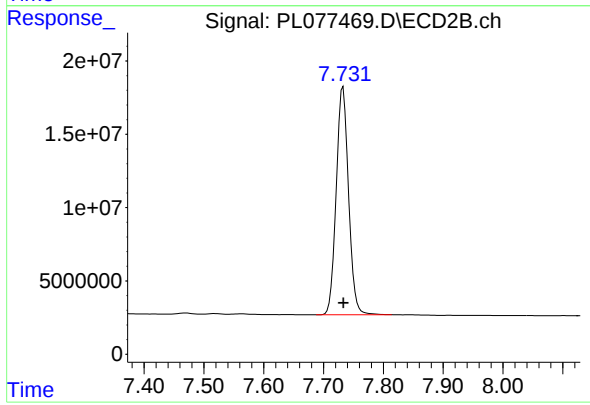

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 223145722
Conc: 95.14 ng/ml