

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 15:21
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 16:22:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 02 16:22:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.630	98204849	225.3E6	70.773	70.129
28)	SA Decachlor...	8.908	7.733	76014530	162.6E6	67.975	69.332
Target Compounds							
23)	Chlordane-1	4.578	3.608	37603462	63493573	705.295	696.468
24)	Chlordane-2	5.112	4.179	39992061	71972030	692.930	688.567
25)	Chlordane-3	5.824	4.803	150.8E6	214.2E6	715.996	700.880
26)	Chlordane-4	5.902	4.864	181.1E6	221.3E6	706.672	703.999
27)	Chlordane-5	6.760	5.528	30188148	56950281	702.284	700.858



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 15:21
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 16:22:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Fri Sep 02 16:22:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

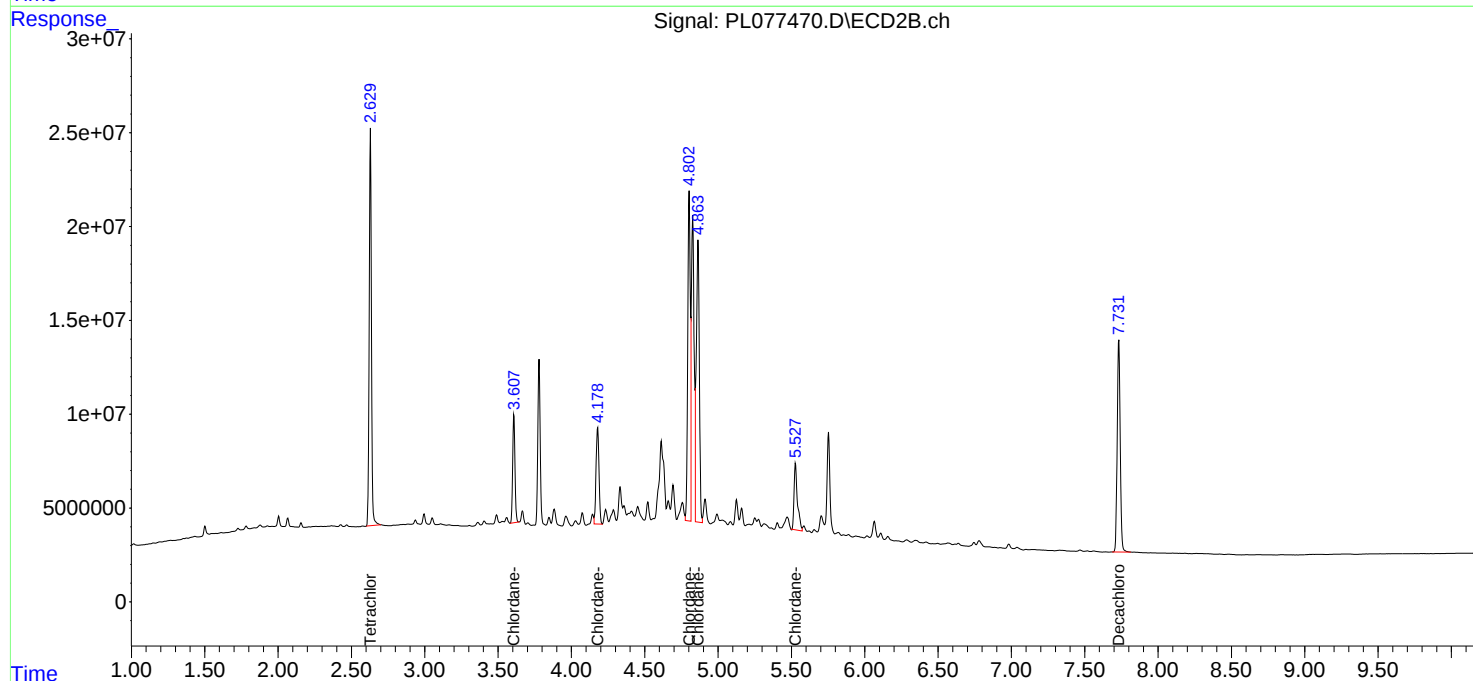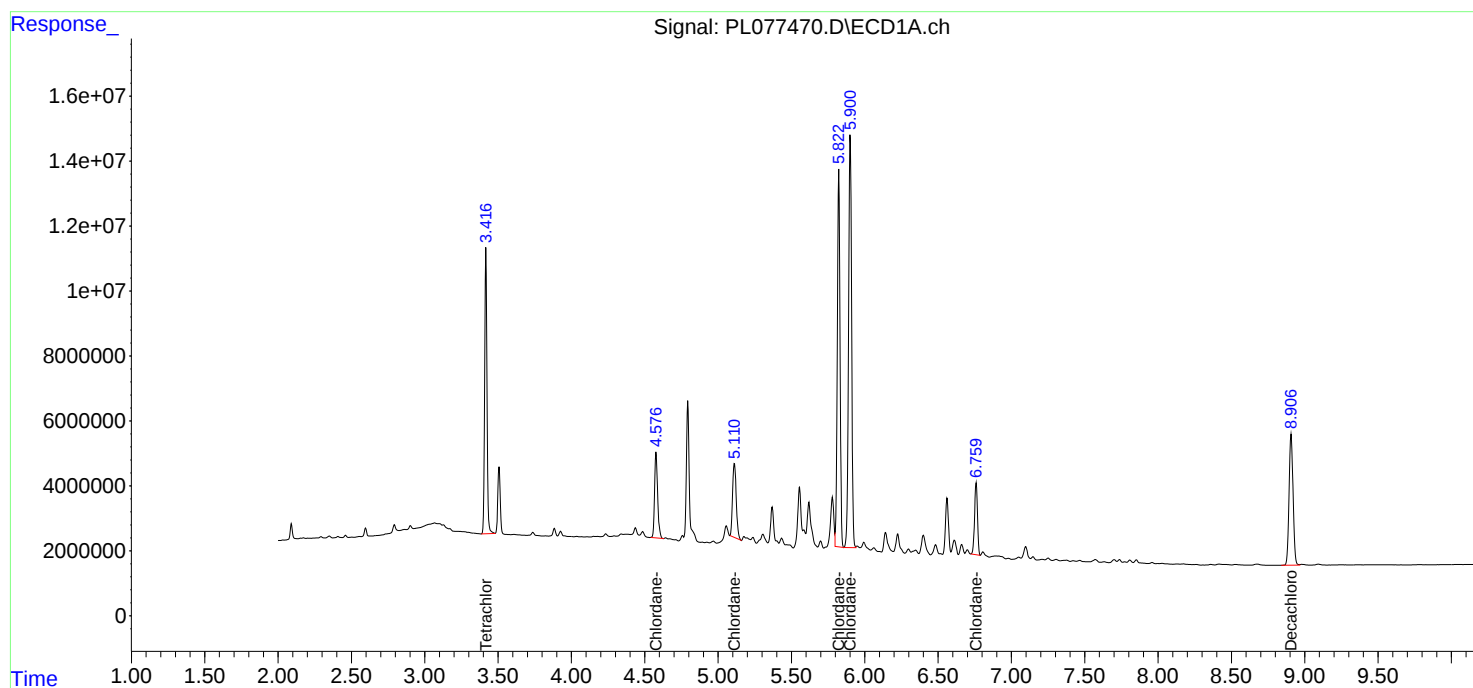


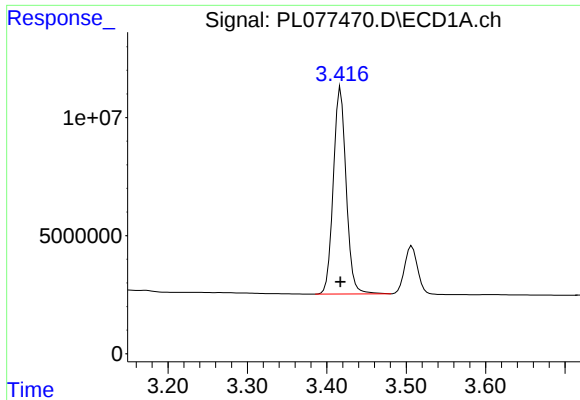

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 98204849
Conc: 70.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

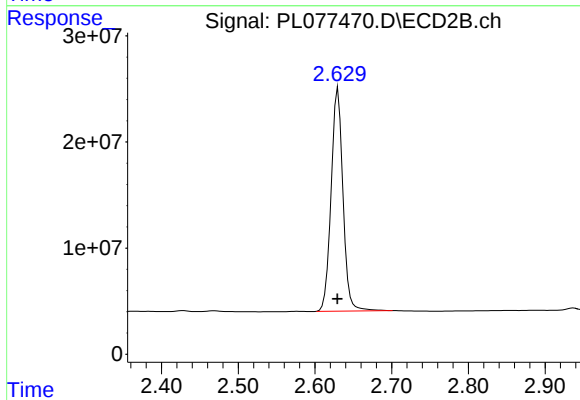


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 225335904
Conc: 70.13 ng/ml

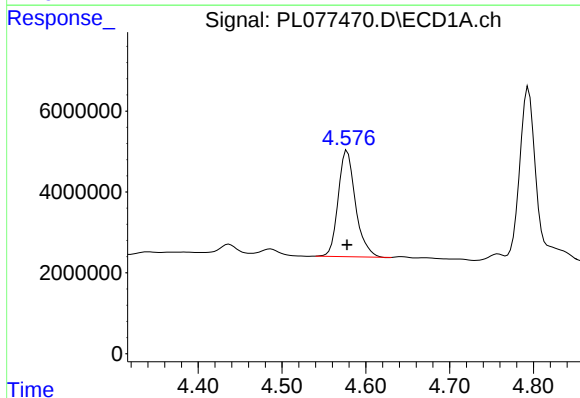


#23 Chlordane-1

R.T.: 4.578 min
Delta R.T.: 0.000 min
Response: 37603462
Conc: 705.30 ng/ml

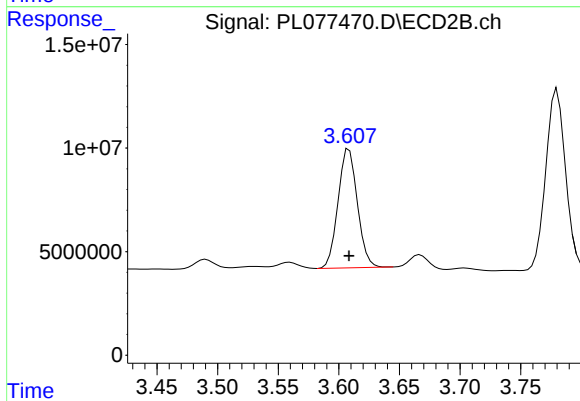

#23 Chlordane-1


R.T.: 3.608 min
Delta R.T.: 0.000 min
Response: 63493573
Conc: 696.47 ng/ml

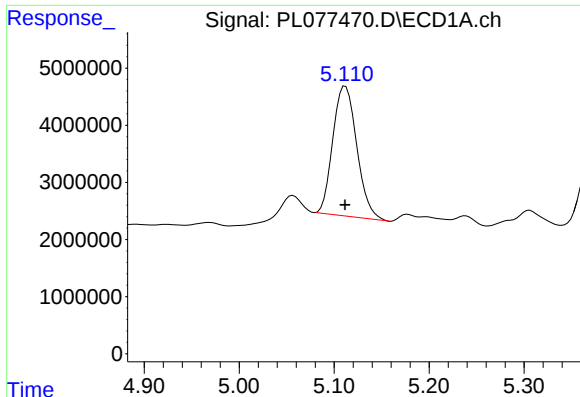

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 39992061
Conc: 692.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

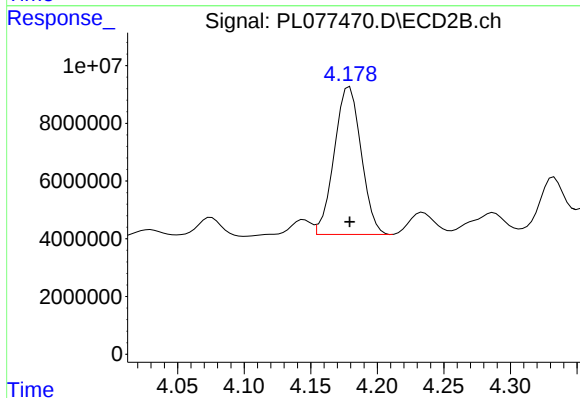


#24 Chlordane-2

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 71972030
Conc: 688.57 ng/ml

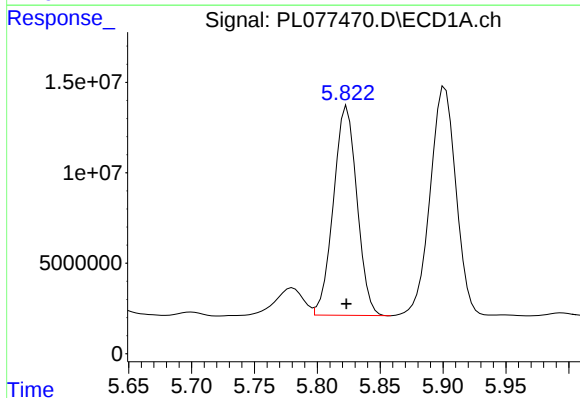


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 150811573
Conc: 716.00 ng/ml

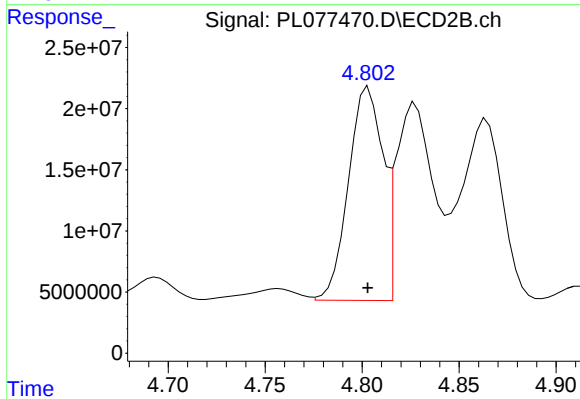

#25 Chlordane-3


R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 214154268
Conc: 700.88 ng/ml

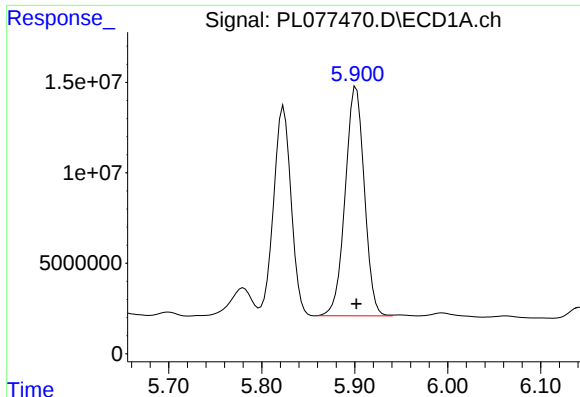

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 181116046
Conc: 706.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

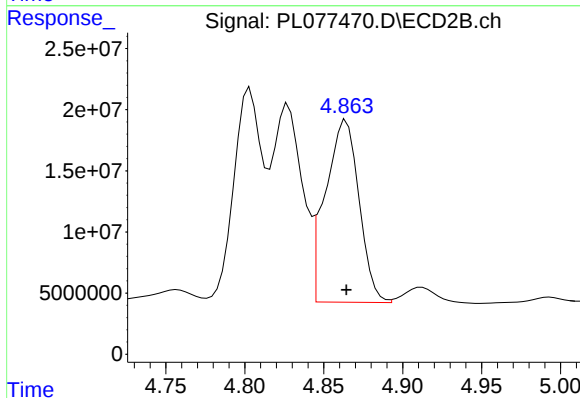


#26 Chlordane-4

R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 221308413
Conc: 704.00 ng/ml

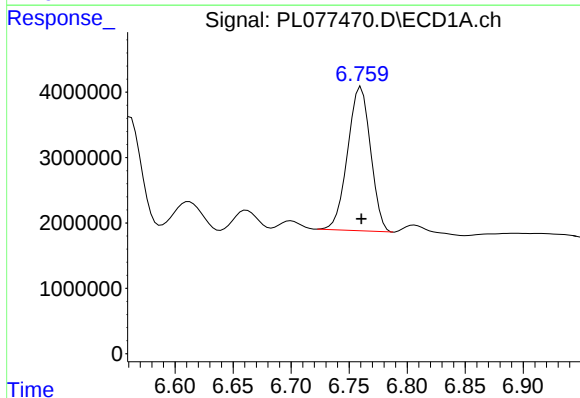


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 30188148
Conc: 702.28 ng/ml

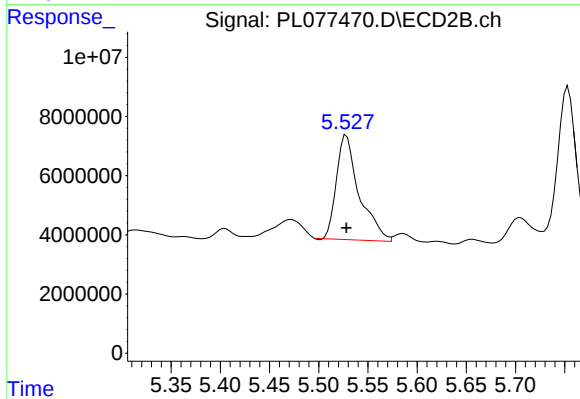

#27 Chlordane-5


R.T.: 5.528 min
Delta R.T.: 0.000 min
Response: 56950281
Conc: 700.86 ng/ml

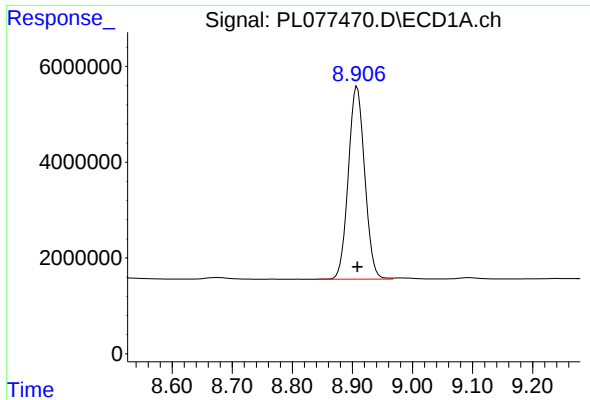

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 76014530
Conc: 67.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

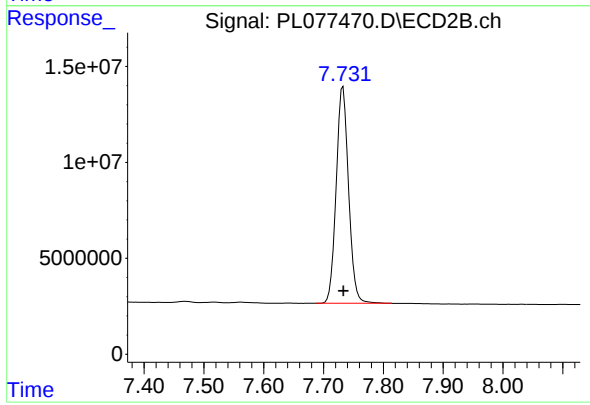

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 162610723
Conc: 69.33 ng/ml