

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
 Data File : PL077480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 18:20
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL090222CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 05:02:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 04:54:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.628	69383368	163.9E6	52.071	52.373
28)	SA Decachlor...	8.903	7.728	56344311	122.7E6	50.482	52.319
Target Compounds							
23)	Chlordane-1	4.575	3.606	26831639	47245316	531.077	535.631
24)	Chlordane-2	5.108	4.176	28507077	53484444	462.896	522.229
25)	Chlordane-3	5.820	4.800	106.7E6	157.8E6	522.967	524.410
26)	Chlordane-4	5.898	4.861	129.1E6	165.1E6	521.960	539.280
27)	Chlordane-5	6.756	5.525	21229665	44011556	510.495	571.568



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090222\
Data File : PL077480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 18:20
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL090222CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 05:02:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 04:54:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

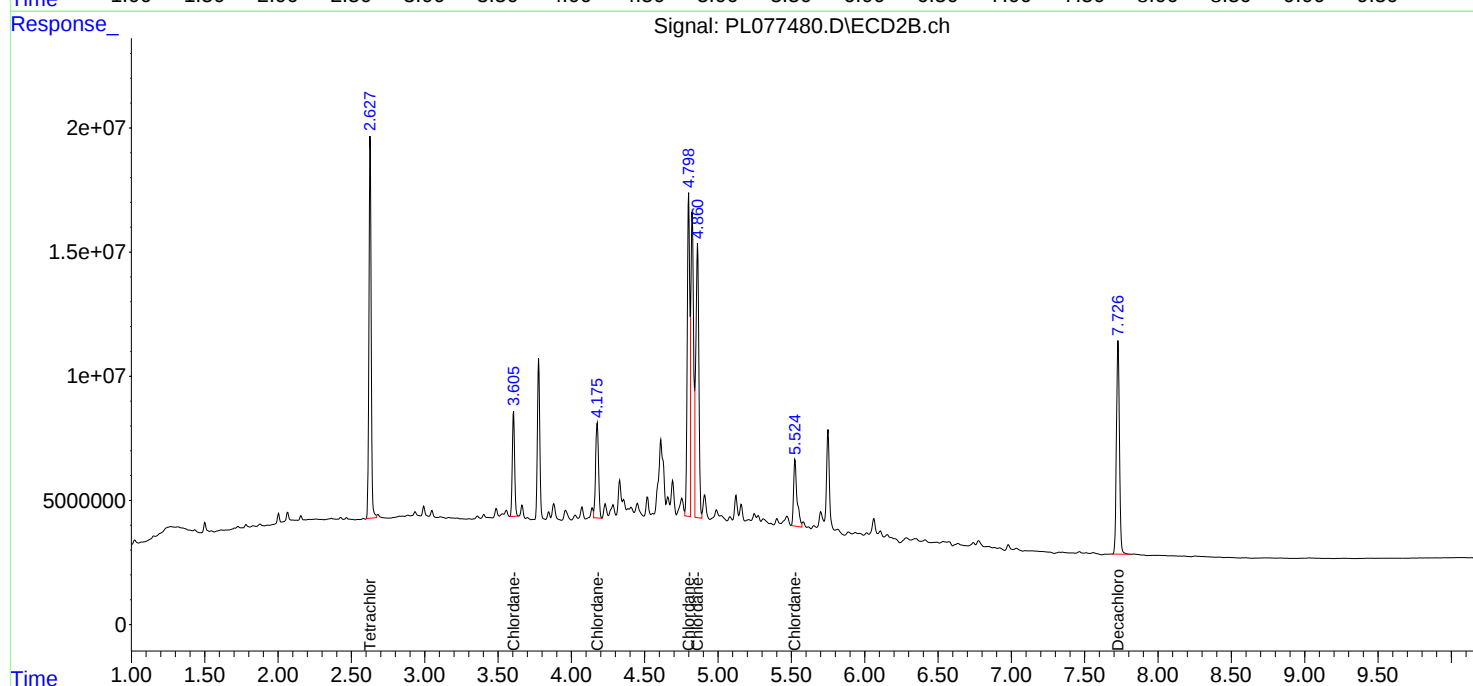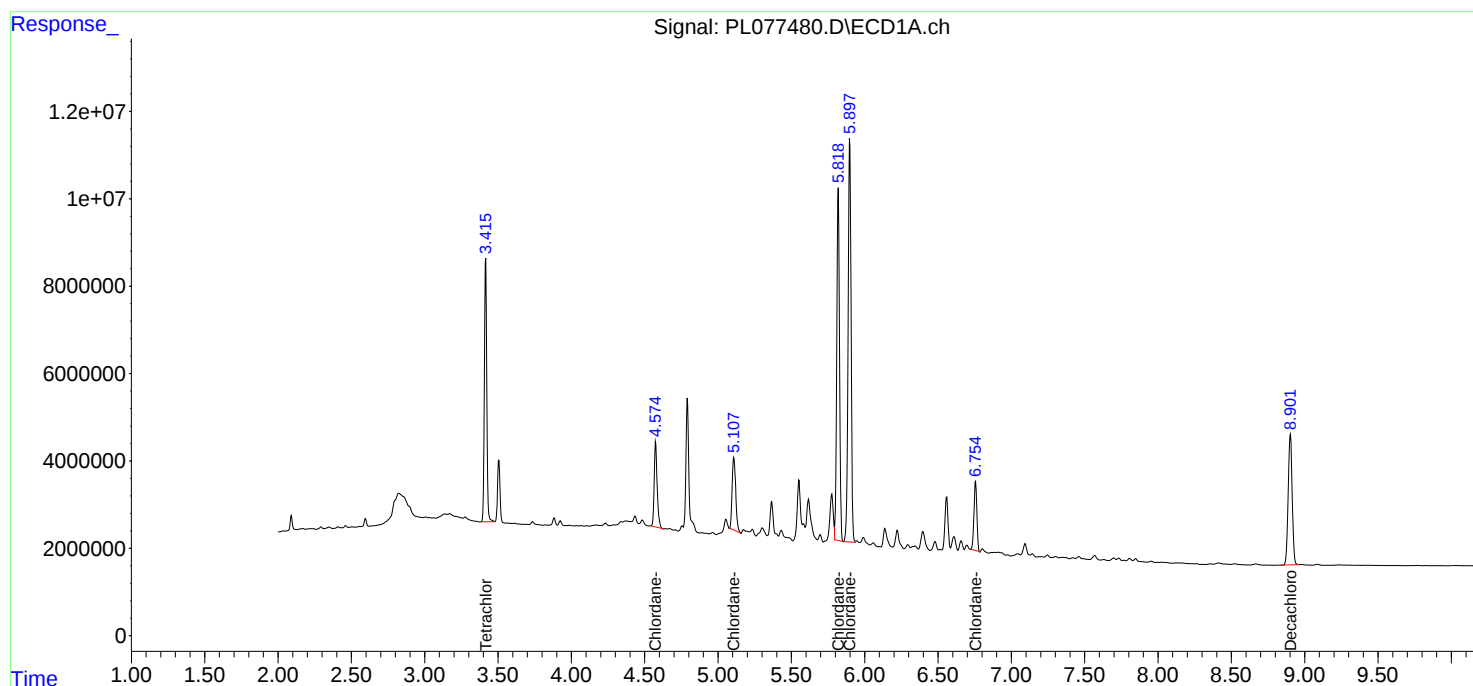


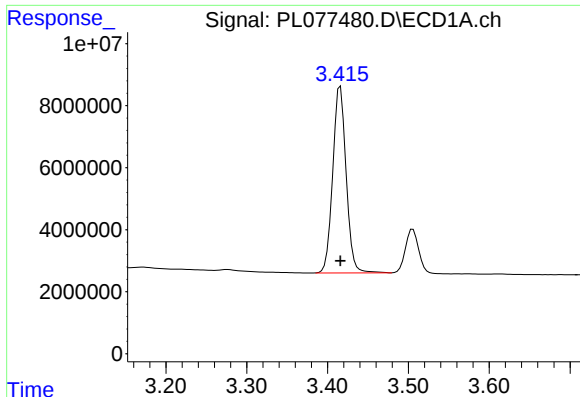

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 69383368
Conc: 52.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090222CHLOR

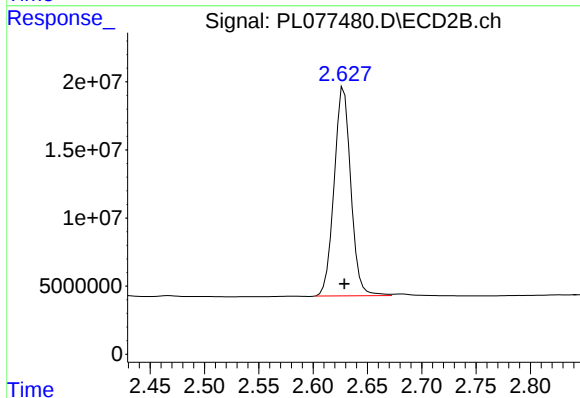


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 163864941
Conc: 52.37 ng/ml

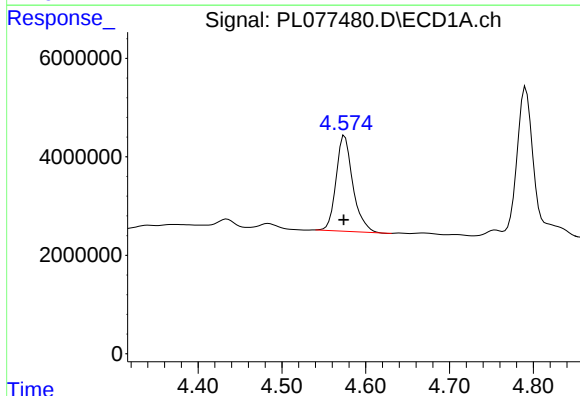


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.001 min
Response: 26831639
Conc: 531.08 ng/ml

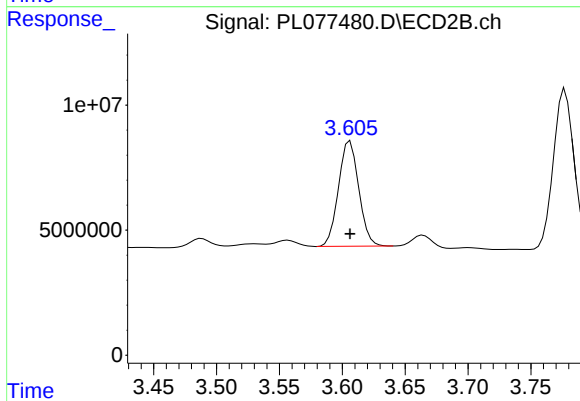

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 47245316
Conc: 535.63 ng/ml

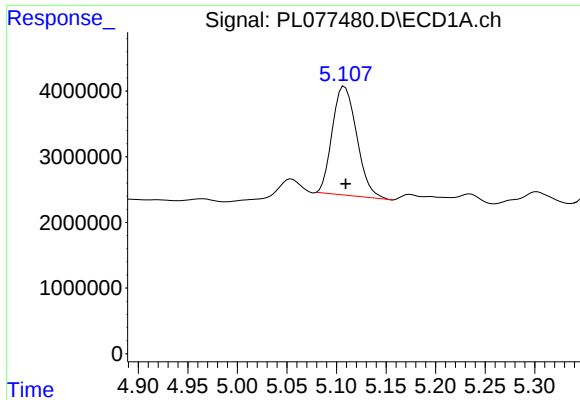

#24 Chlordane-2


R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 28507077
Conc: 462.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090222CHLOR

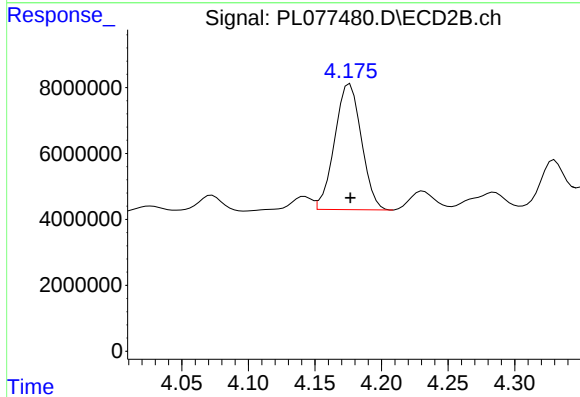


#24 Chlordane-2

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 53484444
Conc: 522.23 ng/ml

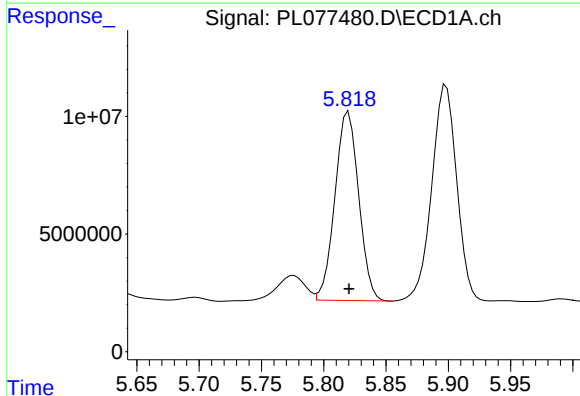


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 106734422
Conc: 522.97 ng/ml

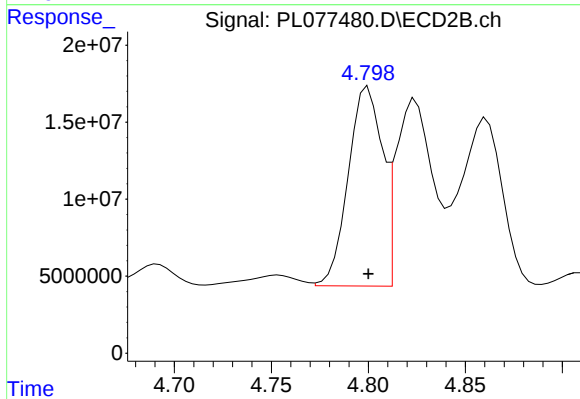

#25 Chlordane-3


R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 157802442
Conc: 524.41 ng/ml

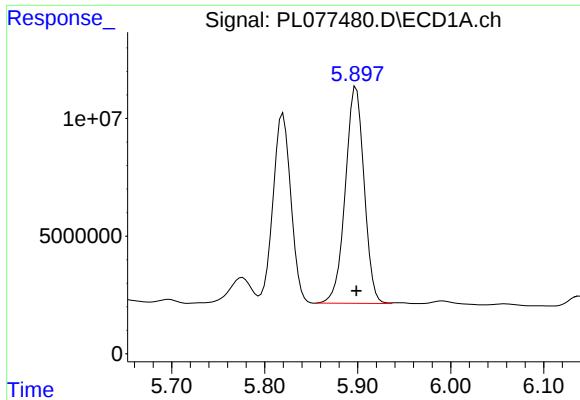

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 129136413
Conc: 521.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090222CHLOR

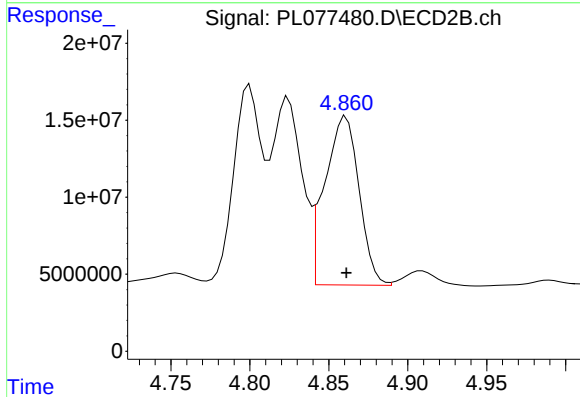


#26 Chlordane-4

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 165073704
Conc: 539.28 ng/ml

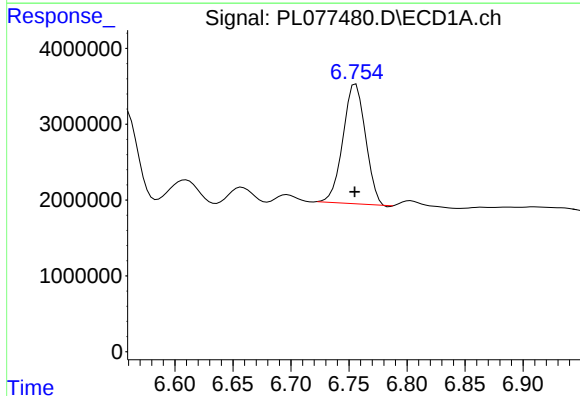


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 21229665
Conc: 510.49 ng/ml

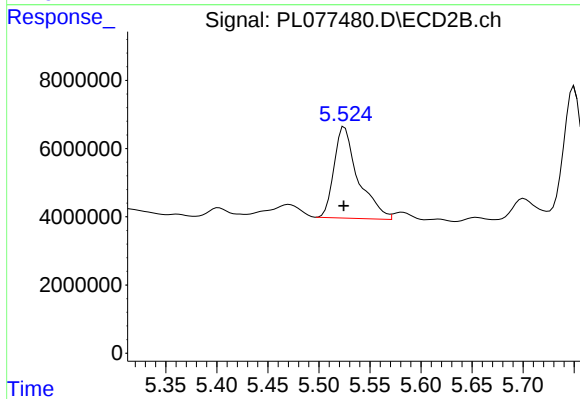

#27 Chlordane-5


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 44011556
Conc: 571.57 ng/ml

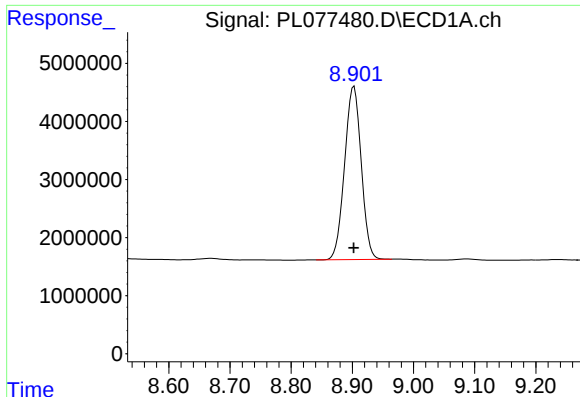

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: 0.000 min
Response: 56344311
Conc: 50.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090222CHLOR

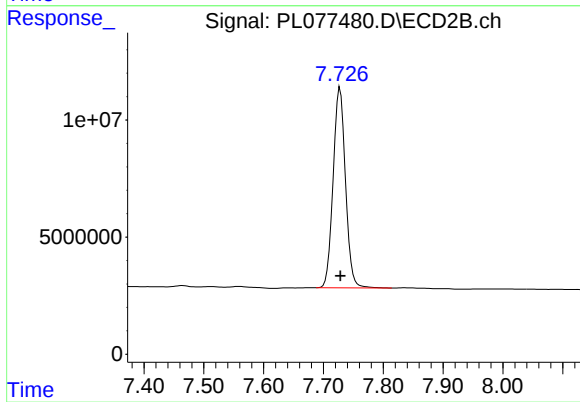

#28 Decachlorobiphenyl

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 122702868
Conc: 52.32 ng/ml