

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
 Data File : PL061217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 13:10
 Operator : DD\AJ
 Sample : L3896-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 16:24:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.009	20758998	27954047	11.249	10.756
28)	SA Decachlor...	8.212	9.098	19809182	20075659	11.759	9.514
Target Compounds							
2)	A alpha-BHC	0.000	4.425f	0	6644586	N.D.	1.636 #
11)	B alpha-Chl...	0.000	6.198	0	2896486	N.D.	0.932 #
24)	Chlordane-2	4.811f	0.000	9343970	0	145.292	N.D. #
26)	Chlordane-4	0.000	6.198	0	2896486	N.D.	6.025 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
Data File : PL061217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 13:10
Operator : DD\AJ
Sample : L3896-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:24:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

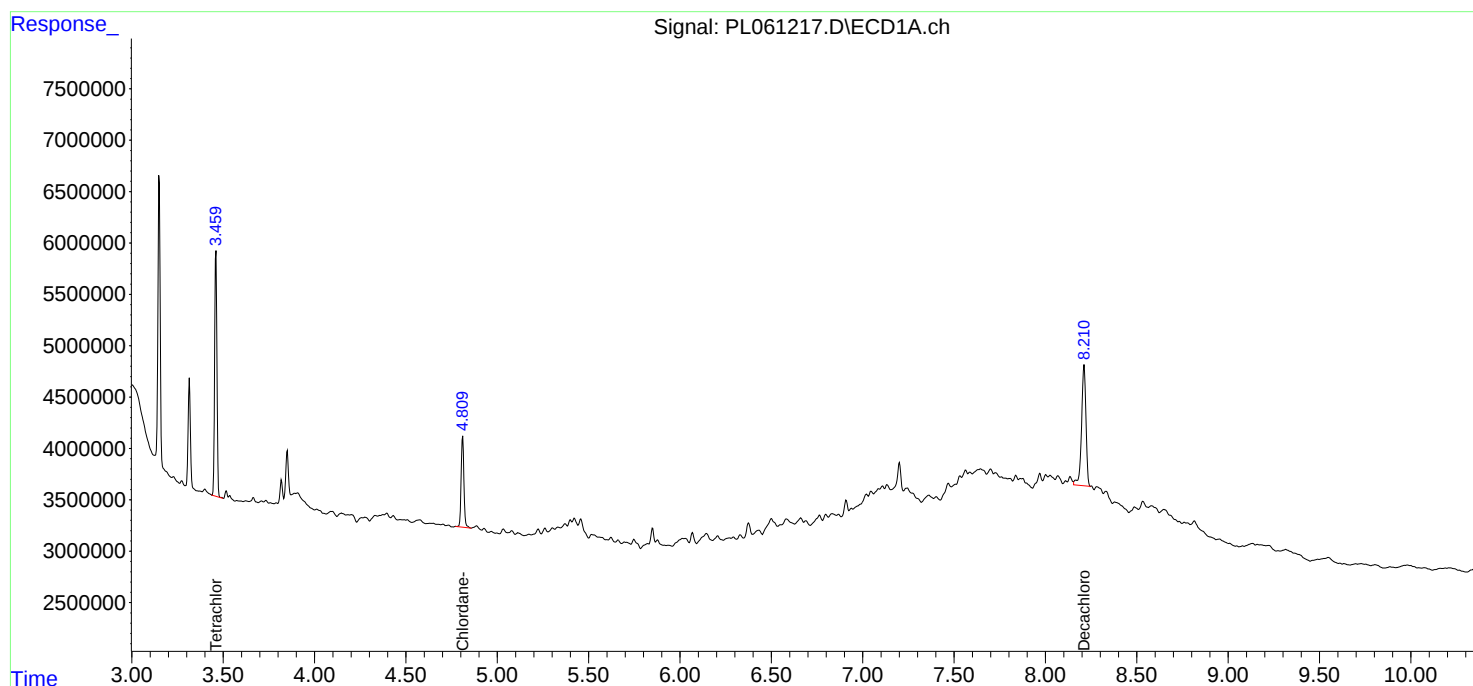


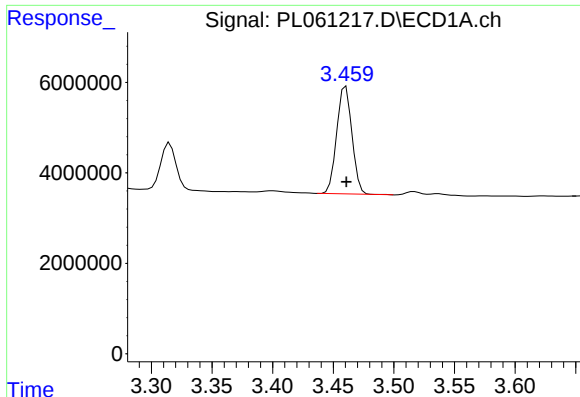

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 20758998
Conc: 11.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

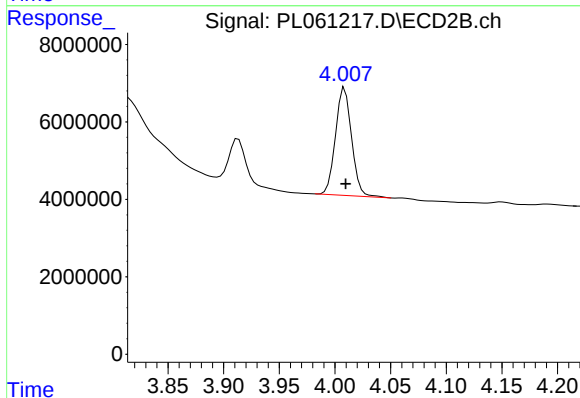


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 27954047
Conc: 10.76 ng/ml

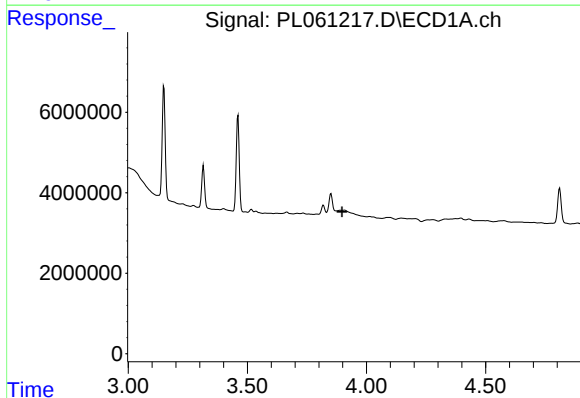


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.898 min
Response: 0
Conc: N.D.

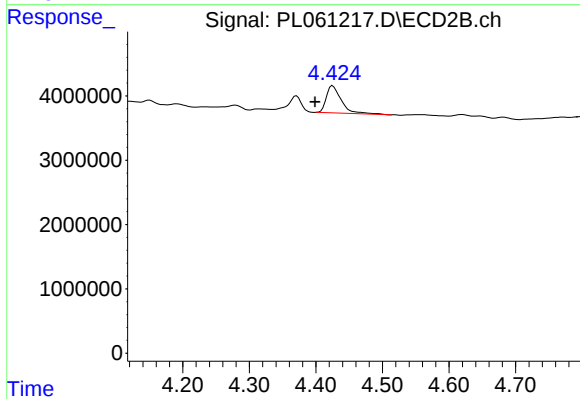

#2 alpha-BHC


R.T.: 4.425 min
Delta R.T.: 0.026 min
Response: 6644586
Conc: 1.64 ng/ml

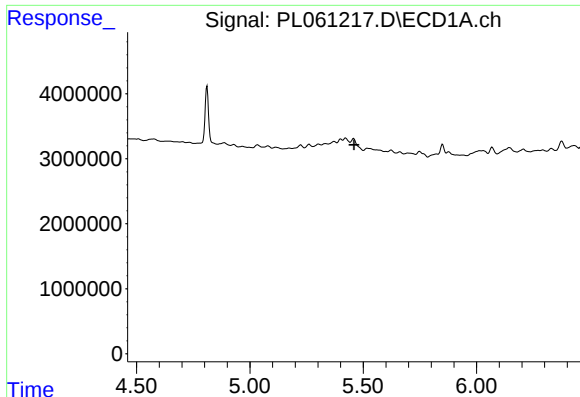

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

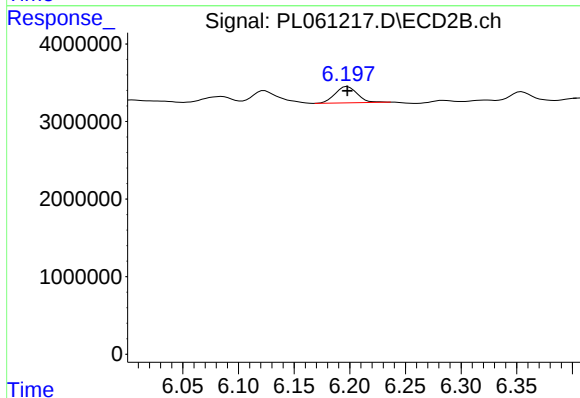


#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 2896486
Conc: 0.93 ng/ml

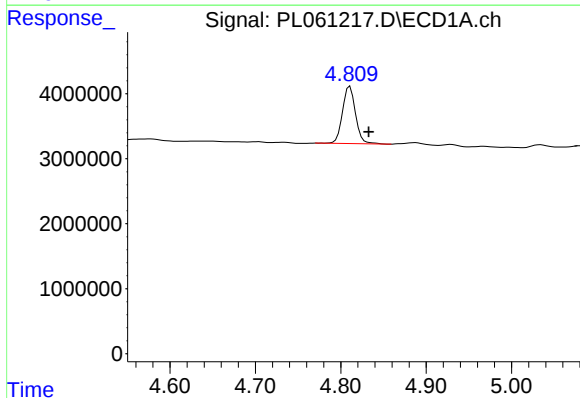


#24 Chlordane-2

R.T.: 4.811 min
Delta R.T.: -0.022 min
Response: 9343970
Conc: 145.29 ng/ml

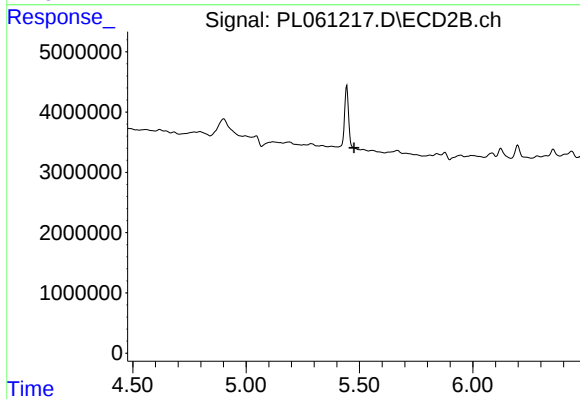

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.476 min
Response: 0
Conc: N.D.

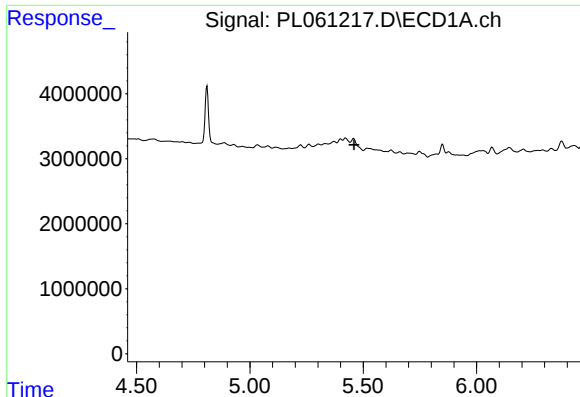

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

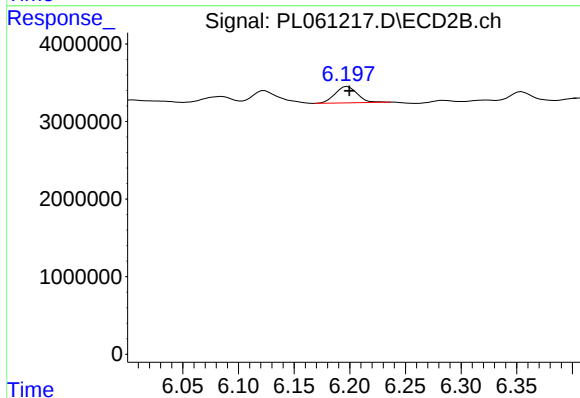


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: -0.002 min
Response: 2896486
Conc: 6.03 ng/ml

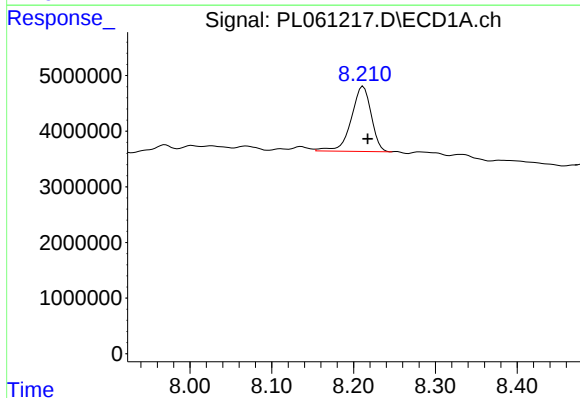

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.005 min
Response: 19809182
Conc: 11.76 ng/ml

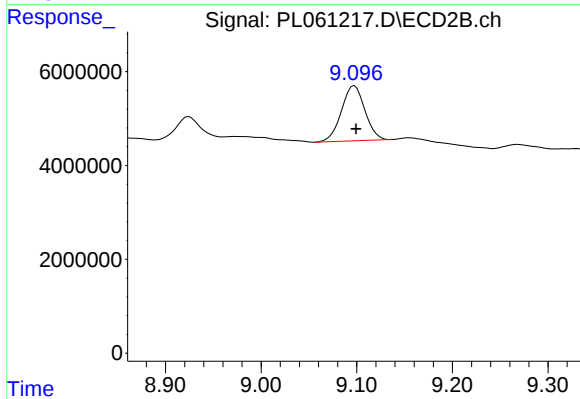

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.001 min
Response: 20075659
Conc: 9.51 ng/ml