

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
 Data File : PL061218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 13:25
 Operator : DD\AJ
 Sample : L3866-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 16:25:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	27056334	33465233	14.662	12.876
28)	SA Decachlor...	8.215	9.099	25491213	29821603	15.132	14.133
Target Compounds							
9)	A Endosulfan I	5.526	0.000	9382820	0	5.164	N.D. #
10)	B gamma-Chl...	0.000	6.125	0	5681865	N.D.	1.829 #
11)	B alpha-Chl...	0.000	6.199	0	4962481	N.D.	1.596 #
23)	Chlordane-1	4.328	0.000	5891506	0	96.491	N.D. #
25)	Chlordane-3	0.000	6.125	0	5681865	N.D.	14.216 #
26)	Chlordane-4	0.000	6.199	0	4962481	N.D.	10.323 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
Data File : PL061218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 13:25
Operator : DD\AJ
Sample : L3866-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:25:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

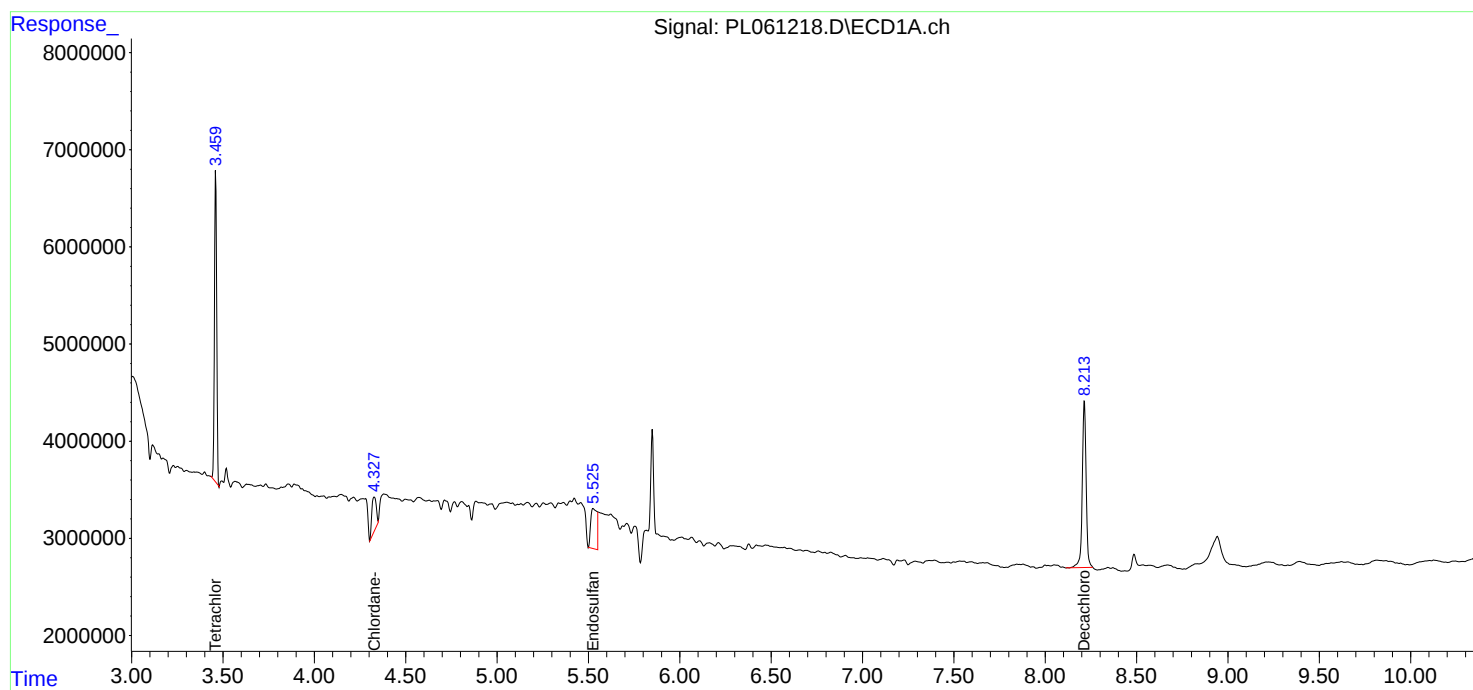


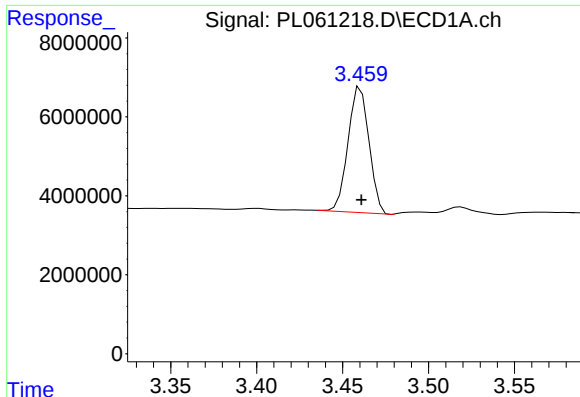

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 27056334
Conc: 14.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

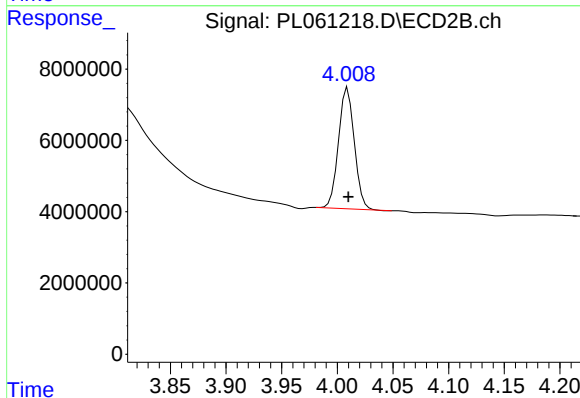


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 33465233
Conc: 12.88 ng/ml

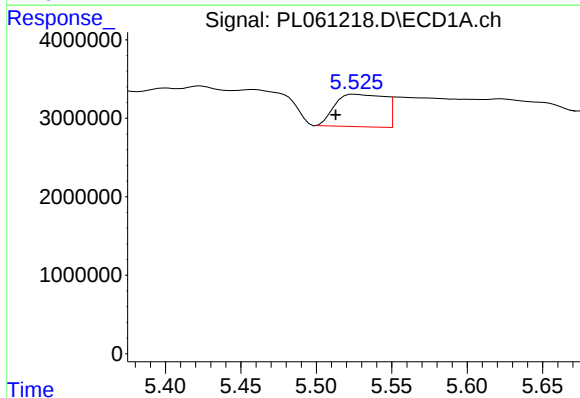


#9 Endosulfan I

R.T.: 5.526 min
Delta R.T.: 0.013 min
Response: 9382820
Conc: 5.16 ng/ml

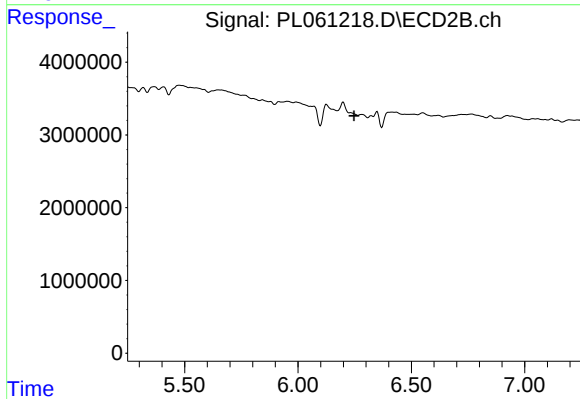

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.248 min
Response: 0
Conc: N.D.

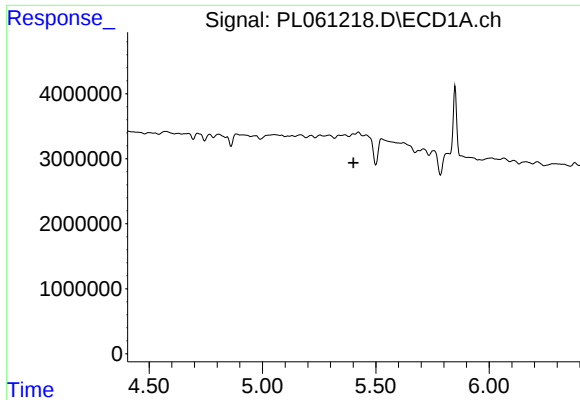

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

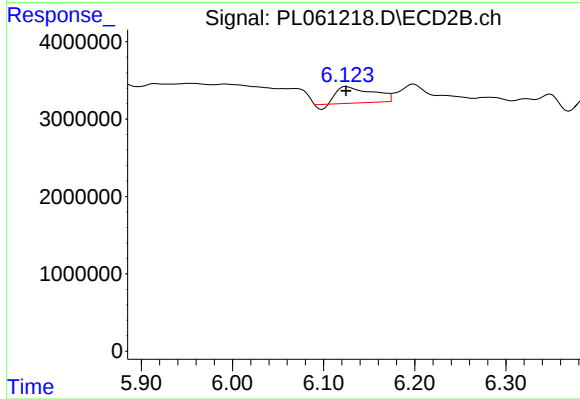


#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 5681865
Conc: 1.83 ng/ml

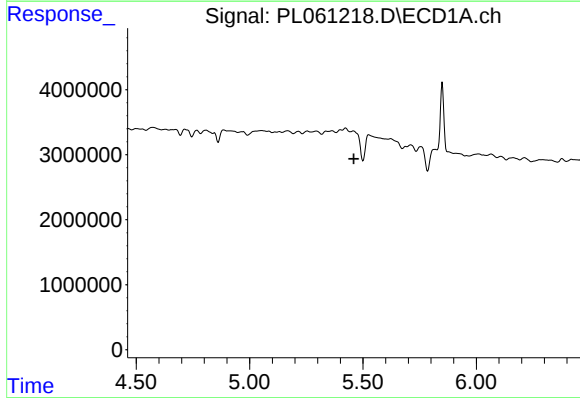


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

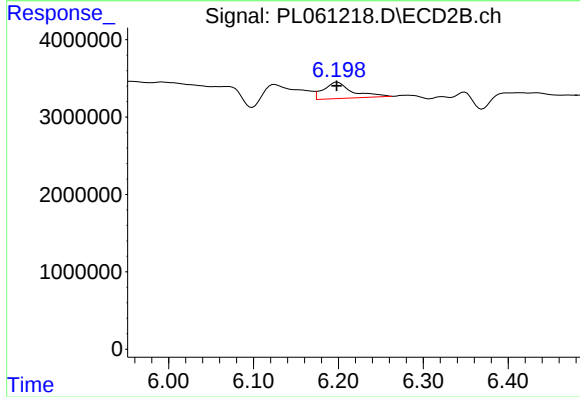

#11 alpha-Chlordane


R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 4962481
Conc: 1.60 ng/ml

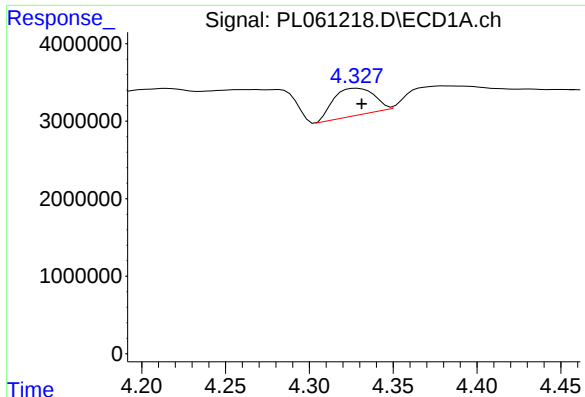

#23 Chlordane-1


R.T.: 4.328 min
Delta R.T.: -0.003 min
Response: 5891506
Conc: 96.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

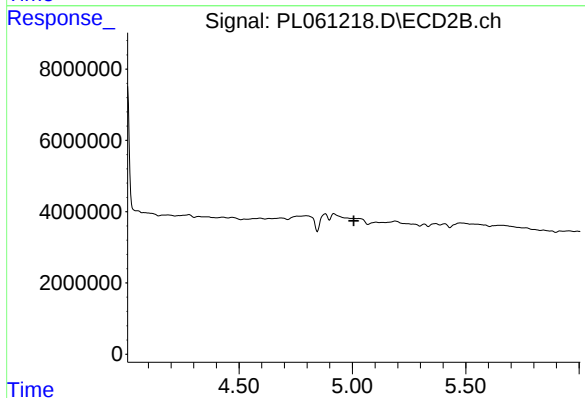


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

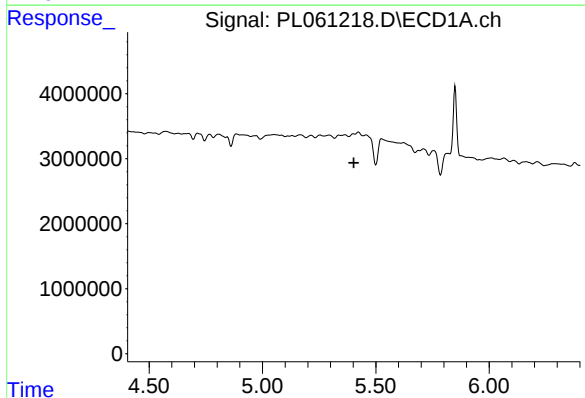


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

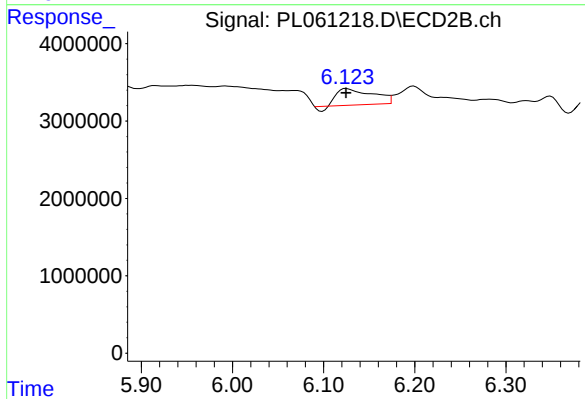

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 5681865
Conc: 14.22 ng/ml

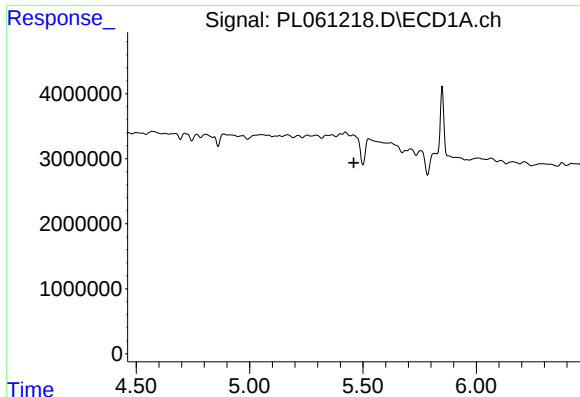

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

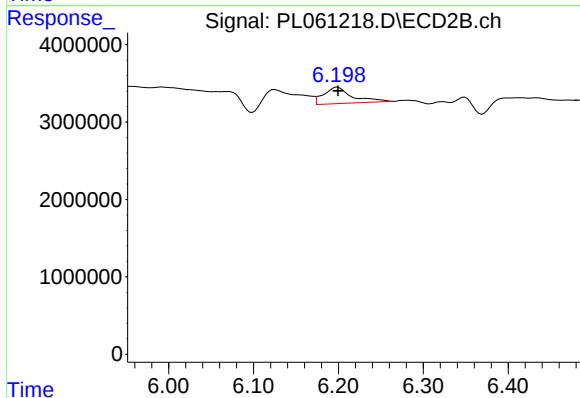


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 4962481
Conc: 10.32 ng/ml

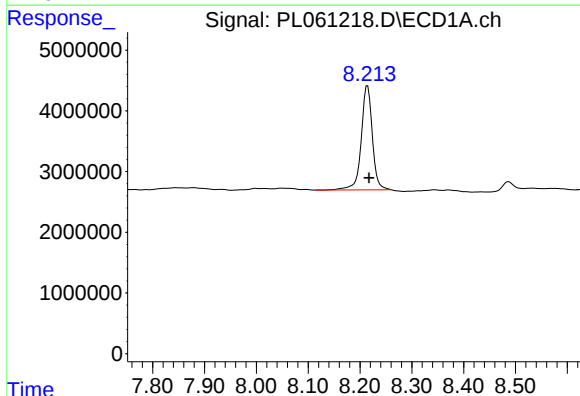

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.003 min
Response: 25491213
Conc: 15.13 ng/ml

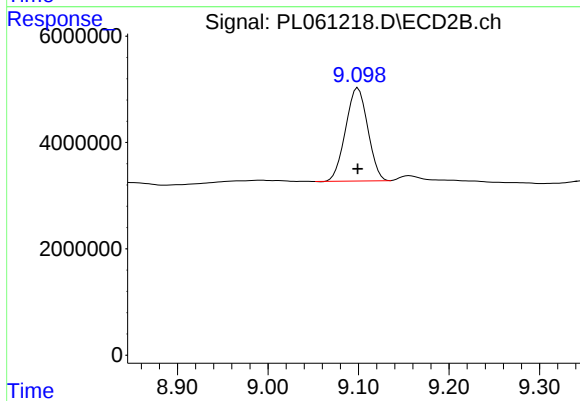

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 29821603
Conc: 14.13 ng/ml