

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
 Data File : PL061220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 13:53
 Operator : DD\AJ
 Sample : L3877-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 9/4/2020 2:41:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 16:25:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.437f	4.007	7483.4E6	137.0E6	4055.167m	52.694 #
28) SA Decachlor...	8.207	9.142f	27095825	1050.2E6	16.084m	497.706m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
Data File : PL061220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 13:53
Operator : DD\AJ
Sample : L3877-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 16:25:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

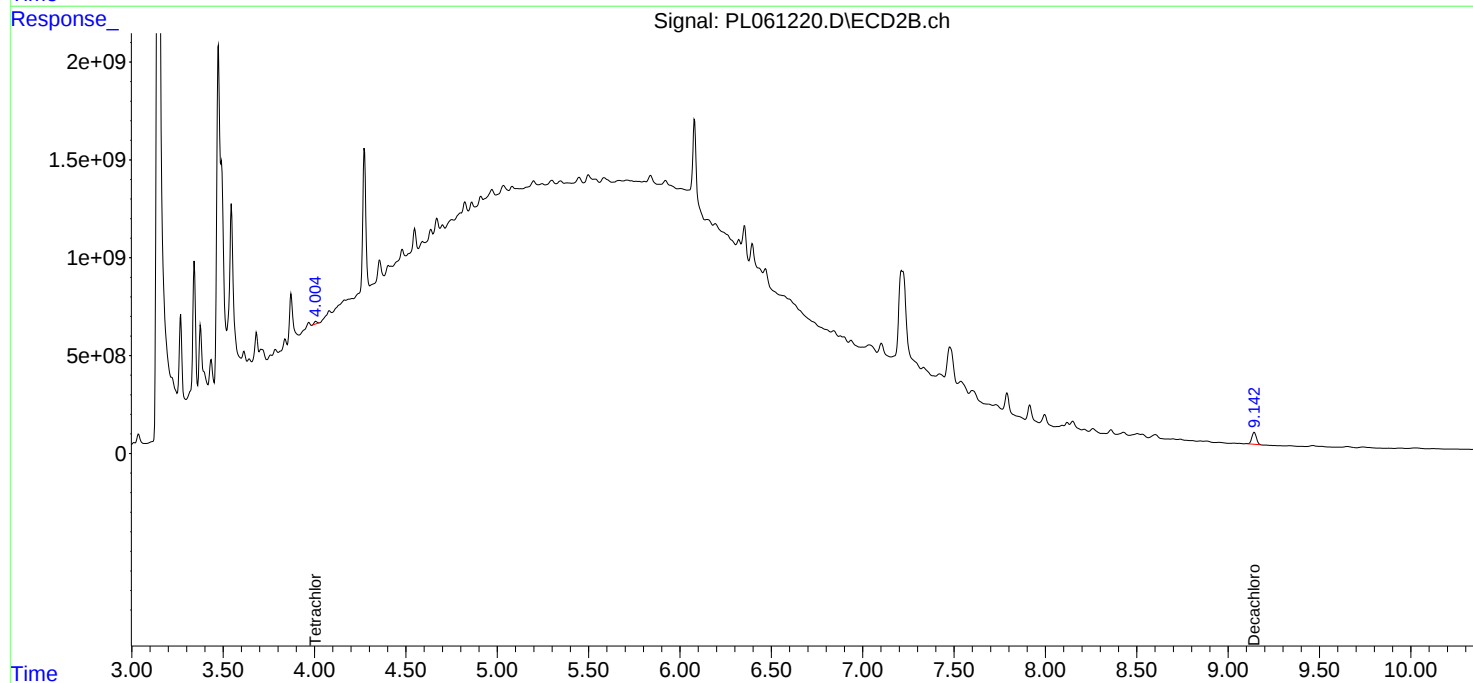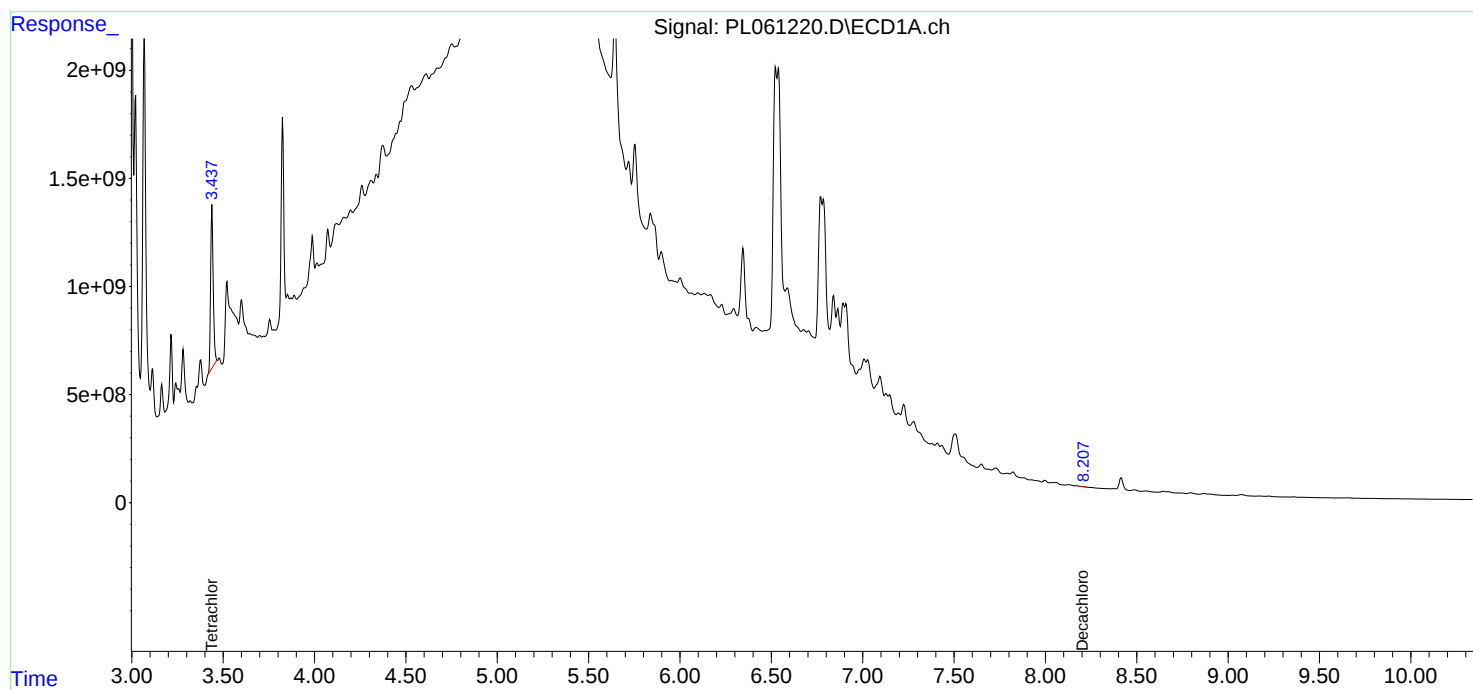

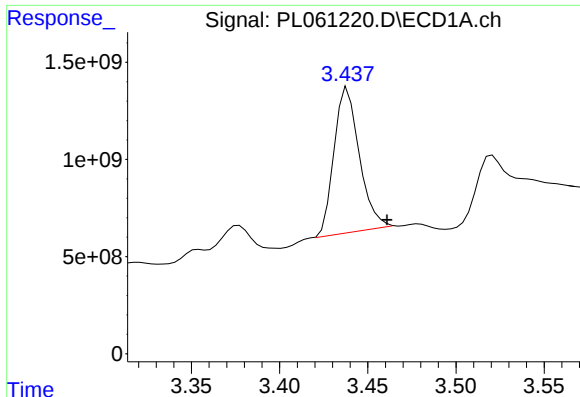

#1 Tetrachloro-m-xylene

R.T.: 3.437 min

Delta R.T.: -0.024 min


Response: 7483372056

Conc: 4055.17 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:00 PM

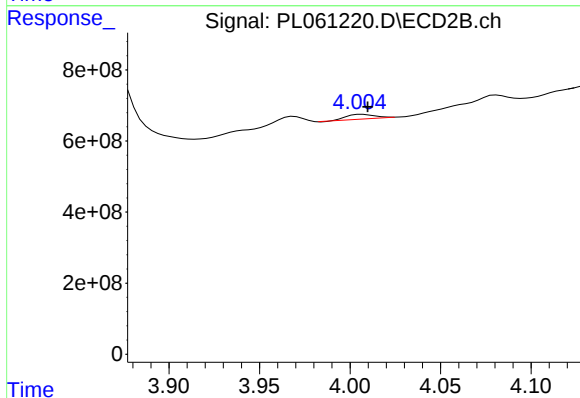


#1 Tetrachloro-m-xylene

R.T.: 4.007 min

Delta R.T.: -0.003 min

Response: 136954082

Conc: 52.69 ng/ml

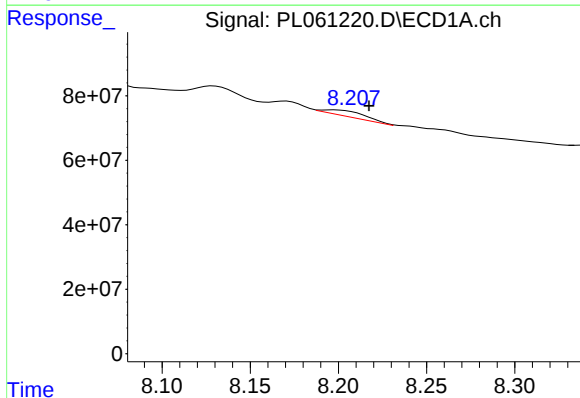


#28 Decachlorobiphenyl

R.T.: 8.207 min

Delta R.T.: -0.010 min

Response: 27095825

Conc: 16.08 ng/ml m

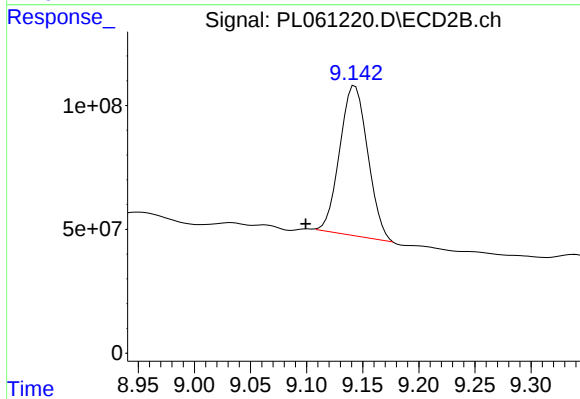

#28 Decachlorobiphenyl

R.T.: 9.142 min

Delta R.T.: 0.043 min

Response: 1050169238

Conc: 497.71 ng/ml m