

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
 Data File : PL061241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 19:21
 Operator : DD\AJ
 Sample : L3877-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 9/4/2020 2:41:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:20:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.010	31396673	46330640	17.014	17.826
28)	SA Decachlor...	8.214	9.100	24684688	33310838	14.653m	15.787
Target Compounds							
2)	A alpha-BHC	3.898	4.401	3141583	1921148	1.111	0.473 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
Data File : PL061241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 19:21
Operator : DD\AJ
Sample : L3877-08
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:20:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

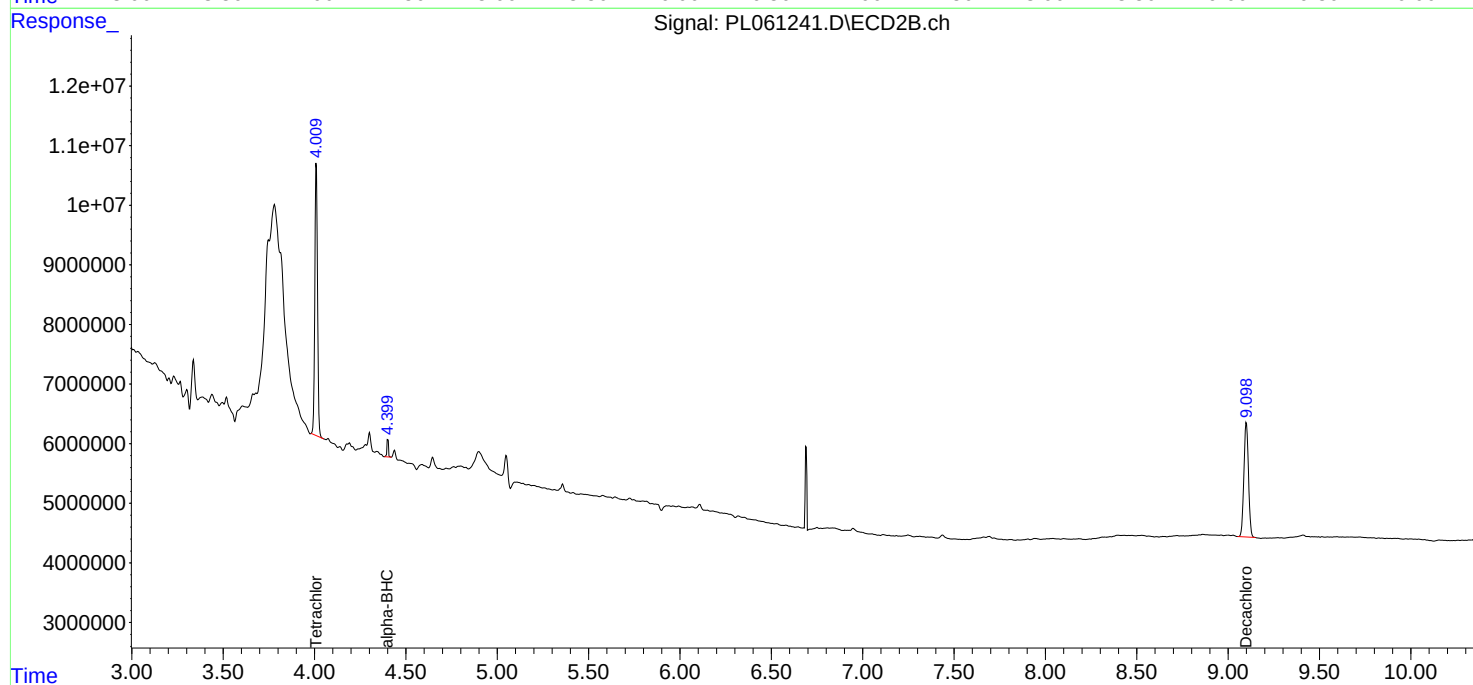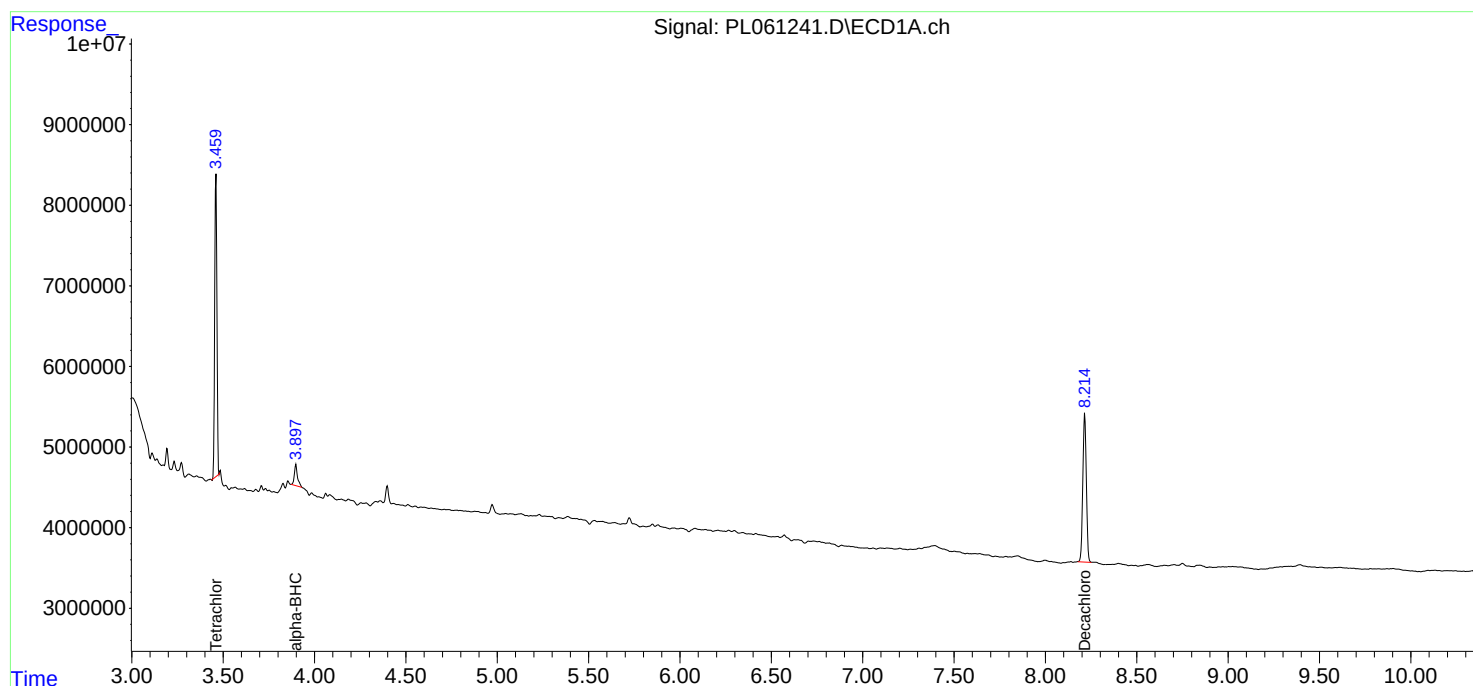

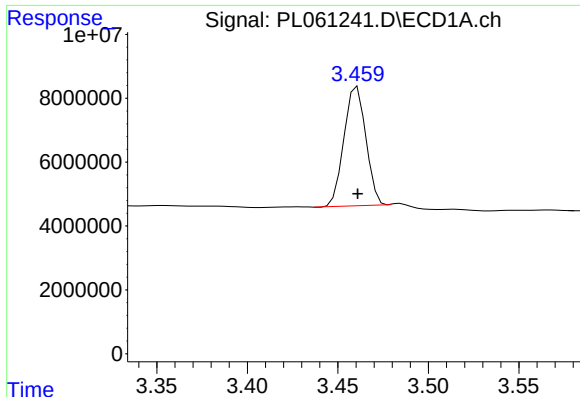


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 31396673
Conc: 17.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:52 PM

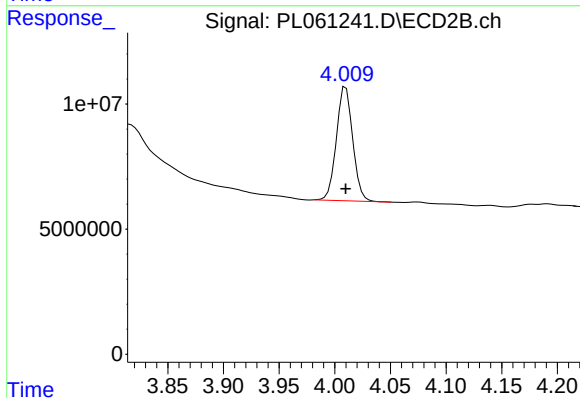


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 46330640
Conc: 17.83 ng/ml

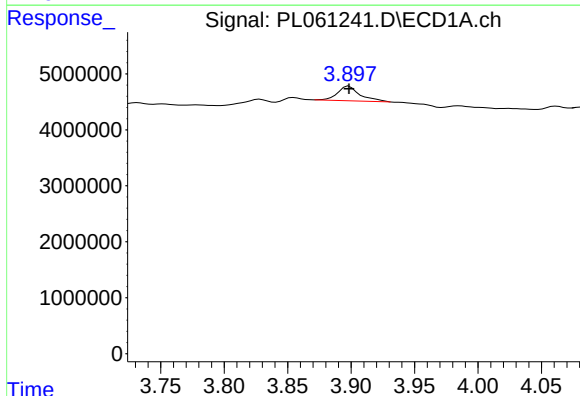


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 3141583
Conc: 1.11 ng/ml

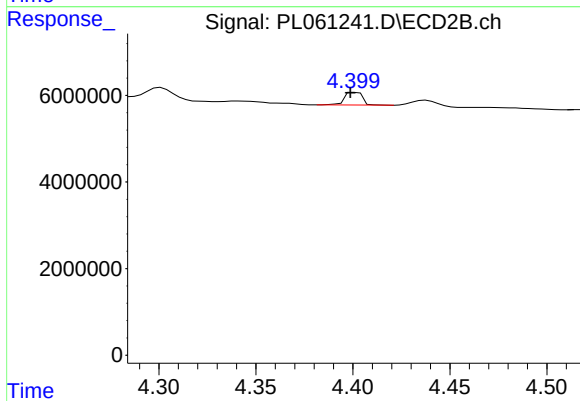

#2 alpha-BHC

R.T.: 4.401 min
Delta R.T.: 0.002 min
Response: 1921148
Conc: 0.47 ng/ml

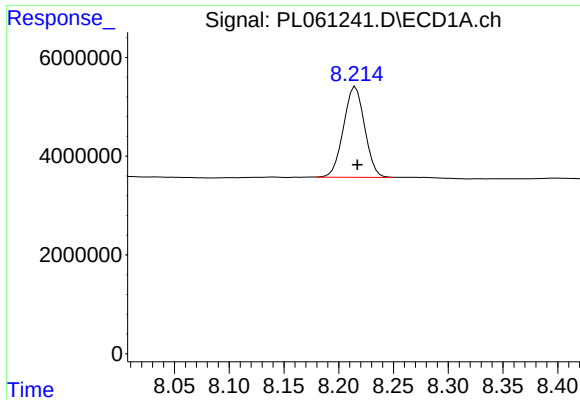


#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.003 min
Response: 24684688
Conc: 14.65 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:52 PM

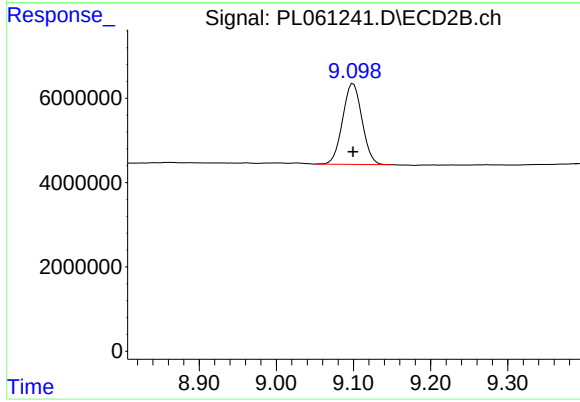

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 33310838
Conc: 15.79 ng/ml