

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
 Data File : PL061243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 19:49
 Operator : DD\AJ
 Sample : L3877-18
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Ankita
 9/4/2020 2:41:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:20:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.009	34510912	34401234	18.701	13.236m#
28)	SA Decachlor...	8.216	9.101	20446220	27591388	12.137	13.076

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090320\
Data File : PL061243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 19:49
Operator : DD\AJ
Sample : L3877-18
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:20:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

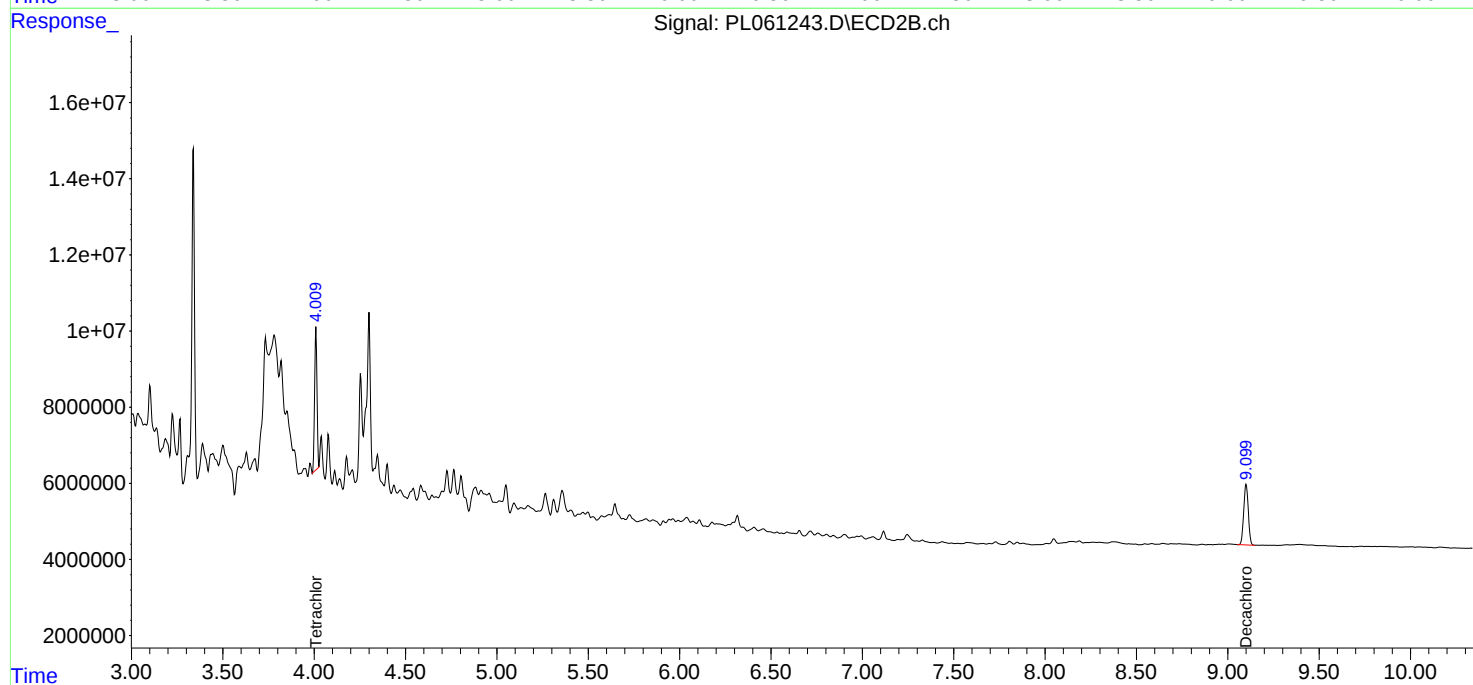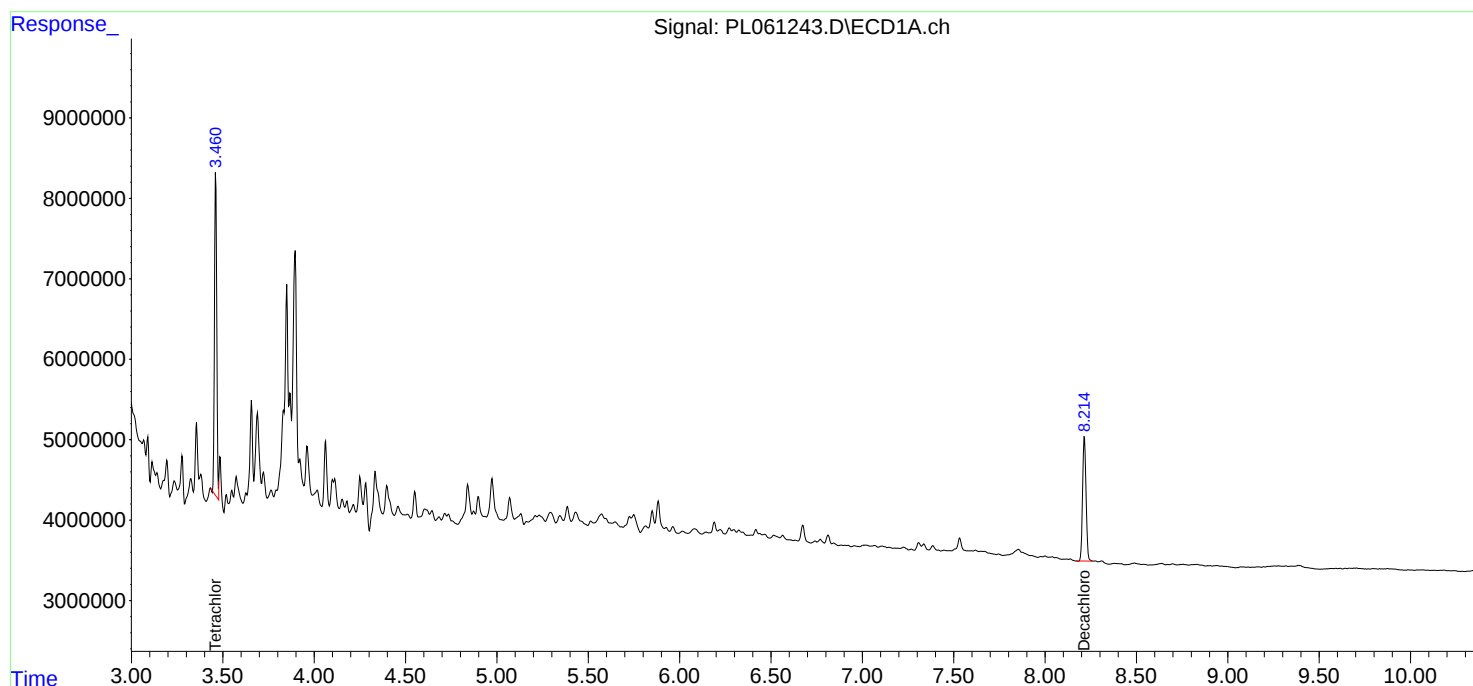

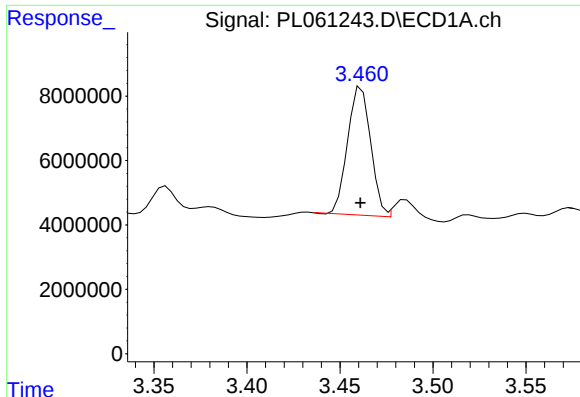


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: 0.000 min
Response: 34510912
Conc: 18.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
9/4/2020 2:41:54 PM

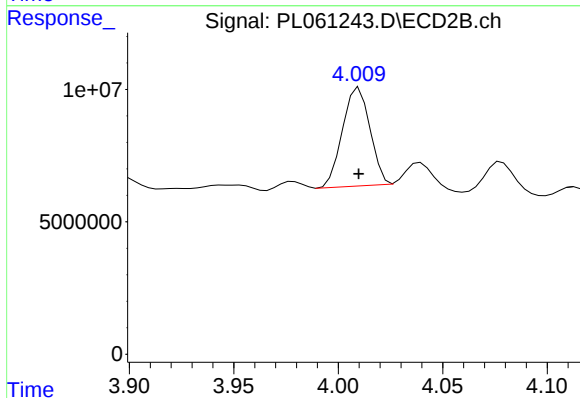


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.001 min
Response: 34401234
Conc: 13.24 ng/ml m

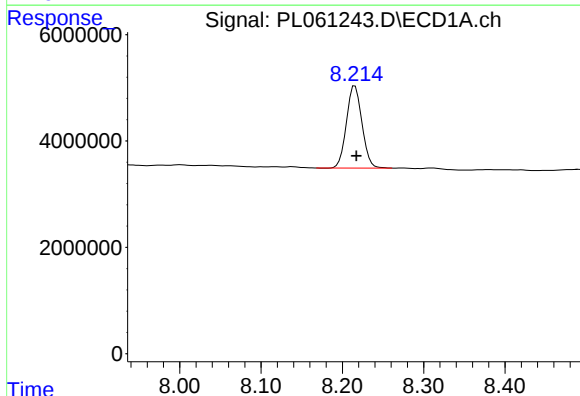

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.002 min
Response: 20446220
Conc: 12.14 ng/ml

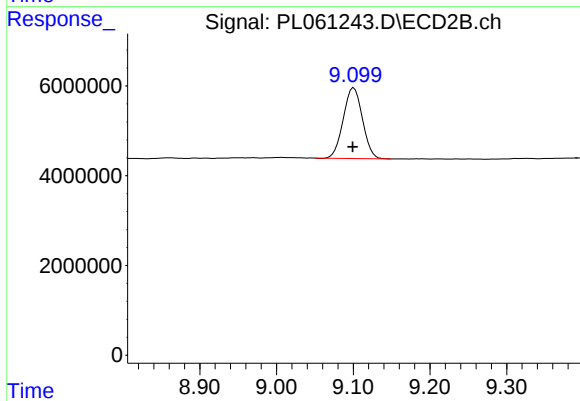

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.001 min
Response: 27591388
Conc: 13.08 ng/ml