

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
 Data File : PL069713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 14:32
 Operator : AR\AJ
 Sample : M3648-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 15:49:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.570	6240537	21513507	20.046	17.100
28)	SA Decachlor...	10.403	11.496	8276332	14998545	14.034	13.291
Target Compounds							
2)	A alpha-BHC	0.000	6.126f	0	515078	N.D.	0.296 #
6)	B beta-BHC	6.115f	0.000	1997088	0	8.322	N.D. #
9)	A Endosulfan I	0.000	8.466f	0	645785	N.D.	0.502 #
11)	B alpha-Chl...	0.000	8.364f	0	635119	N.D.	0.464 #
15)	B Endosulfa...	0.000	9.217f	0	646810	N.D.	0.568 #
21)	B Endrin ke...	0.000	10.097f	0	201940	N.D.	0.170 #
23)	Chlordane-1	0.000	6.927f	0	2385198	N.D.	43.168 #
26)	Chlordane-4	0.000	8.364f	0	635119	N.D.	2.561 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
Data File : PL069713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 14:32
Operator : AR\AJ
Sample : M3648-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 15:49:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

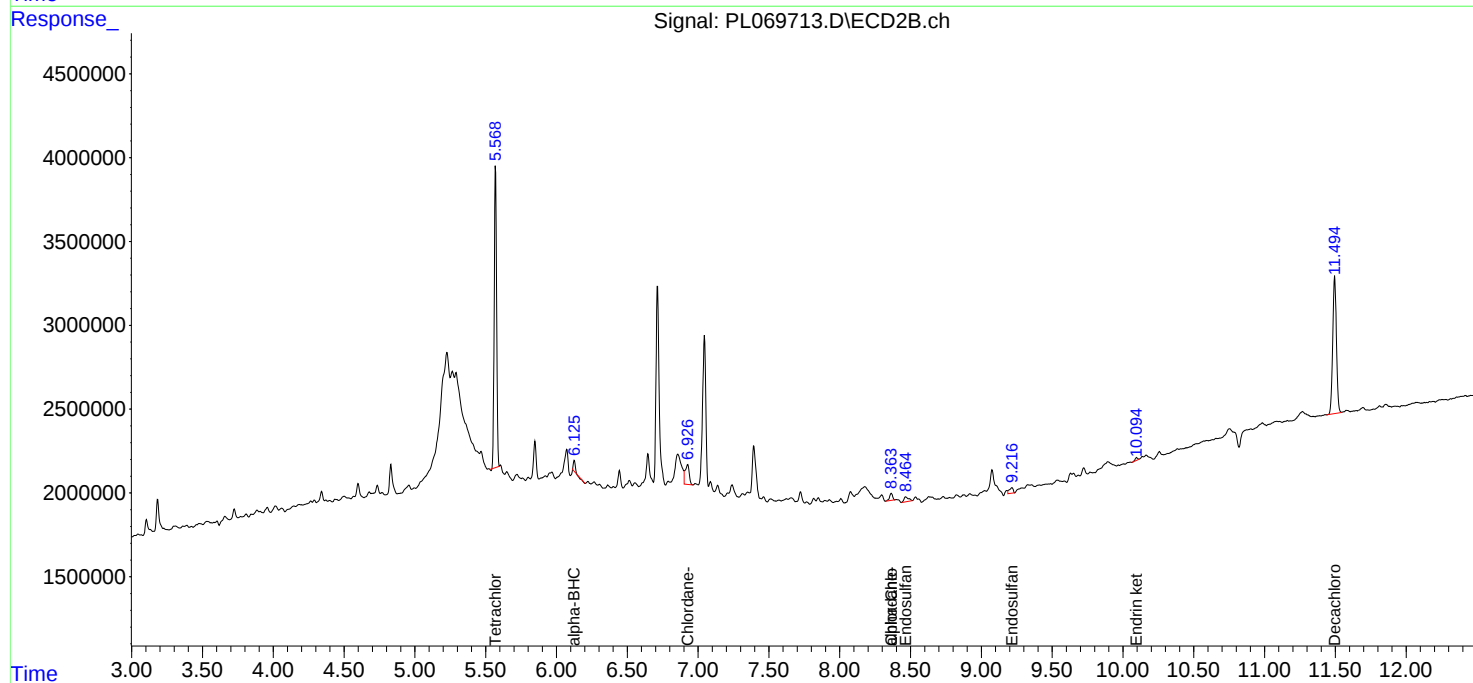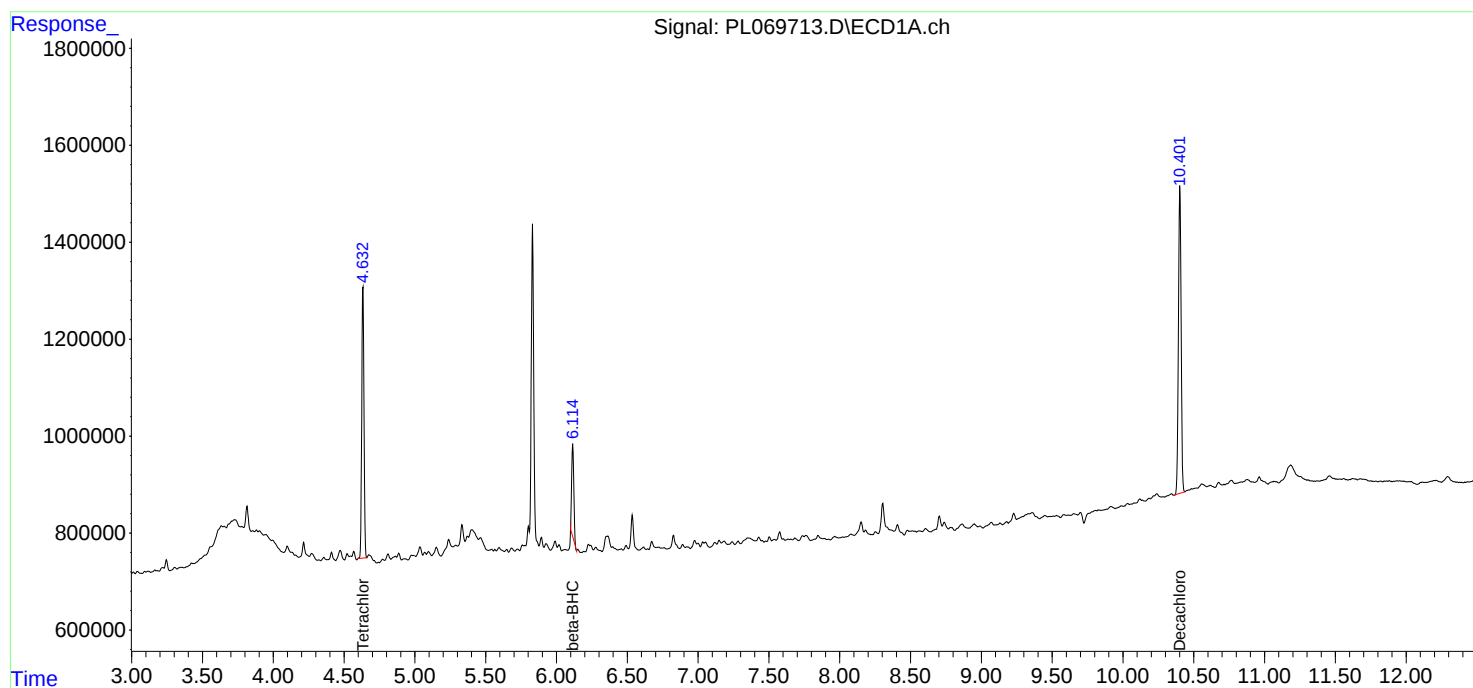


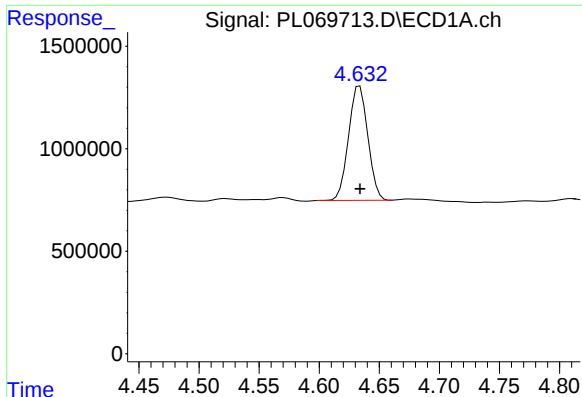

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 6240537
Conc: 20.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

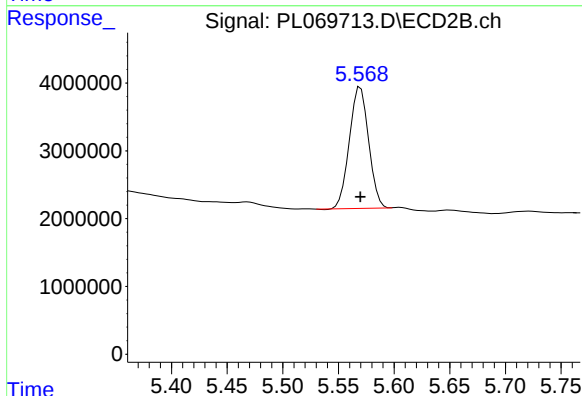


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 21513507
Conc: 17.10 ng/ml

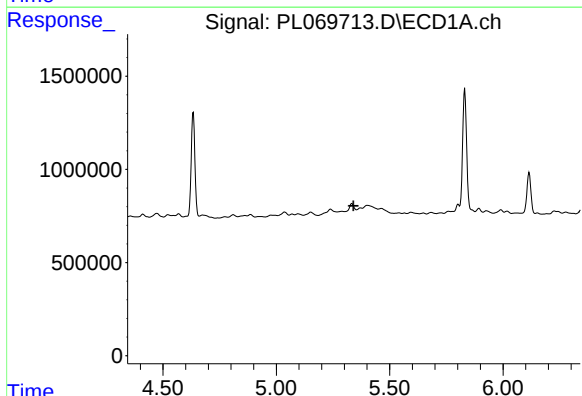


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.341 min
Response: 0
Conc: N.D.

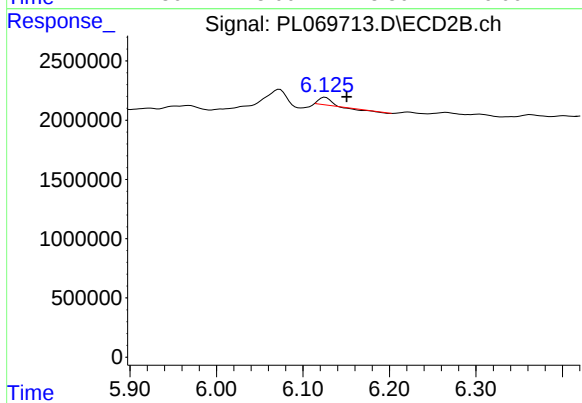

#2 alpha-BHC


R.T.: 6.126 min
Delta R.T.: -0.024 min
Response: 515078
Conc: 0.30 ng/ml

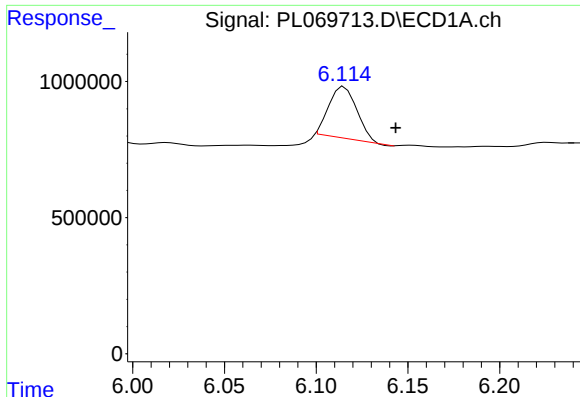

#6 beta-BHC


R.T.: 6.115 min
Delta R.T.: -0.028 min
Response: 1997088
Conc: 8.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

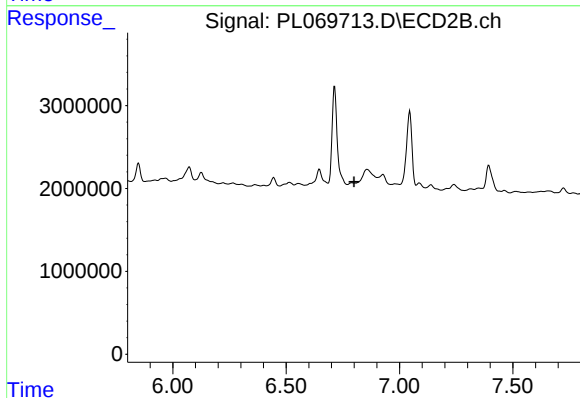


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

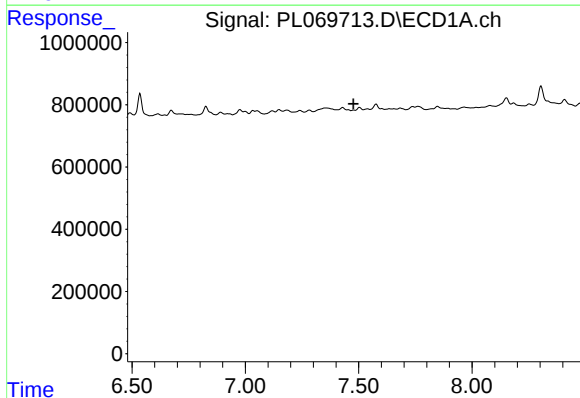


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

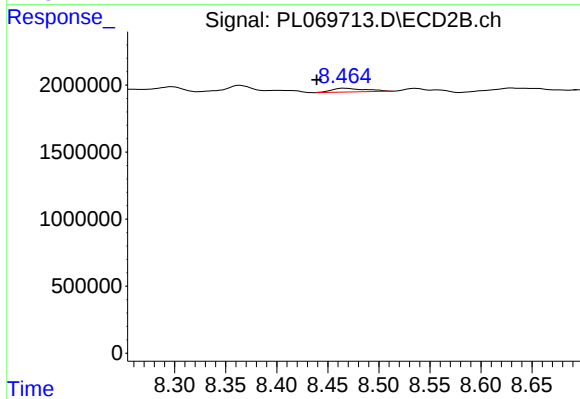

#9 Endosulfan I


R.T.: 8.466 min
Delta R.T.: 0.027 min
Response: 645785
Conc: 0.50 ng/ml

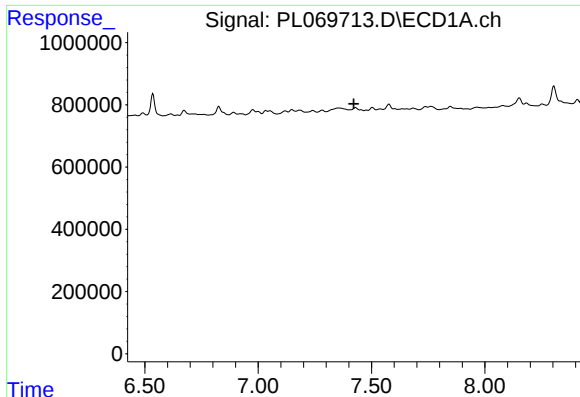

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

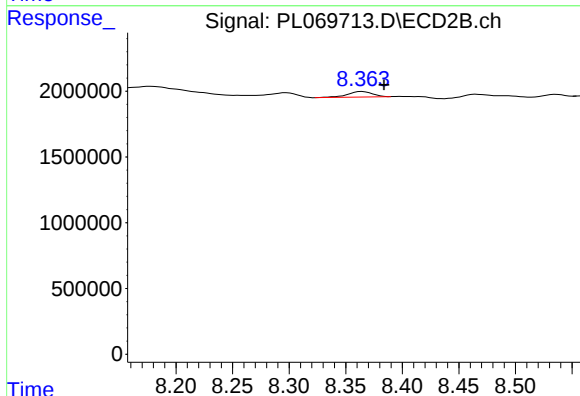


#11 alpha-Chlordane

R.T.: 8.364 min
Delta R.T.: -0.019 min
Response: 635119
Conc: 0.46 ng/ml

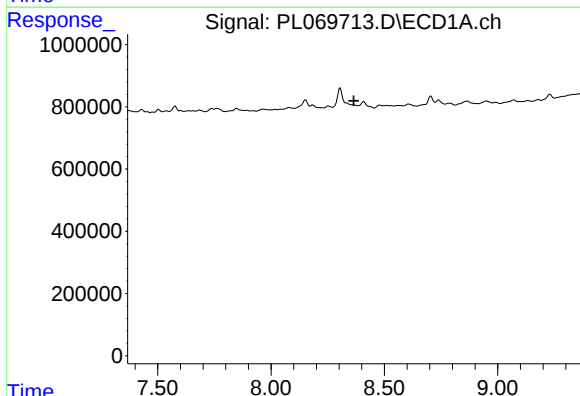


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.365 min
Response: 0
Conc: N.D.

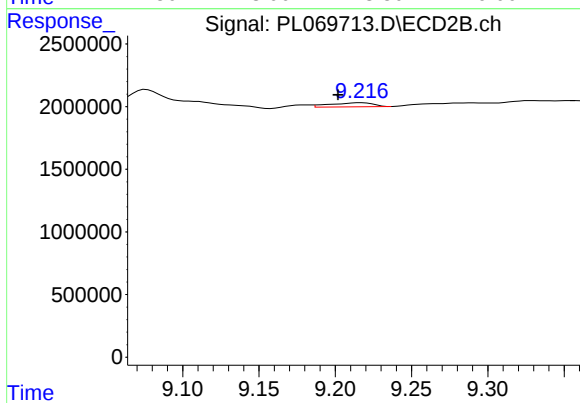

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.015 min
Response: 646810
Conc: 0.57 ng/ml

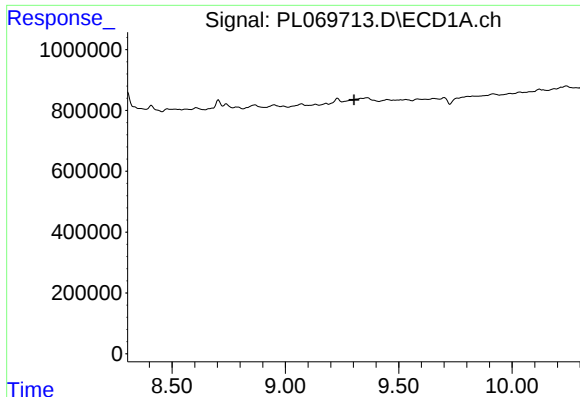

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.303 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

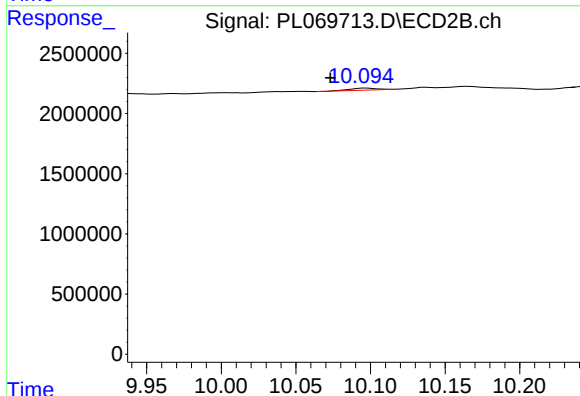


#21 Endrin ketone

R.T.: 10.097 min
Delta R.T.: 0.024 min
Response: 201940
Conc: 0.17 ng/ml

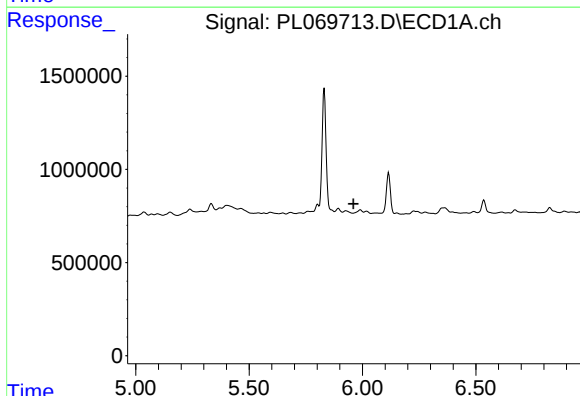


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.961 min
Response: 0
Conc: N.D.

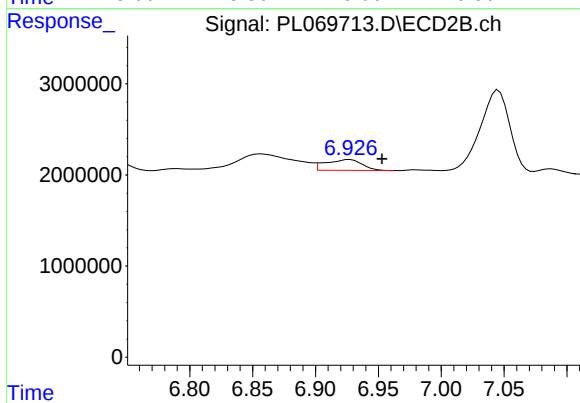

#23 Chlordane-1


R.T.: 6.927 min
Delta R.T.: -0.026 min
Response: 2385198
Conc: 43.17 ng/ml

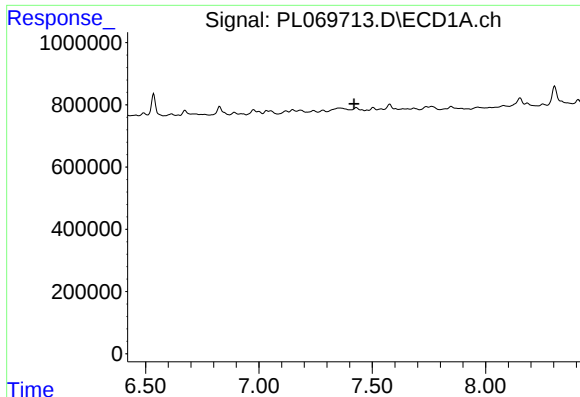

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

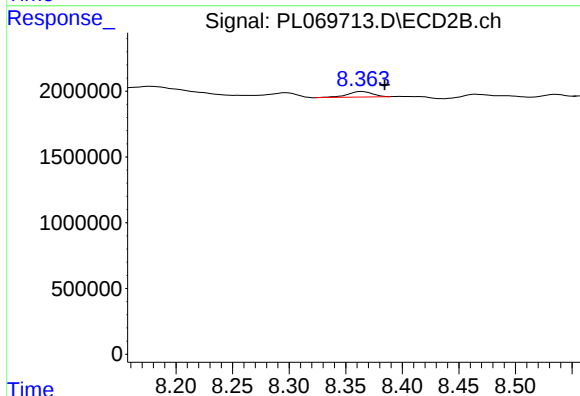


#26 Chlordane-4

R.T.: 8.364 min
Delta R.T.: -0.020 min
Response: 635119
Conc: 2.56 ng/ml

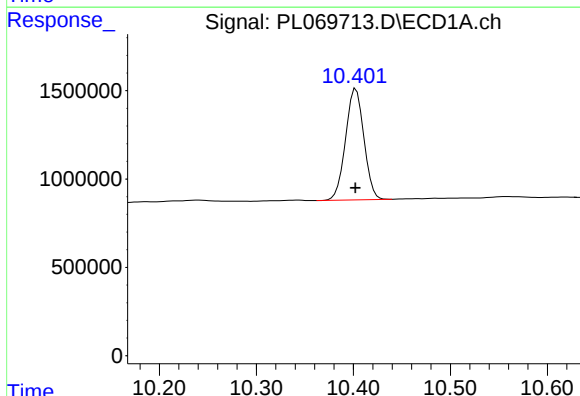

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: 0.000 min
Response: 8276332
Conc: 14.03 ng/ml

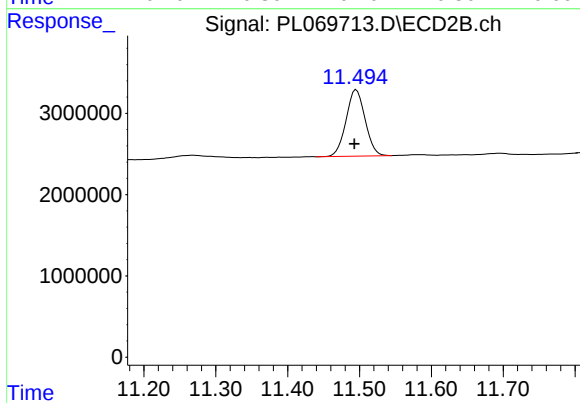

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.003 min
Response: 14998545
Conc: 13.29 ng/ml