

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
 Data File : PL069729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 20:04
 Operator : AR\AJ
 Sample : M3648-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:01:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.631	5.567	7035402	25792748	22.599	20.502
28)	SA Decachlor...	10.397	11.488	9055113	17097609	15.354	15.152
Target Compounds							
10)	B gamma-Chl...	0.000	8.294	0	289228	N.D.	0.208 #
11)	B alpha-Chl...	0.000	8.402f	0	89943	N.D.	0.066 #
14)	MA Endrin	0.000	8.995f	0	783957	N.D.	0.703 #
16)	A 4,4'-DDD	0.000	9.103	0	281286	N.D.	0.259 #
20)	A Methoxychlor	9.051f	9.900	736201	1224173	2.389	2.116
21)	B Endrin ke...	0.000	10.081	0	930039	N.D.	0.783 #
22)	Mirex	0.000	10.559f	0	734737	N.D.	0.819 #
25)	Chlordane-3	0.000	8.294	0	289228	N.D.	1.400 #
26)	Chlordane-4	0.000	8.402f	0	89943	N.D.	0.363 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
Data File : PL069729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 20:04
Operator : AR\AJ
Sample : M3648-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:01:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

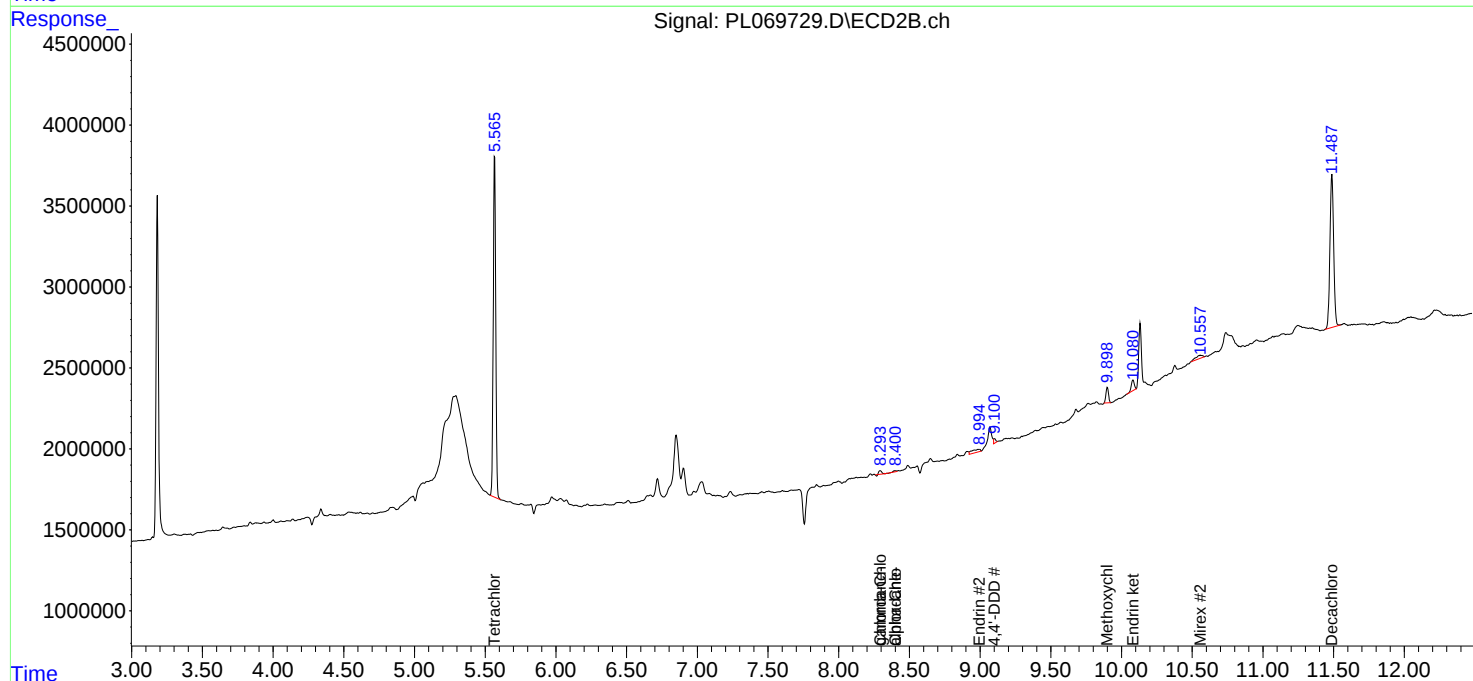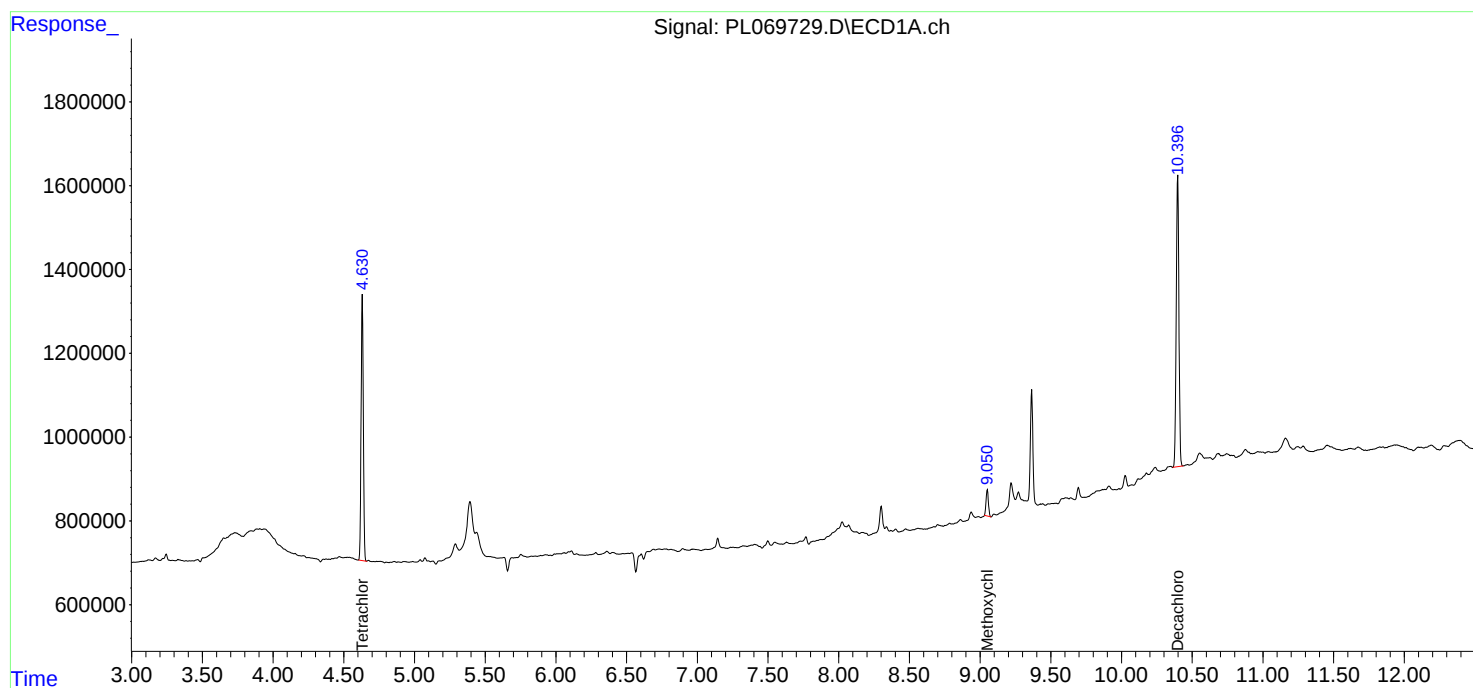


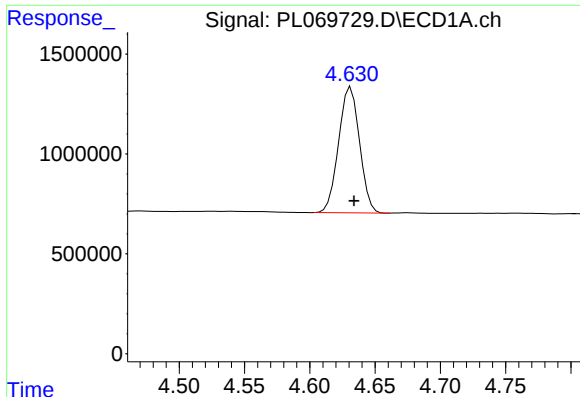

#1 Tetrachloro-m-xylene


R.T.: 4.631 min
Delta R.T.: -0.003 min
Response: 7035402
Conc: 22.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

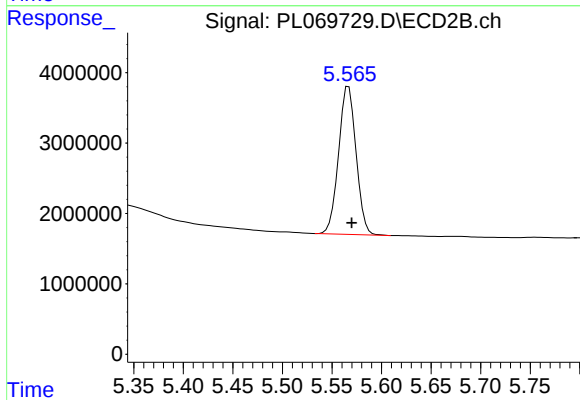


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.003 min
Response: 25792748
Conc: 20.50 ng/ml

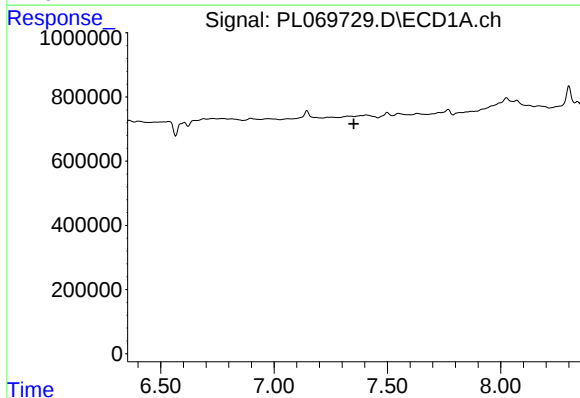


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.352 min
Response: 0
Conc: N.D.

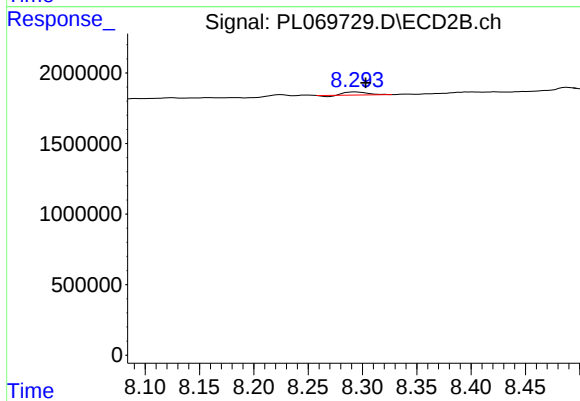

#10 gamma-Chlordane


R.T.: 8.294 min
Delta R.T.: -0.009 min
Response: 289228
Conc: 0.21 ng/ml

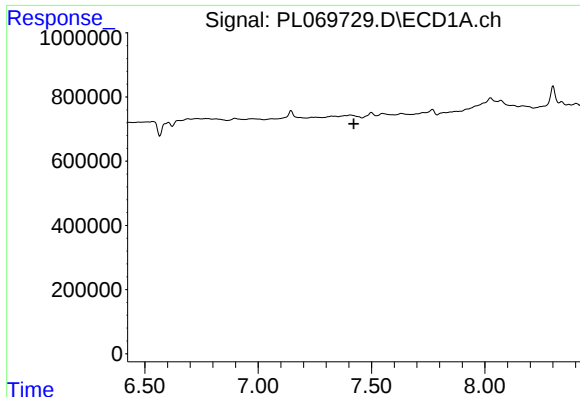

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

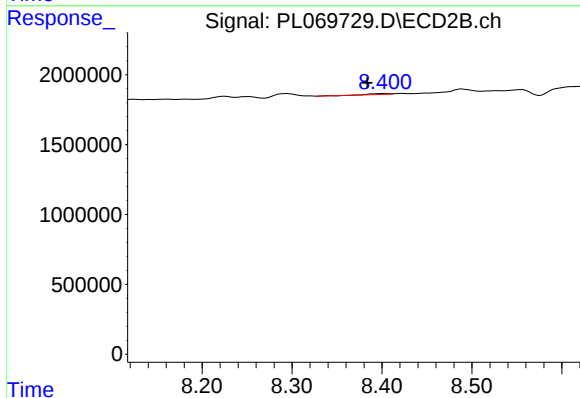


#11 alpha-Chlordane

R.T.: 8.402 min
Delta R.T.: 0.018 min
Response: 89943
Conc: 0.07 ng/ml

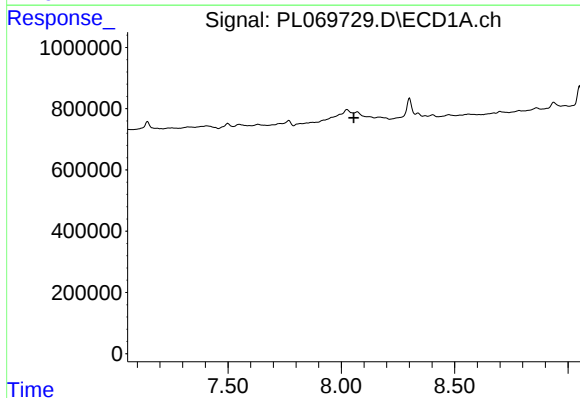


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.055 min
Response: 0
Conc: N.D.

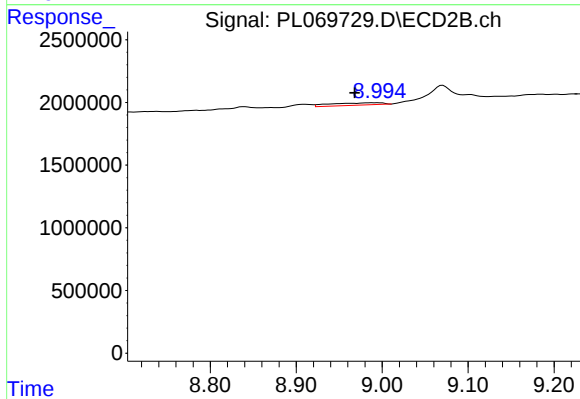

#14 Endrin


R.T.: 8.995 min
Delta R.T.: 0.027 min
Response: 783957
Conc: 0.70 ng/ml

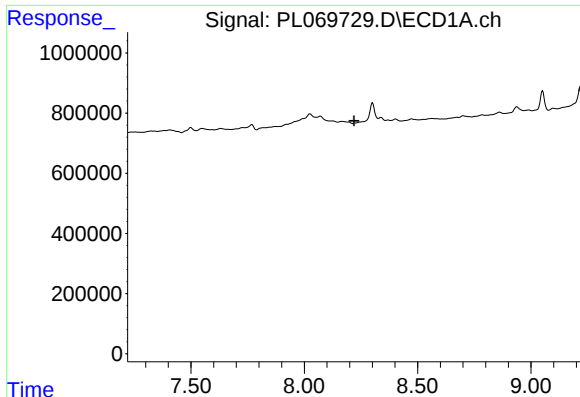

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

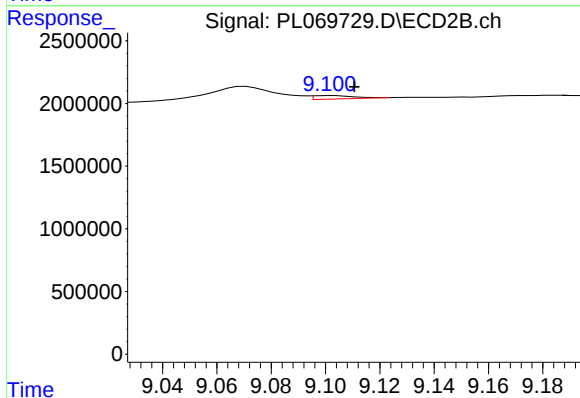


#16 4,4'-DDD

R.T.: 9.103 min
Delta R.T.: -0.008 min
Response: 281286
Conc: 0.26 ng/ml

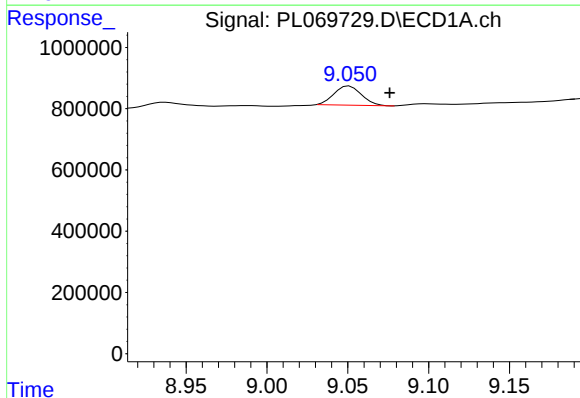


#20 Methoxychlor

R.T.: 9.051 min
Delta R.T.: -0.025 min
Response: 736201
Conc: 2.39 ng/ml

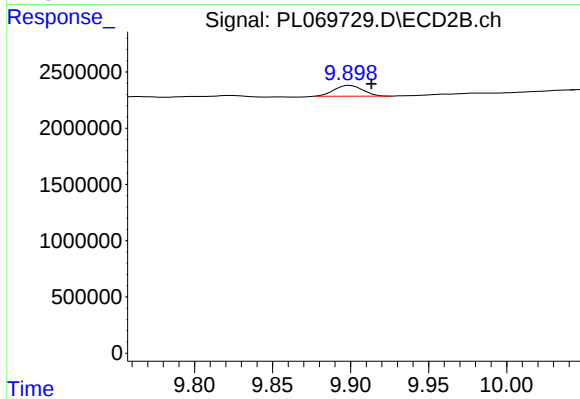

#20 Methoxychlor


R.T.: 9.898 min
Delta R.T.: -0.014 min
Response: 1224173
Conc: 2.12 ng/ml

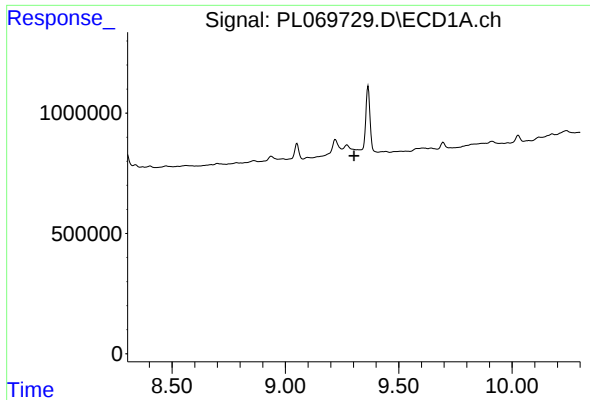

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.303 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

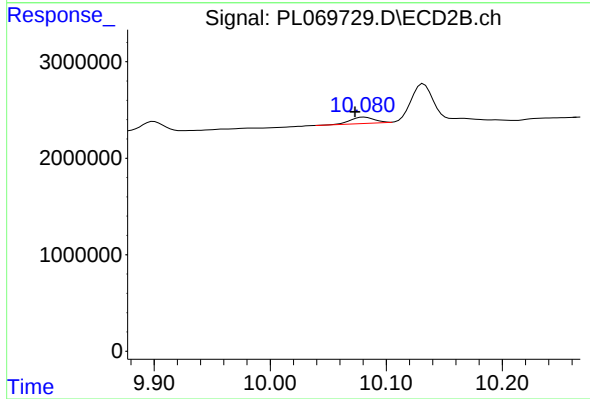


#21 Endrin ketone

R.T.: 10.081 min
Delta R.T.: 0.008 min
Response: 930039
Conc: 0.78 ng/ml

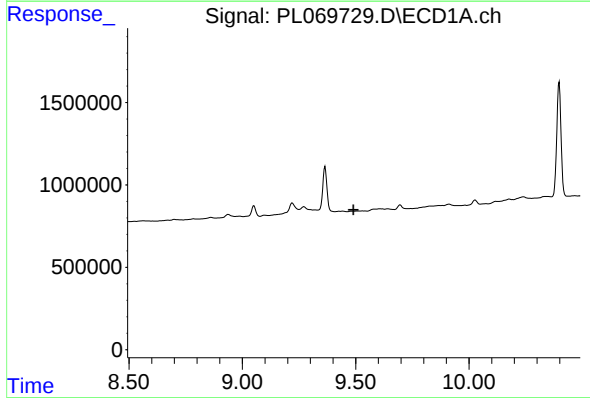


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.491 min
Response: 0
Conc: N.D.

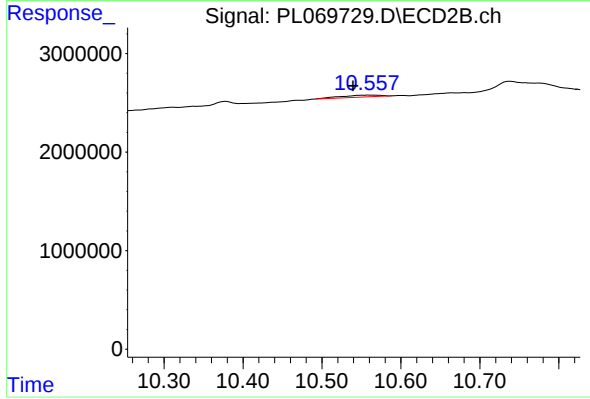

#22 Mirex


R.T.: 10.559 min
Delta R.T.: 0.020 min
Response: 734737
Conc: 0.82 ng/ml

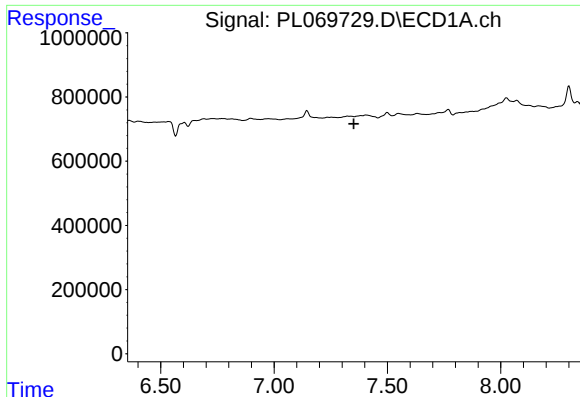

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

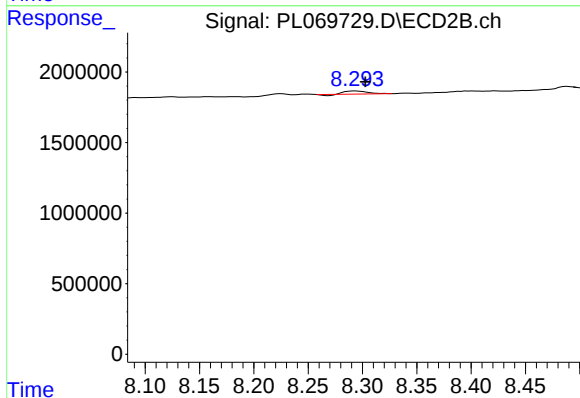


#25 Chlordane-3

R.T.: 8.294 min
Delta R.T.: -0.009 min
Response: 289228
Conc: 1.40 ng/ml

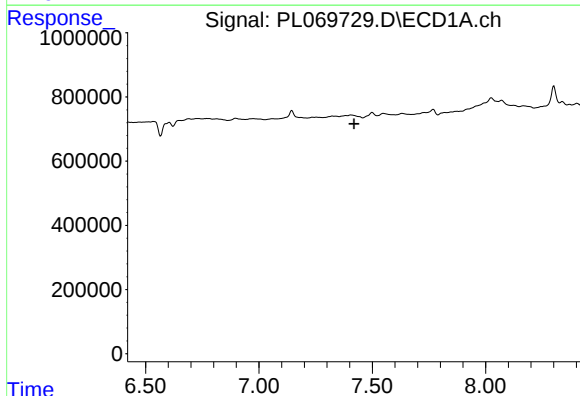


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

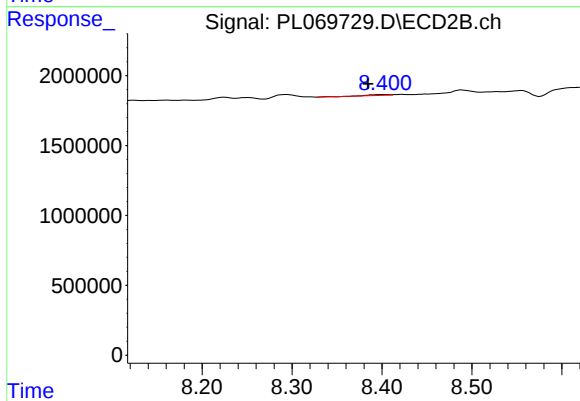

#26 Chlordane-4


R.T.: 8.402 min
Delta R.T.: 0.018 min
Response: 89943
Conc: 0.36 ng/ml

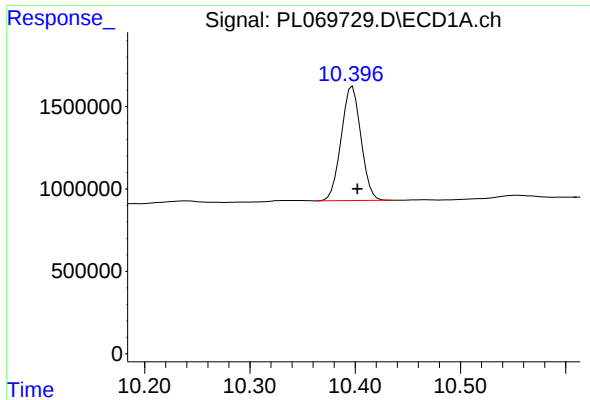

#28 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: -0.005 min
Response: 9055113
Conc: 15.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

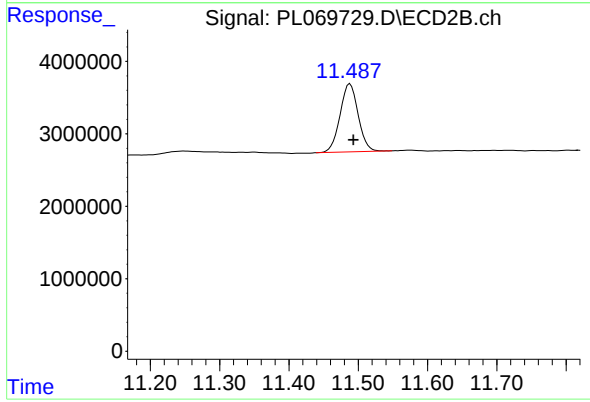

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.005 min
Response: 17097609
Conc: 15.15 ng/ml