

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
 Data File : PL069720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 16:44
 Operator : AR\AJ
 Sample : M3640-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

mohammad
 9/7/2021 8:39:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:58:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.631	5.566	6966252	103.8E6	22.377m	82.504m#
28)	SA Decachlor...	10.398	11.487	1988772	1197664	3.372m	1.061 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
Data File : PL069720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 16:44
Operator : AR\AJ
Sample : M3640-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HP-627


Manual Integrations
APPROVED

mohammad
9/7/2021 8:39:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:58:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

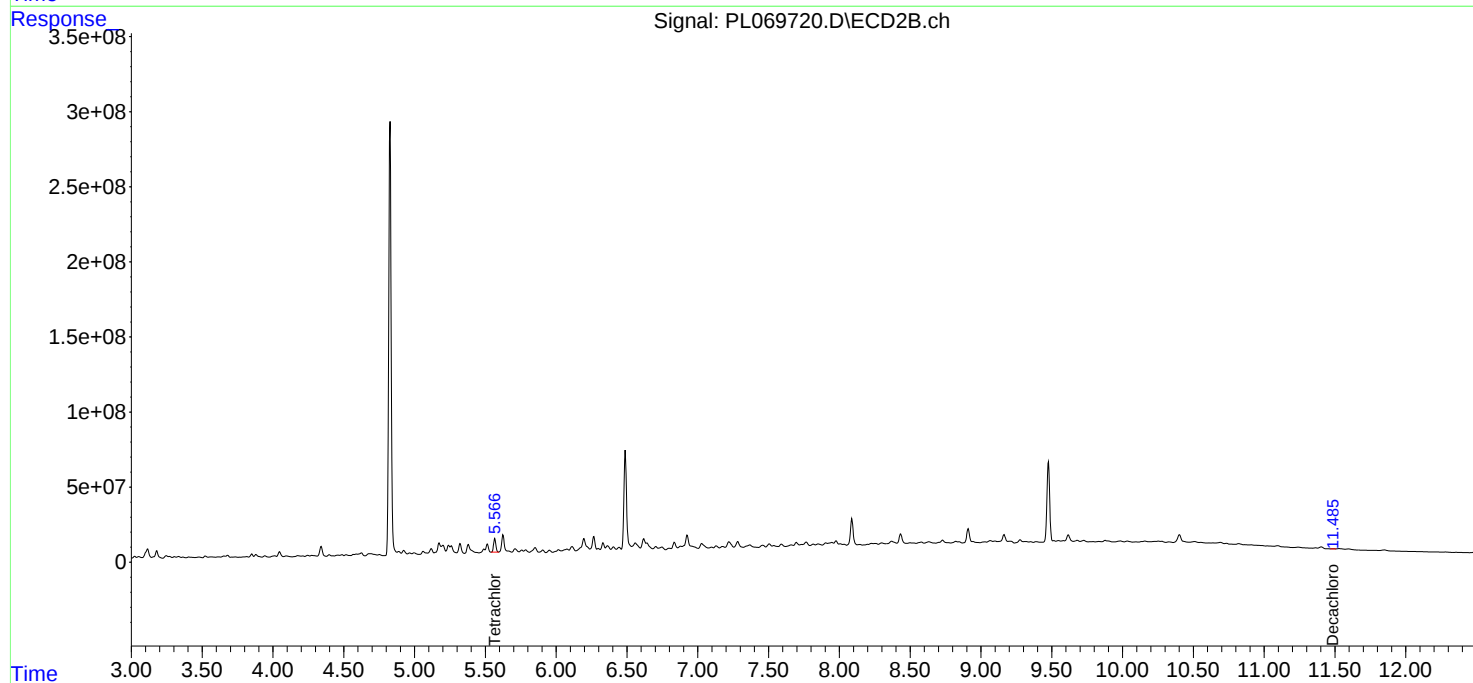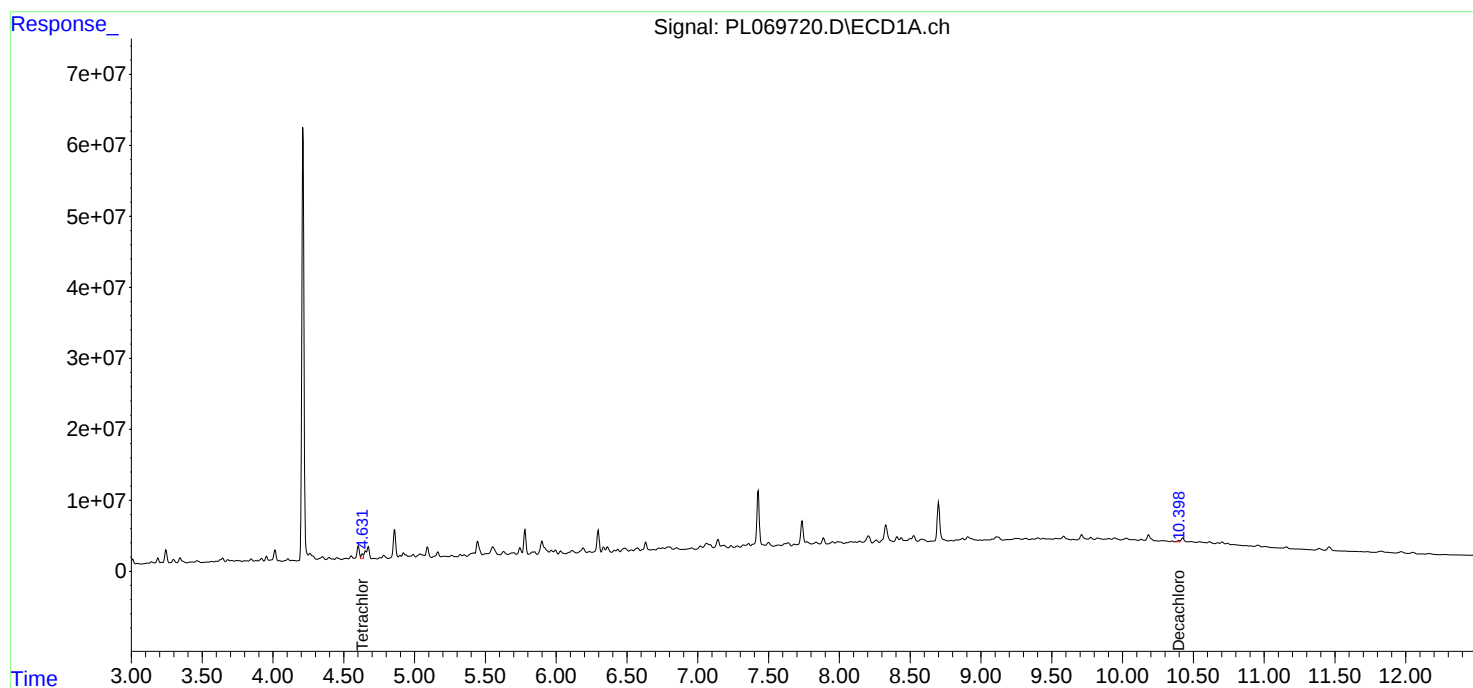

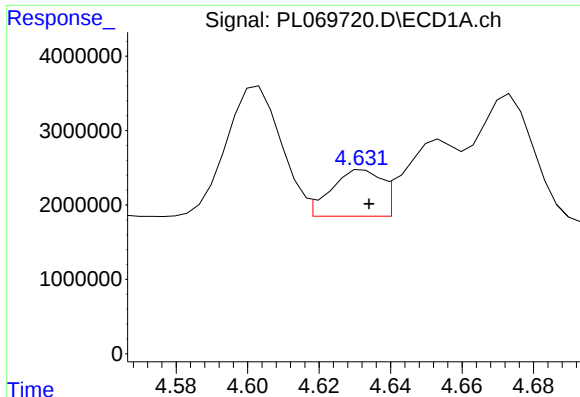


#1 Tetrachloro-m-xylene

R.T.: 4.631 min
Delta R.T.: -0.003 min
Response: 6966252
Conc: 22.38 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

mohammad
9/7/2021 8:39:45 AM

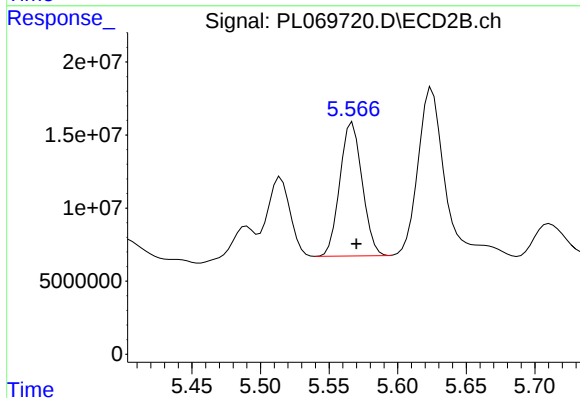


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.004 min
Response: 103796417
Conc: 82.50 ng/ml m

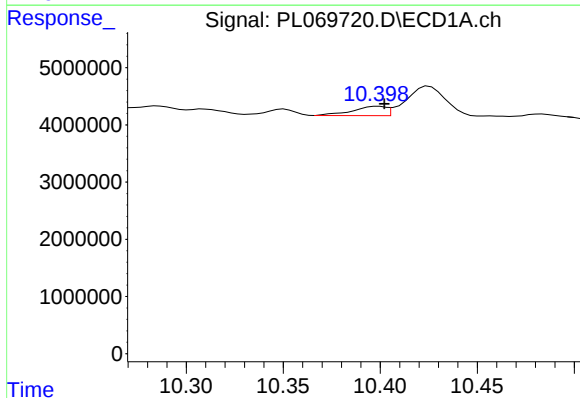

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.004 min
Response: 1988772
Conc: 3.37 ng/ml m

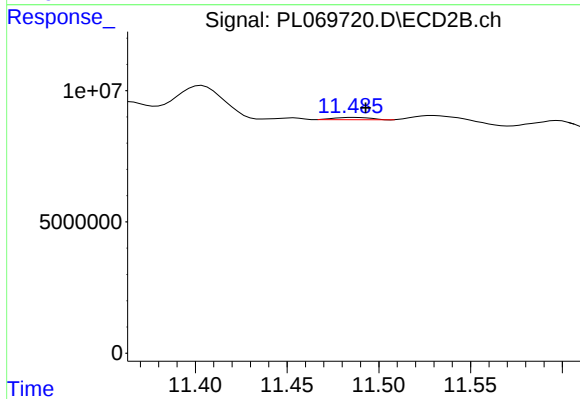

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.006 min
Response: 1197664
Conc: 1.06 ng/ml