

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
 Data File : PL069725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 18:57
 Operator : AR\AJ
 Sample : M3648-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20211052-SI-COMPOSITE-1

Manual Integrations
 APPROVED

mohammad
 9/7/2021 8:39:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 02:00:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.568	7805961	28023142	25.074	22.274
28)	SA Decachlor...	10.400	11.492	11903593	23233159	20.184	20.589
Target Compounds							
12)	B 4,4'-DDE	7.634	8.557	327037	1059092	0.726m	0.800

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090321\
Data File : PL069725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 18:57
Operator : AR\AJ
Sample : M3648-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20211052-SI-COMPOSITE-1


Manual Integrations
APPROVED

mohammad
9/7/2021 8:39:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 02:00:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

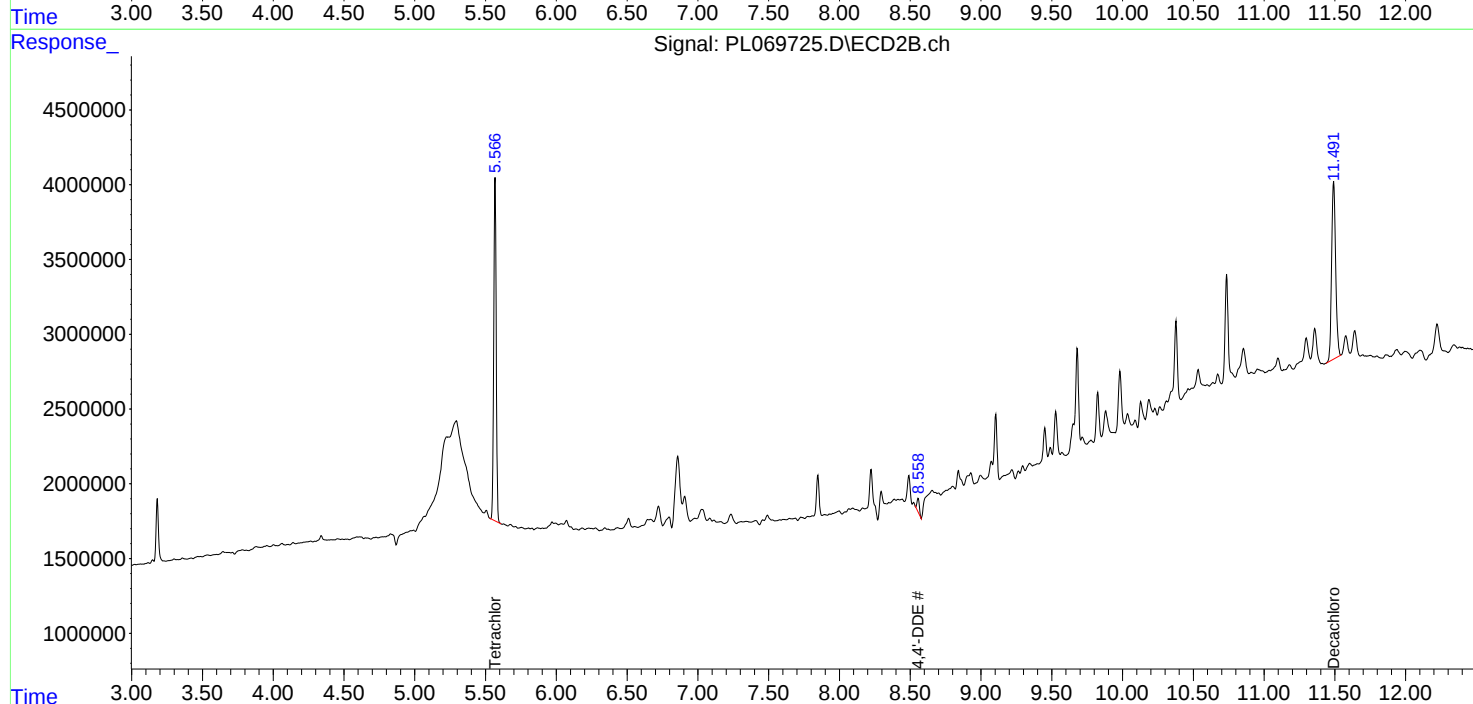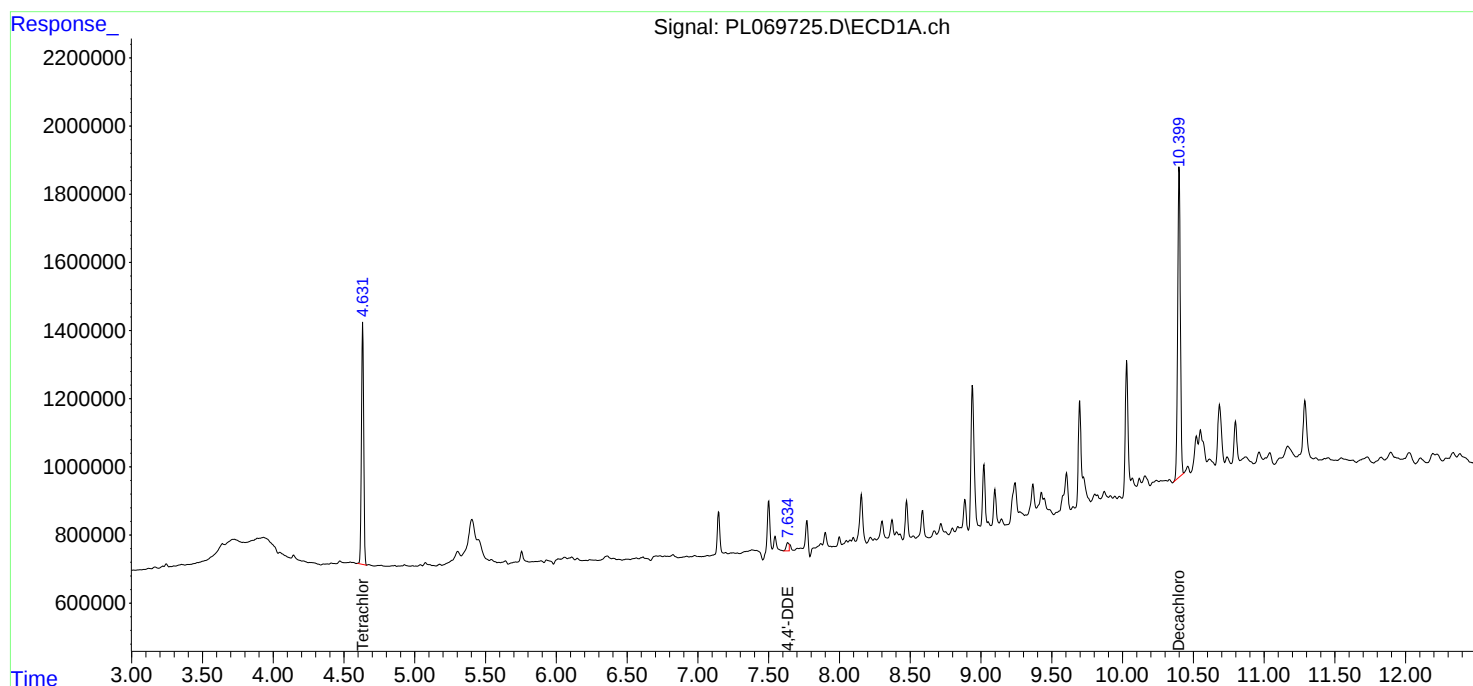

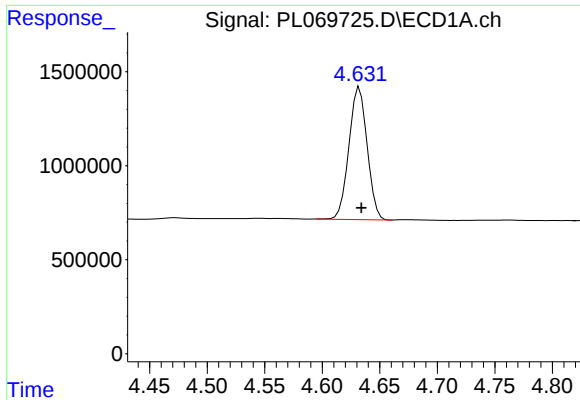


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 7805961
Conc: 25.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211052-SI-COMPOSITE-1


Manual Integrations
APPROVED

mohammad
9/7/2021 8:39:54 AM

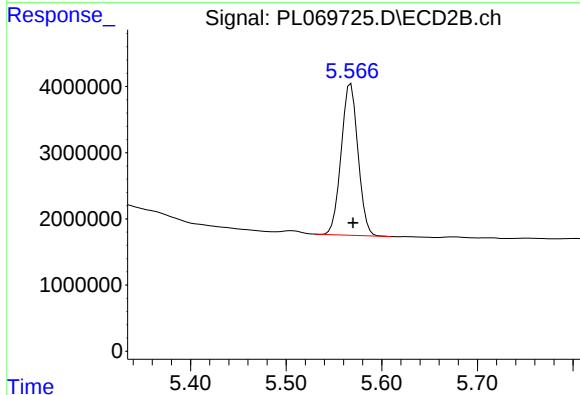


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.002 min
Response: 28023142
Conc: 22.27 ng/ml

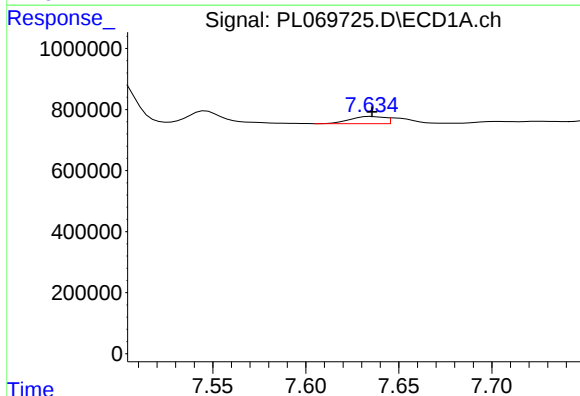


#12 4,4'-DDE

R.T.: 7.634 min
Delta R.T.: -0.002 min
Response: 327037
Conc: 0.73 ng/ml m

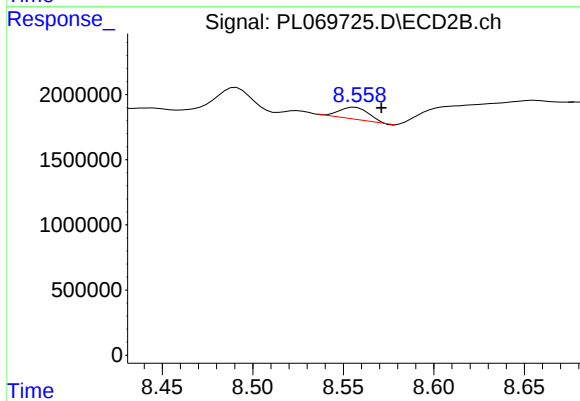

#12 4,4'-DDE

R.T.: 8.557 min
Delta R.T.: -0.014 min
Response: 1059092
Conc: 0.80 ng/ml

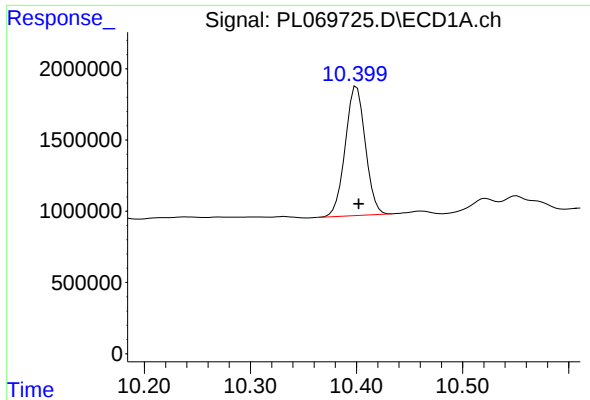


#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.002 min
Response: 11903593
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211052-SI-COMPOSITE-1

Manual Integrations
APPROVED

mohammad
9/7/2021 8:39:54 AM

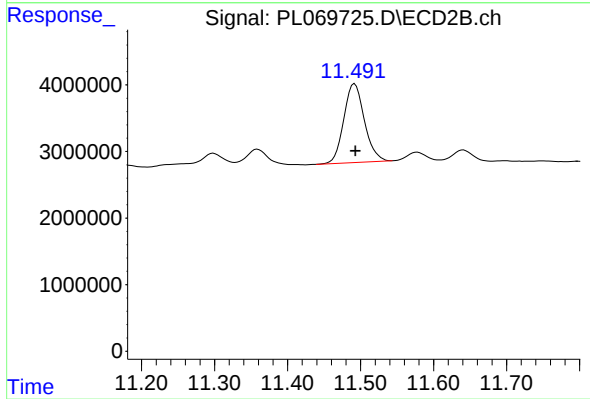

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 23233159
Conc: 20.59 ng/ml