

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090324\
 Data File : PL091482.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 14:39
 Operator : AR\AJ
 Sample : P3812-01 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-083024

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/04/2024
 Supervised By : Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 06:26:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.783	5870832	6392139	2.734m	3.275
28) SA Decachlor...	9.056	7.924	5292026	5513421	3.471m	2.911

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090324\
Data File : PL091482.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 14:39
Operator : AR\AJ
Sample : P3812-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-02-083024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/04/2024
Supervised By : Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 06:26:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

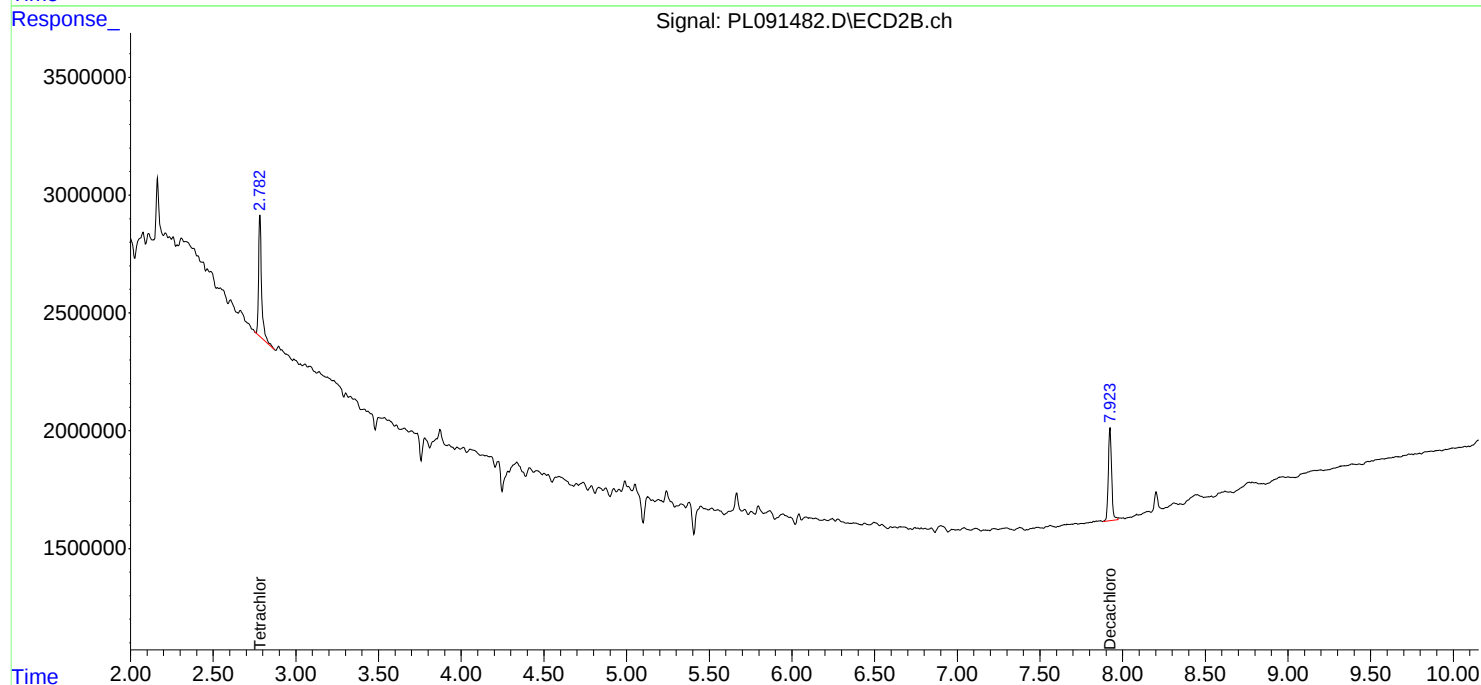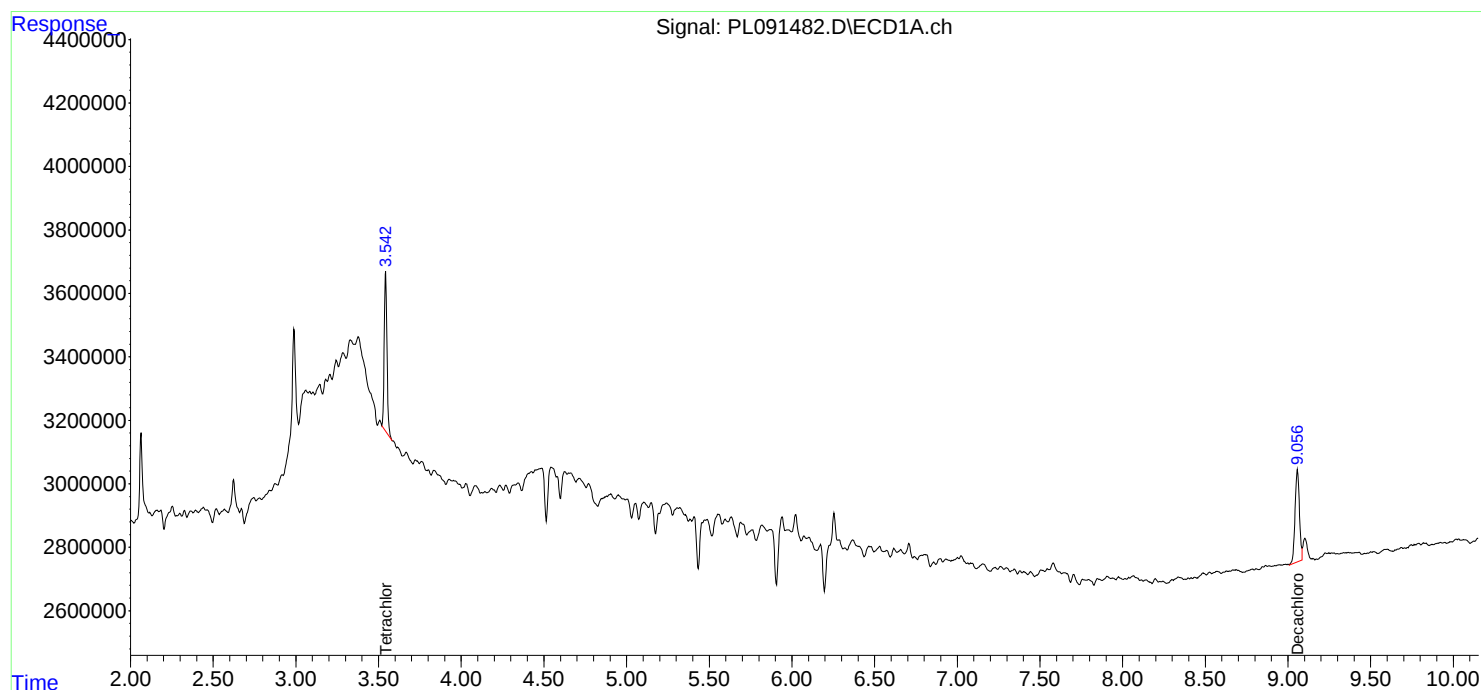

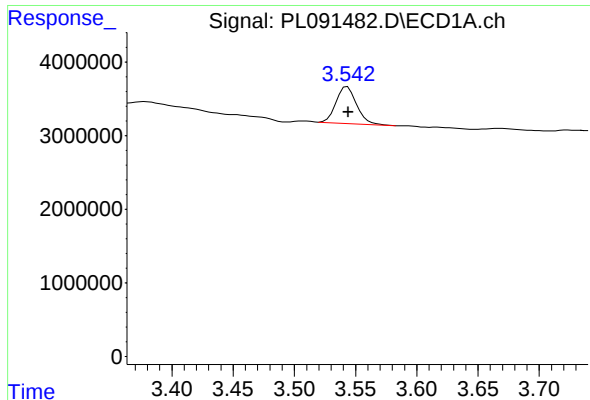


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 5870832
Conc: 2.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-083024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/04/2024
Supervised By :Ankita Jodhani 09/04/2024

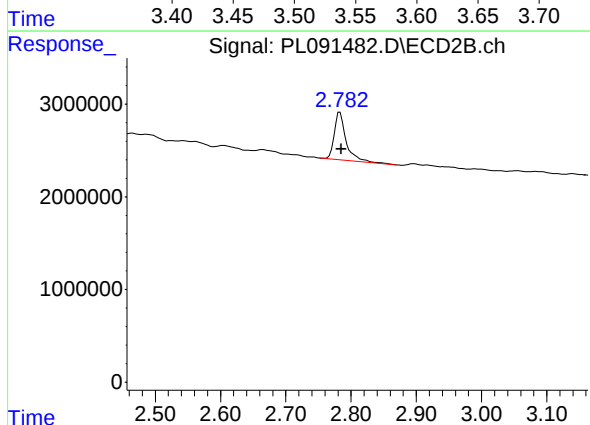


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: -0.002 min
Response: 6392139
Conc: 3.27 ng/ml

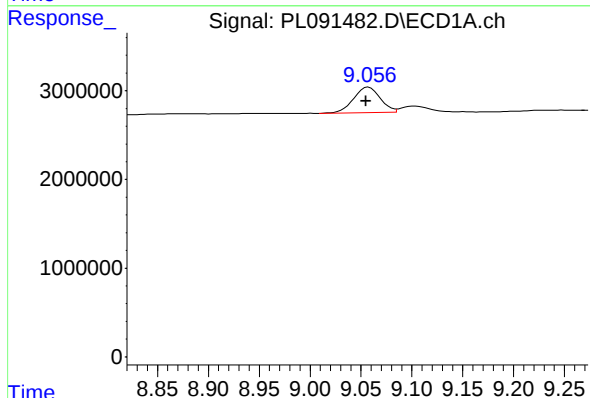

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 5292026
Conc: 3.47 ng/ml m

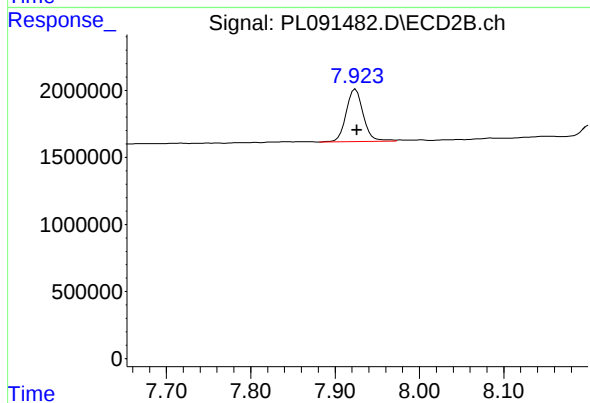

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: -0.002 min
Response: 5513421
Conc: 2.91 ng/ml