

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090418\
 Data File : PL039684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2018 13:13
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:40:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
28)	SA Decachlor...	7.897f	0.000	82513982	0	11.748	N.D.	#
Target Compounds								
9)	A Endosulfan I	5.251f	0.000	1129769	0	0.129	N.D.	#
10)	B gamma-Chl...	5.212	0.000	1295344	0	0.131	N.D.	#
11)	B alpha-Chl...	5.251	0.000	1129769	0	0.118	N.D.	#
13)	MA Dieldrin	5.562	0.000	1171140	0	0.120	N.D.	#
15)	B Endosulfa...	6.002f	0.000	6884400	0	0.792	N.D.	#
16)	A 4,4'-DDD	5.860f	0.000	28593259	0	3.588	N.D.	#
20)	A Methoxychlor	6.636f	0.000	94600296	0	23.117	N.D.	#
21)	B Endrin ke...	6.940	0.000	14552949	0	1.691	N.D.	#
25)	Chlordane-3	5.212	0.000	1295344	0	1.186	N.D.	#
26)	Chlordane-4	5.251	0.000	1129769	0	1.131	N.D.	#
27)	Chlordane-5	6.002	0.000	6884400	0	21.227	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090418\
Data File : PL039684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2018 13:13
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:40:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

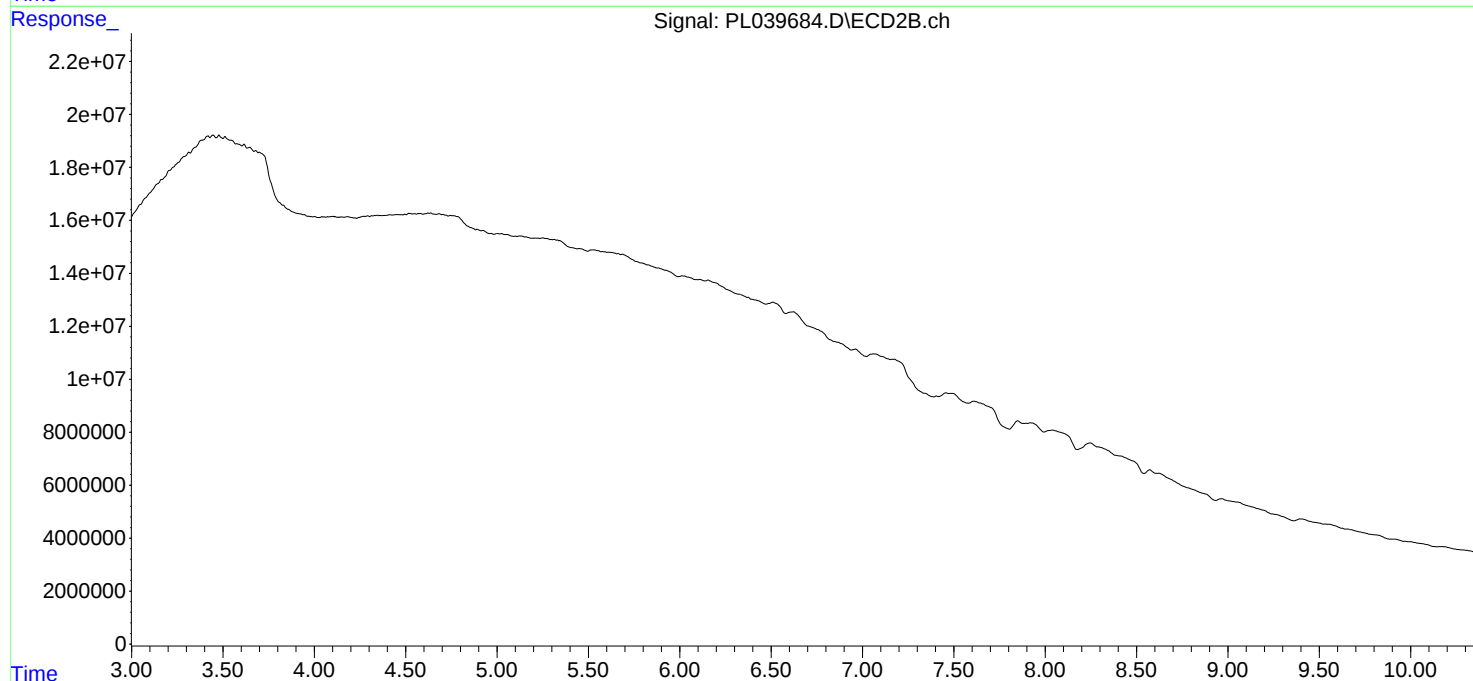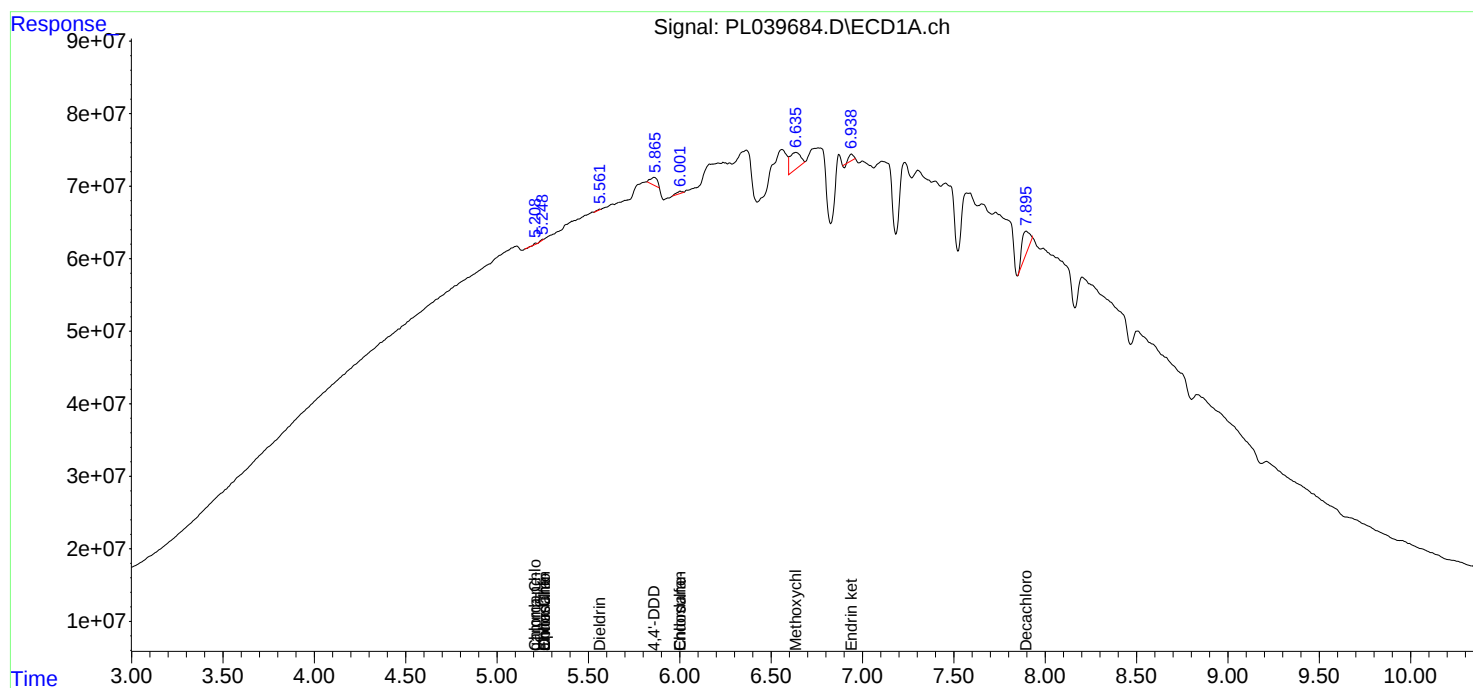


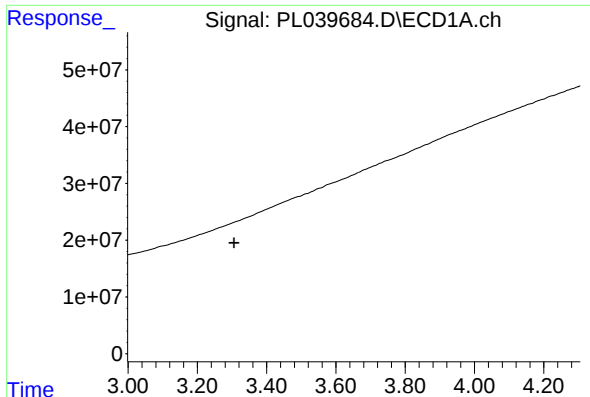

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

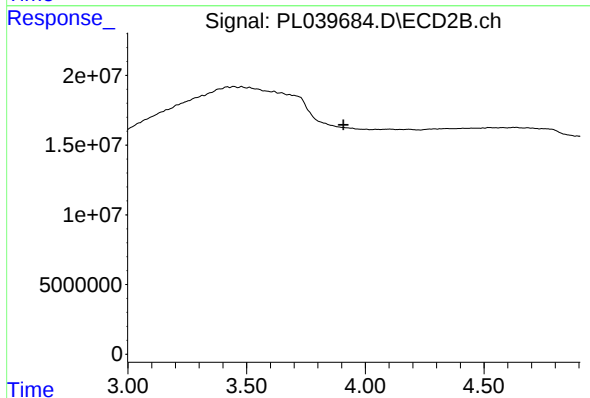


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.907 min
Response: 0
Conc: N.D.

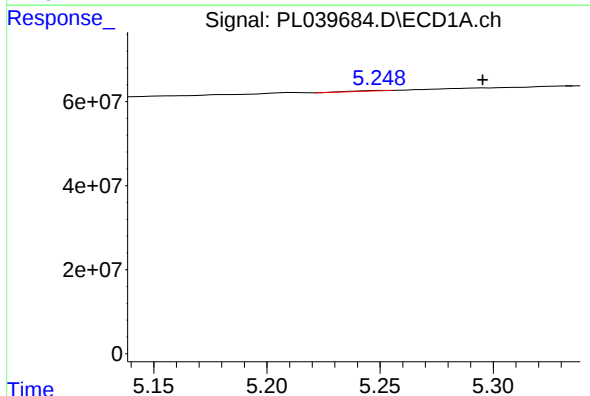


#9 Endosulfan I

R.T.: 5.251 min
Delta R.T.: -0.044 min
Response: 1129769
Conc: 0.13 ng/ml

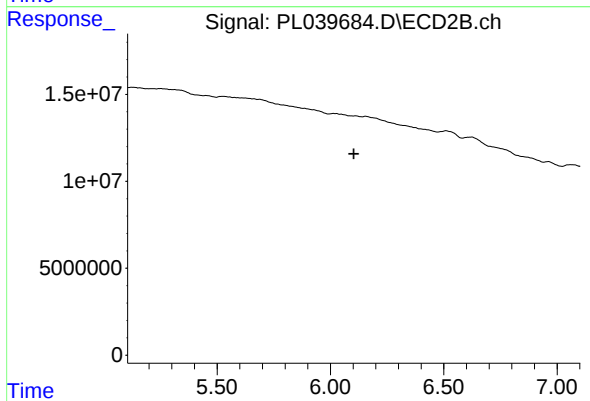

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.102 min
Response: 0
Conc: N.D.

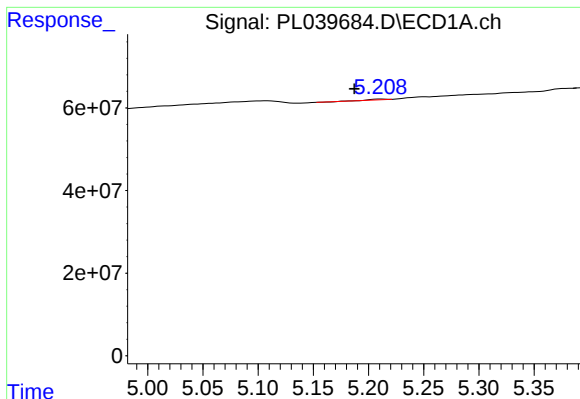

#10 gamma-Chlordane


R.T.: 5.212 min
Delta R.T.: 0.024 min
Response: 1295344
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

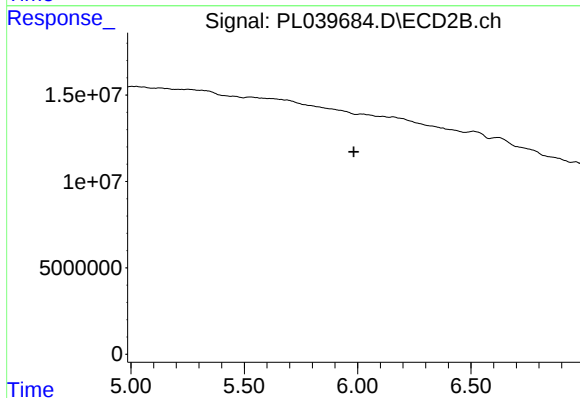


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

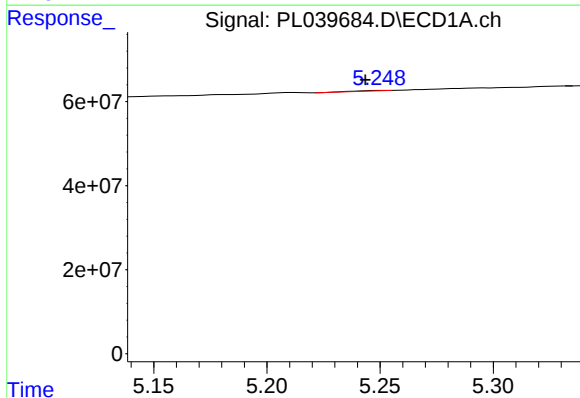


#11 alpha-Chlordane

R.T.: 5.251 min
Delta R.T.: 0.008 min
Response: 1129769
Conc: 0.12 ng/ml

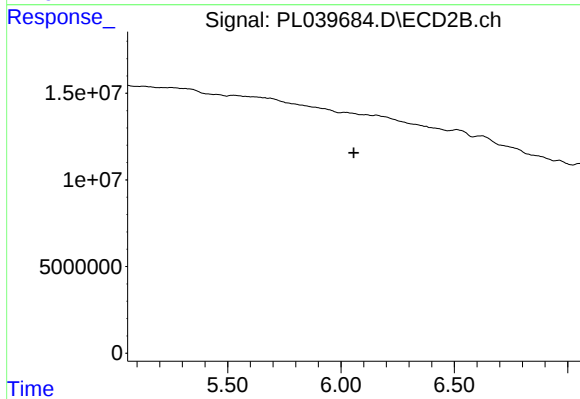

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

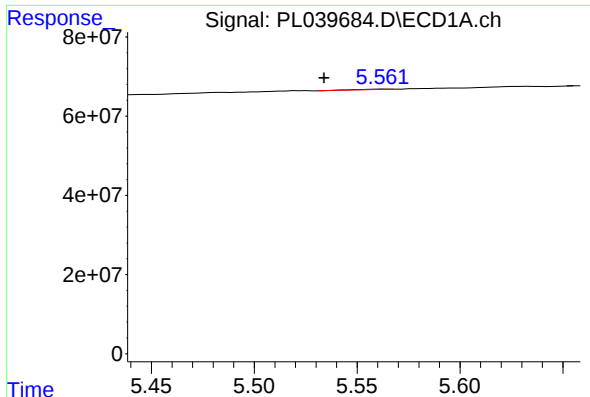

#13 Dieldrin


R.T.: 5.562 min
Delta R.T.: 0.028 min
Response: 1171140
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

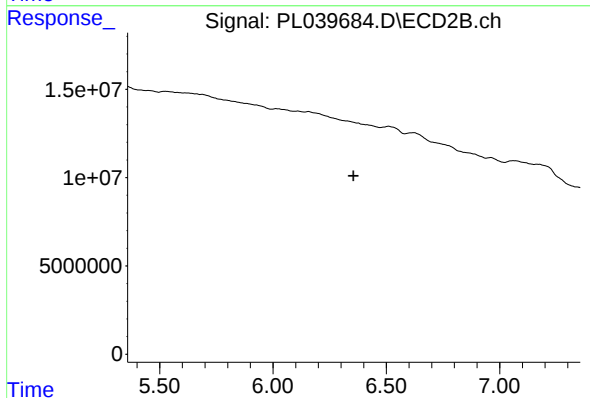


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

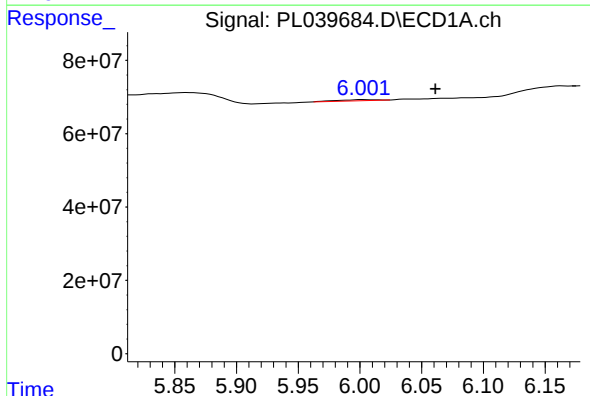


#15 Endosulfan II

R.T.: 6.002 min
Delta R.T.: -0.059 min
Response: 6884400
Conc: 0.79 ng/ml

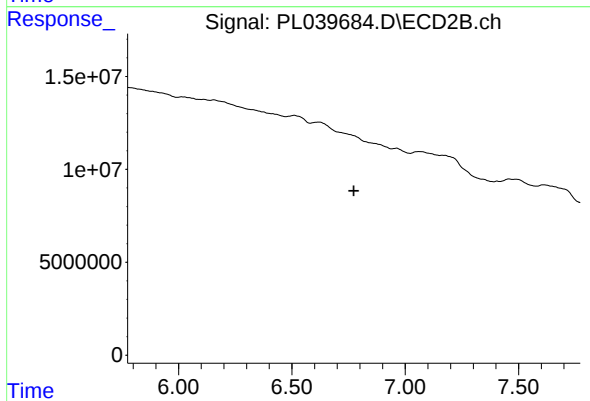

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

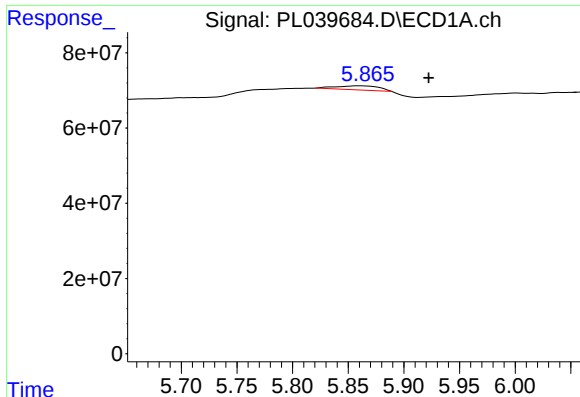

#16 4,4'-DDD


R.T.: 5.860 min
Delta R.T.: -0.062 min
Response: 28593259
Conc: 3.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

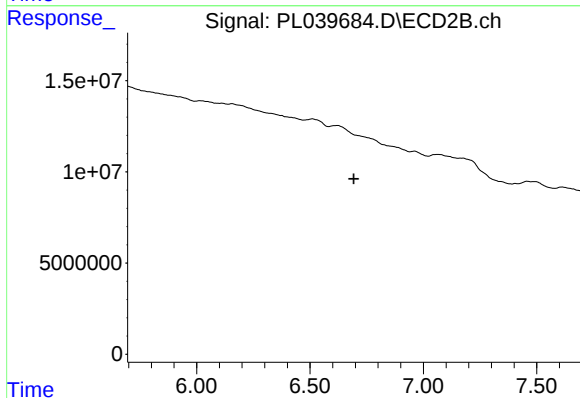


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

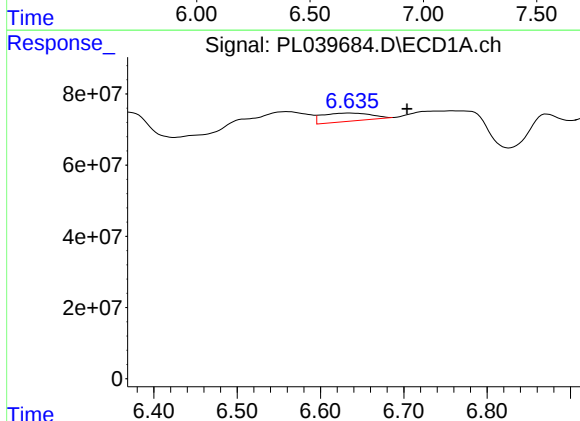


#20 Methoxychlor

R.T.: 6.636 min
Delta R.T.: -0.068 min
Response: 94600296
Conc: 23.12 ng/ml

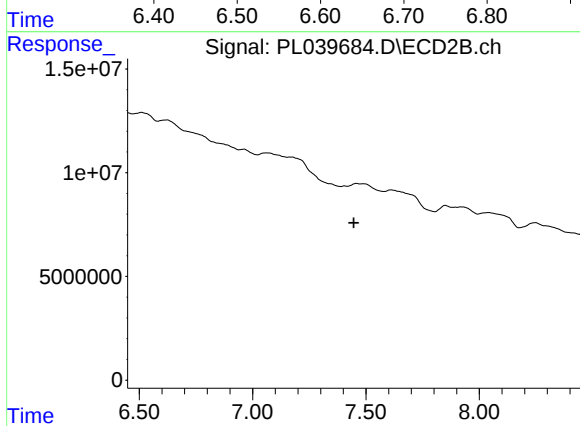

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

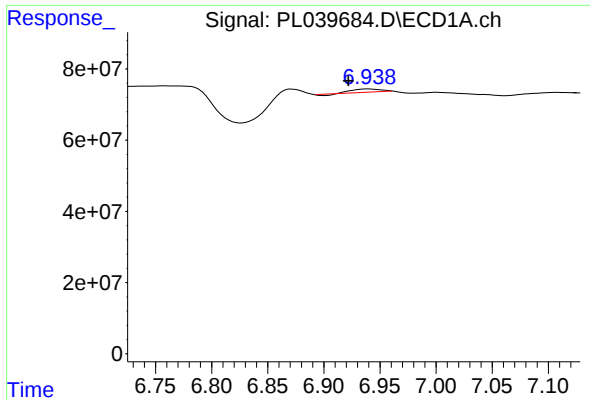

#21 Endrin ketone


R.T.: 6.940 min
Delta R.T.: 0.018 min
Response: 14552949
Conc: 1.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

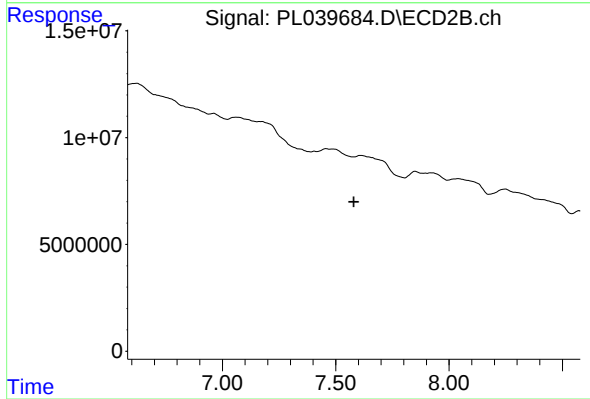


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.580 min
Response: 0
Conc: N.D.

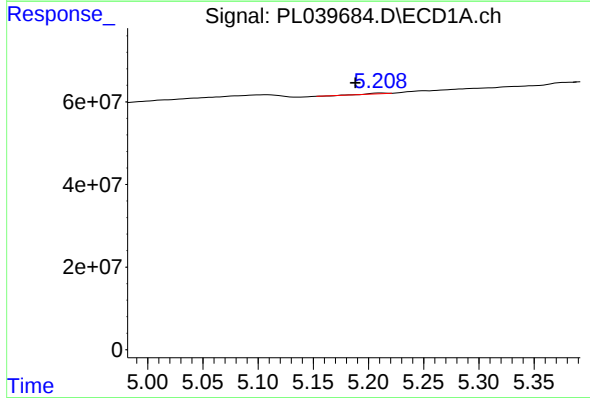


#25 Chlordane-3

R.T.: 5.212 min
Delta R.T.: 0.024 min
Response: 1295344
Conc: 1.19 ng/ml

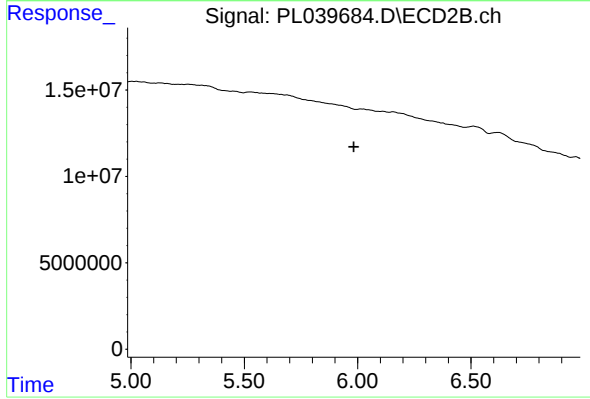

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

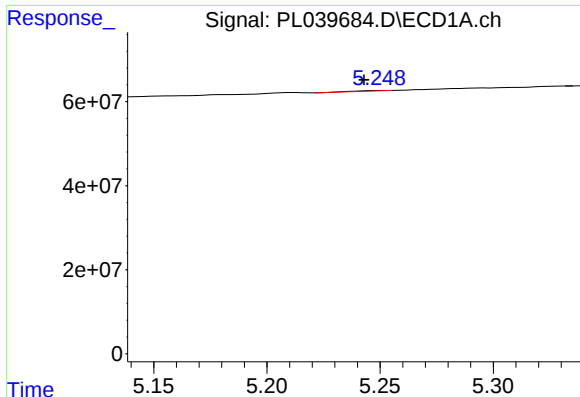

#26 Chlordane-4


R.T.: 5.251 min
Delta R.T.: 0.008 min
Response: 1129769
Conc: 1.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

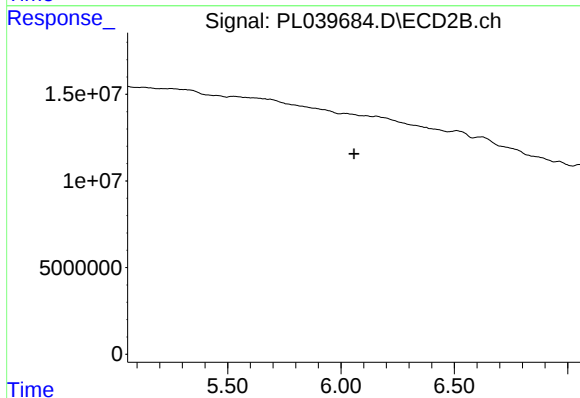


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

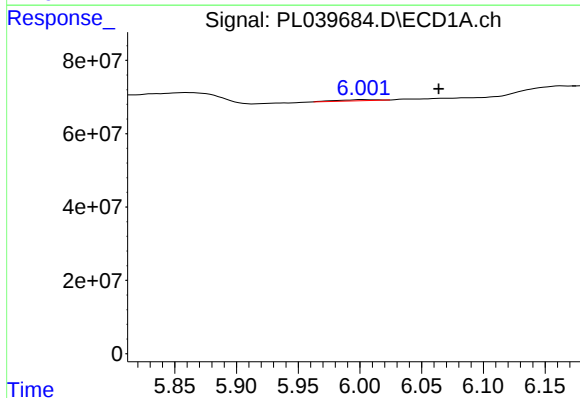


#27 Chlordane-5

R.T.: 6.002 min
Delta R.T.: -0.062 min
Response: 6884400
Conc: 21.23 ng/ml

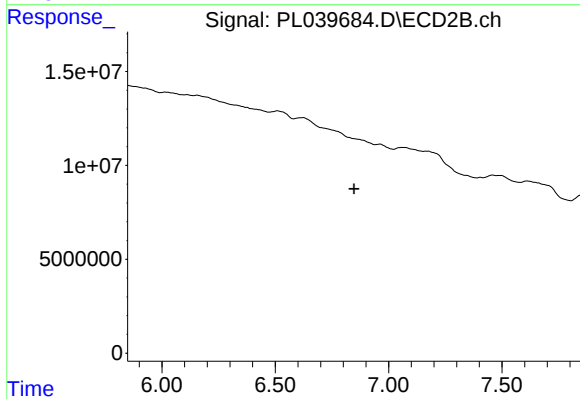

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

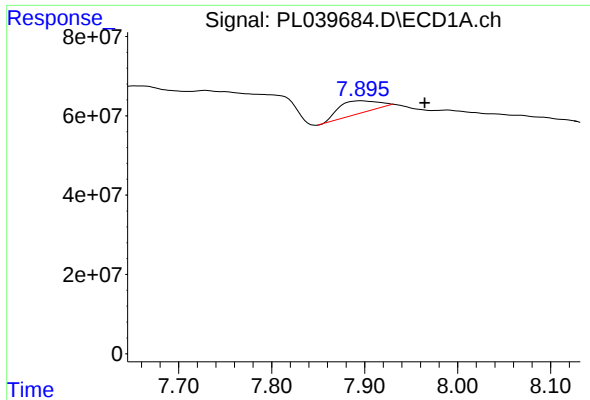

#28 Decachlorobiphenyl

R.T.: 7.897 min
Delta R.T.: -0.068 min
Response: 82513982
Conc: 11.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

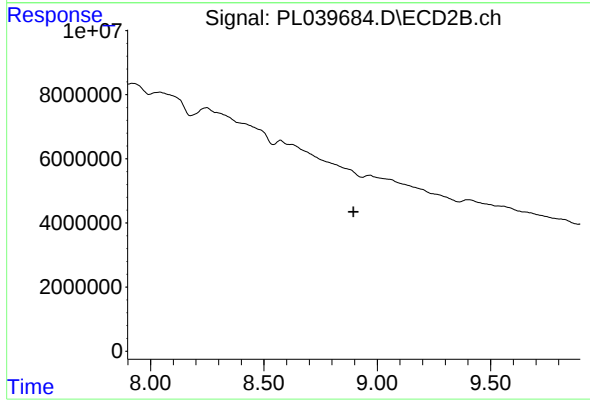

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.