

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090418\
 Data File : PL039693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2018 15:46
 Operator : AJ\SJ
 Sample : J4757-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:44:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.905	78079355	29491182	11.169	11.000
28)	SA Decachlor...	7.955	8.890	59182925	24535484	8.427	10.573 #
Target Compounds							
8)	B Heptachlo...	4.924f	0.000	2778599	0	0.291	N.D. #
10)	B gamma-Chl...	5.186	0.000	49487142	0	5.010	N.D. #
11)	B alpha-Chl...	5.186f	0.000	49487142	0	5.151	N.D. #
12)	B 4,4'-DDE	5.406	6.208	140.2E6	41822900	14.642	13.526
17)	MA 4,4'-DDT	6.148	0.000	5638413	0	0.744	N.D. #
23)	Chlordane-1	4.151	0.000	19456244	0	61.456	N.D. #
24)	Chlordane-2	4.663	0.000	21352209	0	61.078	N.D. #
25)	Chlordane-3	5.186	0.000	49487142	0	45.307	N.D. #
26)	Chlordane-4	5.186	0.000	49487142	0	49.519	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090418\
Data File : PL039693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2018 15:46
Operator : AJ\SJ
Sample : J4757-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:44:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

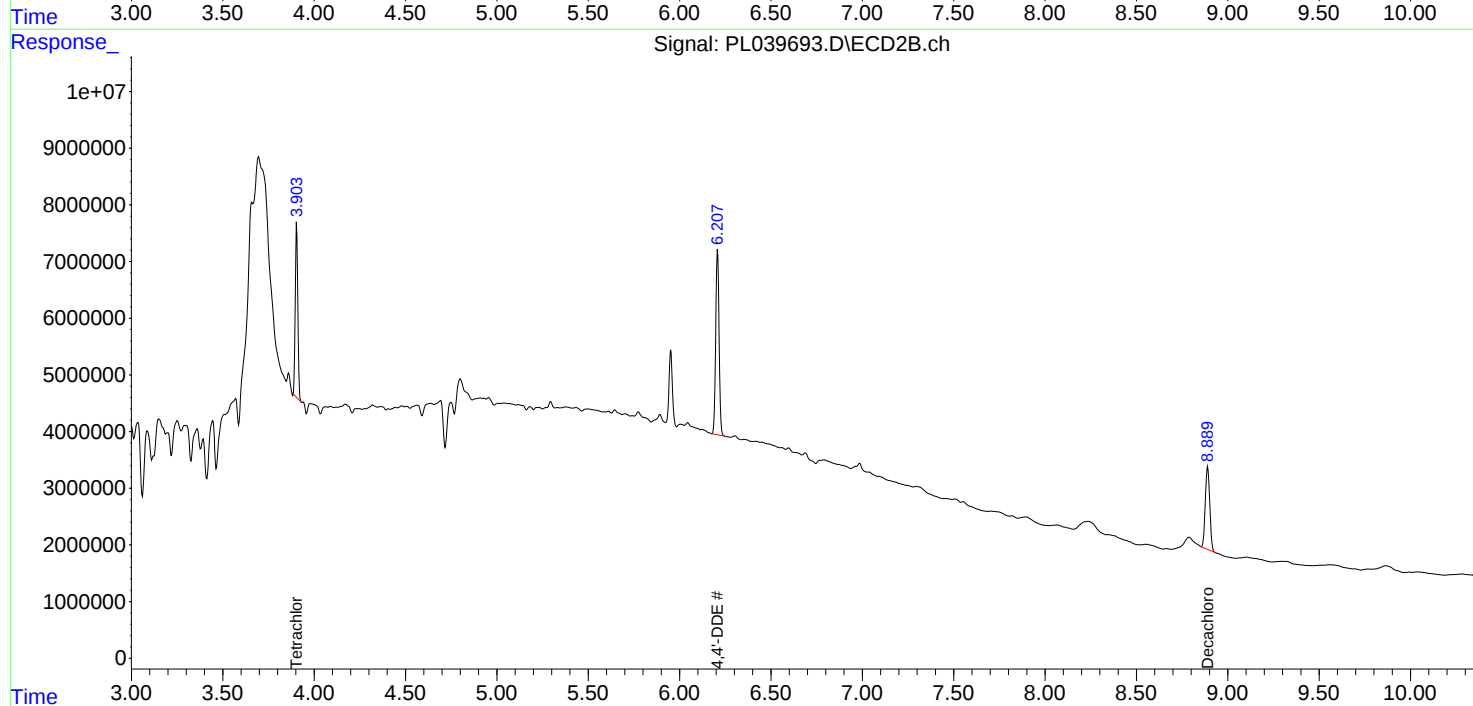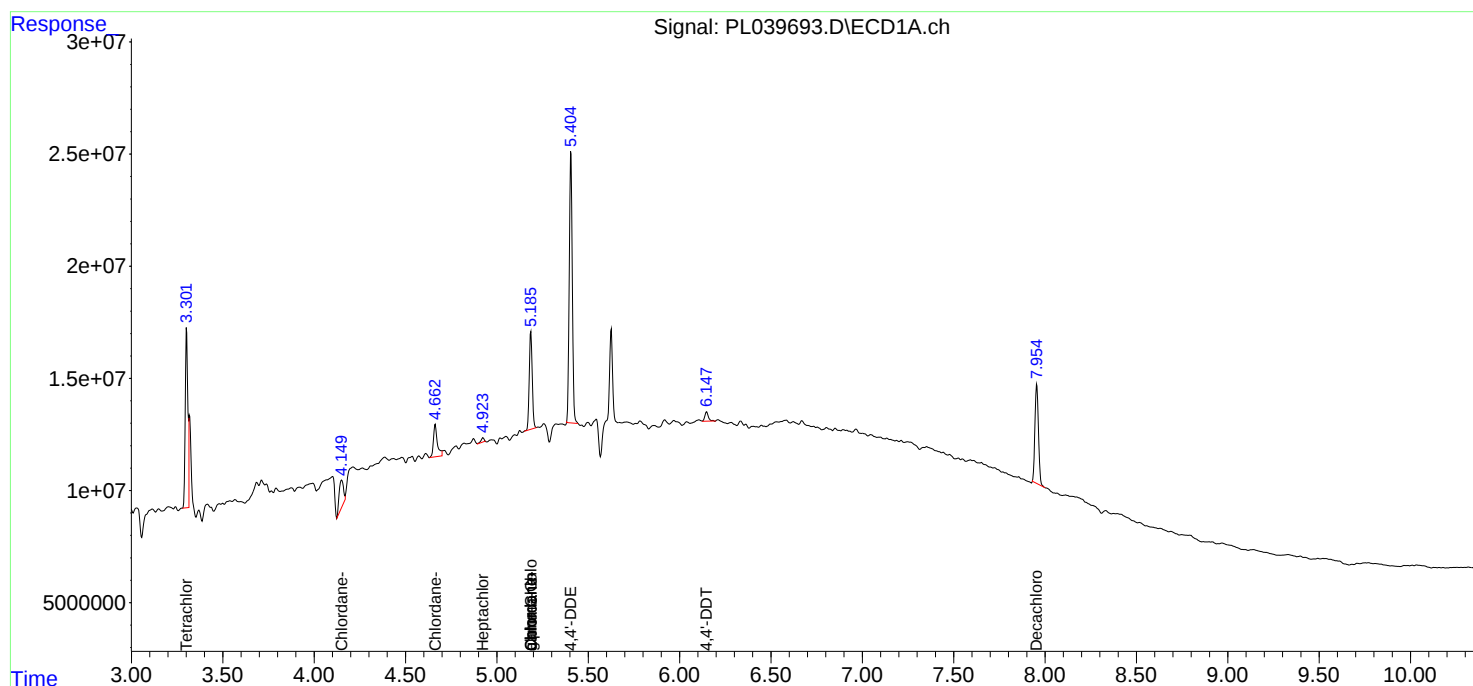


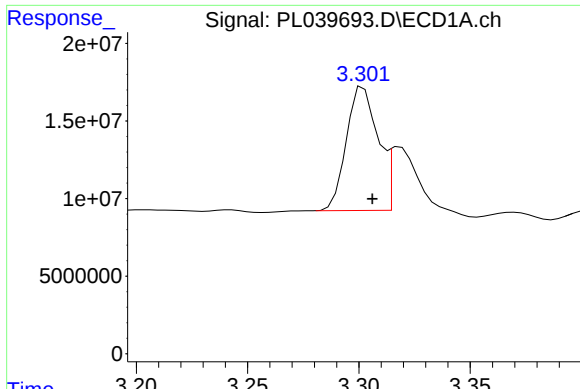

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: -0.004 min
Response: 78079355
Conc: 11.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

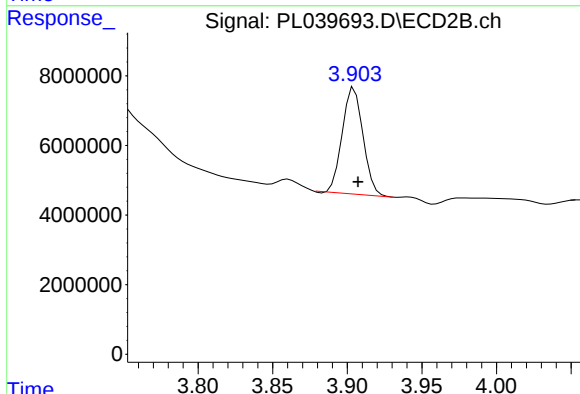


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.003 min
Response: 29491182
Conc: 11.00 ng/ml

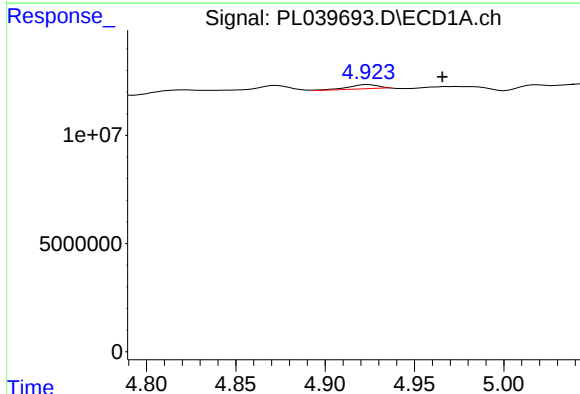


#8 Heptachlor epoxide

R.T.: 4.924 min
Delta R.T.: -0.041 min
Response: 2778599
Conc: 0.29 ng/ml

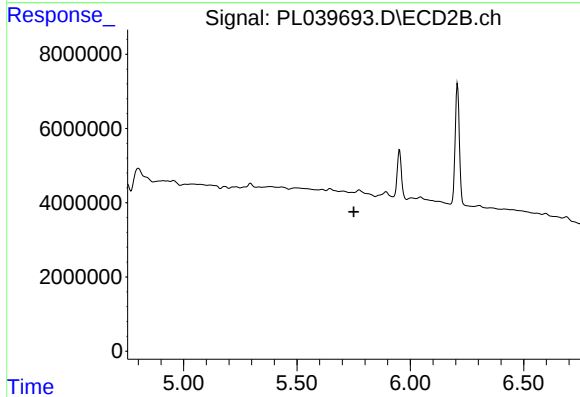

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

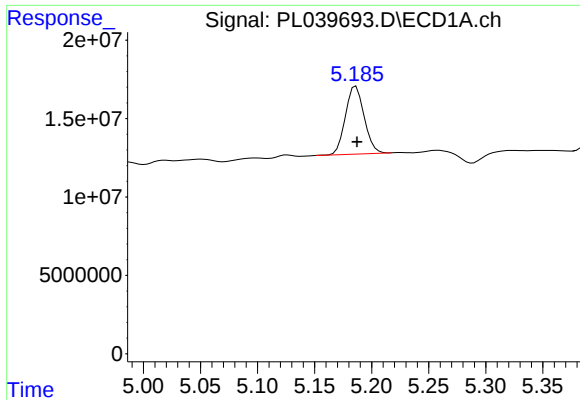

#10 gamma-Chlordane


R.T.: 5.186 min
Delta R.T.: -0.001 min
Response: 49487142
Conc: 5.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

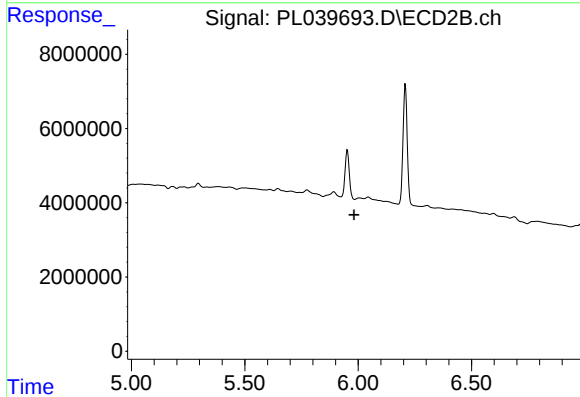


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

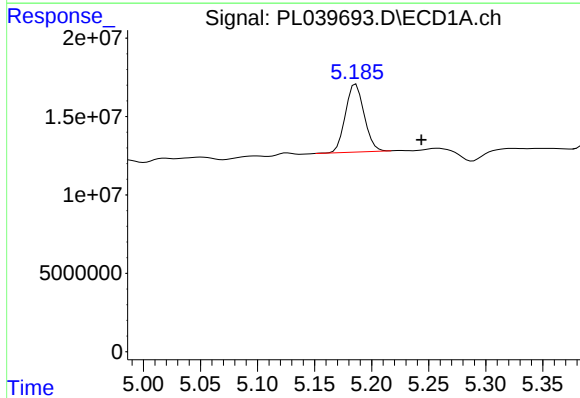


#11 alpha-Chlordane

R.T.: 5.186 min
Delta R.T.: -0.057 min
Response: 49487142
Conc: 5.15 ng/ml

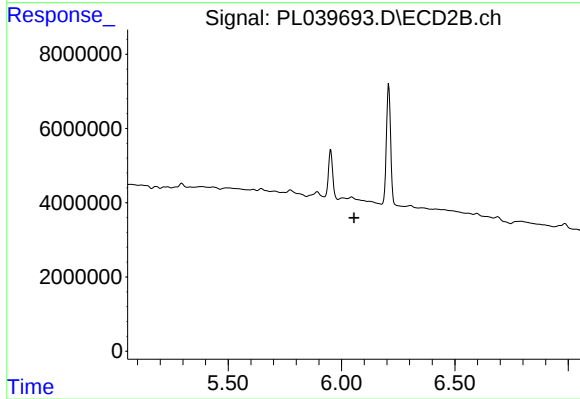

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

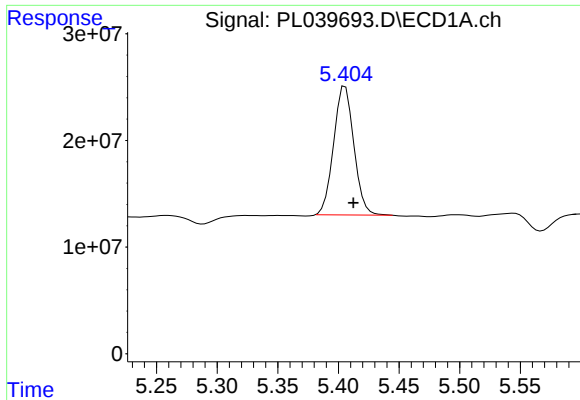

#12 4,4'-DDE


R.T.: 5.406 min
Delta R.T.: -0.007 min
Response: 140214720
Conc: 14.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

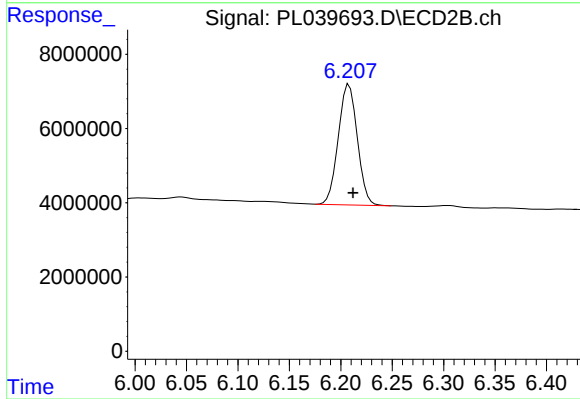


#12 4,4'-DDE

R.T.: 6.208 min
Delta R.T.: -0.004 min
Response: 41822900
Conc: 13.53 ng/ml

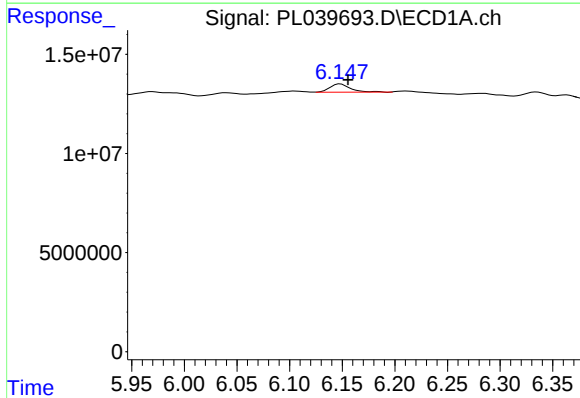


#17 4,4'-DDT

R.T.: 6.148 min
Delta R.T.: -0.007 min
Response: 5638413
Conc: 0.74 ng/ml

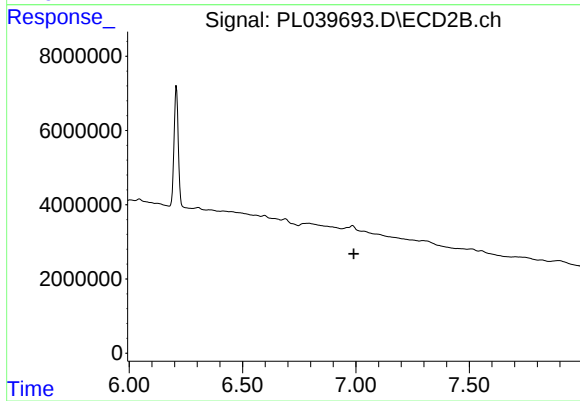

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.991 min
Response: 0
Conc: N.D.

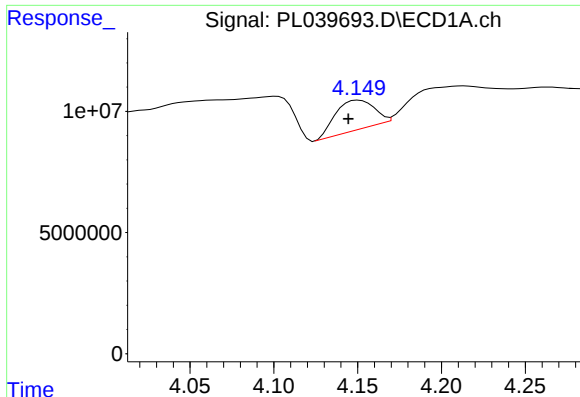

#23 Chlordane-1


R.T.: 4.151 min
Delta R.T.: 0.006 min
Response: 19456244
Conc: 61.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

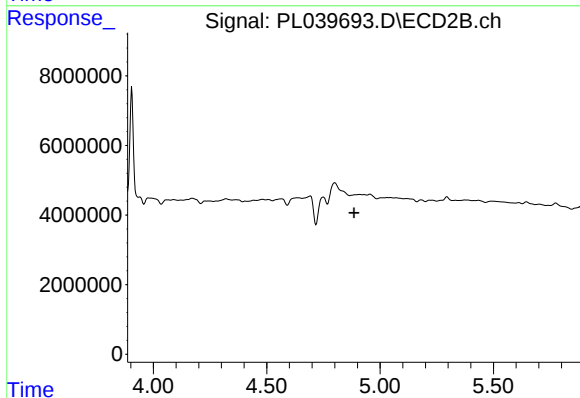


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

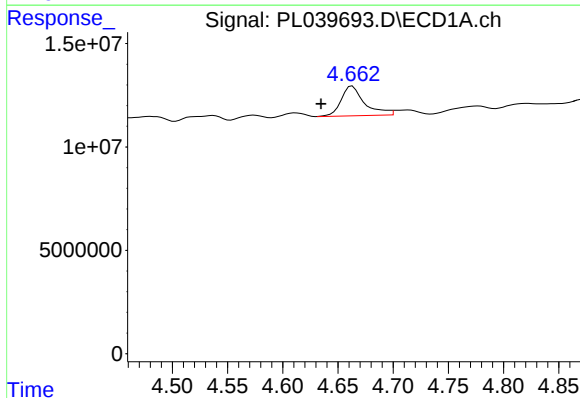


#24 Chlordane-2

R.T.: 4.663 min
Delta R.T.: 0.028 min
Response: 21352209
Conc: 61.08 ng/ml

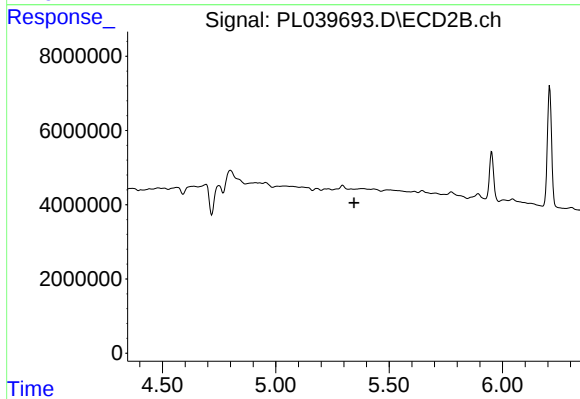

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

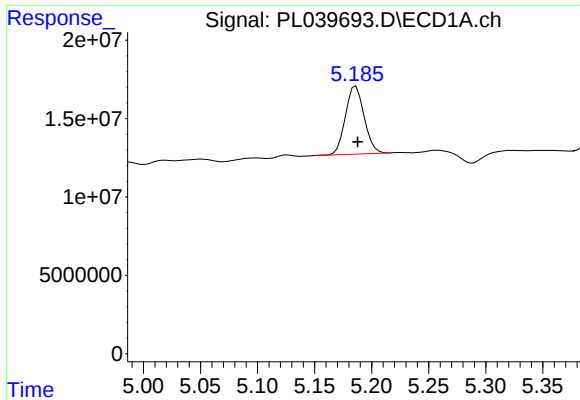

#25 Chlordane-3


R.T.: 5.186 min
Delta R.T.: -0.002 min
Response: 49487142
Conc: 45.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

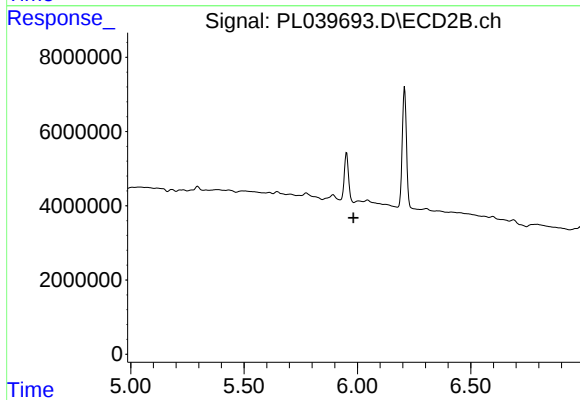


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

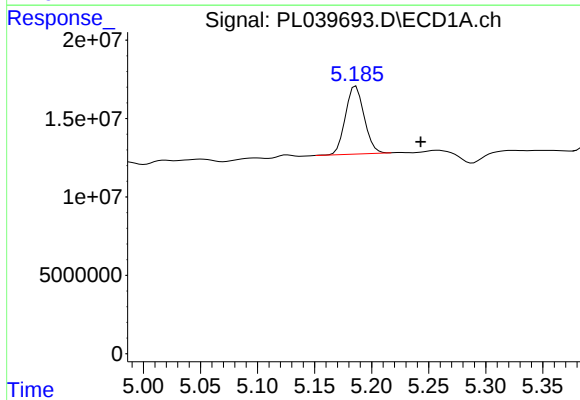


#26 Chlordane-4

R.T.: 5.186 min
Delta R.T.: -0.057 min
Response: 49487142
Conc: 49.52 ng/ml

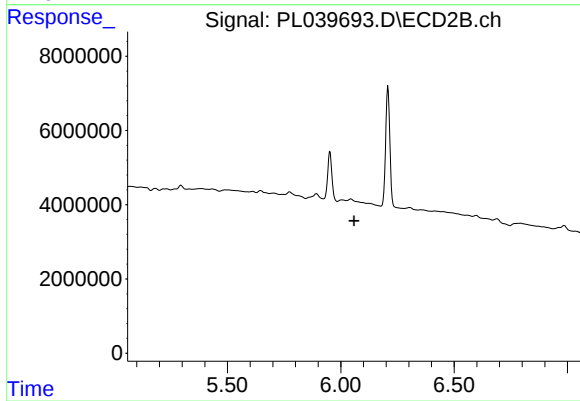

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

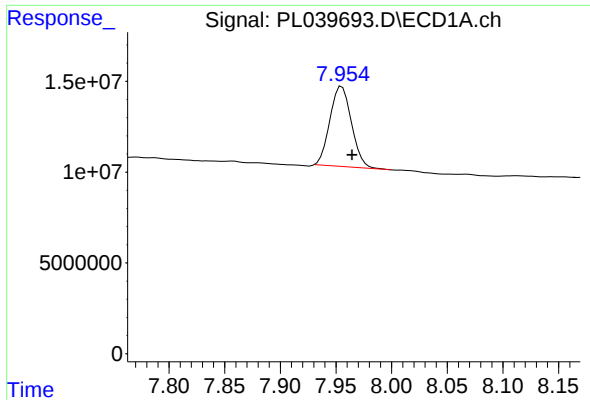

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: -0.009 min
Response: 59182925
Conc: 8.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

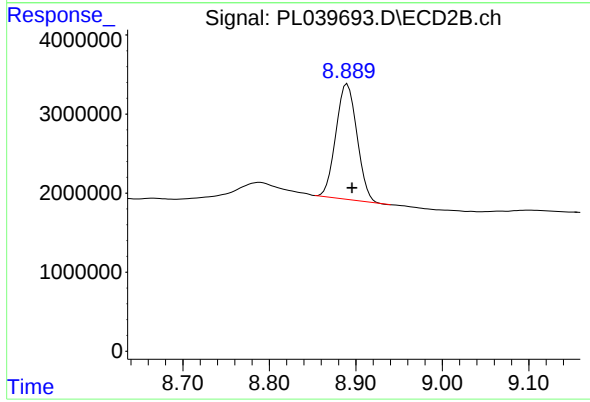

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: -0.005 min
Response: 24535484
Conc: 10.57 ng/ml