

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
 Data File : PL052198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2019 08:54
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 00:46:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	0.000	4.799f	0	1411486	N.D.	0.968 #
8) B	Heptachlo...	0.000	5.788	0	1697224	N.D.	0.503 #
9) A	Endosulfan I	5.329f	6.141	8413178	486107	0.626	0.150 #
11) B	alpha-Chl...	0.000	6.102	0	698852	N.D.	0.203 #
15) B	Endosulfa...	0.000	6.847f	0	682213	N.D.	0.207 #
17) MA	4,4'-DDT	6.160	0.000	7639462	0	0.599	N.D. #
18) B	Endrin al...	6.226	6.946	6974757	777442	0.600	0.275 #
20) A	Methoxychlor	0.000	7.495	0	2080181	N.D.	1.240 #
26)	Chlordane-4	0.000	6.102	0	698852	N.D.	1.287 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
Data File : PL052198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2019 08:54
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 00:46:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

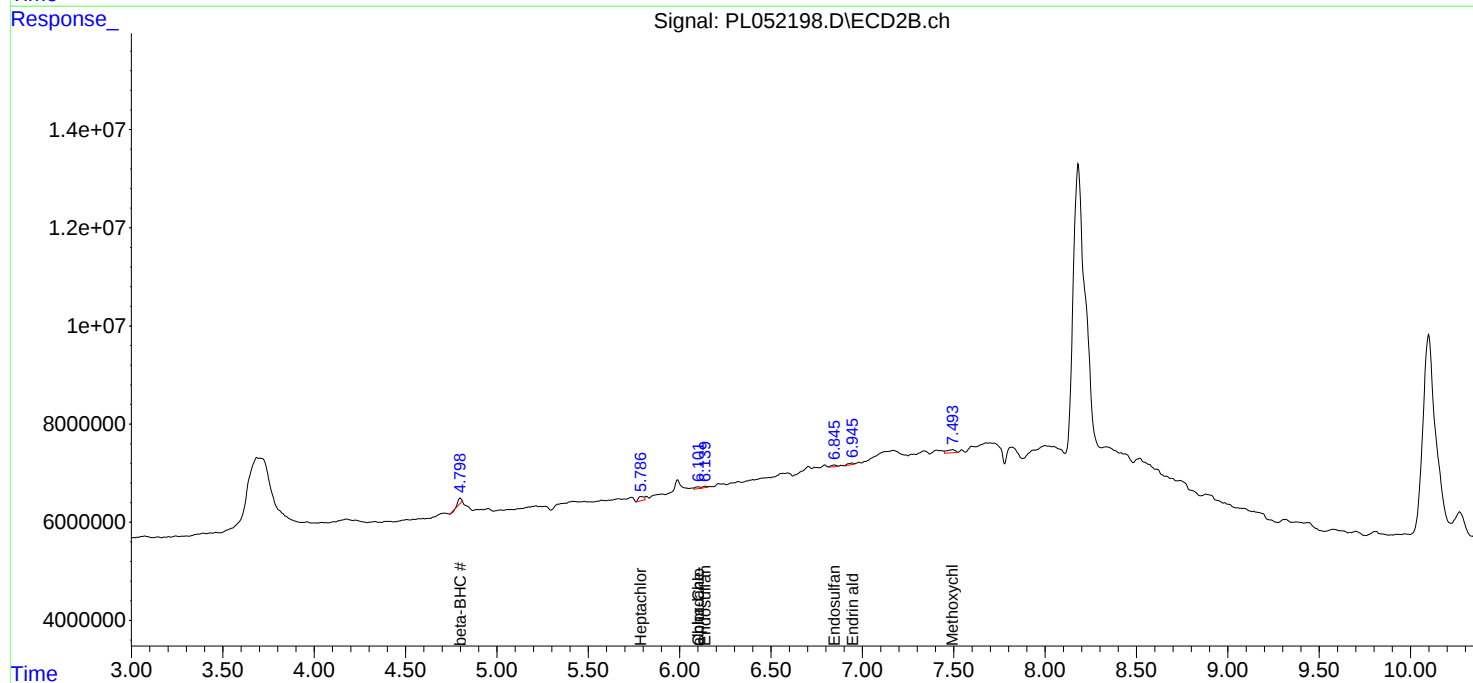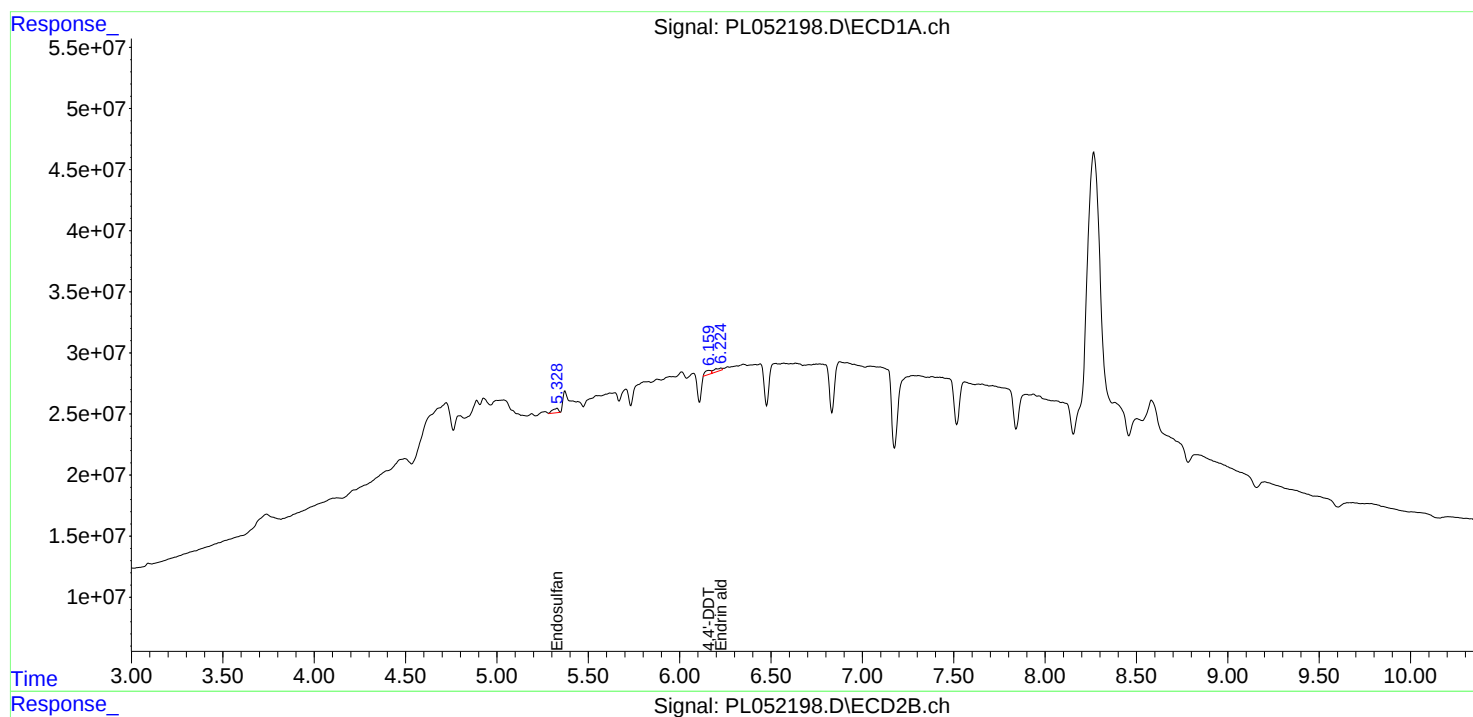


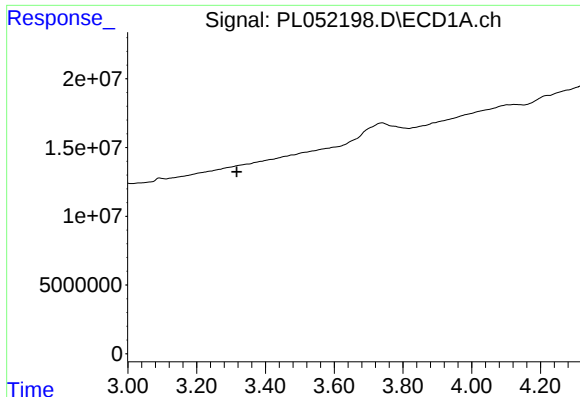

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

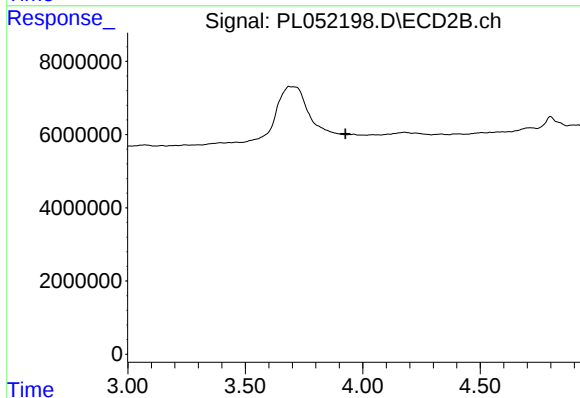


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.927 min
Response: 0
Conc: N.D.

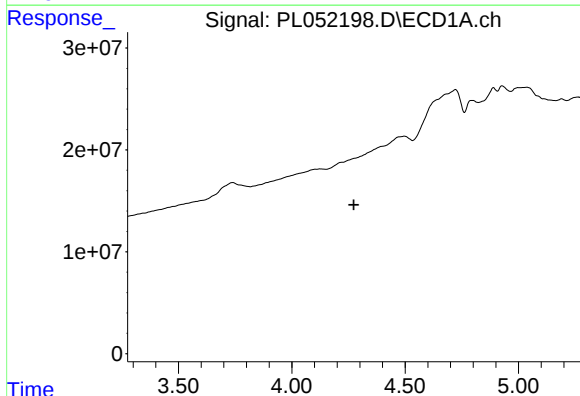


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

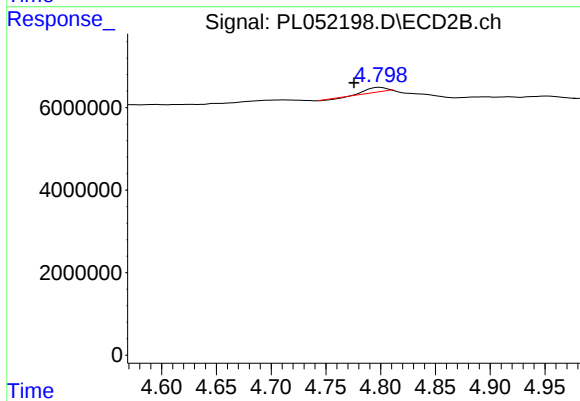

#6 beta-BHC


R.T.: 4.799 min
Delta R.T.: 0.023 min
Response: 1411486
Conc: 0.97 ng/ml

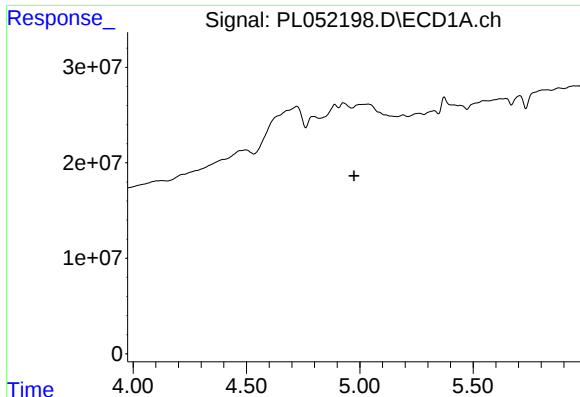

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

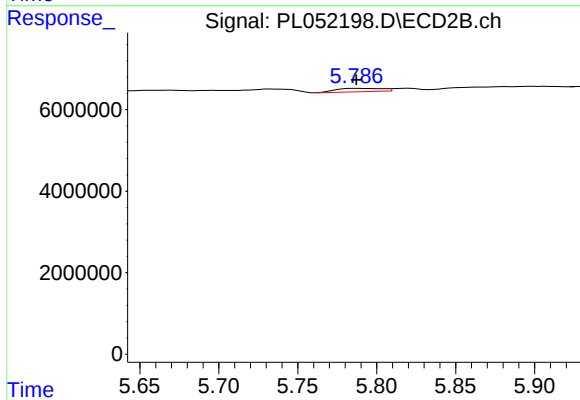


#8 Heptachlor epoxide

R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 1697224
Conc: 0.50 ng/ml

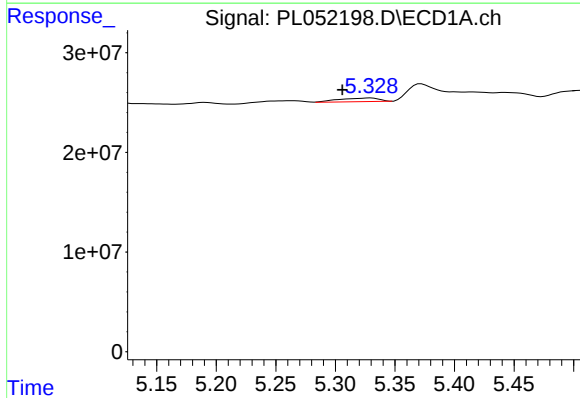


#9 Endosulfan I

R.T.: 5.329 min
Delta R.T.: 0.024 min
Response: 8413178
Conc: 0.63 ng/ml

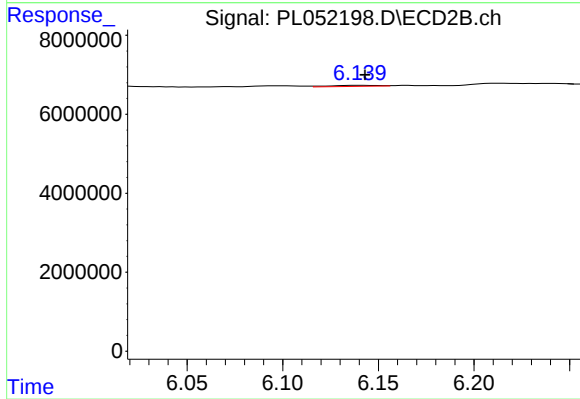

#9 Endosulfan I


R.T.: 6.141 min
Delta R.T.: -0.002 min
Response: 486107
Conc: 0.15 ng/ml

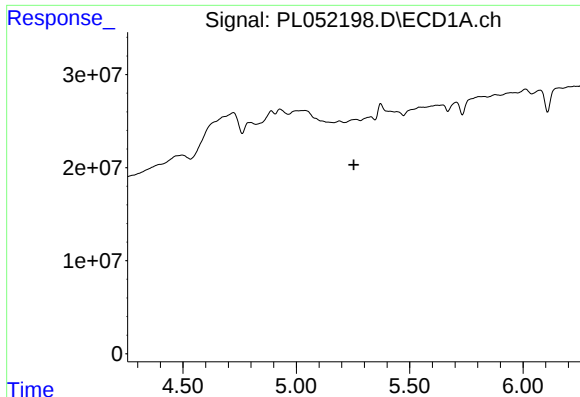

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

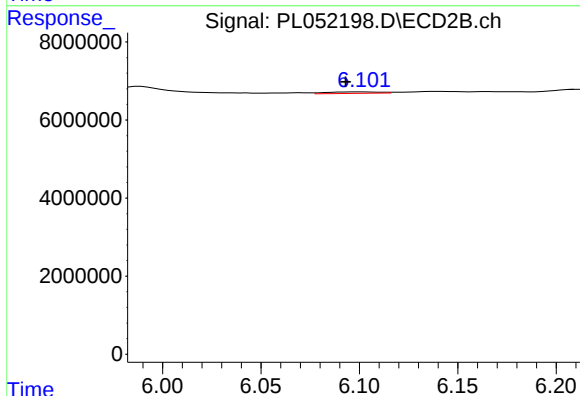


#11 alpha-Chlordane

R.T.: 6.102 min
Delta R.T.: 0.009 min
Response: 698852
Conc: 0.20 ng/ml

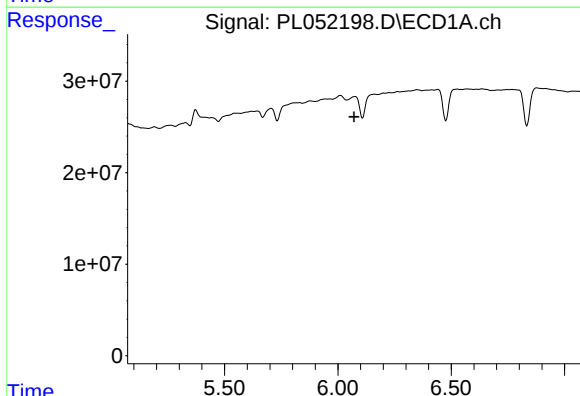


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

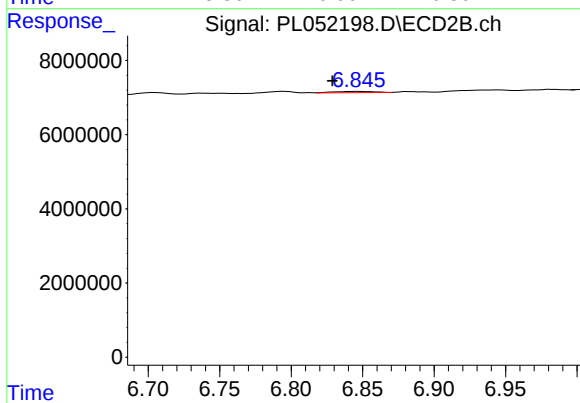

#15 Endosulfan II


R.T.: 6.847 min
Delta R.T.: 0.018 min
Response: 682213
Conc: 0.21 ng/ml

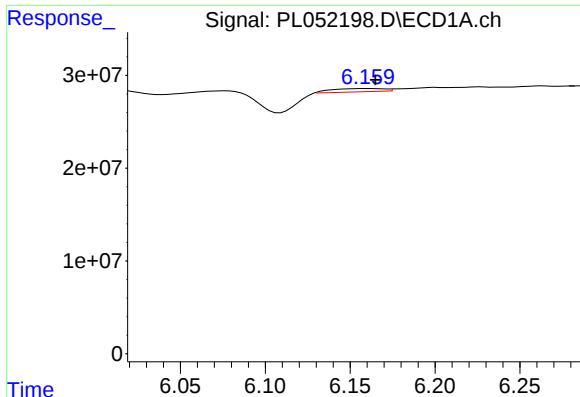

#17 4,4'-DDT


R.T.: 6.160 min
Delta R.T.: -0.005 min
Response: 7639462
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

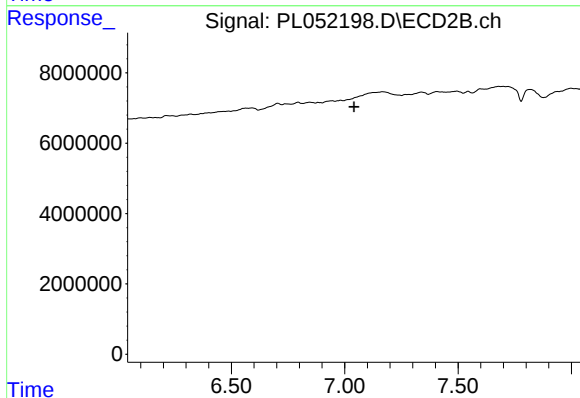


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

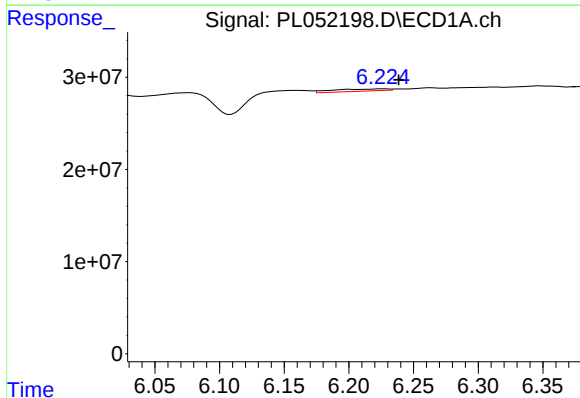


#18 Endrin aldehyde

R.T.: 6.226 min
Delta R.T.: -0.013 min
Response: 6974757
Conc: 0.60 ng/ml

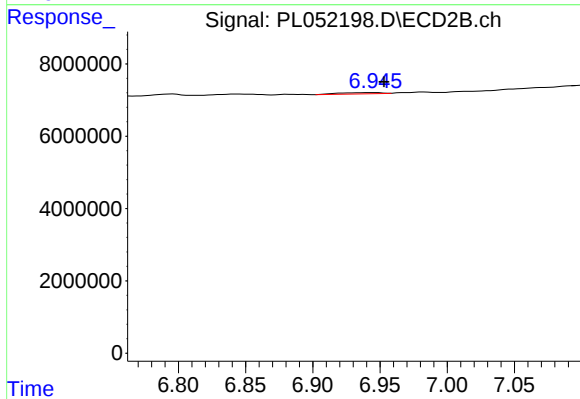

#18 Endrin aldehyde


R.T.: 6.946 min
Delta R.T.: -0.007 min
Response: 777442
Conc: 0.28 ng/ml

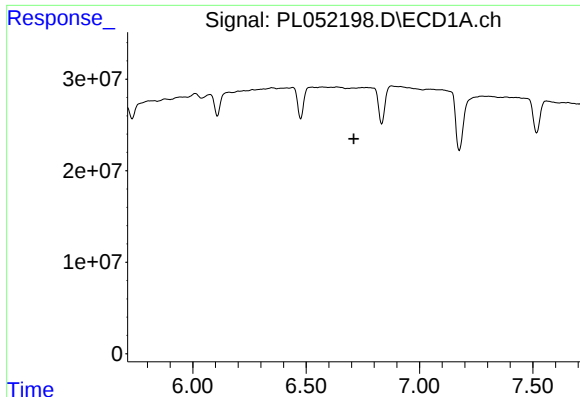

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

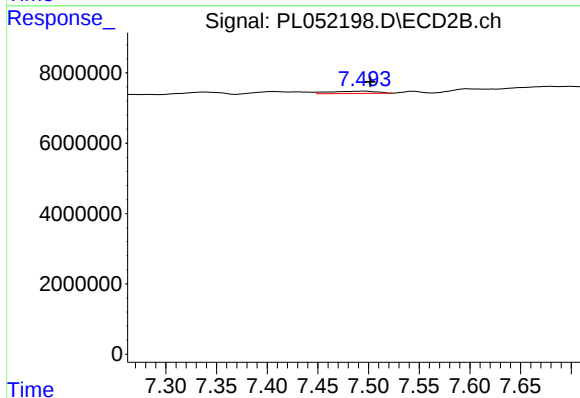


#20 Methoxychlor

R.T.: 7.495 min
Delta R.T.: -0.007 min
Response: 2080181
Conc: 1.24 ng/ml

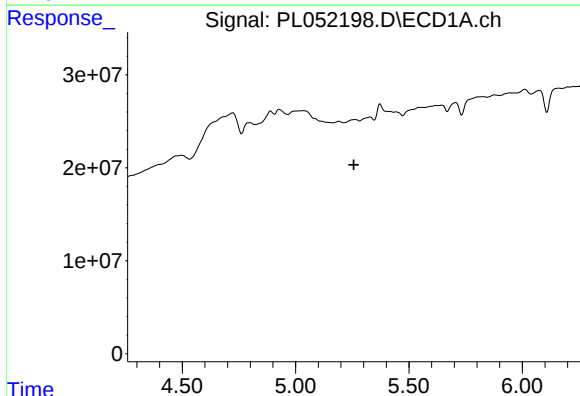


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

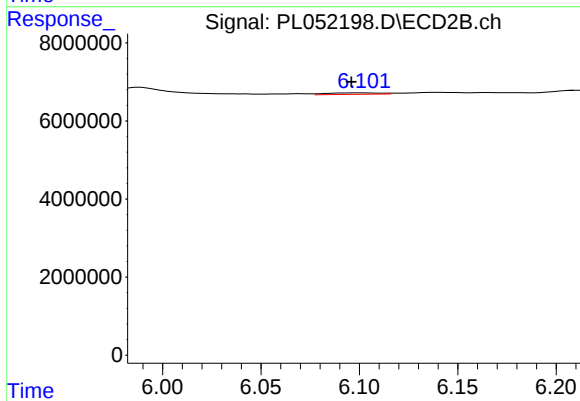

#26 Chlordane-4


R.T.: 6.102 min
Delta R.T.: 0.006 min
Response: 698852
Conc: 1.29 ng/ml

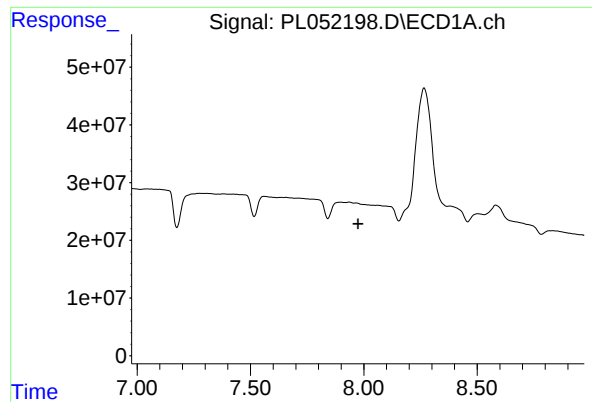

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

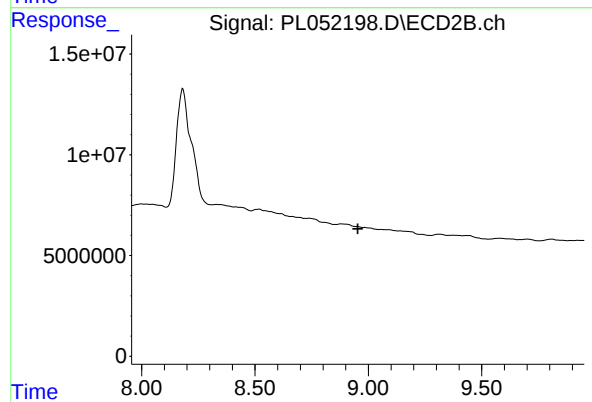

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.954 min
Response: 0
Conc: N.D.