

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
 Data File : PL052220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2019 18:03
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 00:55:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	217.9E6	54961499	25.463	25.156
28)	SA Decachlor...	7.969	8.948	243.7E6	65676911	20.077	21.577
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	521869	N.D.	0.358 #
8)	B Heptachlo...	0.000	5.784	0	5550061	N.D.	1.645 #
9)	A Endosulfan I	5.323f	0.000	9134106	0	0.679	N.D. #
13)	MA Dieldrin	5.538	6.408	5764261	-89009	0.379	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052220.D
Data File : PL052220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2019 18:03
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 00:55:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

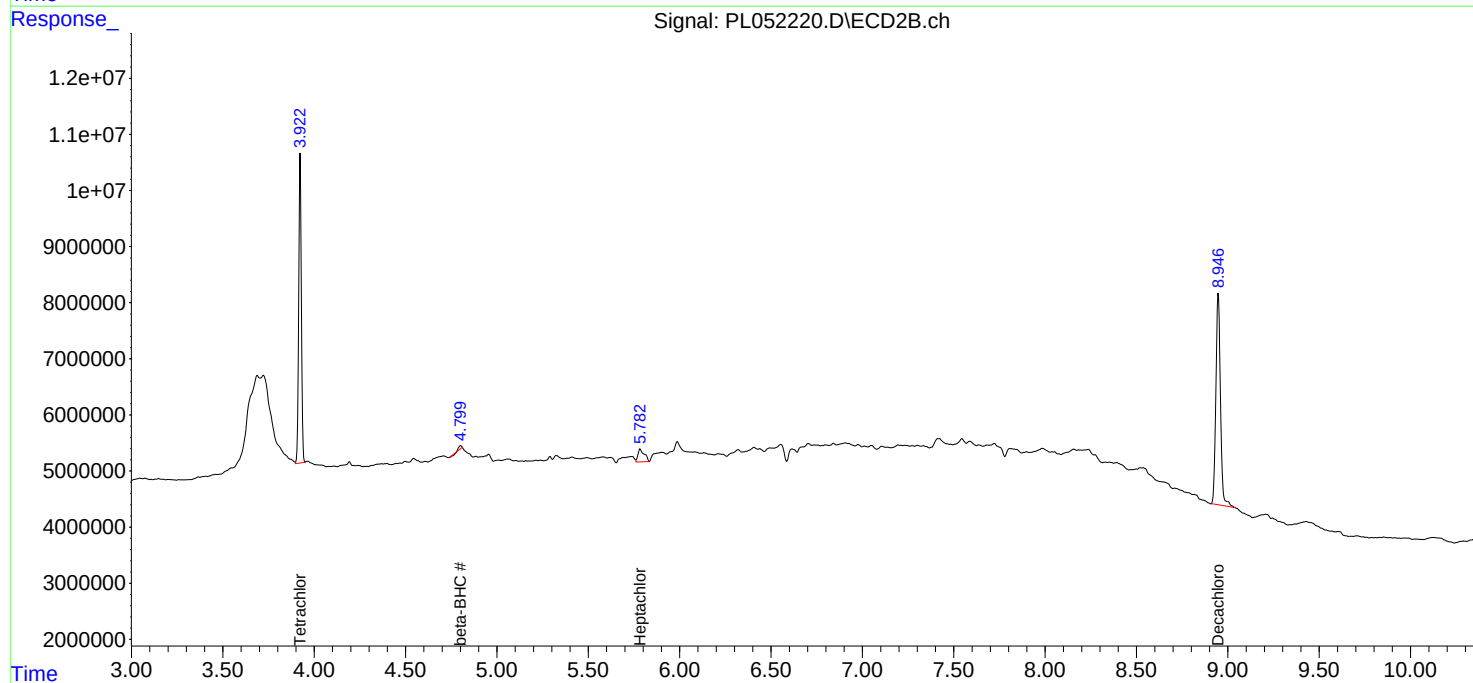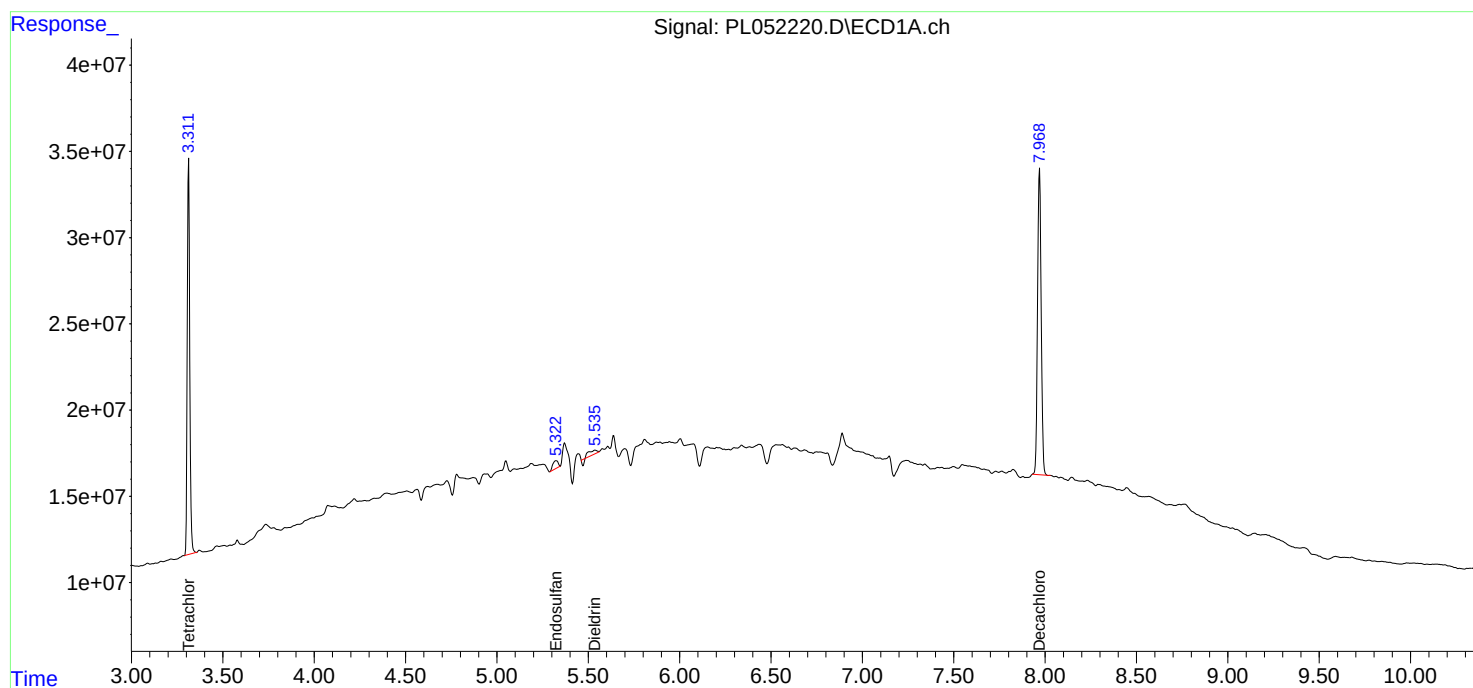


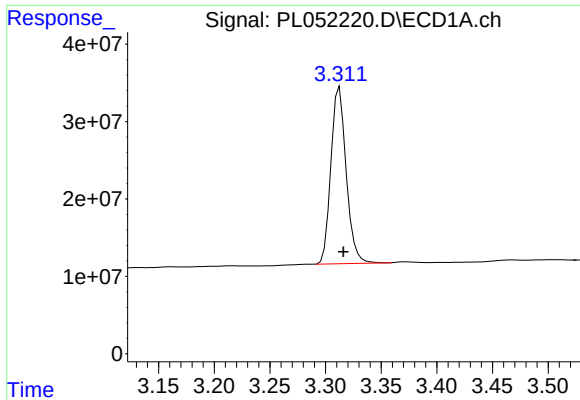

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 217929138
Conc: 25.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

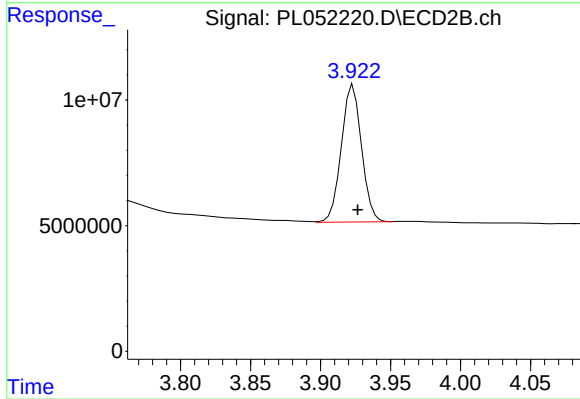


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 54961499
Conc: 25.16 ng/ml

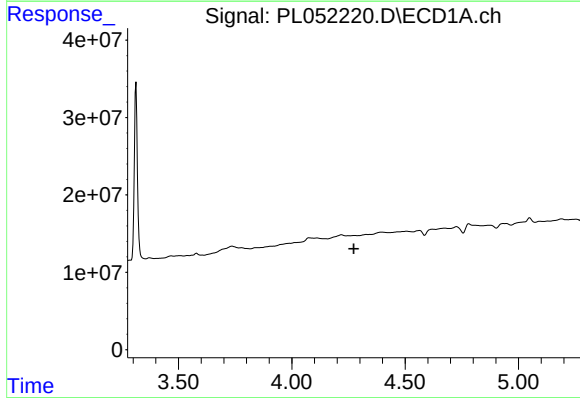


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

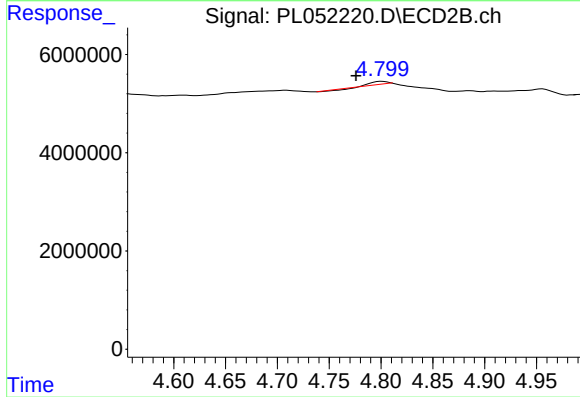

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 521869
Conc: 0.36 ng/ml

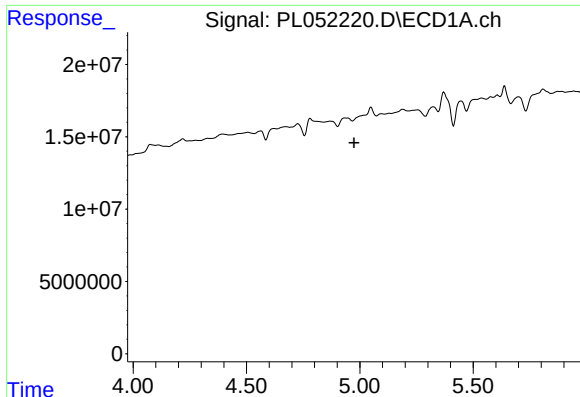

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

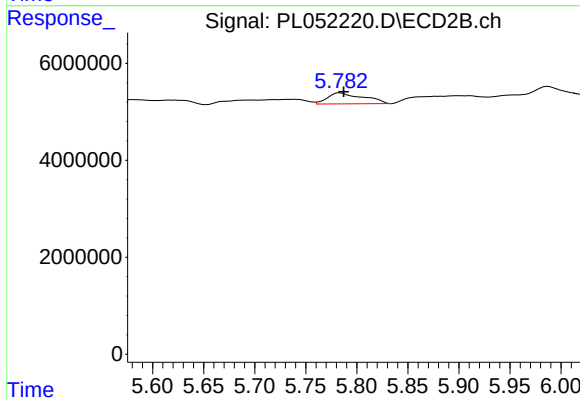


#8 Heptachlor epoxide

R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 5550061
Conc: 1.64 ng/ml

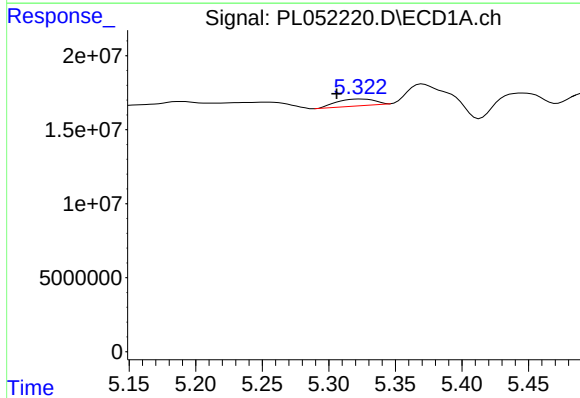


#9 Endosulfan I

R.T.: 5.323 min
Delta R.T.: 0.017 min
Response: 9134106
Conc: 0.68 ng/ml

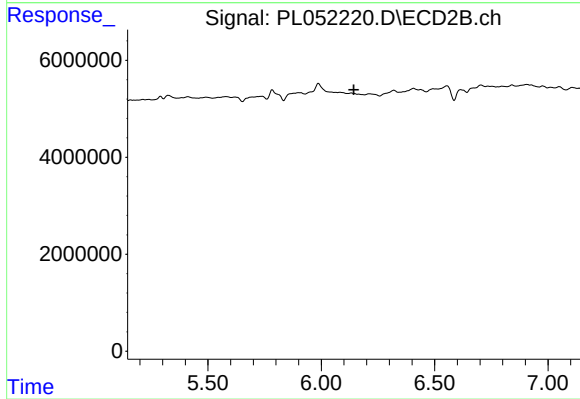

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

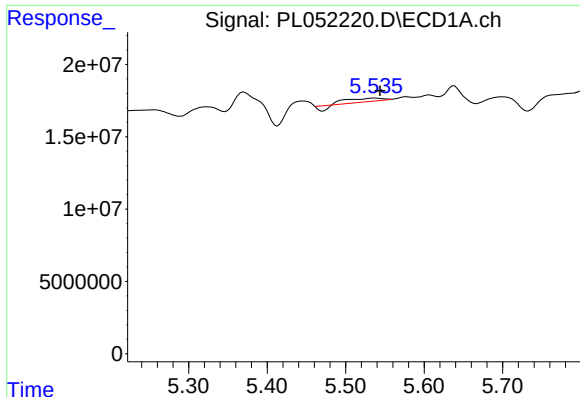

#13 Dieldrin


R.T.: 5.538 min
Delta R.T.: -0.006 min
Response: 5764261
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

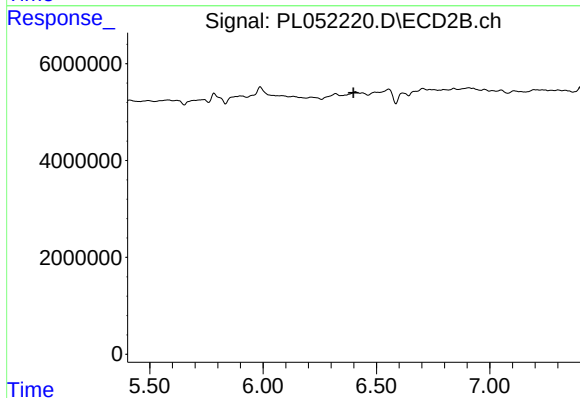


#13 Dieldrin

R.T.: 6.408 min
Delta R.T.: 0.008 min
Response: -89009
Conc: N.D.

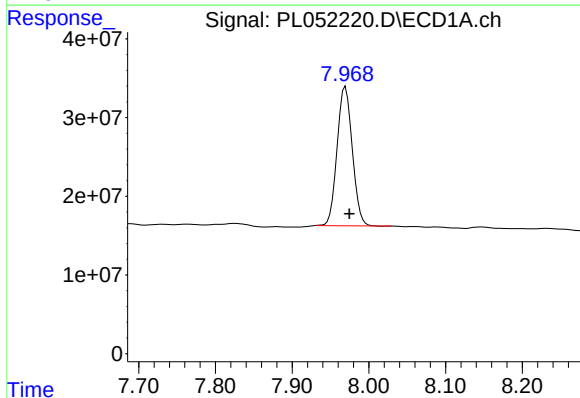

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.005 min
Response: 243695049
Conc: 20.08 ng/ml

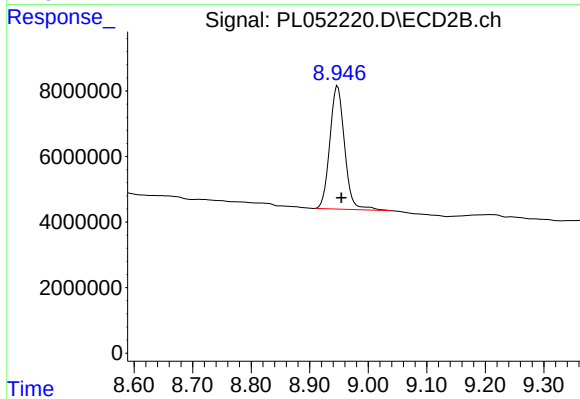

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.006 min
Response: 65676911
Conc: 21.58 ng/ml