

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
 Data File : PL052235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2019 21:34
 Operator : SG\AJ
 Sample : K4680-27
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 01:01:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.923	185.7E6	47722918	21.698	21.843
28)	SA Decachlor...	7.970	8.948	235.0E6	55640507	19.362	18.280
Target Compounds							
3)	MA gamma-BHC...	0.000	4.600	0	18679	N.D.	0.006 #
5)	MB Aldrin	4.569f	0.000	3176183	0	0.220	N.D. #
8)	B Heptachlo...	0.000	5.781	0	716471	N.D.	0.212 #
11)	B alpha-Chl...	5.256	0.000	10717731	0	0.741	N.D. #
13)	MA Dieldrin	5.536	0.000	5204862	0	0.342	N.D. #
15)	B Endosulfa...	0.000	6.843	0	4166806	N.D.	1.264 #
24)	Chlordane-2	4.677f	0.000	12933547	0	31.644	N.D. #
26)	Chlordane-4	5.256	0.000	10717731	0	8.790	N.D. #
27)	Chlordane-5	0.000	6.919f	0	2395155	N.D.	24.296 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
Data File : PL052235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2019 21:34
Operator : SG\AJ
Sample : K4680-27
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 01:01:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

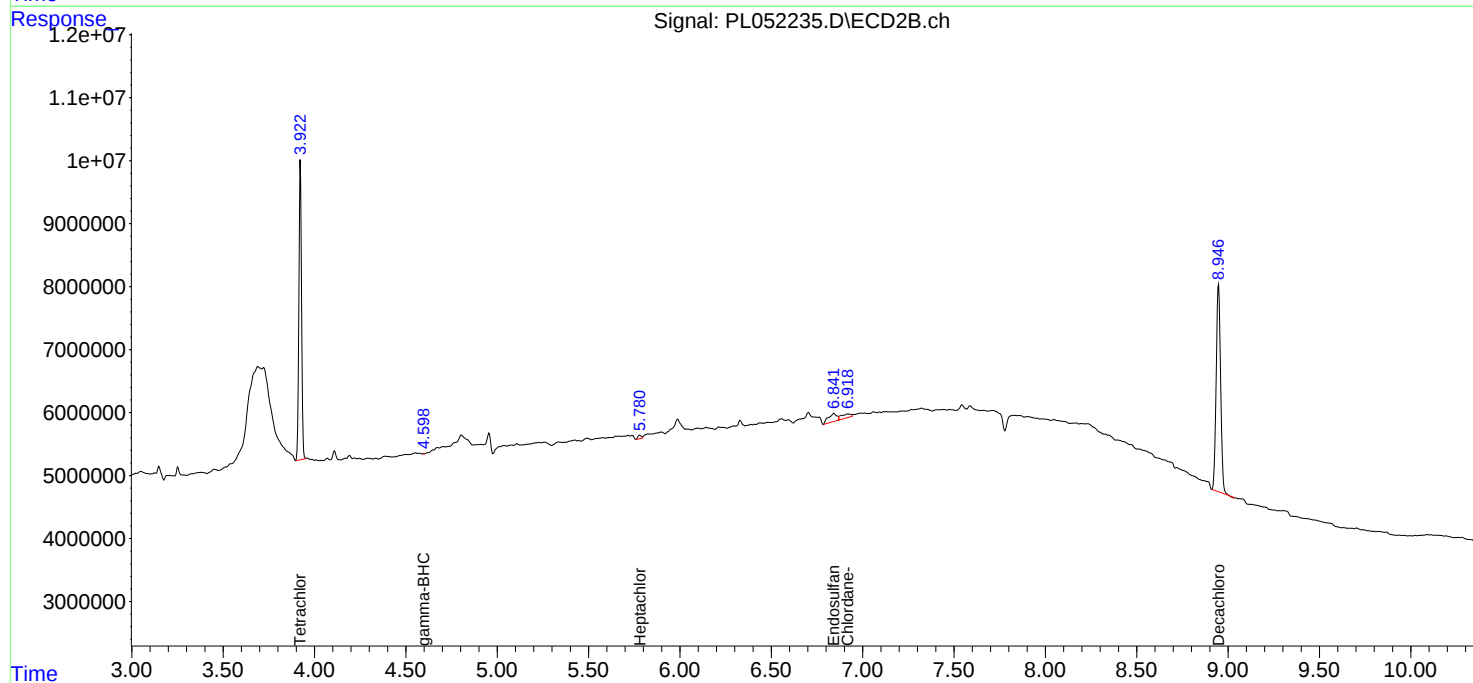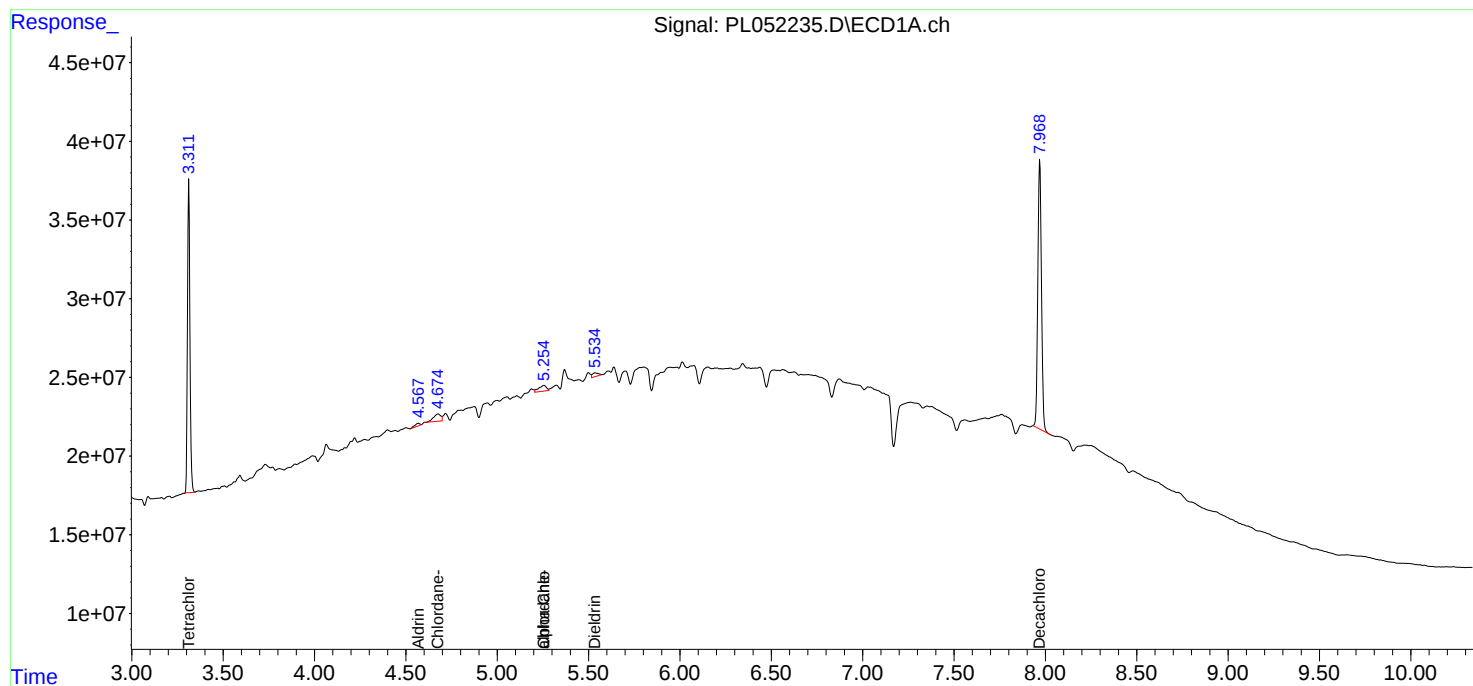


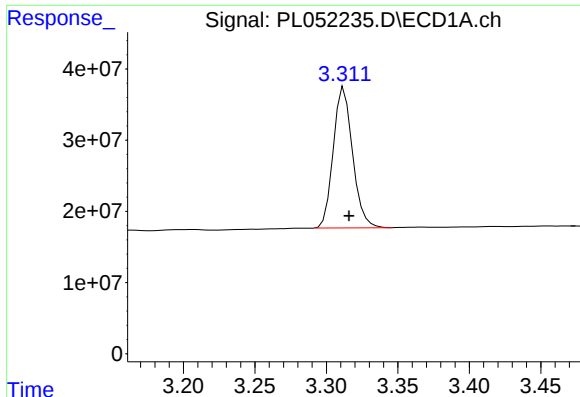

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 185704723
Conc: 21.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

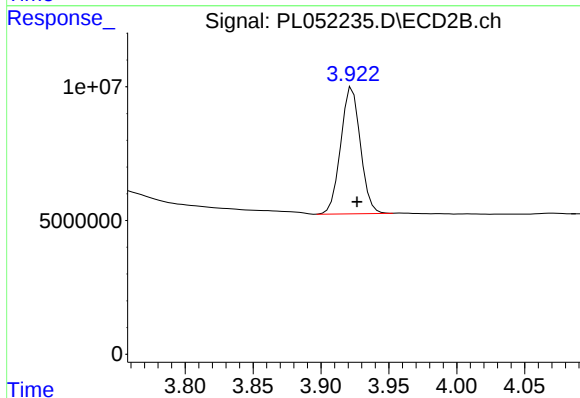


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.004 min
Response: 47722918
Conc: 21.84 ng/ml

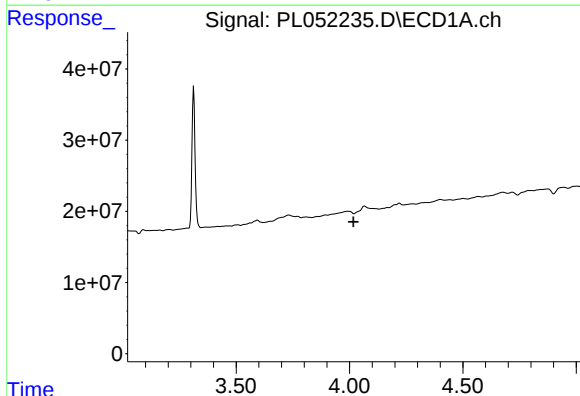


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.018 min
Response: 0
Conc: N.D.

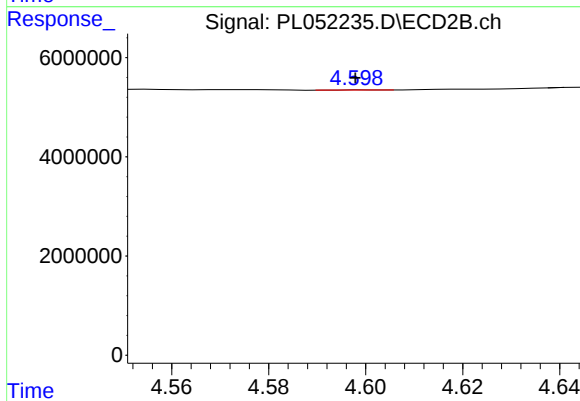

#3 gamma-BHC (Lindane)


R.T.: 4.600 min
Delta R.T.: 0.002 min
Response: 18679
Conc: 0.01 ng/ml

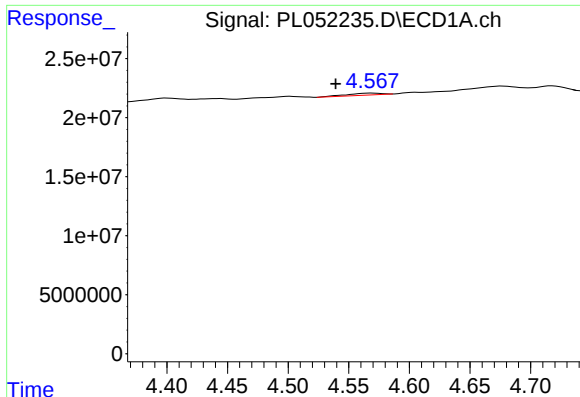

#5 Aldrin


R.T.: 4.569 min
Delta R.T.: 0.030 min
Response: 3176183
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

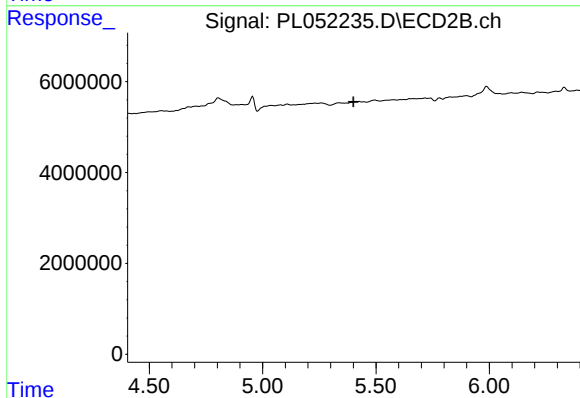


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.401 min
Response: 0
Conc: N.D.

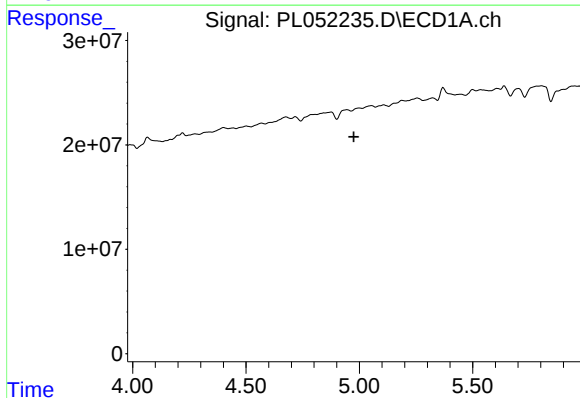


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

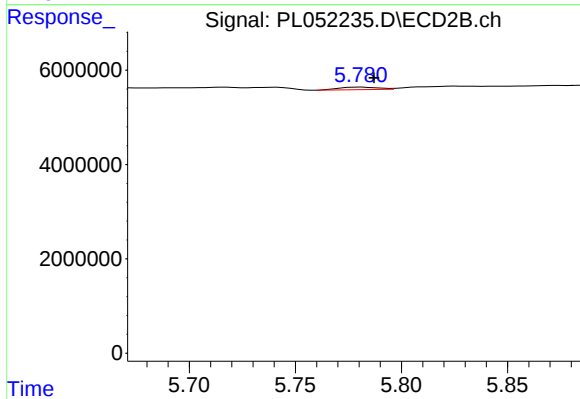

#8 Heptachlor epoxide


R.T.: 5.781 min
Delta R.T.: -0.007 min
Response: 716471
Conc: 0.21 ng/ml

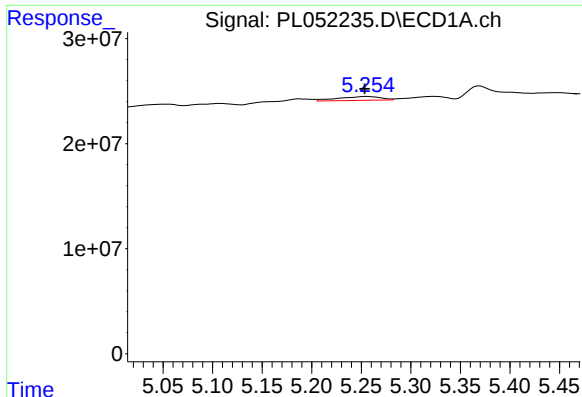

#11 alpha-Chlordane


R.T.: 5.256 min
Delta R.T.: 0.003 min
Response: 10717731
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

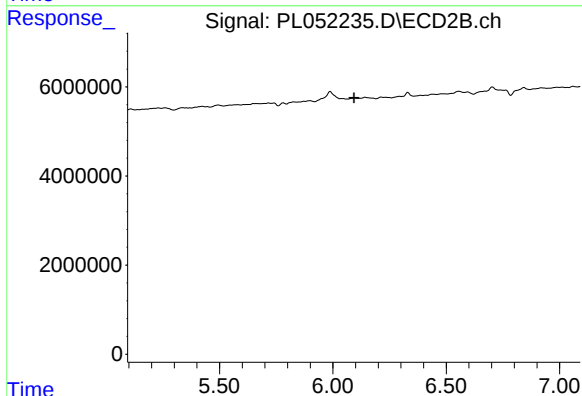


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

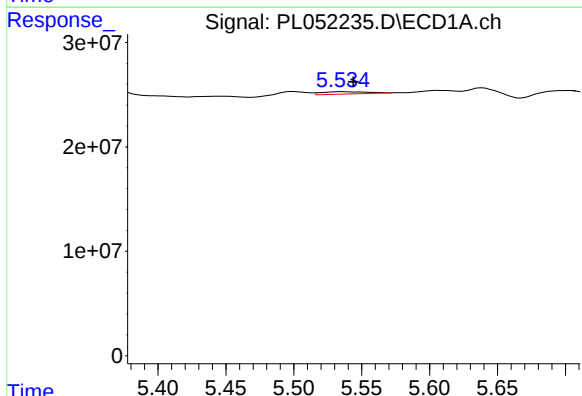


#13 Dieldrin

R.T.: 5.536 min
Delta R.T.: -0.008 min
Response: 5204862
Conc: 0.34 ng/ml

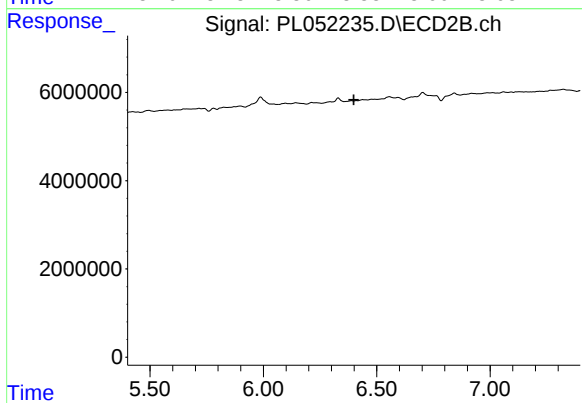

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

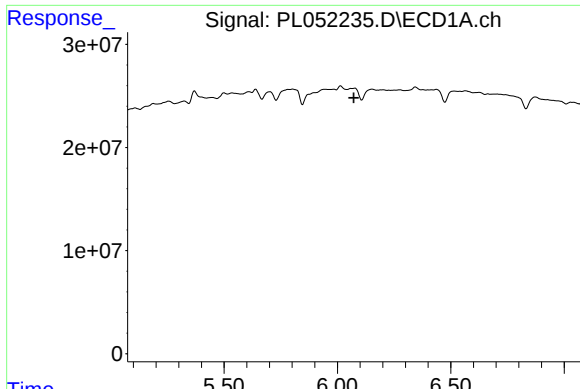

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

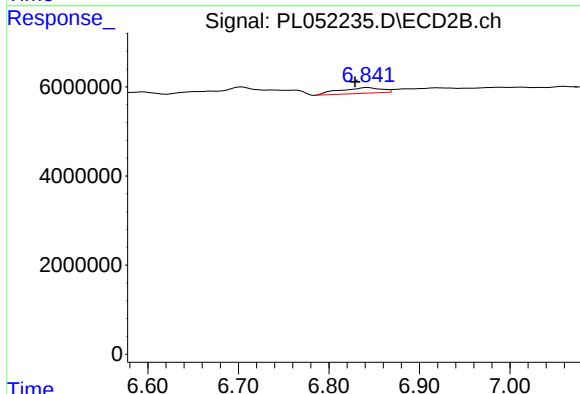


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.014 min
Response: 4166806
Conc: 1.26 ng/ml

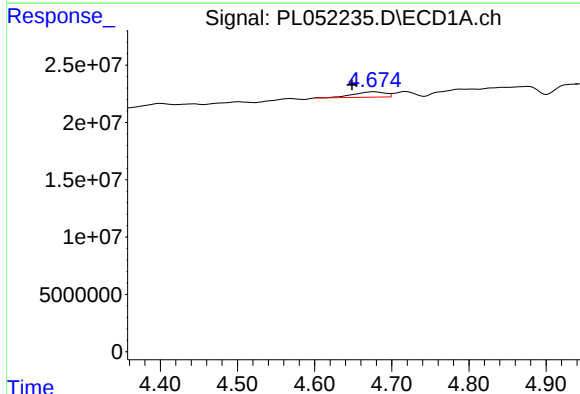


#24 Chlordane-2

R.T.: 4.677 min
Delta R.T.: 0.028 min
Response: 12933547
Conc: 31.64 ng/ml

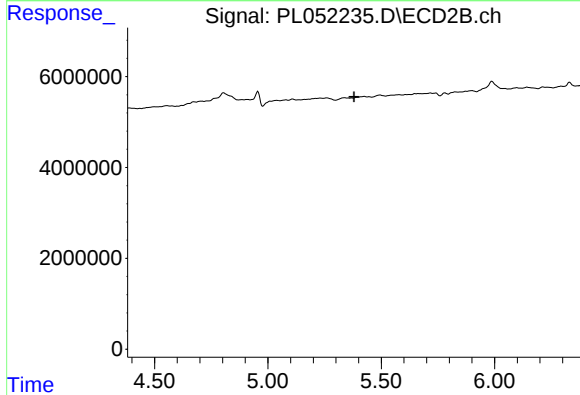

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

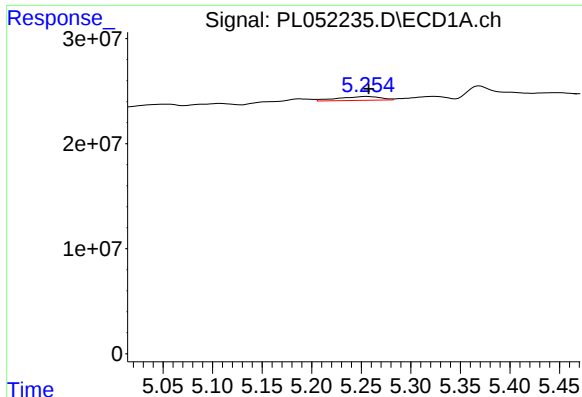

#26 Chlordane-4


R.T.: 5.256 min
Delta R.T.: -0.001 min
Response: 10717731
Conc: 8.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

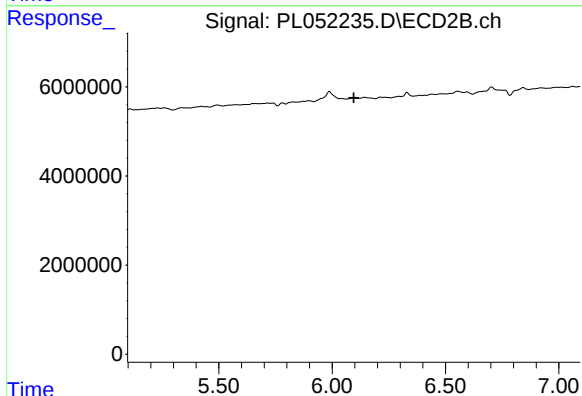


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

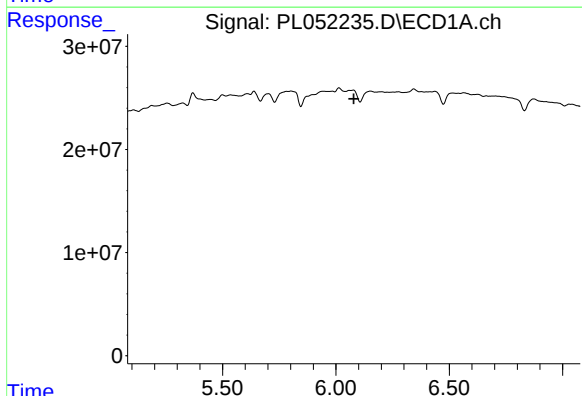


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

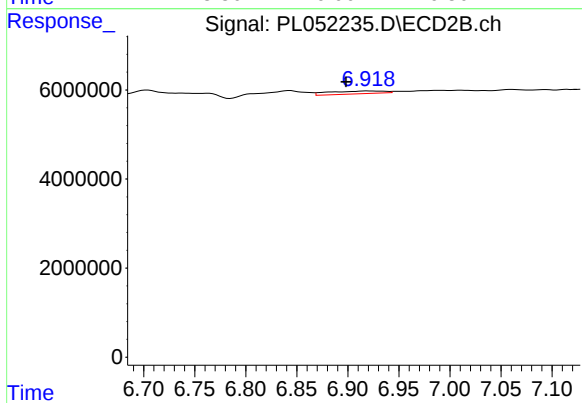

#27 Chlordane-5


R.T.: 6.919 min
Delta R.T.: 0.021 min
Response: 2395155
Conc: 24.30 ng/ml

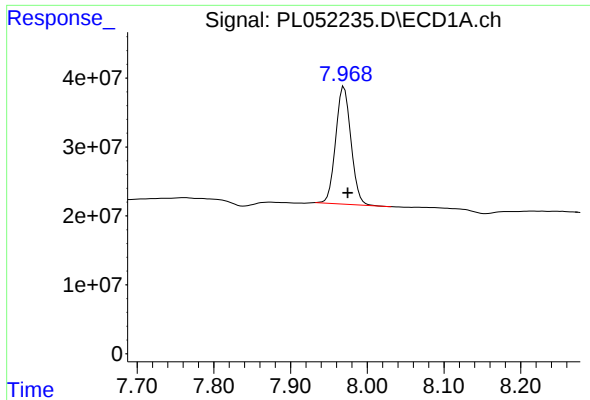

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.005 min
Response: 235010473
Conc: 19.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

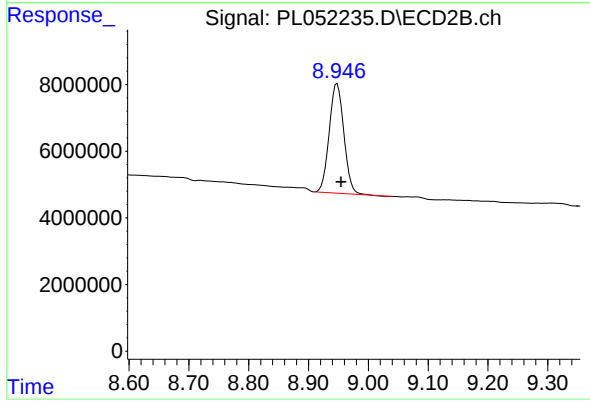

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.006 min
Response: 55640507
Conc: 18.28 ng/ml