

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
 Data File : PL052236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2019 21:48
 Operator : SG\AJ
 Sample : K4680-30
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 01:02:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	197.4E6	50792490	23.060	23.248
28)	SA Decachlor...	7.969	8.947	269.5E6	62444132	22.201	20.515
Target Compounds							
6)	B beta-BHC	0.000	4.803f	0	715479	N.D.	0.491 #
8)	B Heptachlo...	0.000	5.782	0	631626	N.D.	0.187 #
11)	B alpha-Chl...	5.257	0.000	7636680	0	0.528	N.D. #
13)	MA Dieldrin	5.540	0.000	1172985	0	0.077	N.D. #
15)	B Endosulfa...	0.000	6.843	0	3685757	N.D.	1.118 #
18)	B Endrin al...	0.000	6.977f	0	2713464	N.D.	0.960 #
24)	Chlordane-2	4.678f	0.000	12659199	0	30.973	N.D. #
25)	Chlordane-3	5.229f	0.000	8109807	0	6.246	N.D. #
26)	Chlordane-4	5.257	0.000	7636680	0	6.263	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090519\
Data File : PL052236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2019 21:48
Operator : SG\AJ
Sample : K4680-30
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 01:02:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

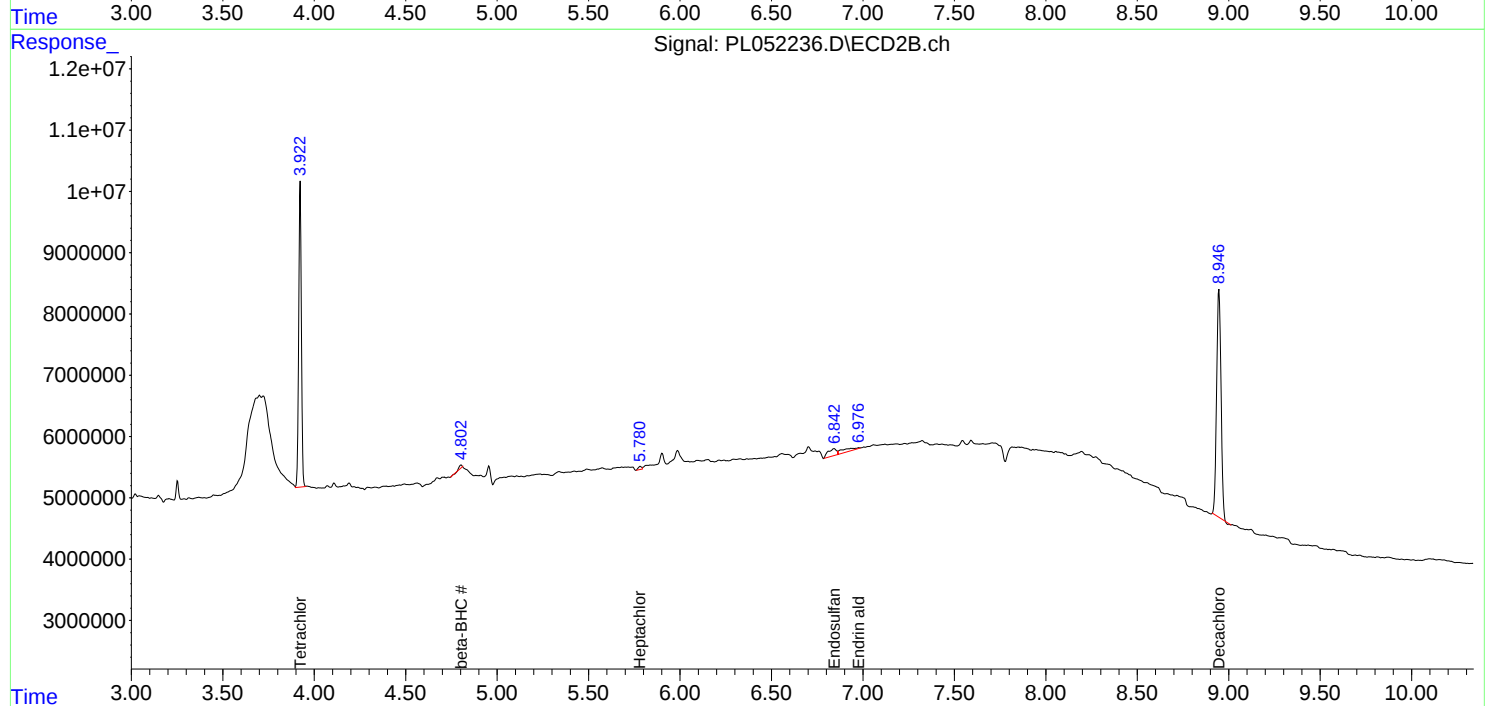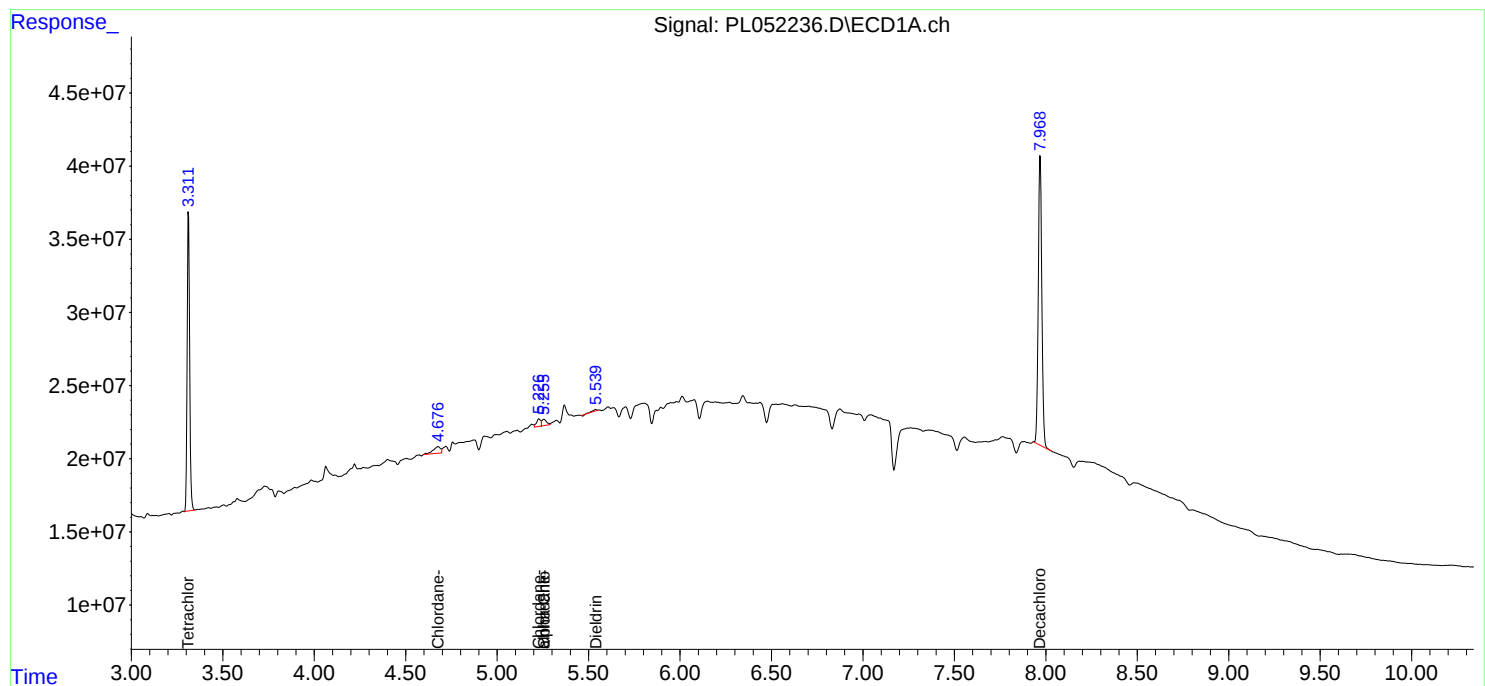


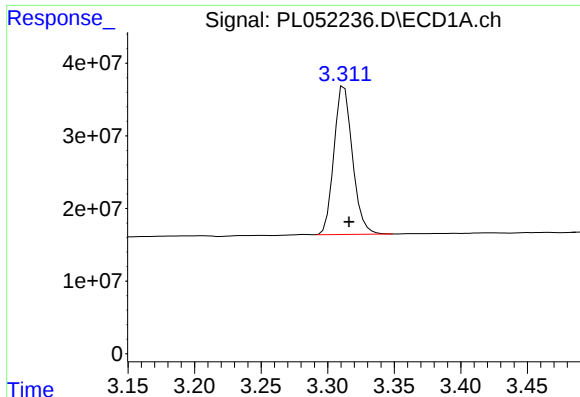

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 197365438
Conc: 23.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

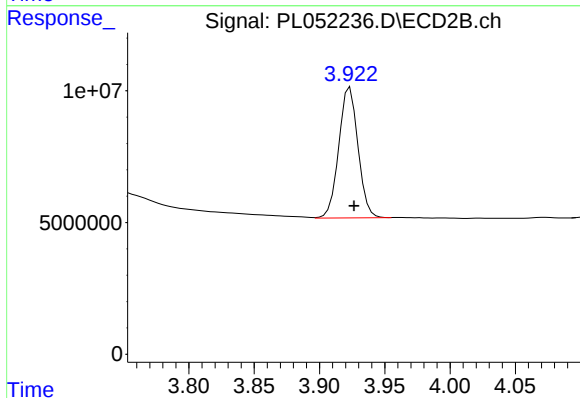


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 50792490
Conc: 23.25 ng/ml

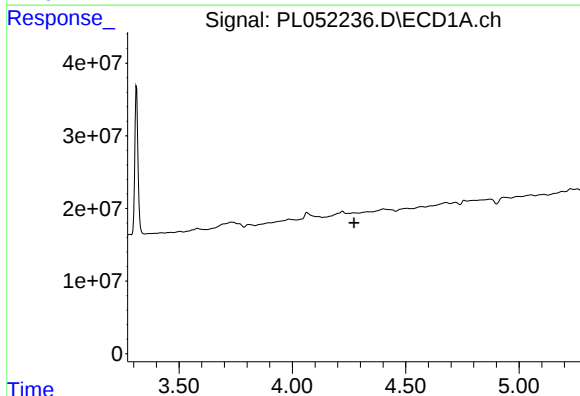


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

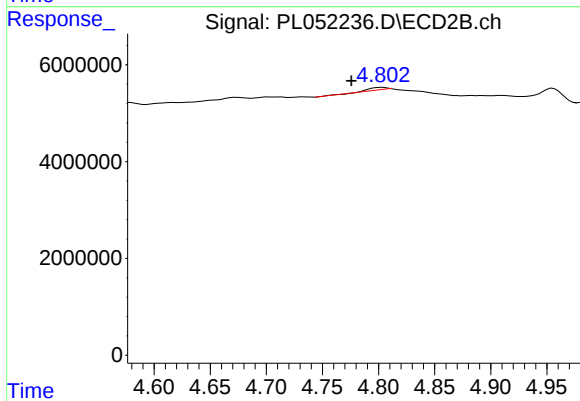

#6 beta-BHC


R.T.: 4.803 min
Delta R.T.: 0.027 min
Response: 715479
Conc: 0.49 ng/ml

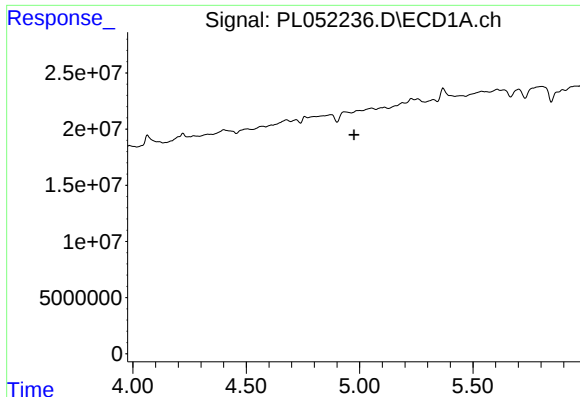

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

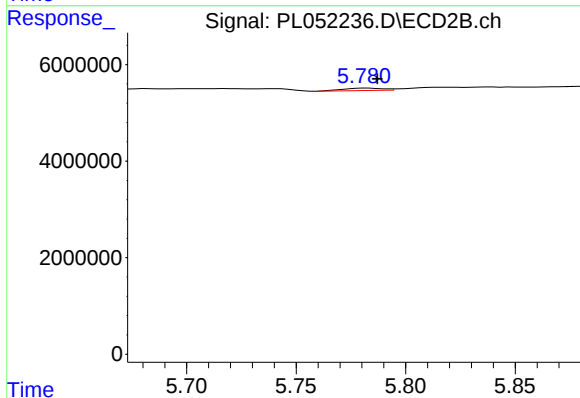


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.005 min
Response: 631626
Conc: 0.19 ng/ml

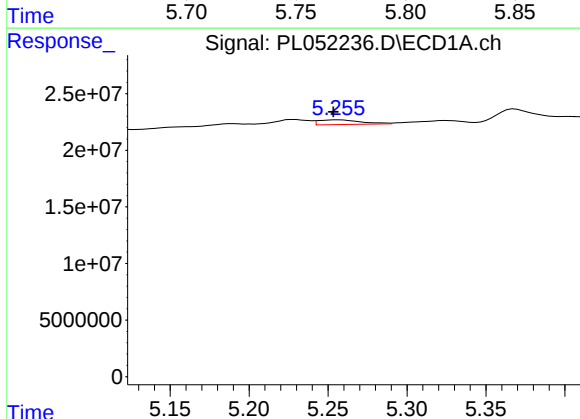


#11 alpha-Chlordane

R.T.: 5.257 min
Delta R.T.: 0.003 min
Response: 7636680
Conc: 0.53 ng/ml

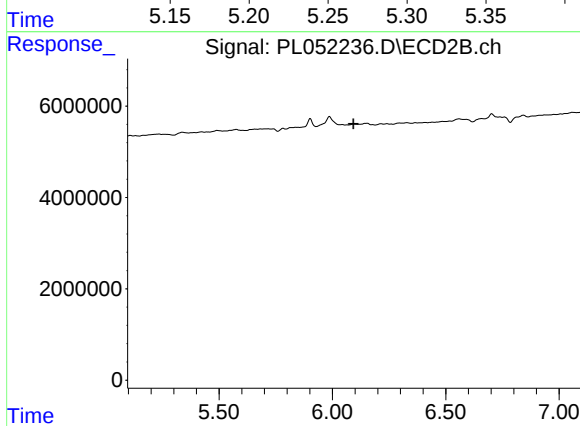

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.093 min
Response: 0
Conc: N.D.

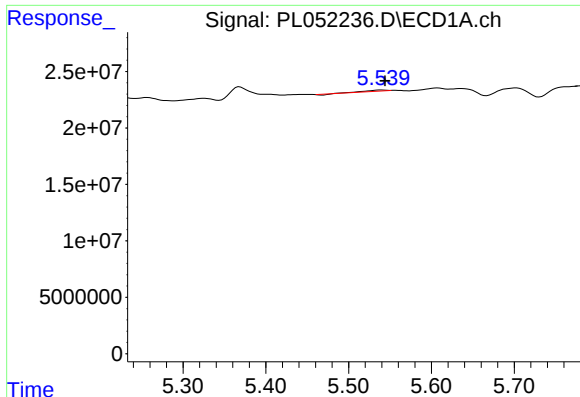

#13 Dieldrin


R.T.: 5.540 min
Delta R.T.: -0.004 min
Response: 1172985
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

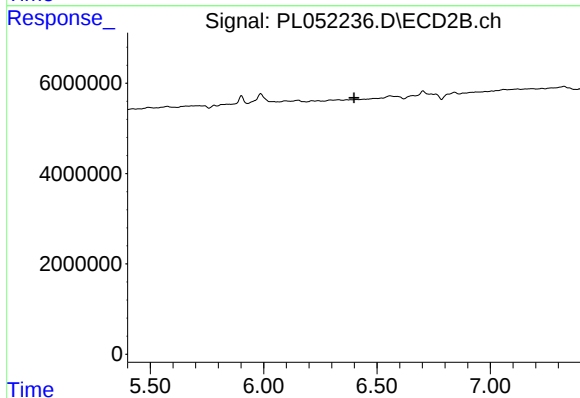


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

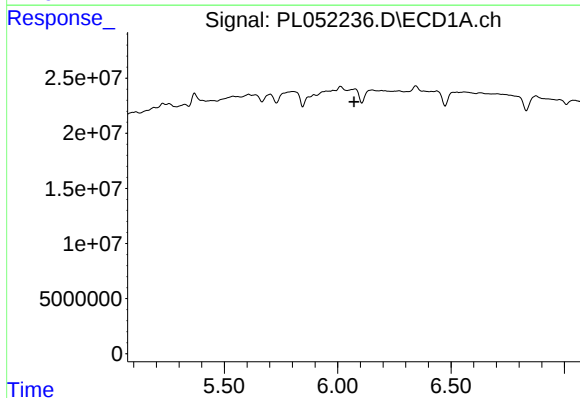


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

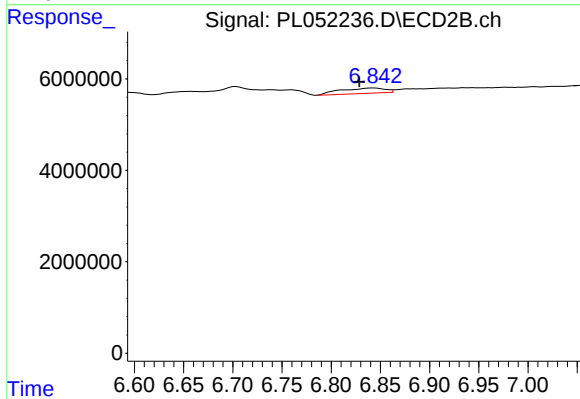

#15 Endosulfan II


R.T.: 6.843 min
Delta R.T.: 0.014 min
Response: 3685757
Conc: 1.12 ng/ml

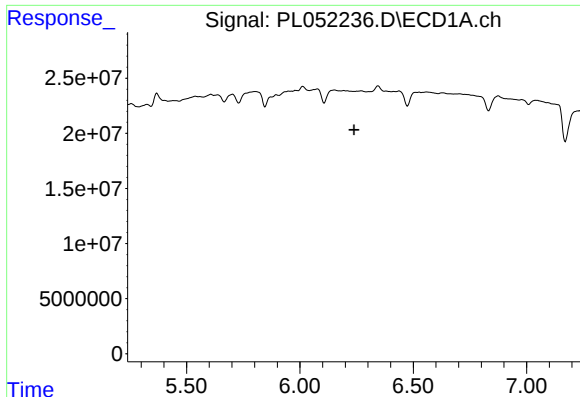

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

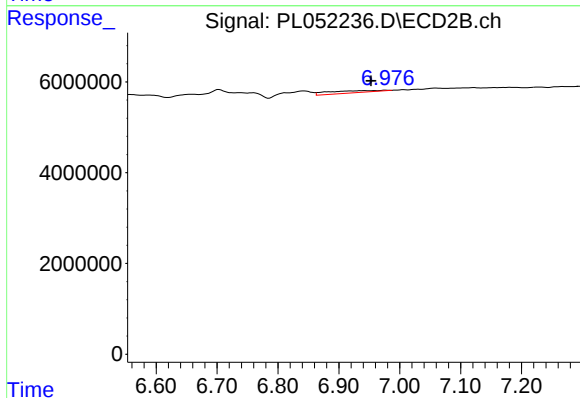


#18 Endrin aldehyde

R.T.: 6.977 min
Delta R.T.: 0.024 min
Response: 2713464
Conc: 0.96 ng/ml

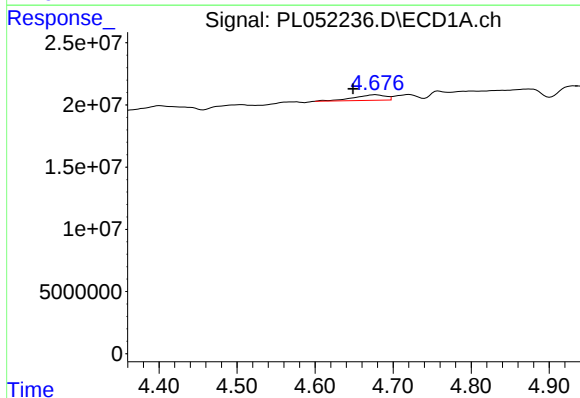


#24 Chlordane-2

R.T.: 4.678 min
Delta R.T.: 0.029 min
Response: 12659199
Conc: 30.97 ng/ml

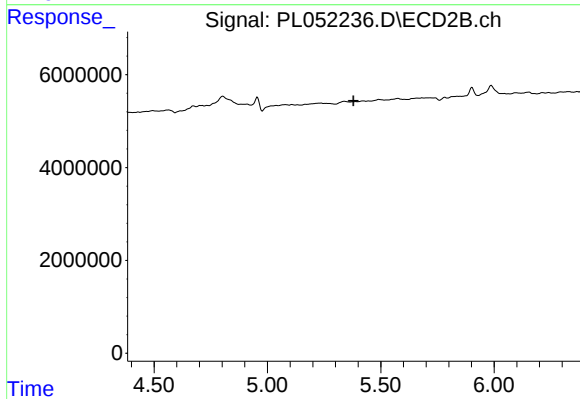

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

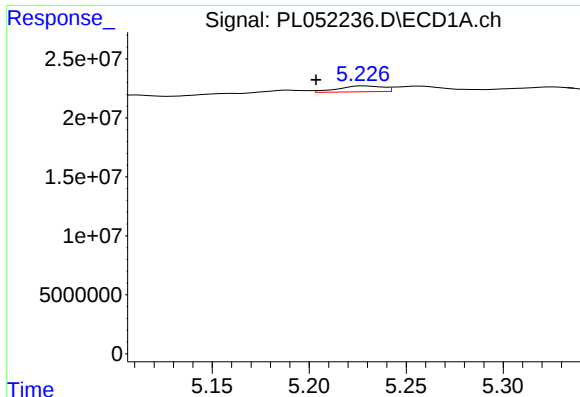

#25 Chlordane-3


R.T.: 5.229 min
Delta R.T.: 0.025 min
Response: 8109807
Conc: 6.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

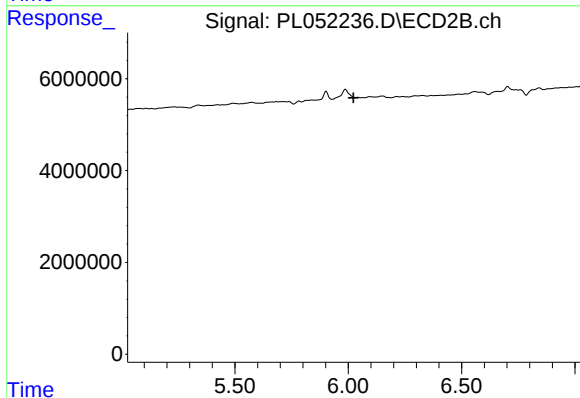


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

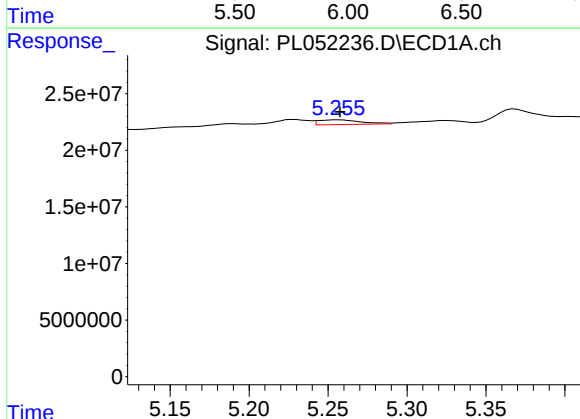


#26 Chlordane-4

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 7636680
Conc: 6.26 ng/ml

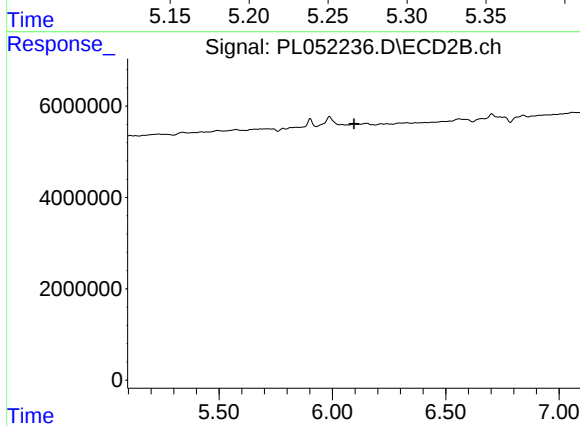

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

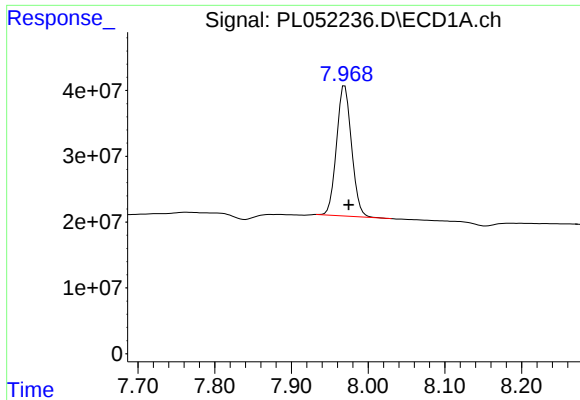

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.005 min
Response: 269474534
Conc: 22.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

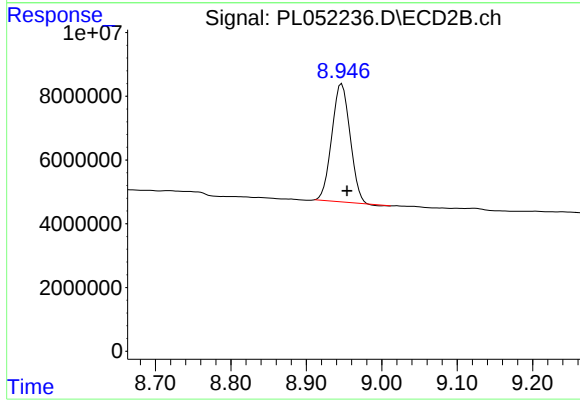

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.007 min
Response: 62444132
Conc: 20.51 ng/ml