

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
 Data File : PL085107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 11:39
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 15:07:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 14:57:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.683	225.0E6	135.9E6	98.903	99.648
28)	SA Decachlor...	9.027	7.864	137.5E6	118.3E6	95.785	97.356
Target Compounds							
23)	Chlordane-1	4.644	3.685	96522435	38961431	981.346	998.524
24)	Chlordane-2	5.178	4.266	97050558	45827539	961.693	973.581
25)	Chlordane-3	5.892	4.899	356.9E6	139.8E6	996.870	1008.459
26)	Chlordane-4	5.974	4.962	421.4E6	147.0E6	990.277	1004.170
27)	Chlordane-5	6.825	5.861	68095135	51338817	978.804	998.733



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
Data File : PL085107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 11:39
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 15:07:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 14:57:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

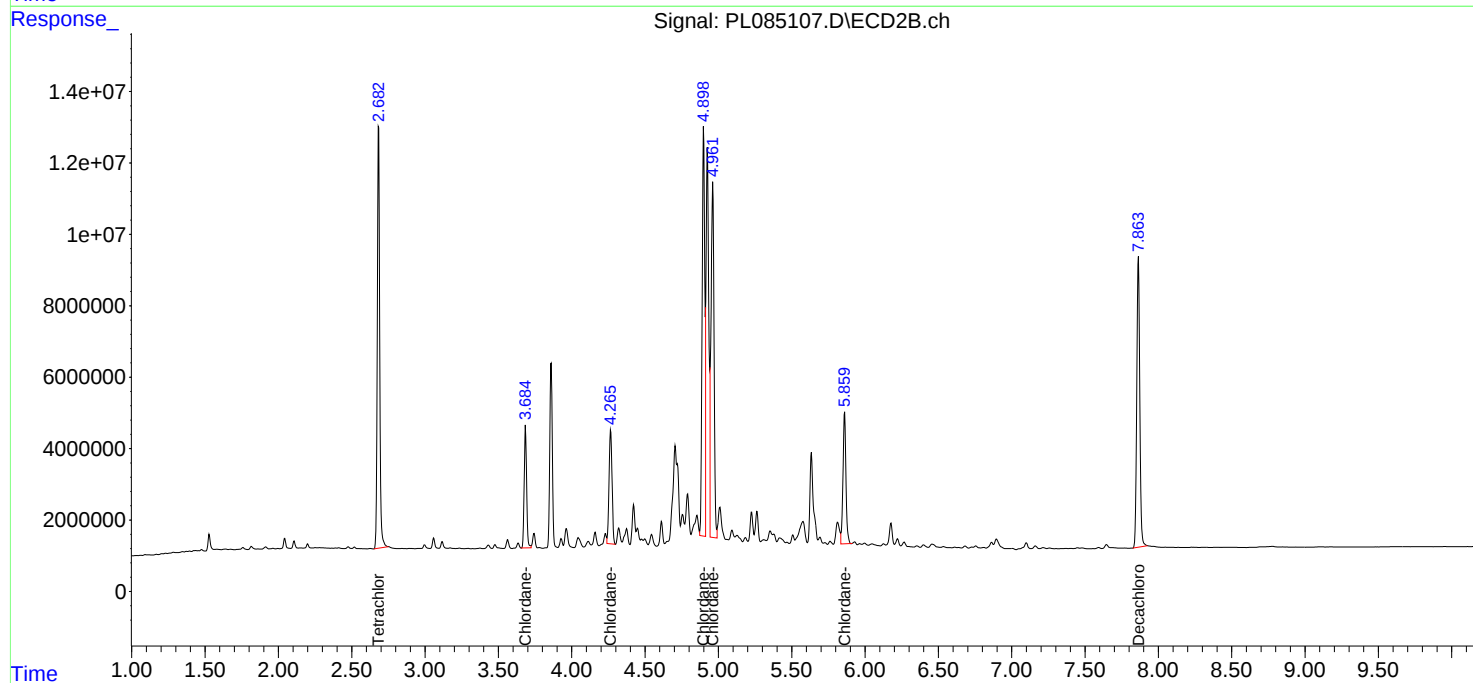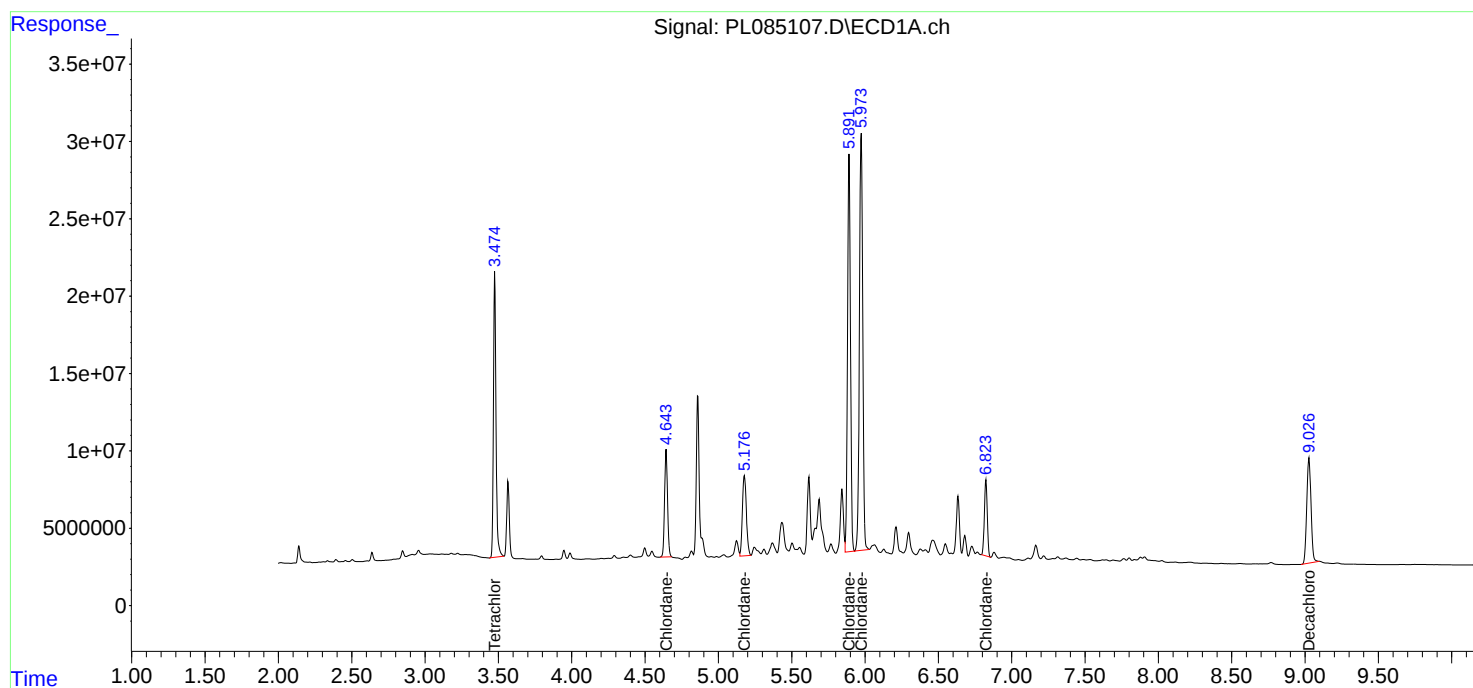


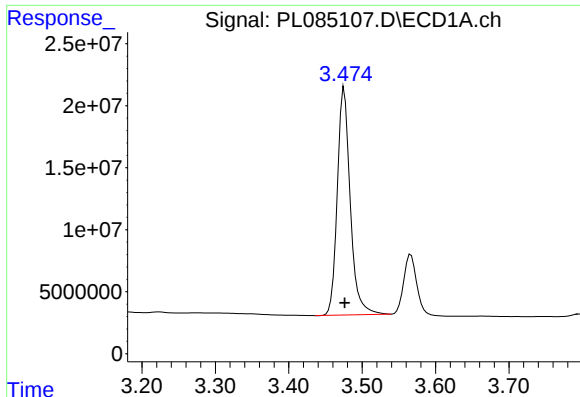

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 224960660
Conc: 98.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

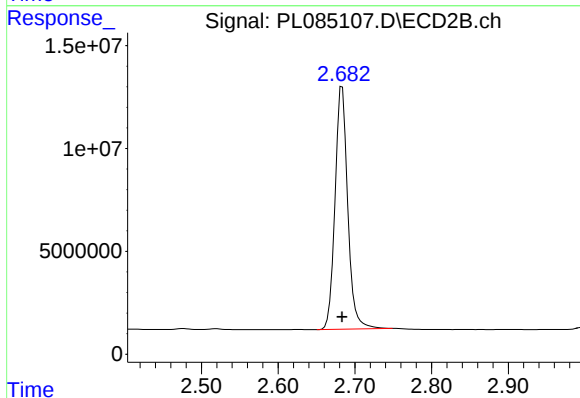


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 135917800
Conc: 99.65 ng/ml

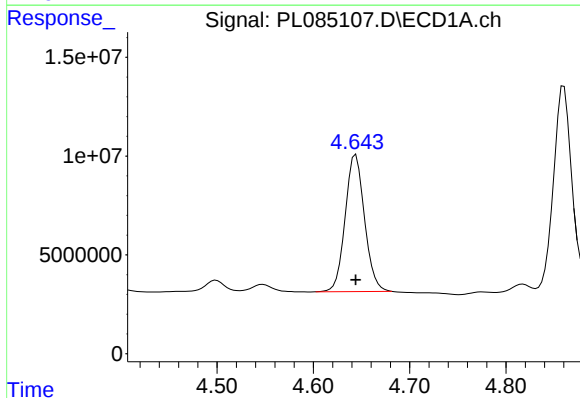


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 96522435
Conc: 981.35 ng/ml

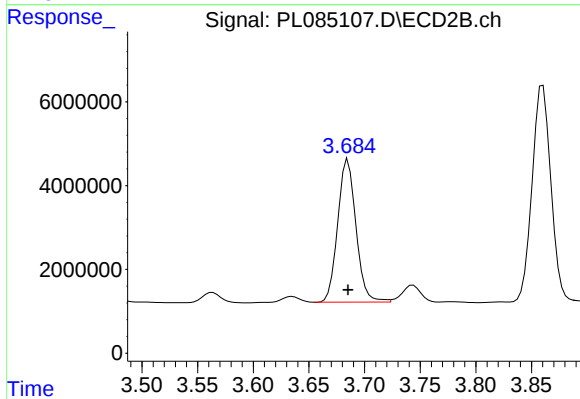

#23 Chlordane-1


R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 38961431
Conc: 998.52 ng/ml

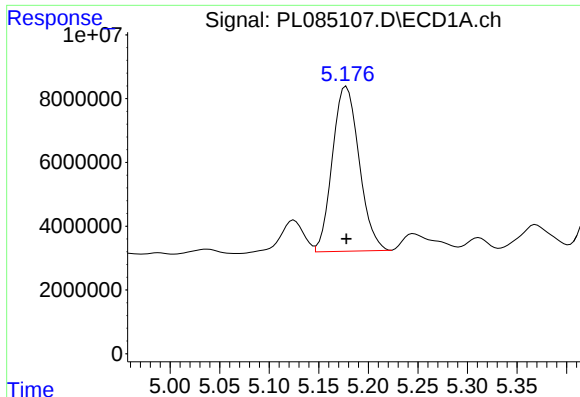

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 97050558
Conc: 961.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

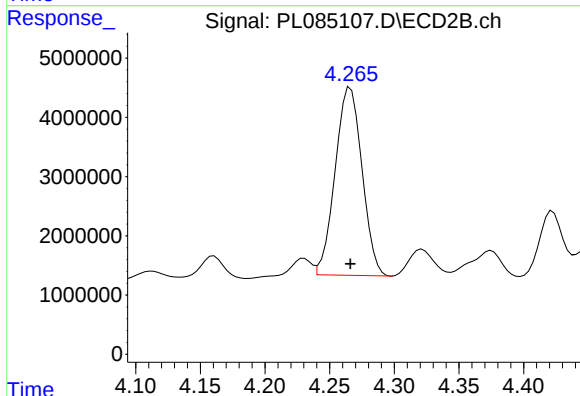


#24 Chlordane-2

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 45827539
Conc: 973.58 ng/ml

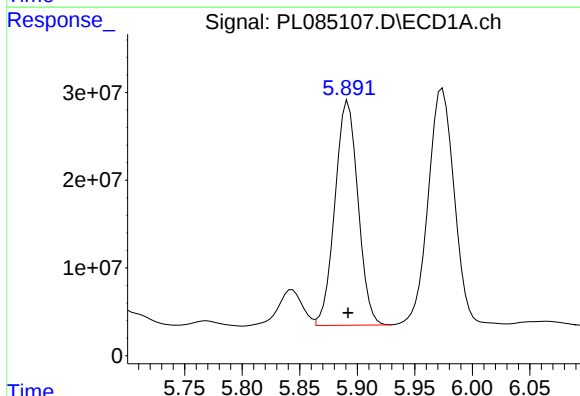


#25 Chlordane-3

R.T.: 5.892 min
Delta R.T.: 0.000 min
Response: 356869375
Conc: 996.87 ng/ml

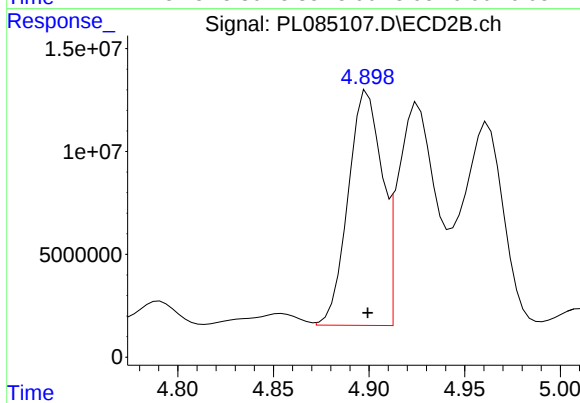

#25 Chlordane-3


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 139789225
Conc: 1008.46 ng/ml

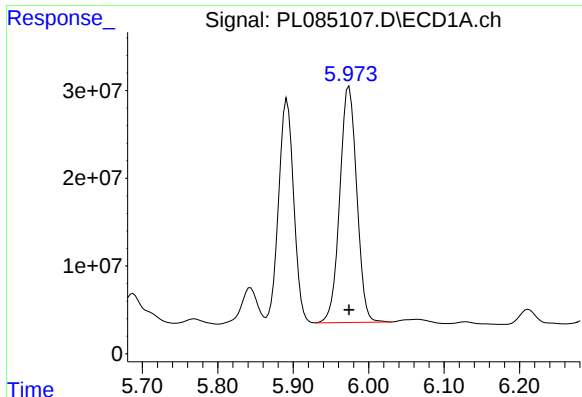

#26 Chlordane-4


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 421446971
Conc: 990.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

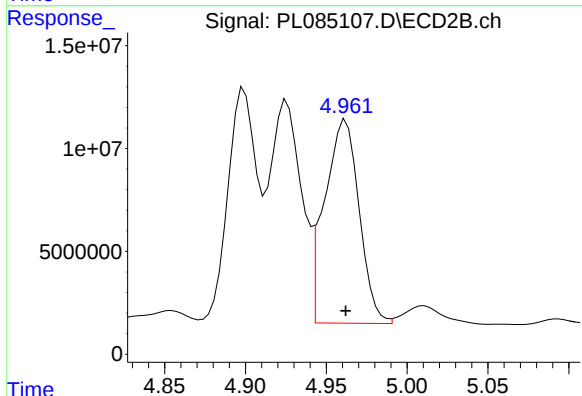


#26 Chlordane-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 146969323
Conc: 1004.17 ng/ml

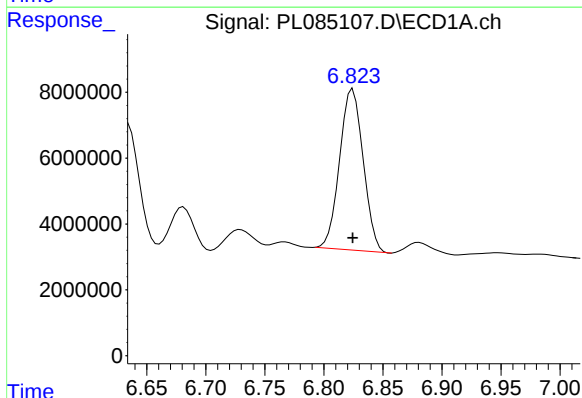


#27 Chlordane-5

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 68095135
Conc: 978.80 ng/ml

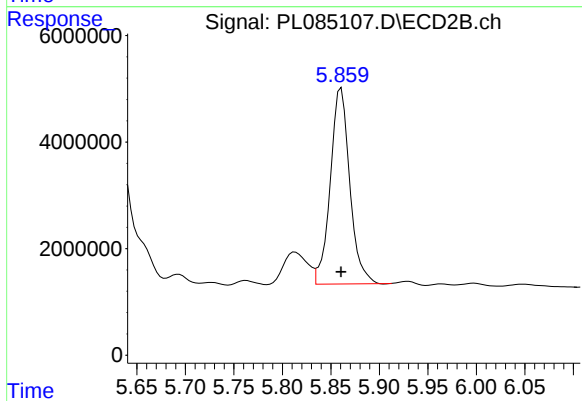

#27 Chlordane-5


R.T.: 5.861 min
Delta R.T.: 0.000 min
Response: 51338817
Conc: 998.73 ng/ml

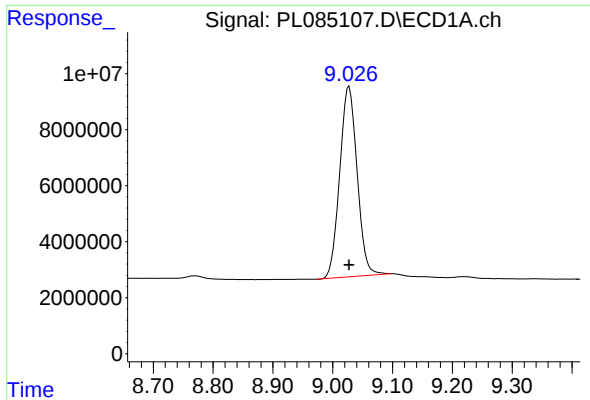

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.000 min
Response: 137545989
Conc: 95.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

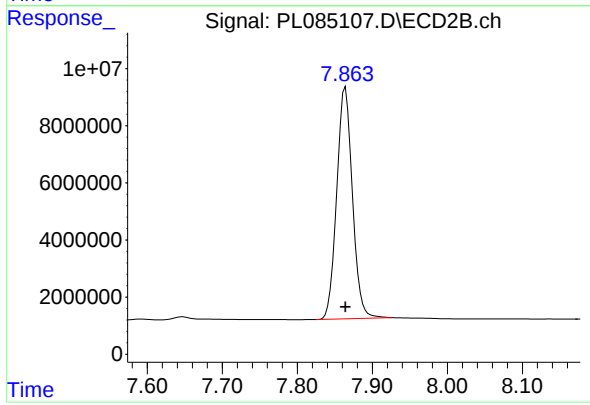

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 118258359
Conc: 97.36 ng/ml