

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
 Data File : PL085108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 11:53
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 15:09:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 14:57:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.683	169.5E6	102.2E6	74.668	74.943
28)	SA Decachlor...	9.028	7.864	106.3E6	89901172	74.358	74.338
Target Compounds							
23)	Chlordane-1	4.644	3.686	72695542	29191633	742.696	748.758
24)	Chlordane-2	5.178	4.267	74599880	35061215	742.782	746.563
25)	Chlordane-3	5.892	4.899	267.2E6	104.4E6	747.512	751.951
26)	Chlordane-4	5.975	4.962	316.8E6	109.8E6	746.261	750.110
27)	Chlordane-5	6.825	5.861	51486429	38612152	743.350	750.767



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
Data File : PL085108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 11:53
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 15:09:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 14:57:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

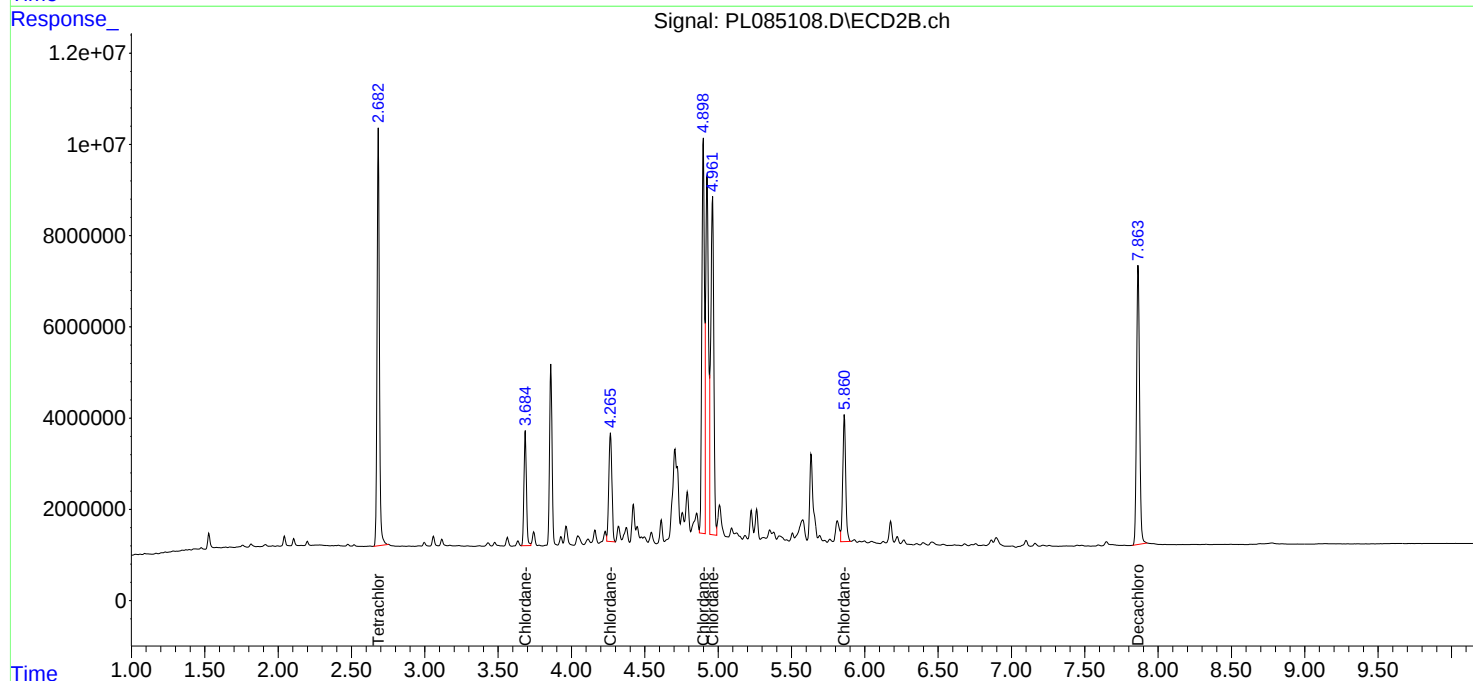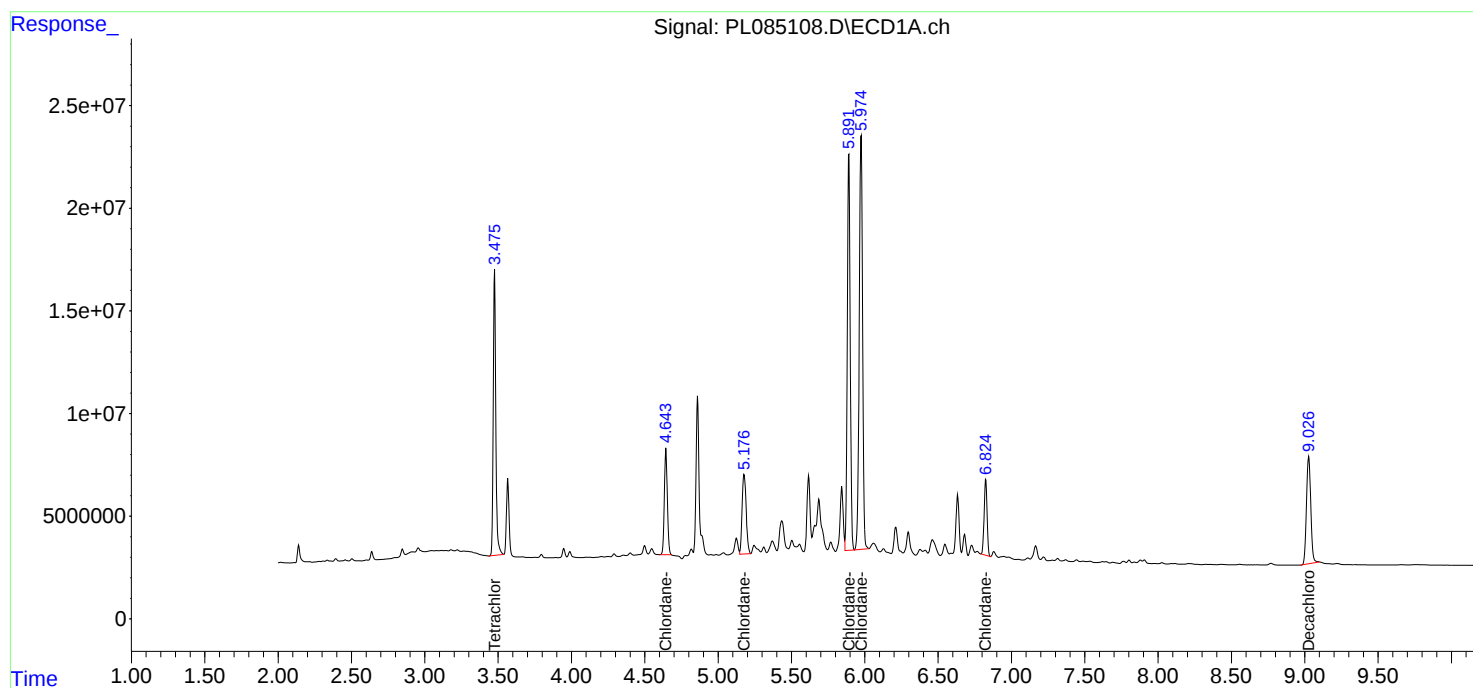


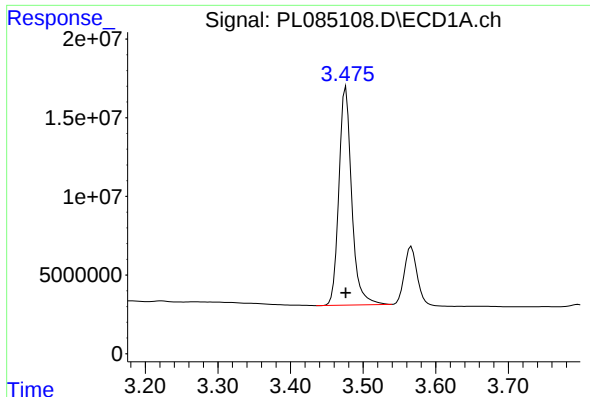

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 169462216
Conc: 74.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

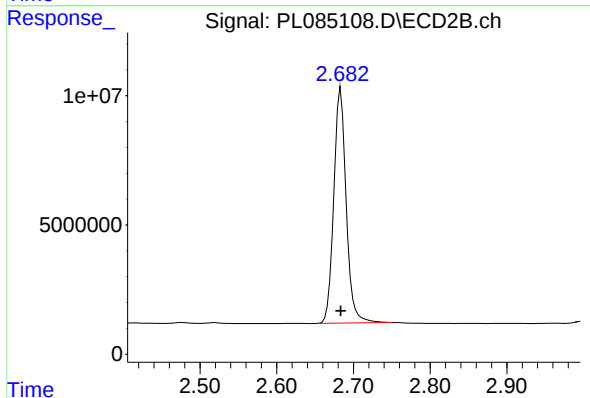


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 102180859
Conc: 74.94 ng/ml

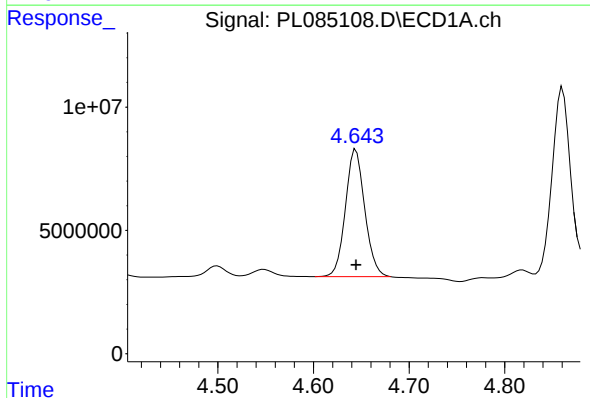


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 72695542
Conc: 742.70 ng/ml

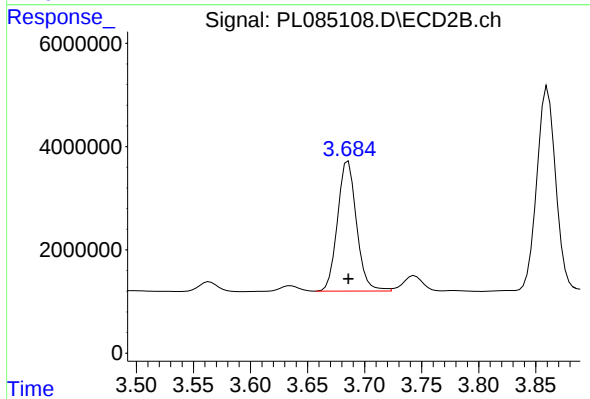

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 29191633
Conc: 748.76 ng/ml

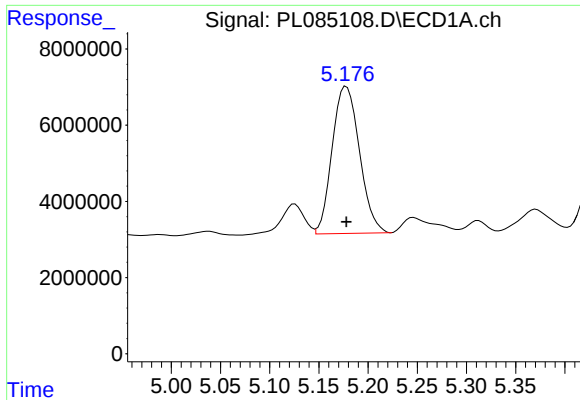

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 74599880
Conc: 742.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

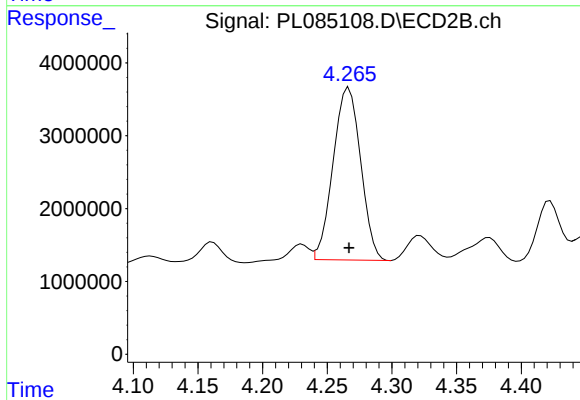


#24 Chlordane-2

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 35061215
Conc: 746.56 ng/ml

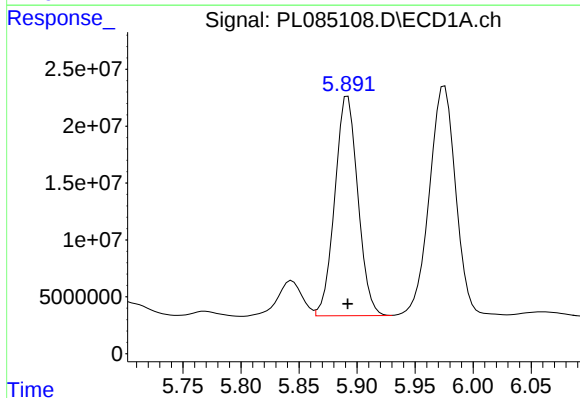


#25 Chlordane-3

R.T.: 5.892 min
Delta R.T.: 0.000 min
Response: 267158517
Conc: 747.51 ng/ml

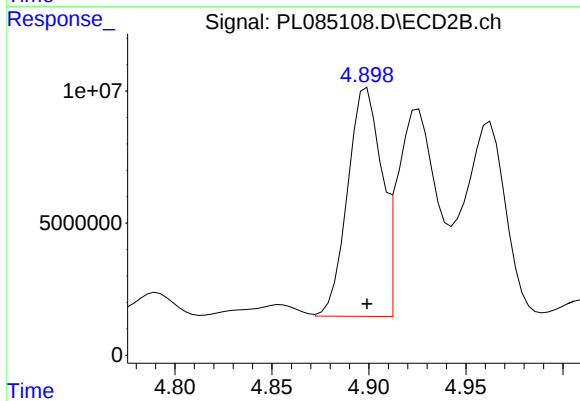

#25 Chlordane-3


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 104368701
Conc: 751.95 ng/ml

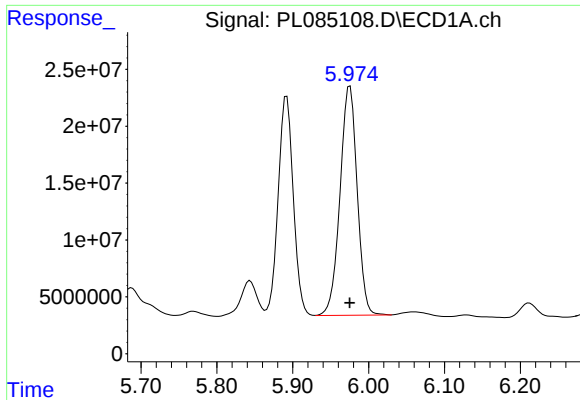

#26 Chlordane-4


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 316807667
Conc: 746.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

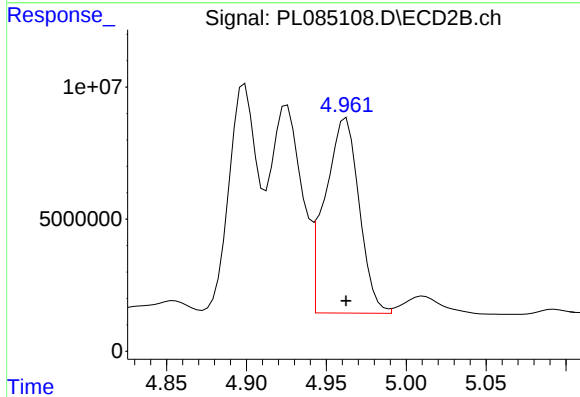


#26 Chlordane-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 109793502
Conc: 750.11 ng/ml

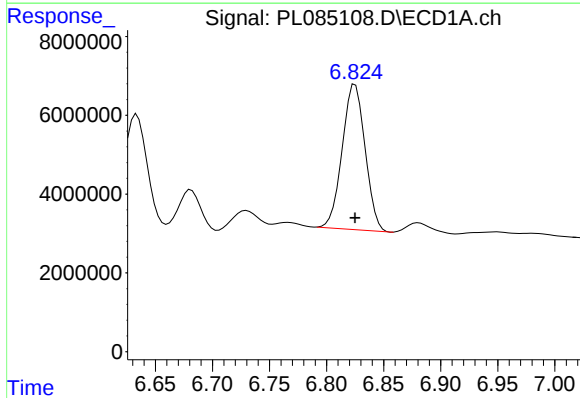


#27 Chlordane-5

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 51486429
Conc: 743.35 ng/ml

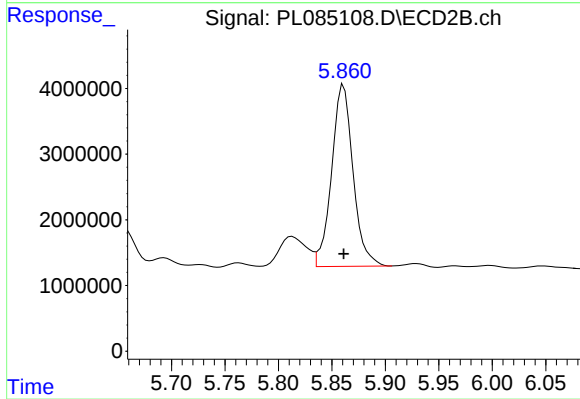

#27 Chlordane-5


R.T.: 5.861 min
Delta R.T.: 0.000 min
Response: 38612152
Conc: 750.77 ng/ml

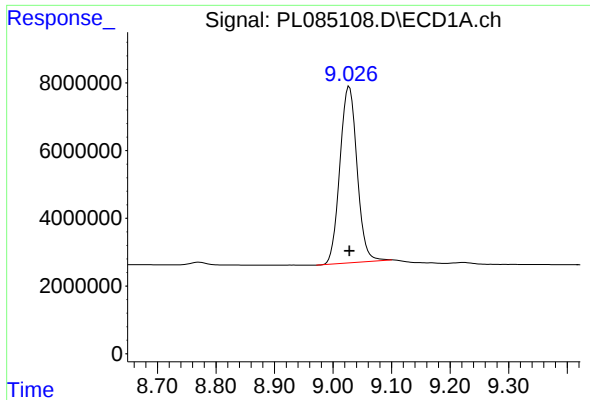

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: 0.000 min
Response: 106321551
Conc: 74.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

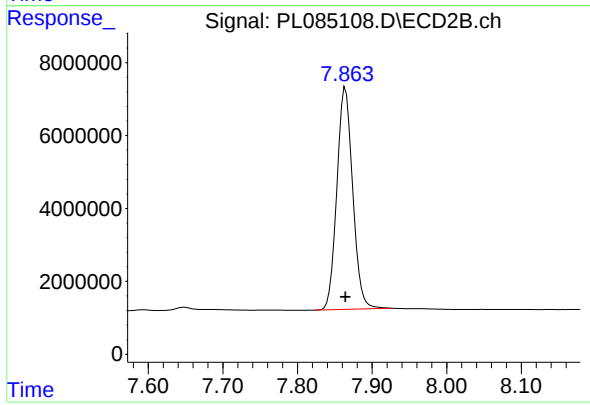

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 89901172
Conc: 74.34 ng/ml