

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
 Data File : PL085109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 12:07
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 15:00:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 14:57:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.683	115.0E6	68438909	50.000	50.000
28)	SA Decachlor...	9.027	7.864	74825639	62340993	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.645	3.686	50095947	19538293	500.000	500.000
24)	Chlordane-2	5.178	4.267	52391034	24157350	500.000	500.000
25)	Chlordane-3	5.892	4.900	179.6E6	68721989	500.000	500.000
26)	Chlordane-4	5.975	4.963	214.9E6	72874342	500.000	500.000
27)	Chlordane-5	6.825	5.861	35522158	25734529	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
Data File : PL085109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 12:07
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 15:00:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 14:57:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

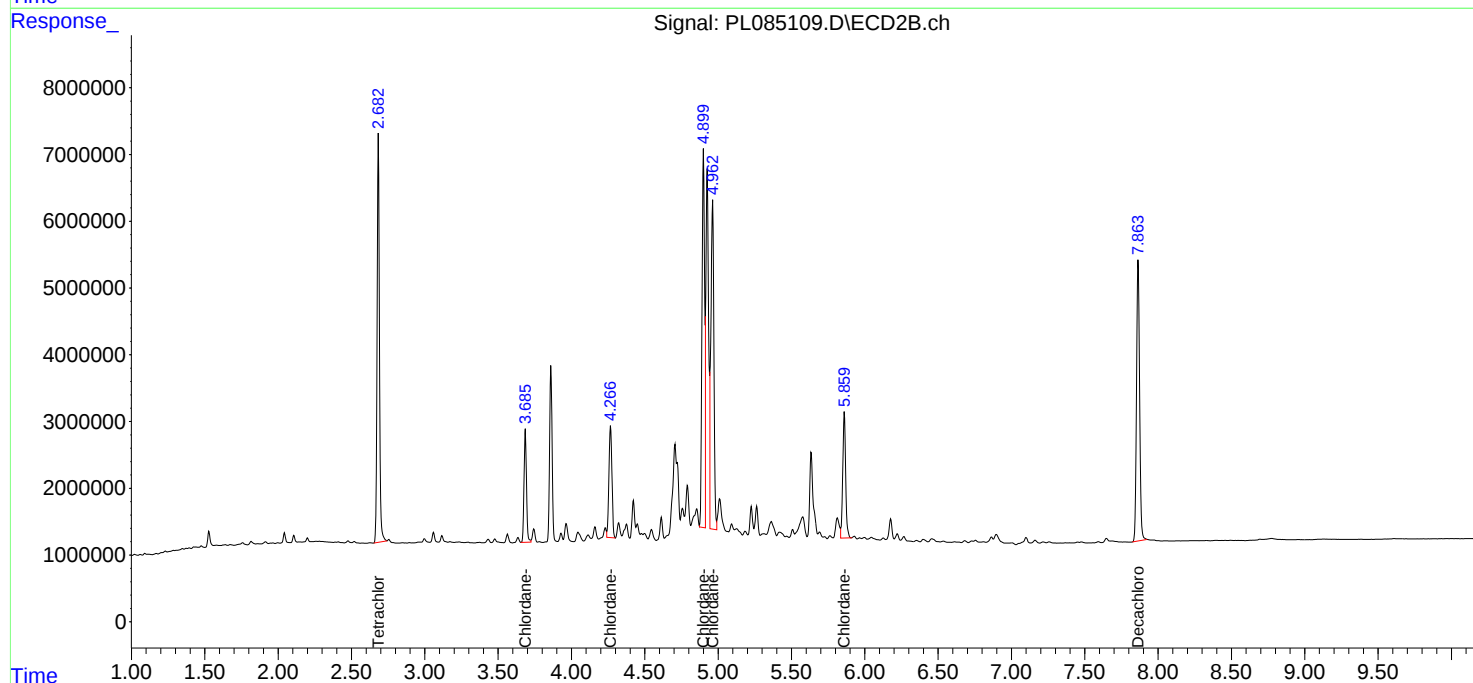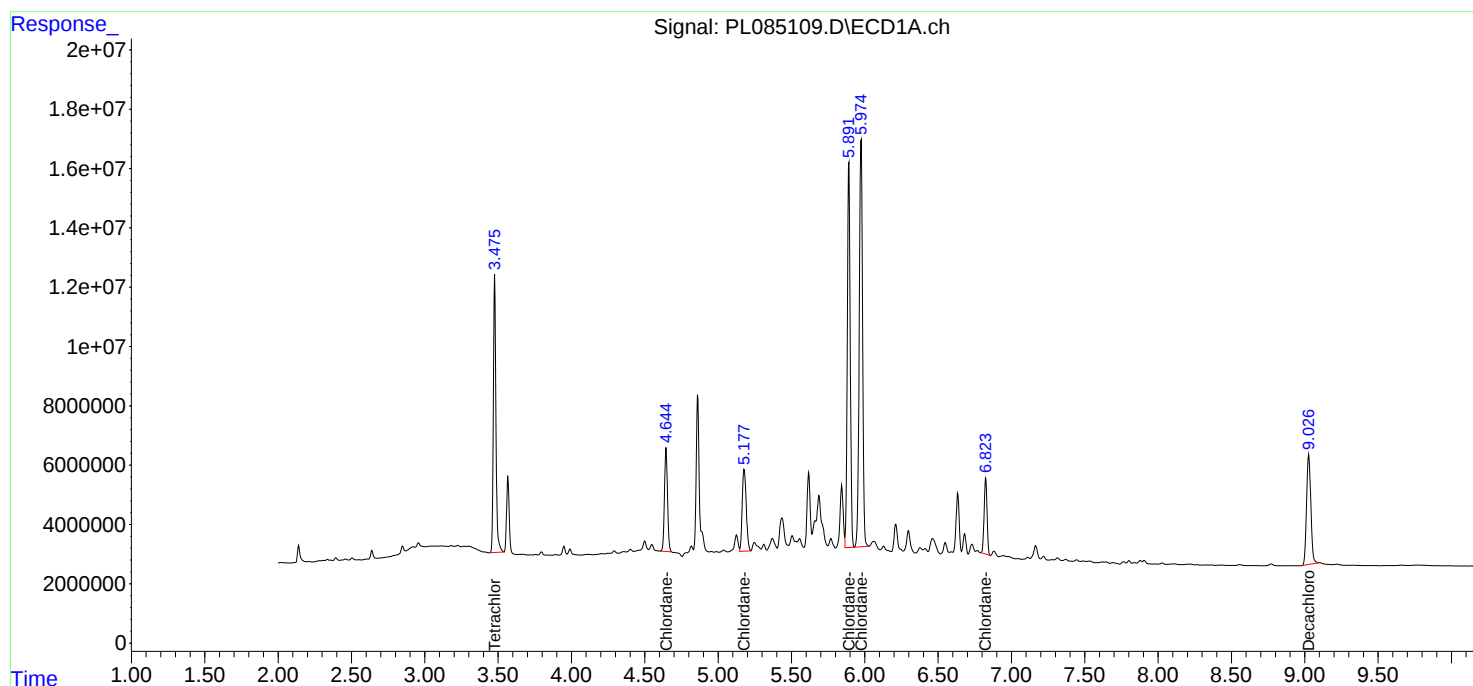


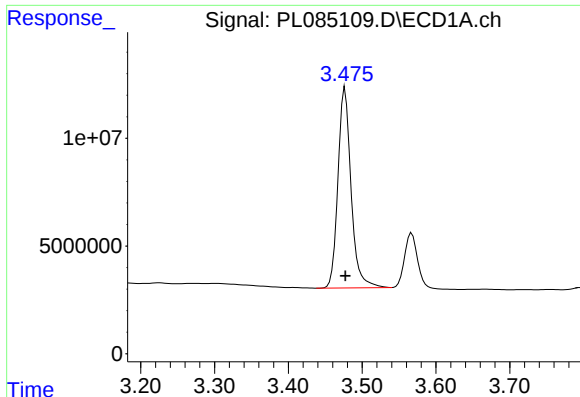

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 114976477
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

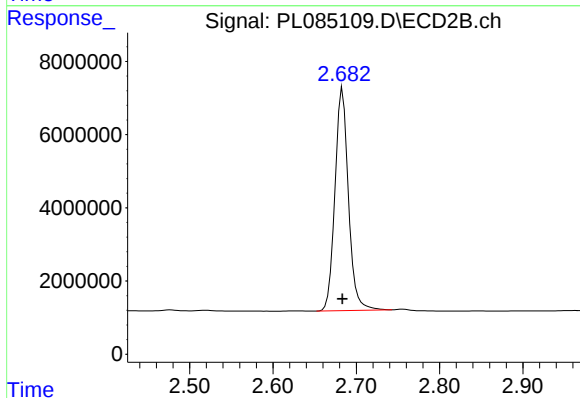


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 68438909
Conc: 50.00 ng/ml

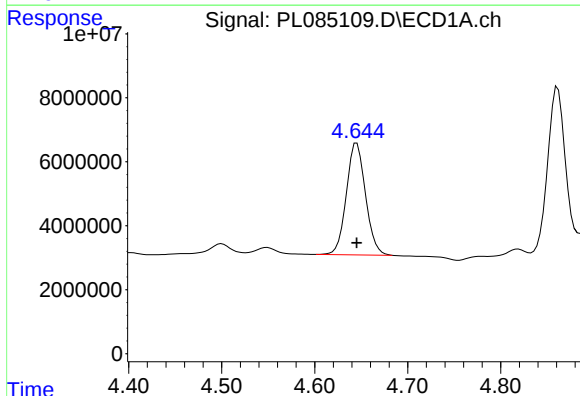


#23 Chlordane-1

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 50095947
Conc: 500.00 ng/ml

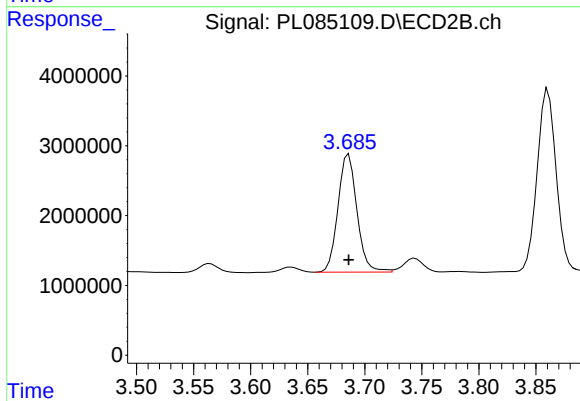

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 19538293
Conc: 500.00 ng/ml

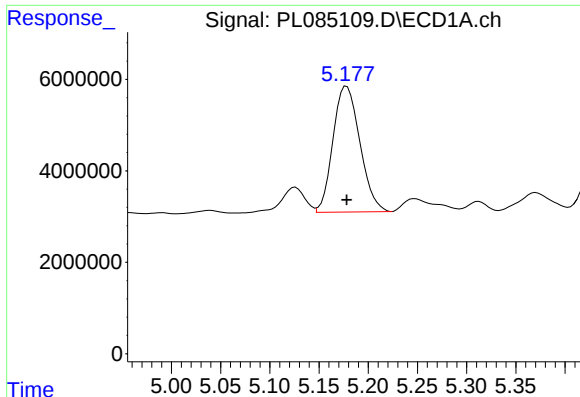

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 52391034
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

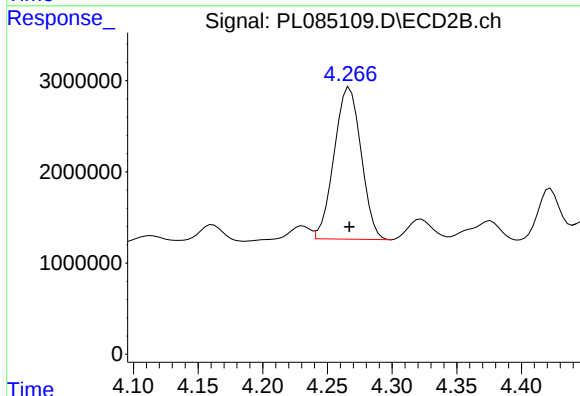


#24 Chlordane-2

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 24157350
Conc: 500.00 ng/ml

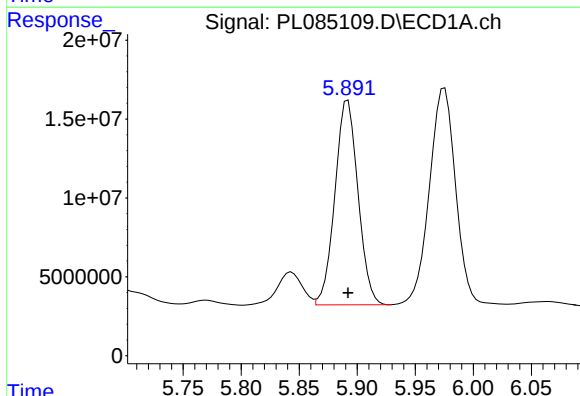


#25 Chlordane-3

R.T.: 5.892 min
Delta R.T.: 0.000 min
Response: 179555222
Conc: 500.00 ng/ml

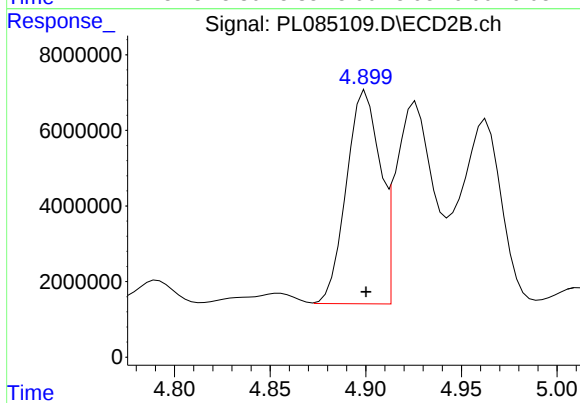

#25 Chlordane-3


R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 68721989
Conc: 500.00 ng/ml

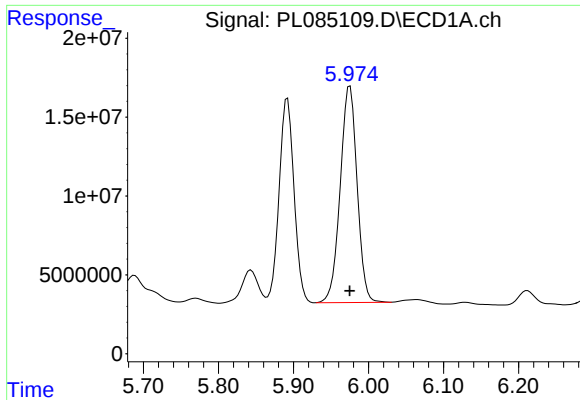

#26 Chlordane-4


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 214861331
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

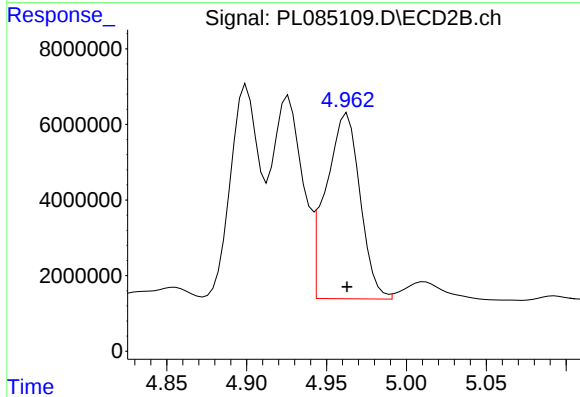


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 72874342
Conc: 500.00 ng/ml

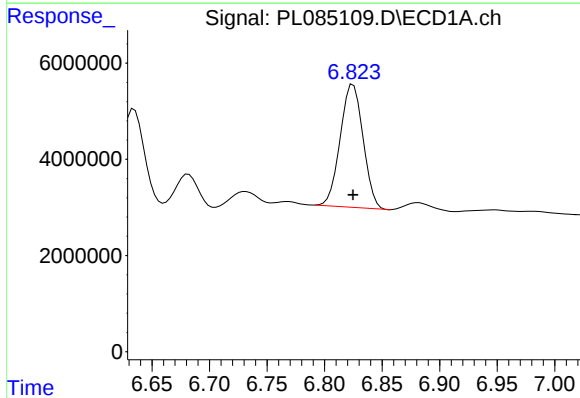


#27 Chlordane-5

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 35522158
Conc: 500.00 ng/ml

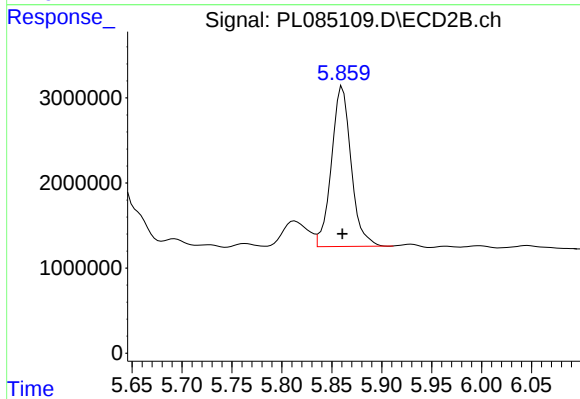

#27 Chlordane-5


R.T.: 5.861 min
Delta R.T.: 0.000 min
Response: 25734529
Conc: 500.00 ng/ml

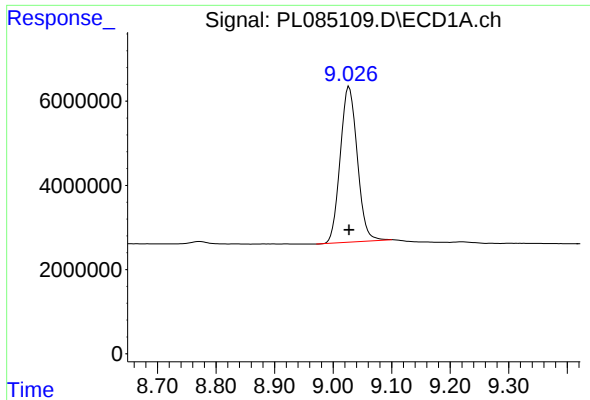

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.000 min
Response: 74825639
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

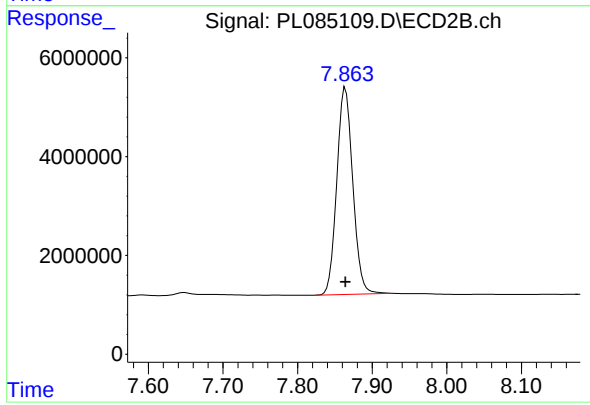

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 62340993
Conc: 50.00 ng/ml