

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
 Data File : PL085110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 12:21
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 15:11:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 14:57:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.684	55153968	32327262	24.473	24.020
28)	SA Decachlor...	9.027	7.864	38365184	31176018	26.349	25.580
Target Compounds							
23)	Chlordane-1	4.644	3.686	24461042	9284313	249.930	240.998
24)	Chlordane-2	5.177	4.267	26432874	11959484	259.763	253.475
25)	Chlordane-3	5.891	4.900	86073576	31432062	243.062	231.920
26)	Chlordane-4	5.975	4.963	104.4E6	34465146	246.981	238.939
27)	Chlordane-5	6.825	5.861	16892554	12464235	245.390	244.220



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
Data File : PL085110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 12:21
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 15:11:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 14:57:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

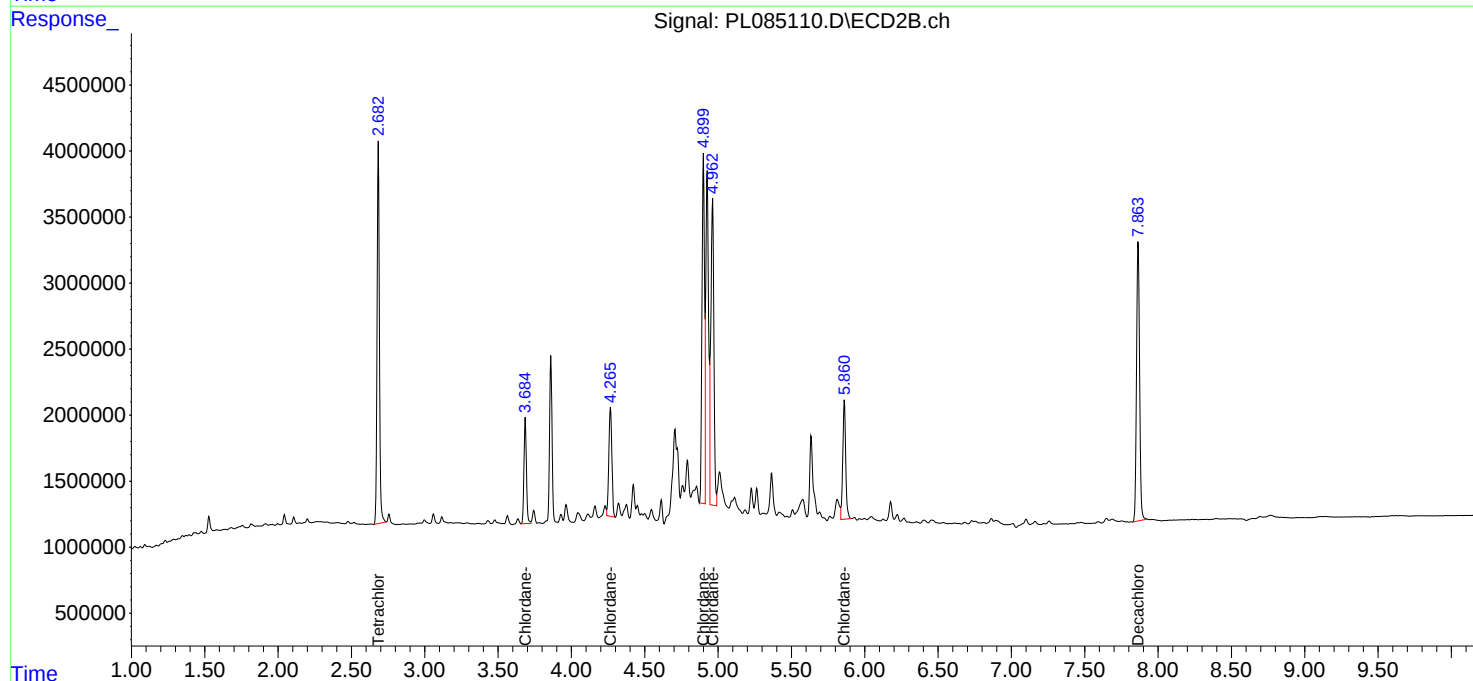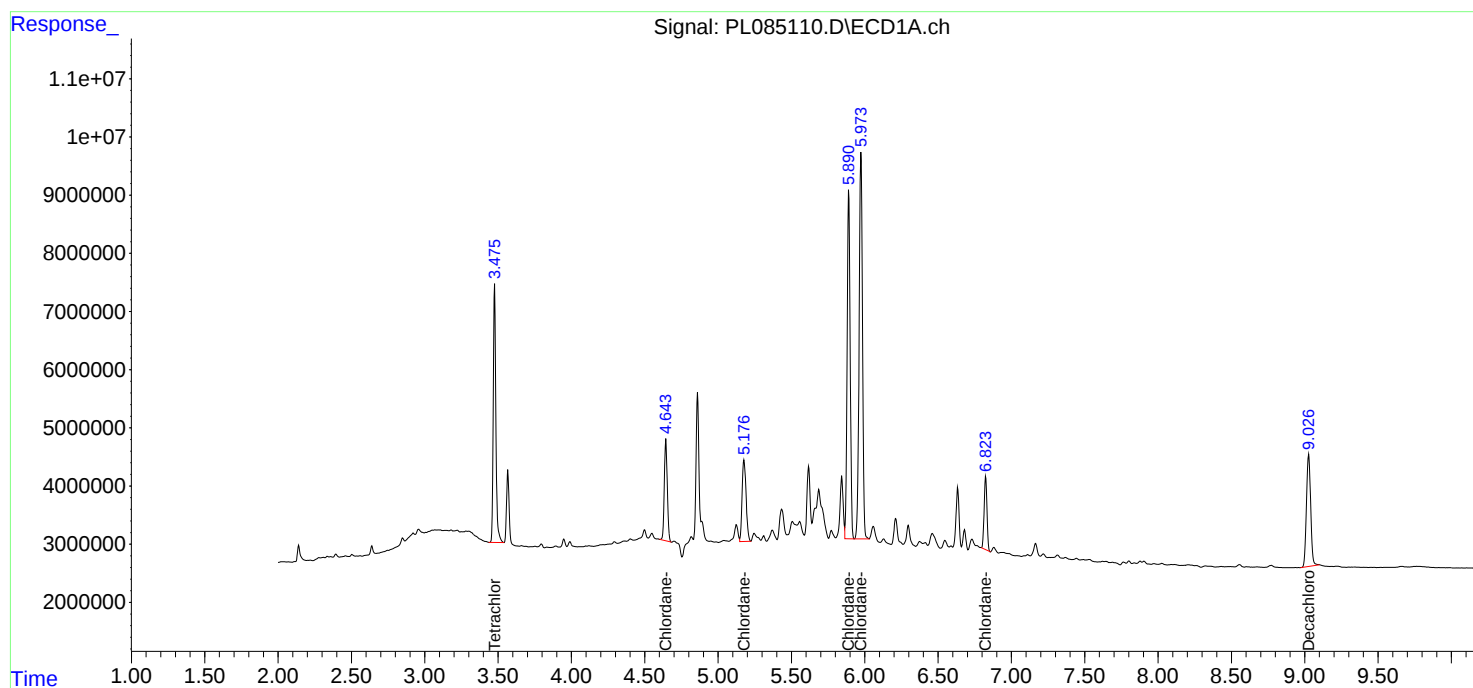


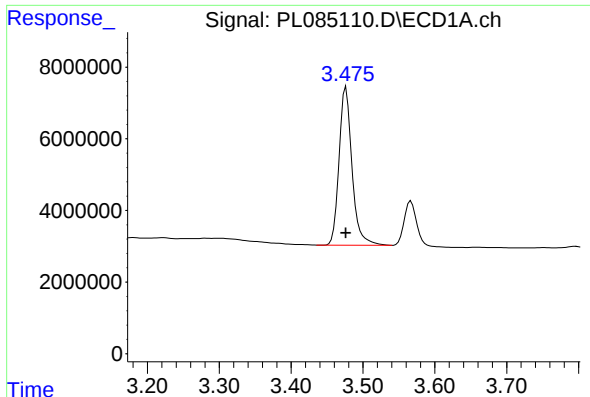

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 55153968
Conc: 24.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

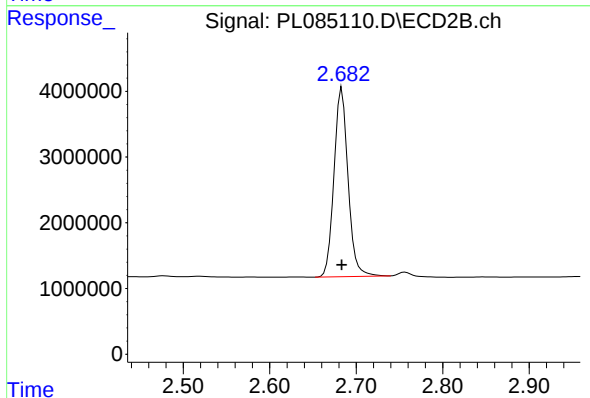


#1 Tetrachloro-m-xylene

R.T.: 2.684 min
Delta R.T.: 0.000 min
Response: 32327262
Conc: 24.02 ng/ml

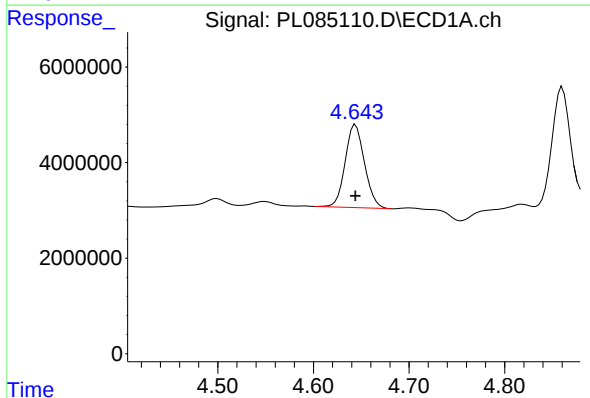


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 24461042
Conc: 249.93 ng/ml

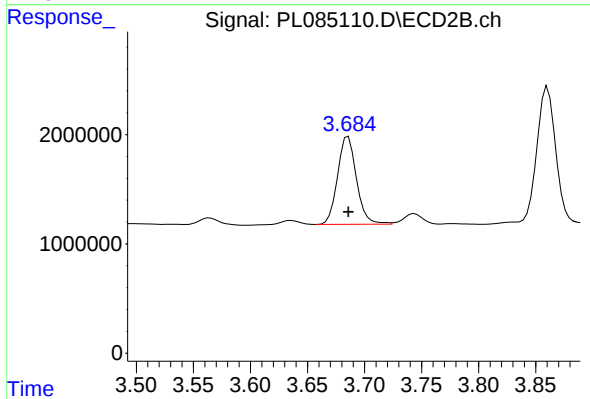

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 9284313
Conc: 241.00 ng/ml

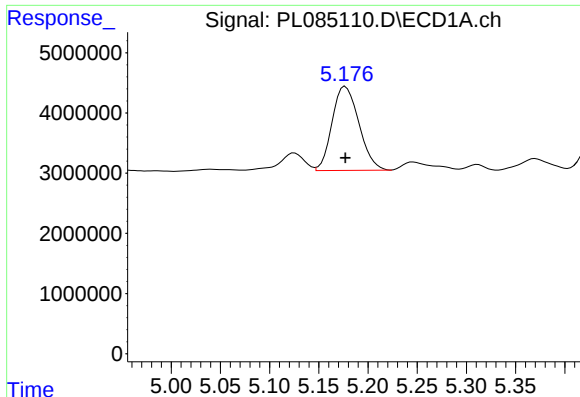

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 26432874
Conc: 259.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

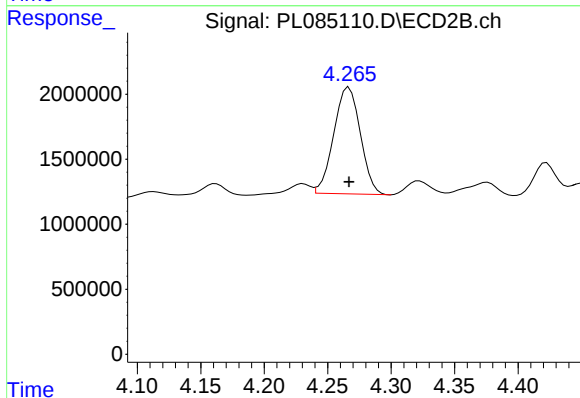


#24 Chlordane-2

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 11959484
Conc: 253.47 ng/ml

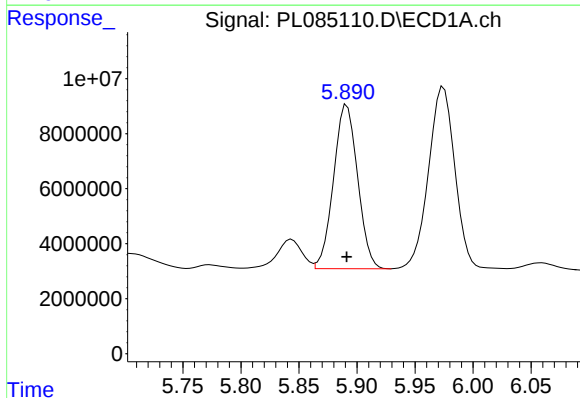


#25 Chlordane-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 86073576
Conc: 243.06 ng/ml

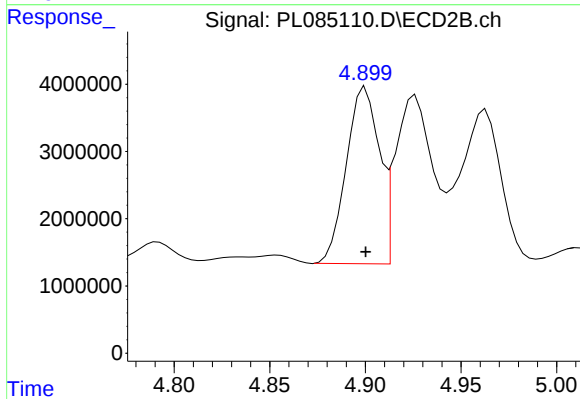

#25 Chlordane-3


R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 31432062
Conc: 231.92 ng/ml

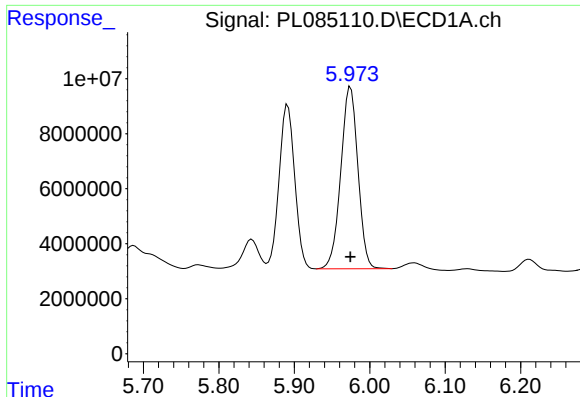

#26 Chlordane-4


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 104429529
Conc: 246.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

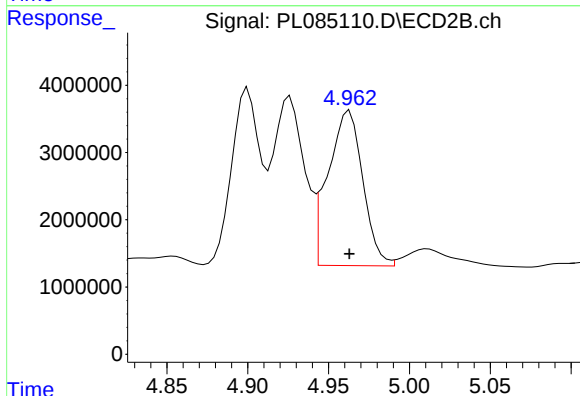


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 34465146
Conc: 238.94 ng/ml

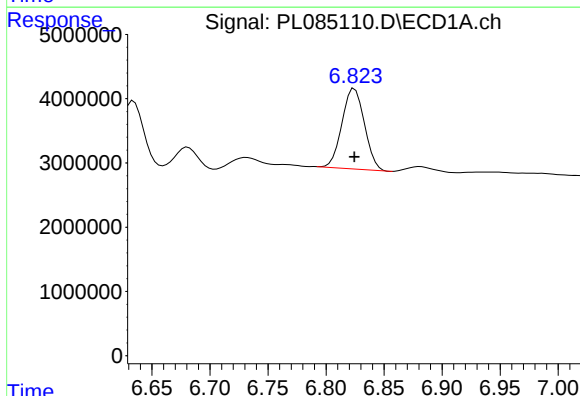


#27 Chlordane-5

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 16892554
Conc: 245.39 ng/ml

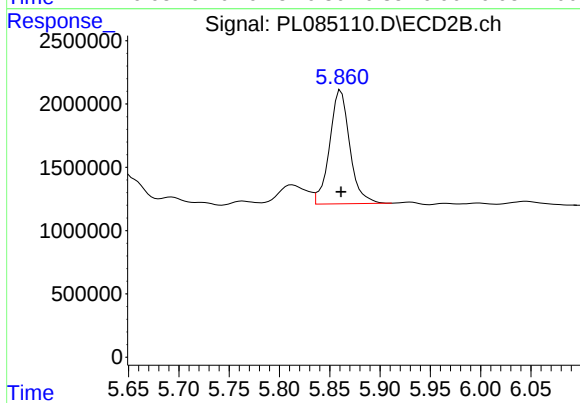

#27 Chlordane-5


R.T.: 5.861 min
Delta R.T.: 0.000 min
Response: 12464235
Conc: 244.22 ng/ml

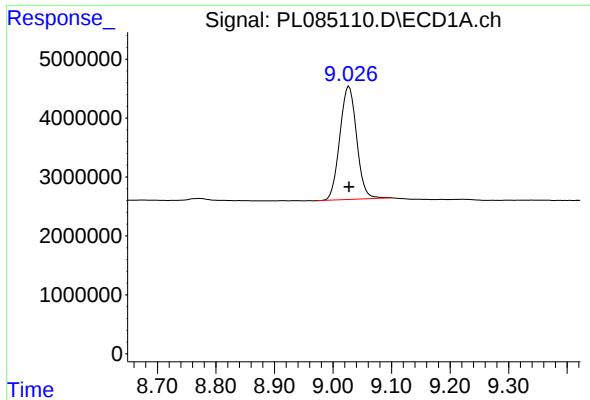

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.000 min
Response: 38365184
Conc: 26.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

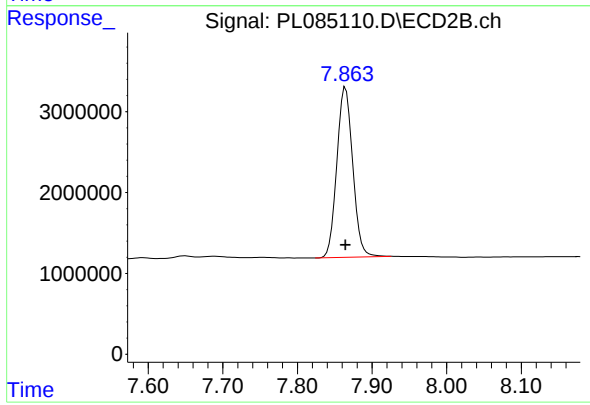

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 31176018
Conc: 25.58 ng/ml