

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
 Data File : PL085111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 12:35
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 15:14:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 14:57:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.683	12241994	7006519	5.340	5.163
28)	SA Decachlor...	9.027	7.864	8730970	7234351	5.767	5.722
Target Compounds							
23)	Chlordane-1	4.644	3.685	5302542	2010363	53.288	51.732
24)	Chlordane-2	5.178	4.266	5838613	2612729	55.733	54.210
25)	Chlordane-3	5.892	4.899	19536420	6463586	54.051	48.136
26)	Chlordane-4	5.975	4.962	23896946	8328382	55.081	56.005
27)	Chlordane-5	6.825	5.860	3686663	2518869	52.804	49.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
Data File : PL085111.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 12:35
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 15:14:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 14:57:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

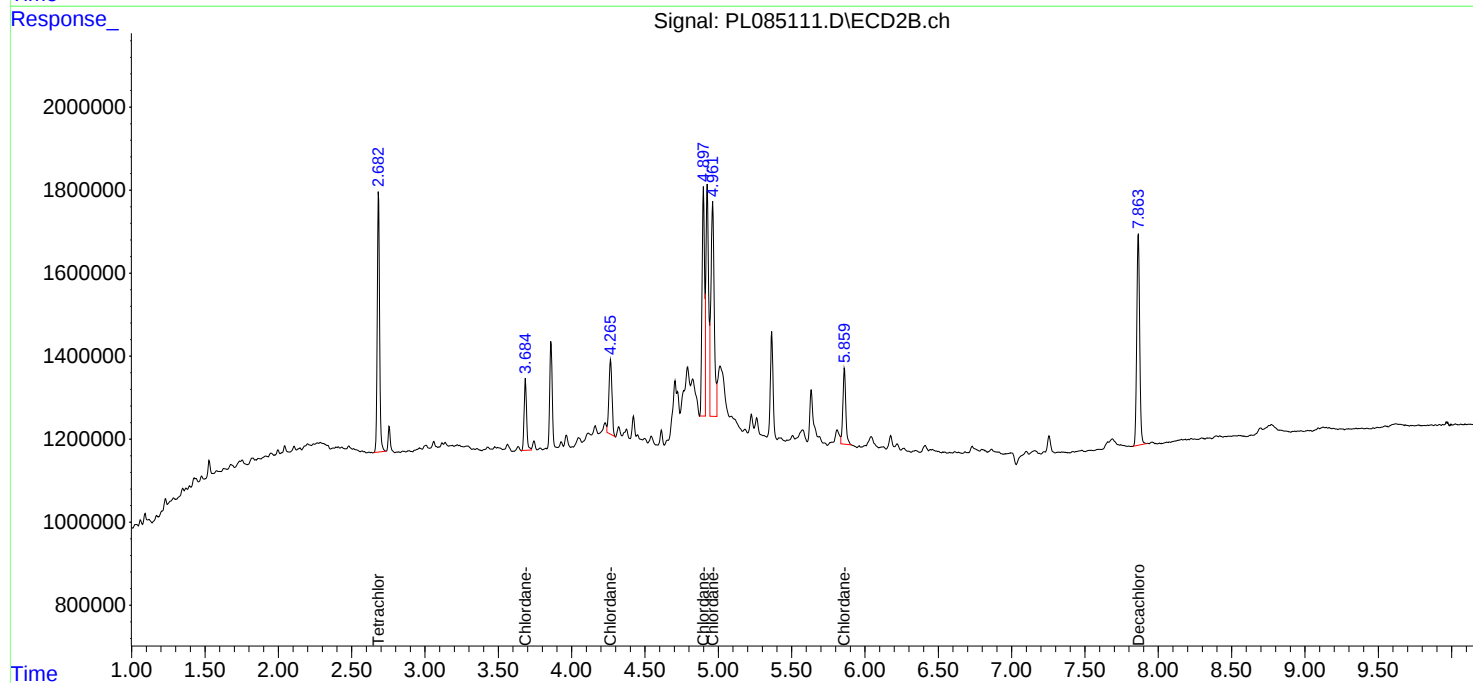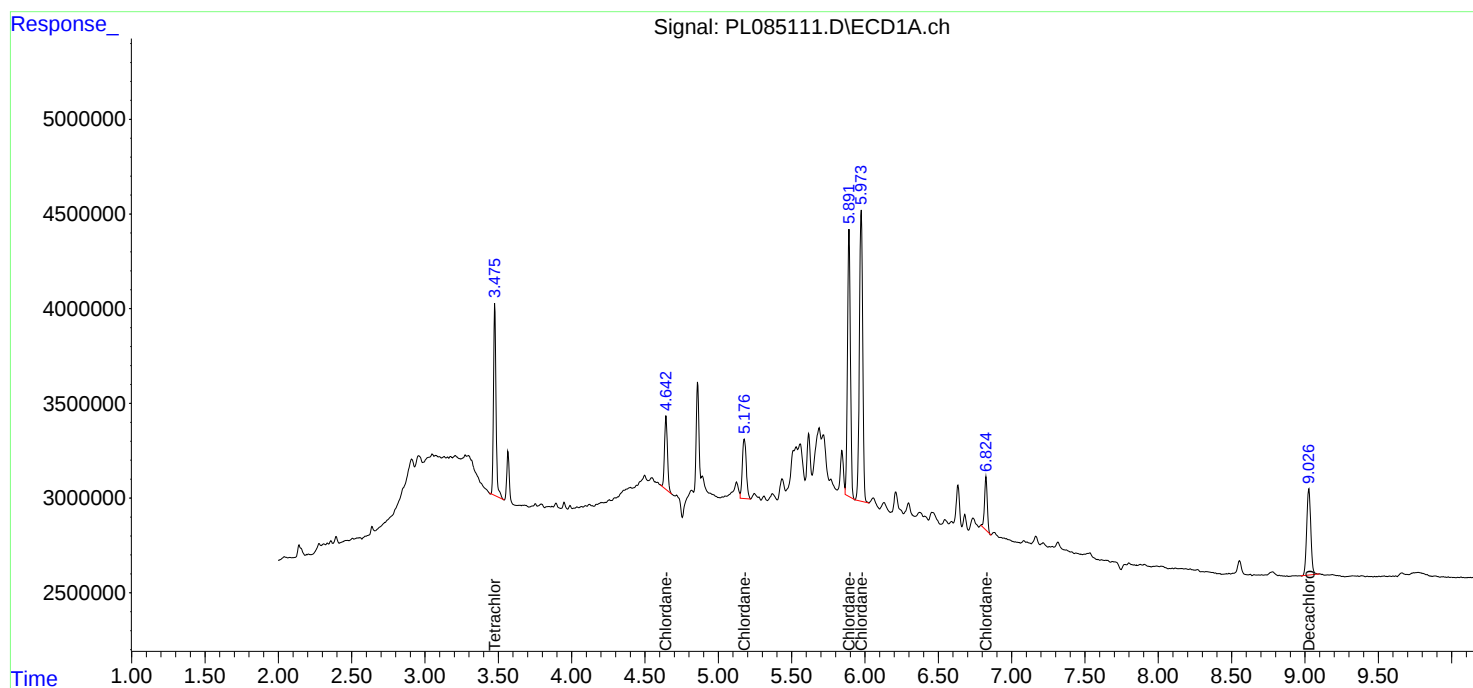


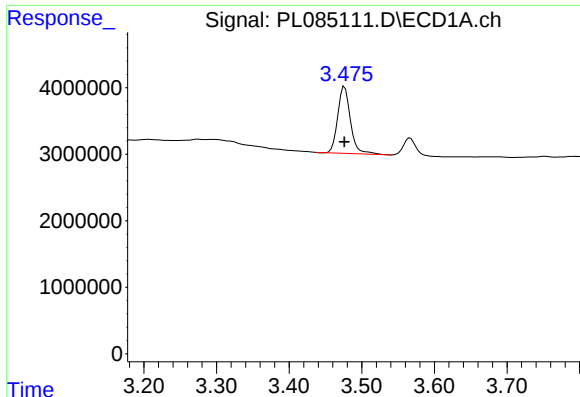

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 12241994
Conc: 5.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

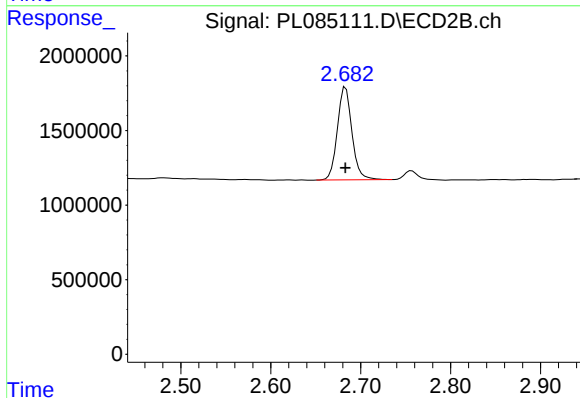


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 7006519
Conc: 5.16 ng/ml

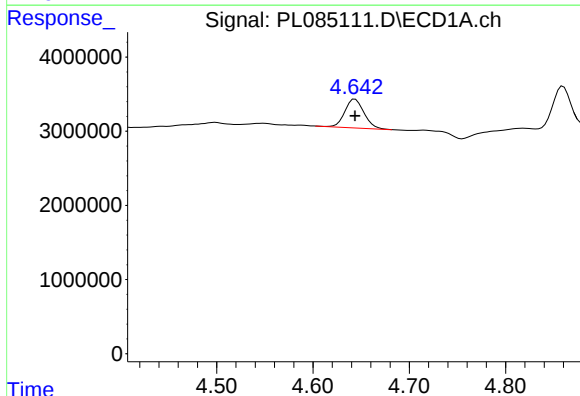


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 5302542
Conc: 53.29 ng/ml

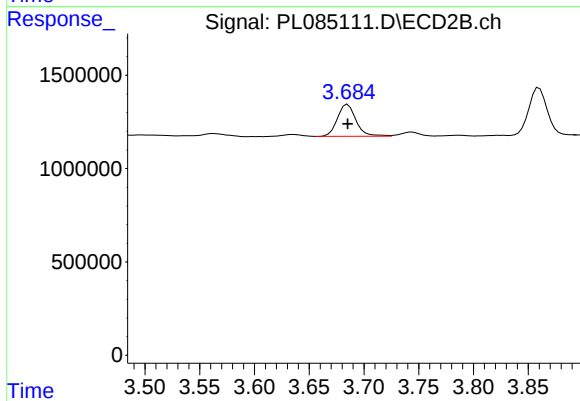

#23 Chlordane-1


R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 2010363
Conc: 51.73 ng/ml

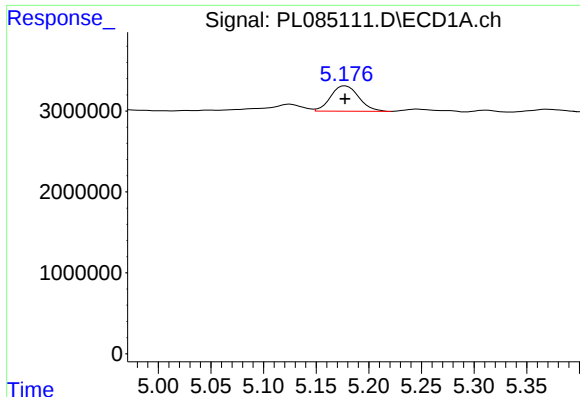

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 5838613
Conc: 55.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

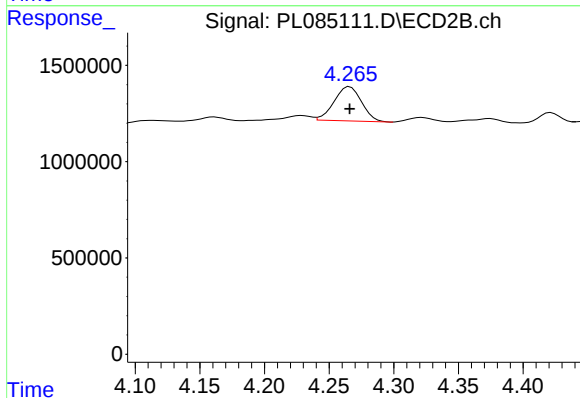


#24 Chlordane-2

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 2612729
Conc: 54.21 ng/ml

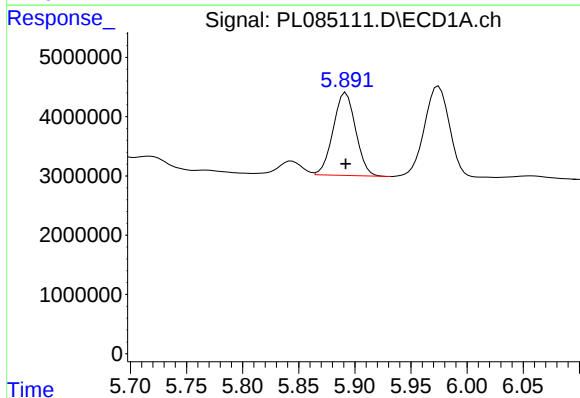


#25 Chlordane-3

R.T.: 5.892 min
Delta R.T.: 0.000 min
Response: 19536420
Conc: 54.05 ng/ml

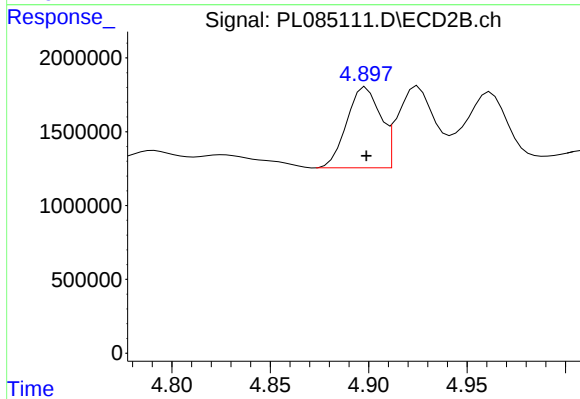

#25 Chlordane-3


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 6463586
Conc: 48.14 ng/ml

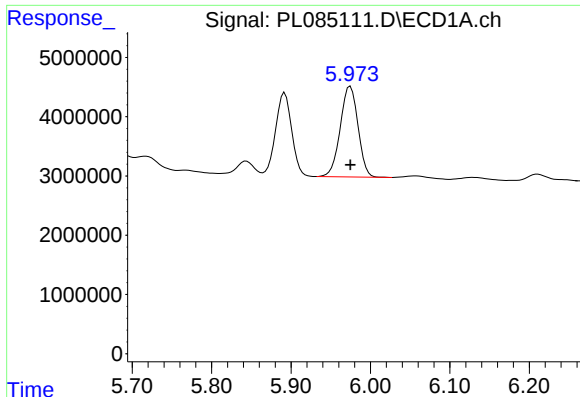

#26 Chlordane-4


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 23896946
Conc: 55.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

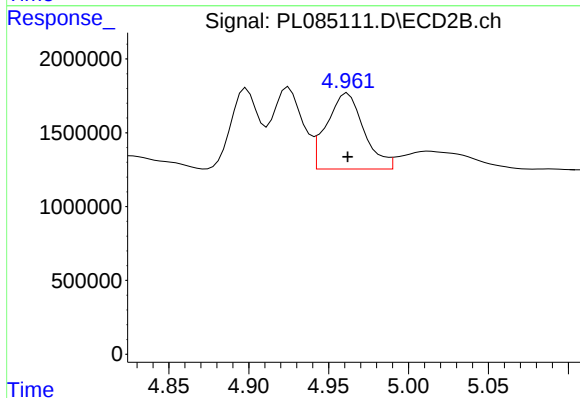


#26 Chlordane-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 8328382
Conc: 56.01 ng/ml

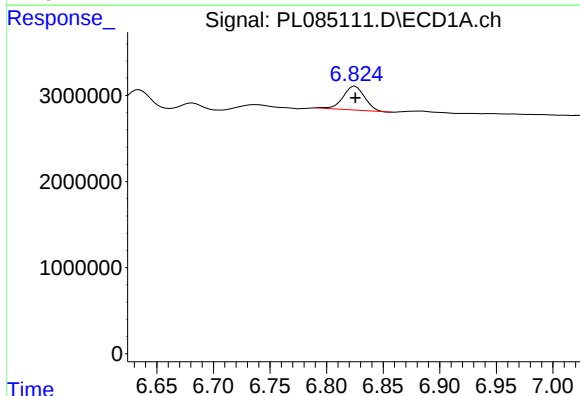


#27 Chlordane-5

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 3686663
Conc: 52.80 ng/ml

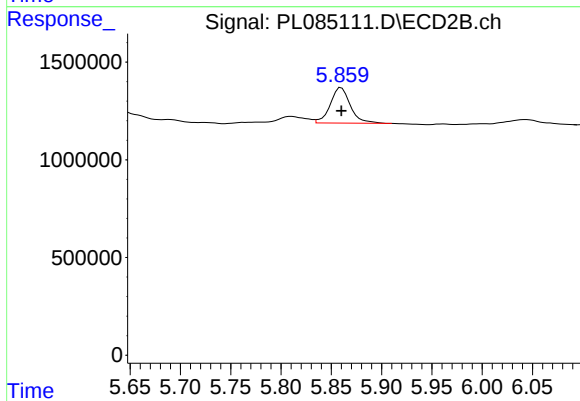

#27 Chlordane-5


R.T.: 5.860 min
Delta R.T.: 0.000 min
Response: 2518869
Conc: 49.48 ng/ml

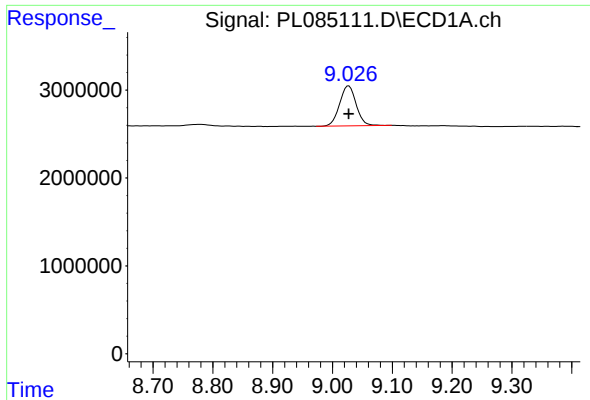

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.000 min
Response: 8730970
Conc: 5.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

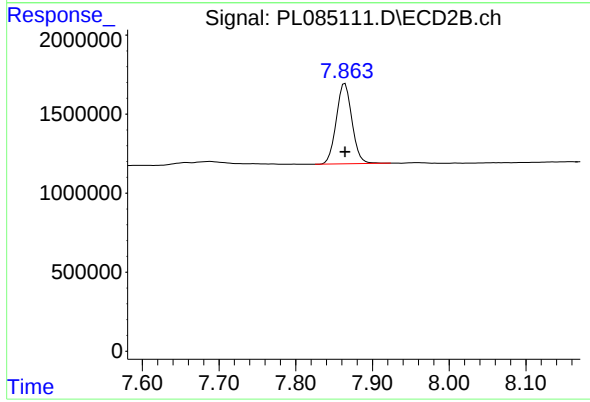

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 7234351
Conc: 5.72 ng/ml