

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
 Data File : PL085118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 14:26
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL090523CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 15:17:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:17:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.683	111.7E6	67555077	48.725	49.784
28)	SA Decachlor...	9.026	7.863	73193451	61321794	48.342	48.499
Target Compounds							
23)	Chlordane-1	4.644	3.685	48608433	19249215	488.491	495.336
24)	Chlordane-2	5.177	4.266	50941041	23784501	486.262	493.489
25)	Chlordane-3	5.891	4.899	174.3E6	67507823	482.133	502.746
26)	Chlordane-4	5.974	4.962	208.8E6	71745440	481.208	482.460
27)	Chlordane-5	6.824	5.860	34607870	25502276	495.685	500.978



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090523\
Data File : PL085118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 14:26
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL090523CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 15:17:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:17:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

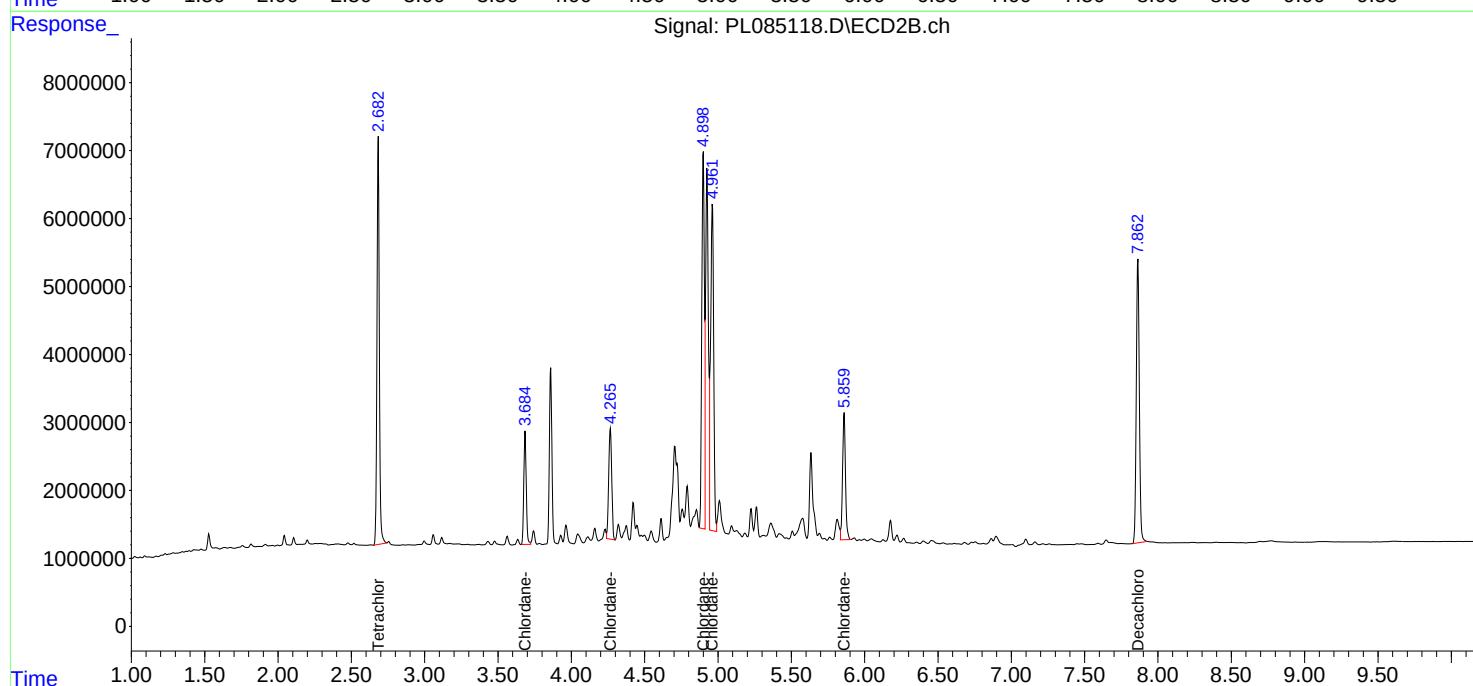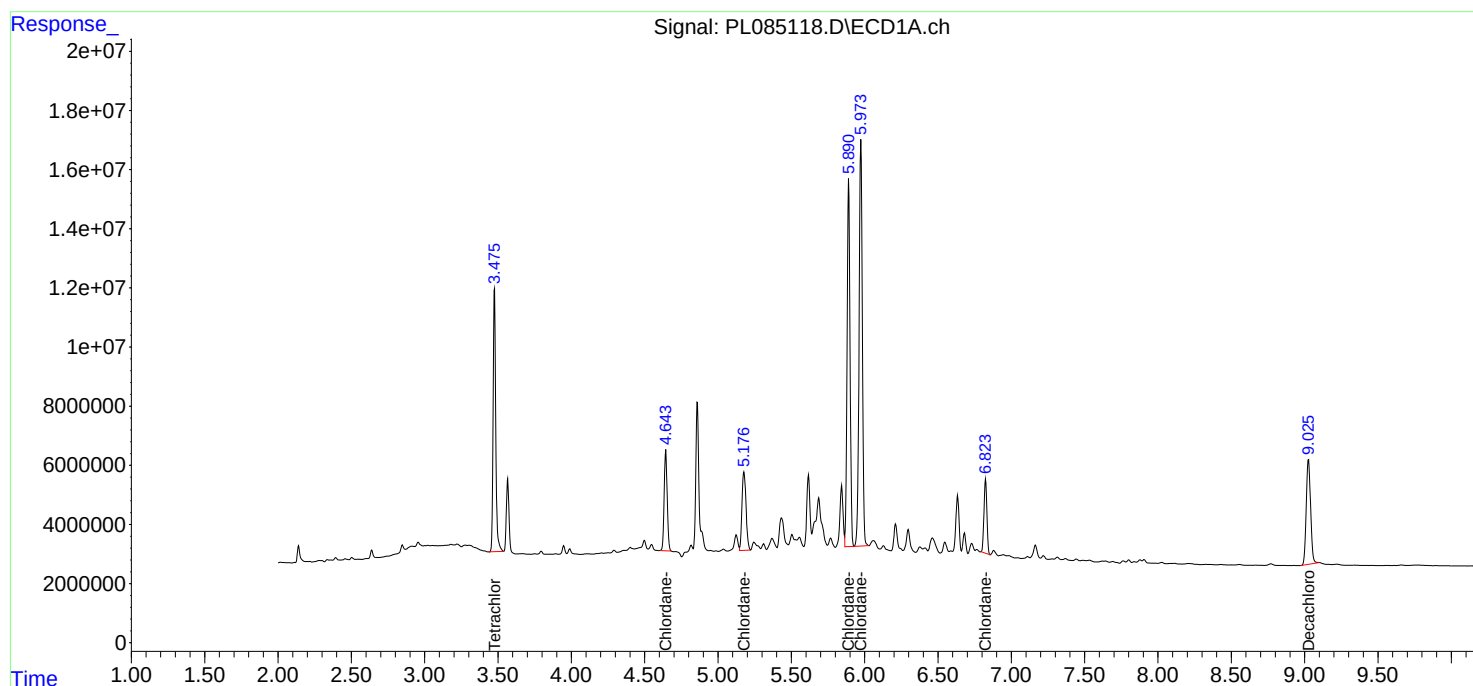


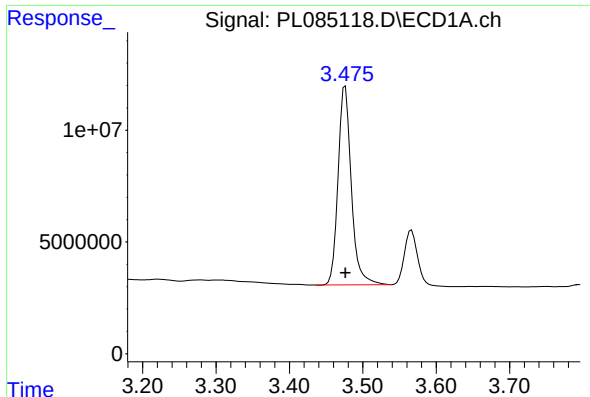

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 111709381
Conc: 48.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090523CHLOR

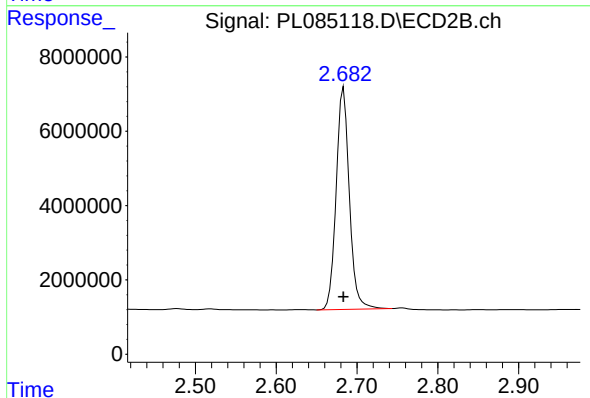


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 67555077
Conc: 49.78 ng/ml

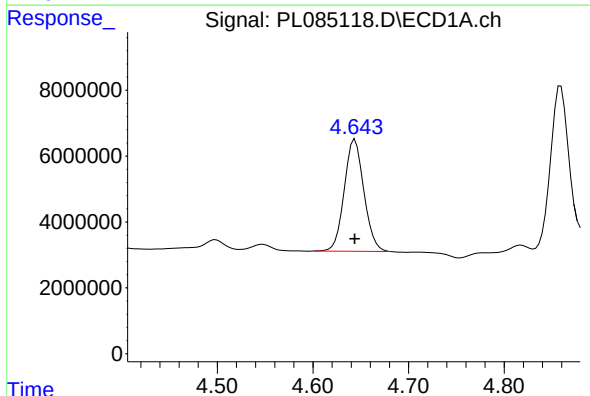


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 48608433
Conc: 488.49 ng/ml

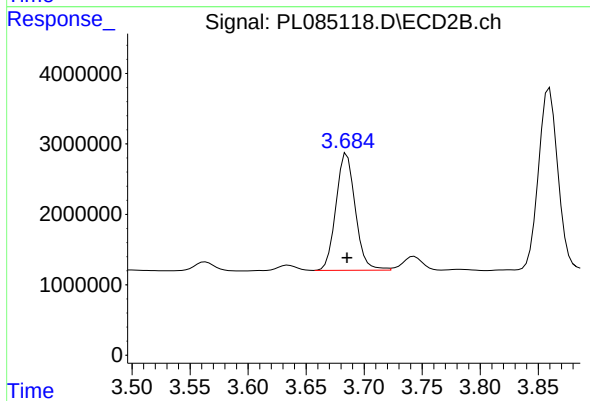

#23 Chlordane-1


R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 19249215
Conc: 495.34 ng/ml

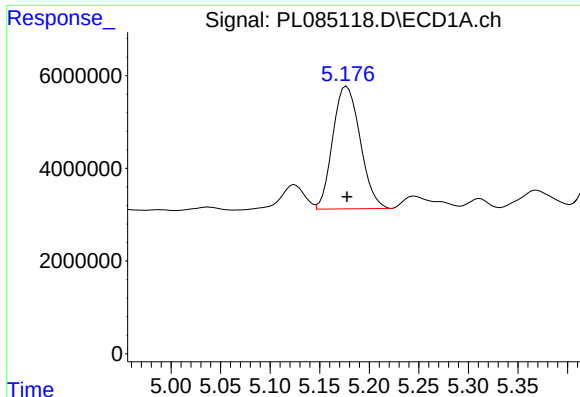

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 50941041
Conc: 486.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090523CHLOR

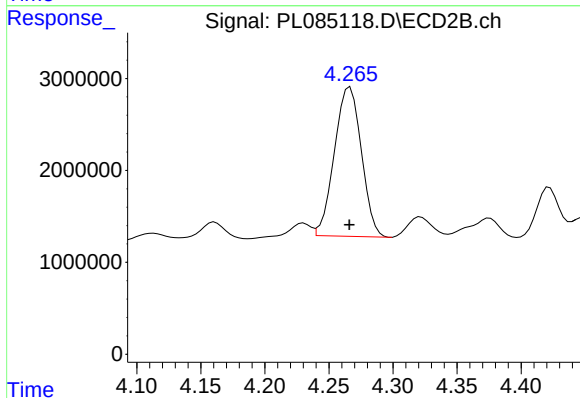


#24 Chlordane-2

R.T.: 4.266 min
Delta R.T.: 0.000 min
Response: 23784501
Conc: 493.49 ng/ml

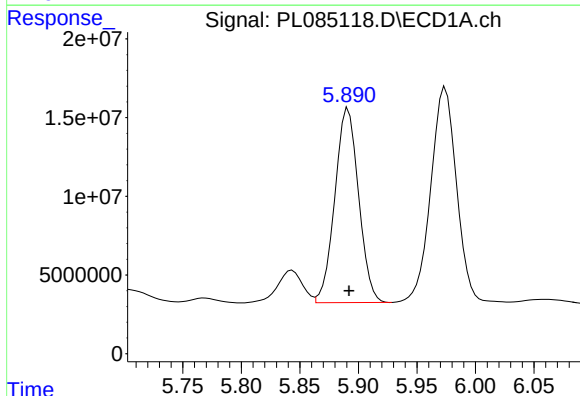


#25 Chlordane-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 174263332
Conc: 482.13 ng/ml

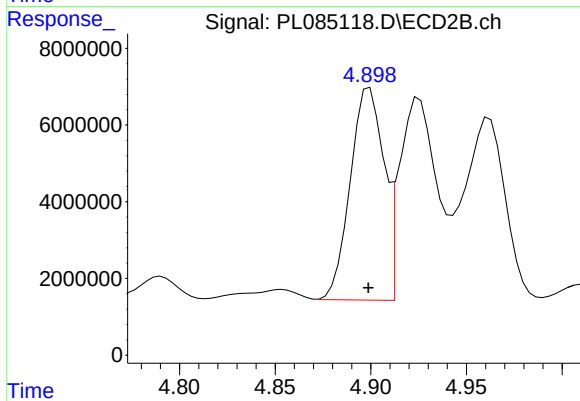

#25 Chlordane-3


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 67507823
Conc: 502.75 ng/ml

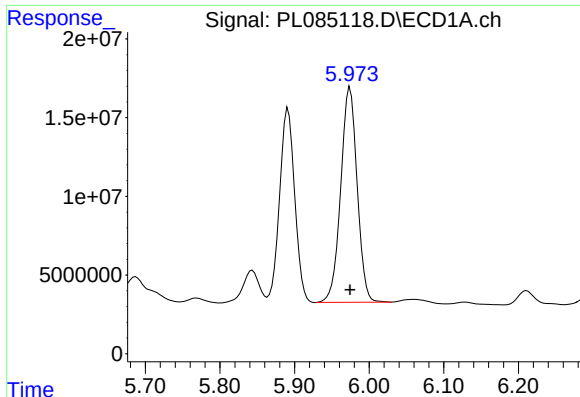

#26 Chlordane-4


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 208770943
Conc: 481.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090523CHLOR

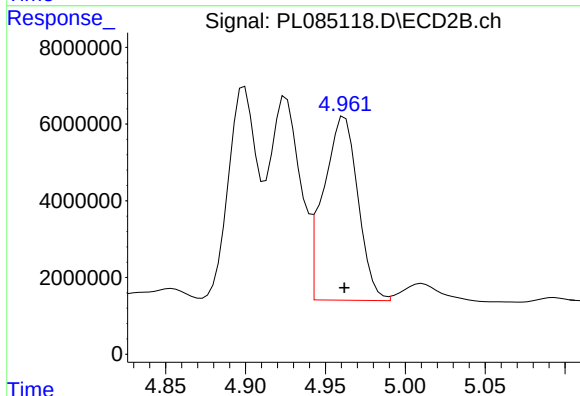


#26 Chlordane-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 71745440
Conc: 482.46 ng/ml

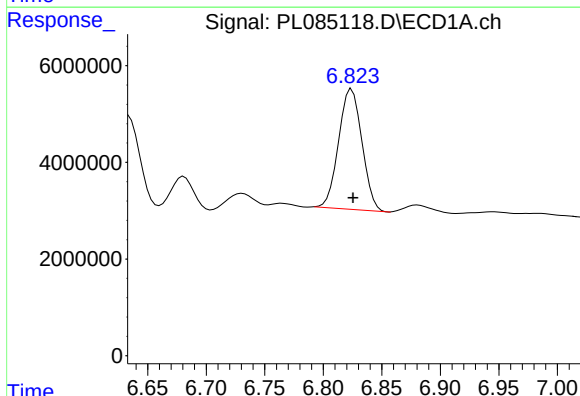


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: -0.001 min
Response: 34607870
Conc: 495.68 ng/ml

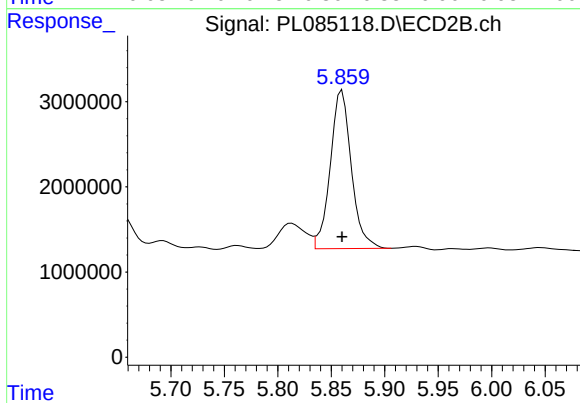

#27 Chlordane-5


R.T.: 5.860 min
Delta R.T.: 0.000 min
Response: 25502276
Conc: 500.98 ng/ml

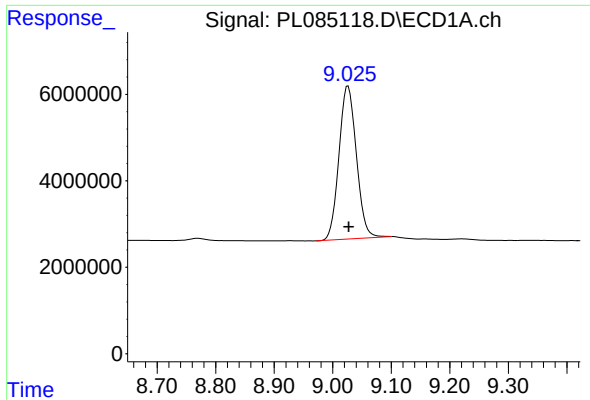

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.001 min
Response: 73193451
Conc: 48.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL090523CHLOR

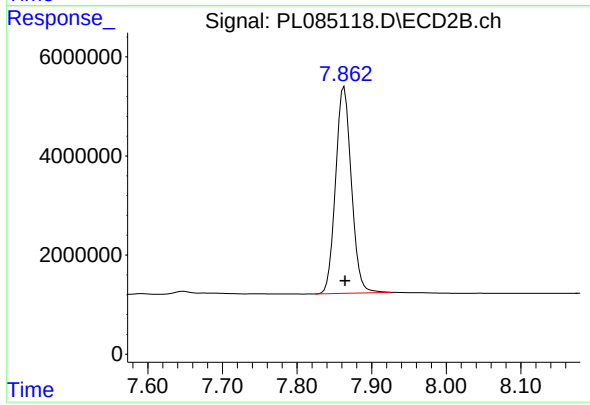

#28 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: 0.000 min
Response: 61321794
Conc: 48.50 ng/ml