

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
 Data File : PL039732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2018 18:15
 Operator : AJ\SJ
 Sample : PB112643TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:12:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.905	155.5E6	65115779	22.241	24.289
28)	SA Decachlor...	7.956	8.891	153.7E6	56446840	21.885	24.324
Target Compounds							
3)	MA gamma-BHC...	4.048f	0.000	342.6E6	0	32.297	N.D. #
7)	B delta-BHC	0.000	4.950	0	26734185	N.D.	6.714 #
8)	B Heptachlo...	4.913f	5.771	4758243	18095514	0.498	5.381 #
15)	B Endosulfa...	6.009f	0.000	13972598	0	1.607	N.D. #
23)	Chlordane-1	0.000	4.950	0	26734185	N.D.	213.985 #
27)	Chlordane-5	6.009	0.000	13972598	0	43.081	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
Data File : PL039732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2018 18:15
Operator : AJ\SJ
Sample : PB112643TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:12:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

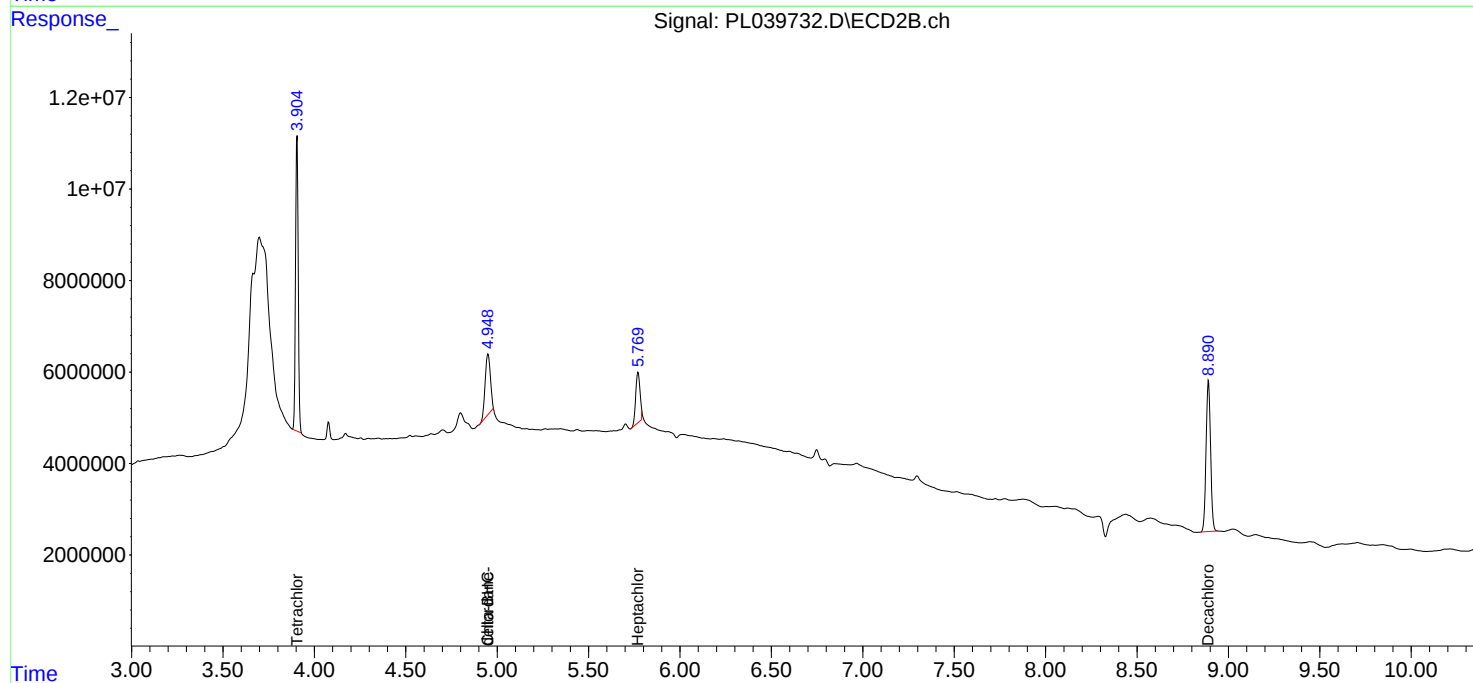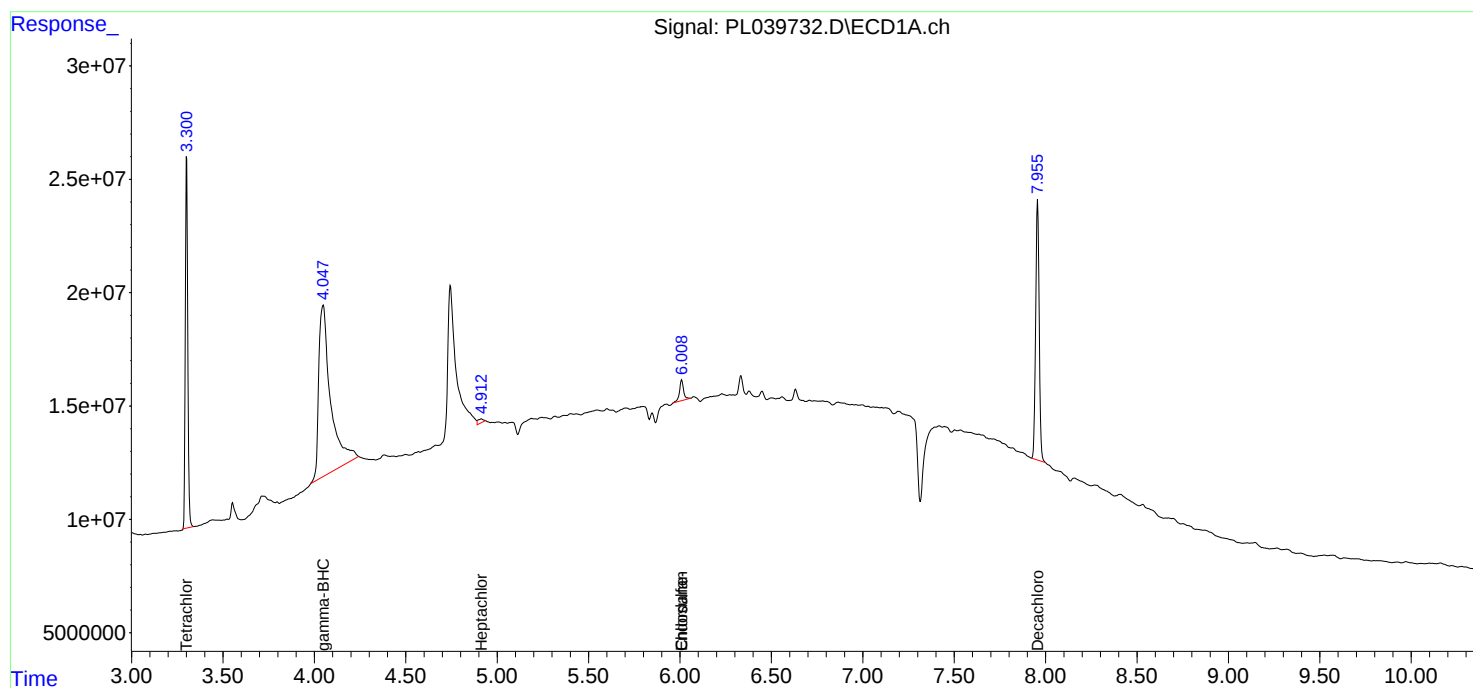


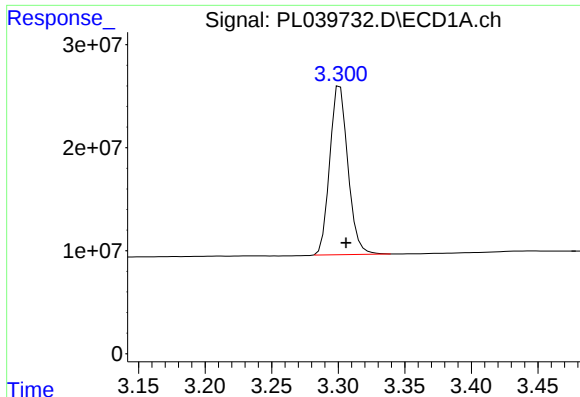

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: -0.005 min
Response: 155472837
Conc: 22.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

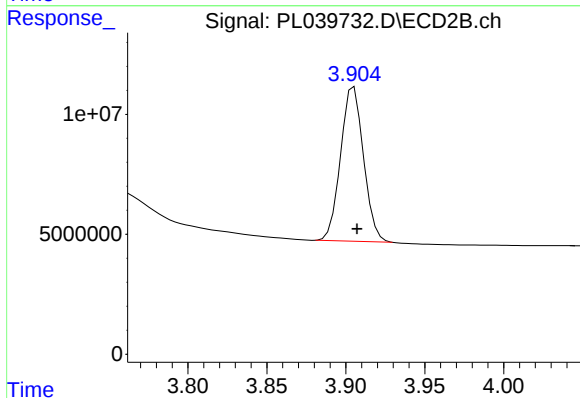


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 65115779
Conc: 24.29 ng/ml

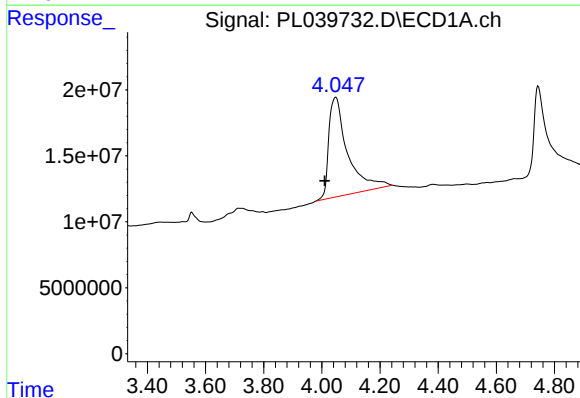


#3 gamma-BHC (Lindane)

R.T.: 4.048 min
Delta R.T.: 0.039 min
Response: 342558801
Conc: 32.30 ng/ml

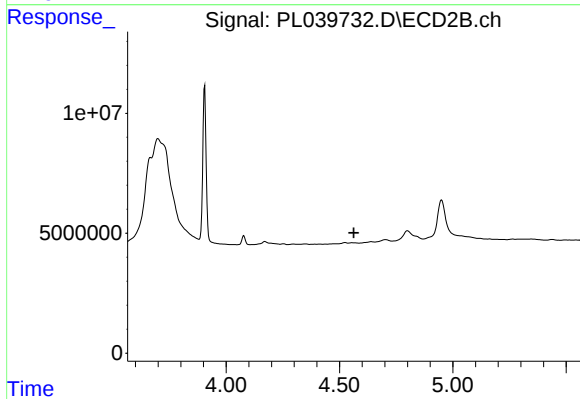

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

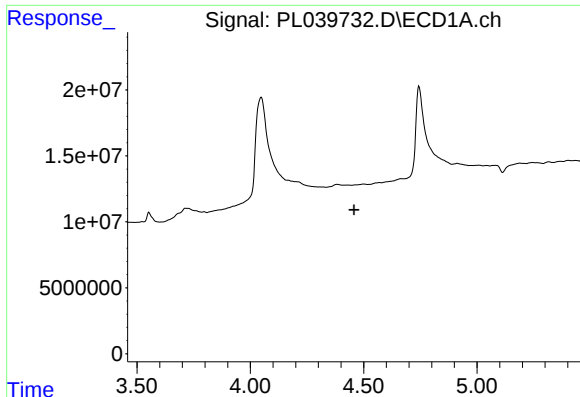

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

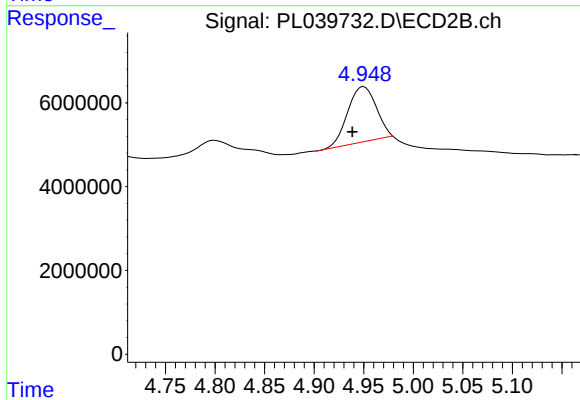


#7 delta-BHC

R.T.: 4.950 min
Delta R.T.: 0.012 min
Response: 26734185
Conc: 6.71 ng/ml

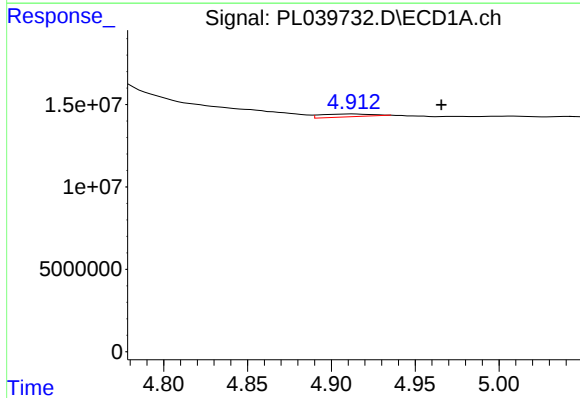


#8 Heptachlor epoxide

R.T.: 4.913 min
Delta R.T.: -0.052 min
Response: 4758243
Conc: 0.50 ng/ml

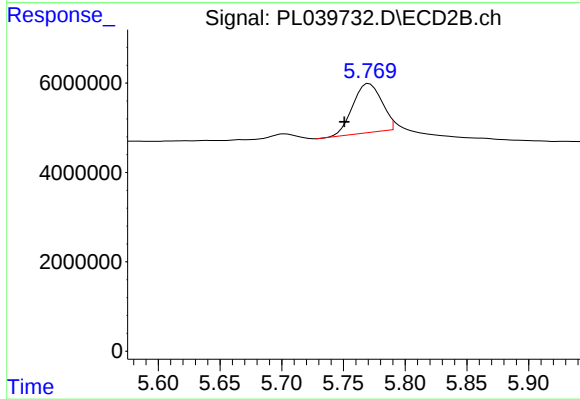

#8 Heptachlor epoxide


R.T.: 5.771 min
Delta R.T.: 0.020 min
Response: 18095514
Conc: 5.38 ng/ml

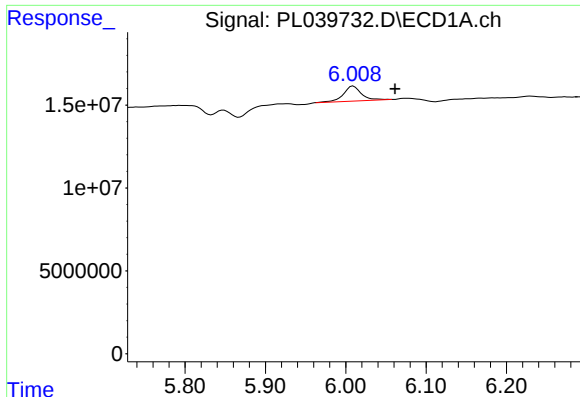

#15 Endosulfan II


R.T.: 6.009 min
Delta R.T.: -0.052 min
Response: 13972598
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

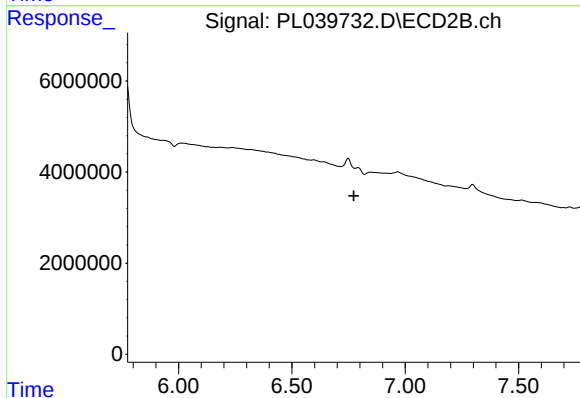


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

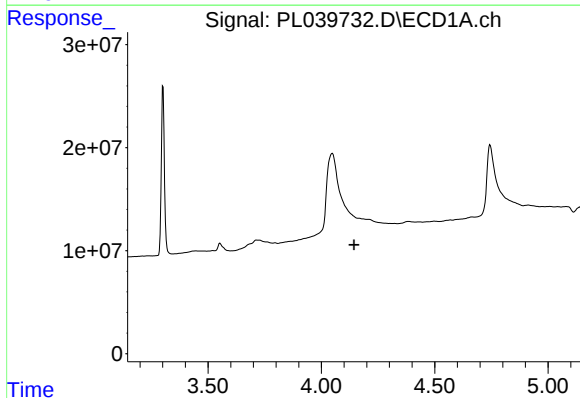


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.145 min
Response: 0
Conc: N.D.

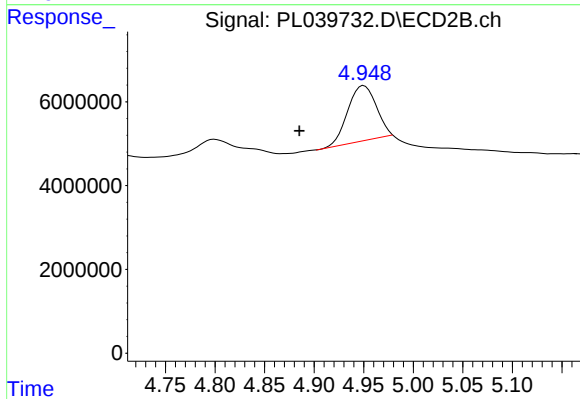

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.065 min
Response: 26734185
Conc: 213.99 ng/ml

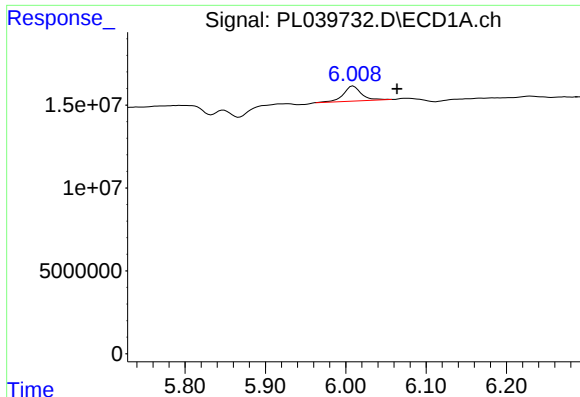

#27 Chlordane-5


R.T.: 6.009 min
Delta R.T.: -0.054 min
Response: 13972598
Conc: 43.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

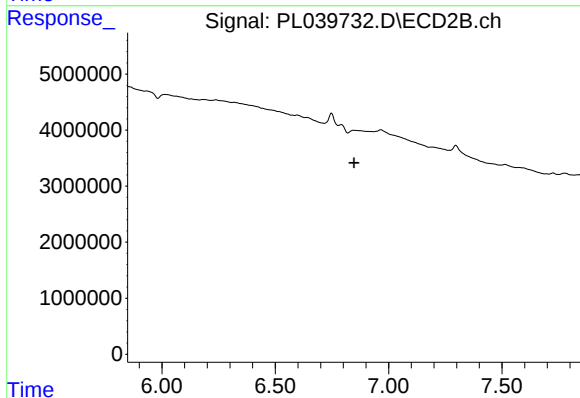


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.848 min
Response: 0
Conc: N.D.

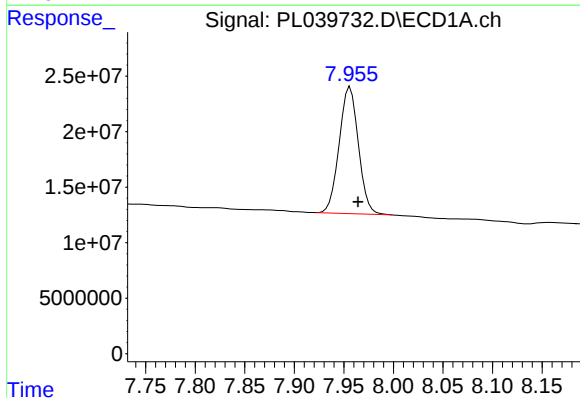

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.008 min
Response: 153704307
Conc: 21.88 ng/ml

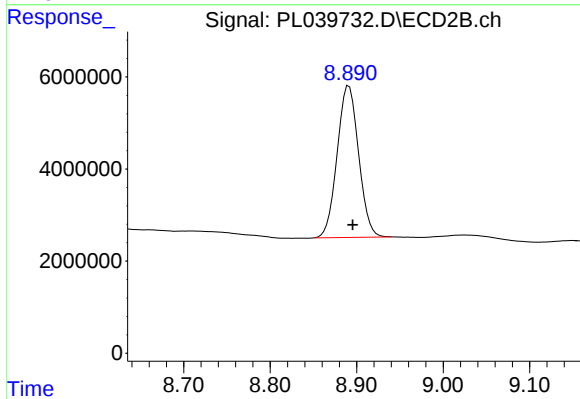

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: -0.004 min
Response: 56446840
Conc: 24.32 ng/ml