

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
 Data File : PL039736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2018 19:11
 Operator : AJ\SJ
 Sample : J4793-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:12:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.905	136.8E6	57451113	19.574	21.430
28)	SA Decachlor...	7.956	8.892	104.1E6	39156556	14.816	16.873
Target Compounds							
3)	MA gamma-BHC...	4.051f	0.000	214.7E6	0	20.241	N.D. #
7)	B delta-BHC	0.000	4.952	0	23905983	N.D.	6.004 #
8)	B Heptachlo...	4.917f	5.772	3559700	9158616	0.373	2.723 #
10)	B gamma-Chl...	5.212	0.000	7386069	0	0.748	N.D. #
11)	B alpha-Chl...	5.212	0.000	7386069	0	0.769	N.D. #
15)	B Endosulfa...	6.078	0.000	11593037	0	1.333	N.D. #
23)	Chlordane-1	4.137	4.952	28285554	23905983	89.345	191.348 #
24)	Chlordane-2	4.666	0.000	7366334	0	21.071	N.D. #
25)	Chlordane-3	5.212	0.000	7386069	0	6.762	N.D. #
26)	Chlordane-4	5.212	0.000	7386069	0	7.391	N.D. #
27)	Chlordane-5	6.078	0.000	11593037	0	35.745	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
Data File : PL039736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2018 19:11
Operator : AJ\SJ
Sample : J4793-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:12:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

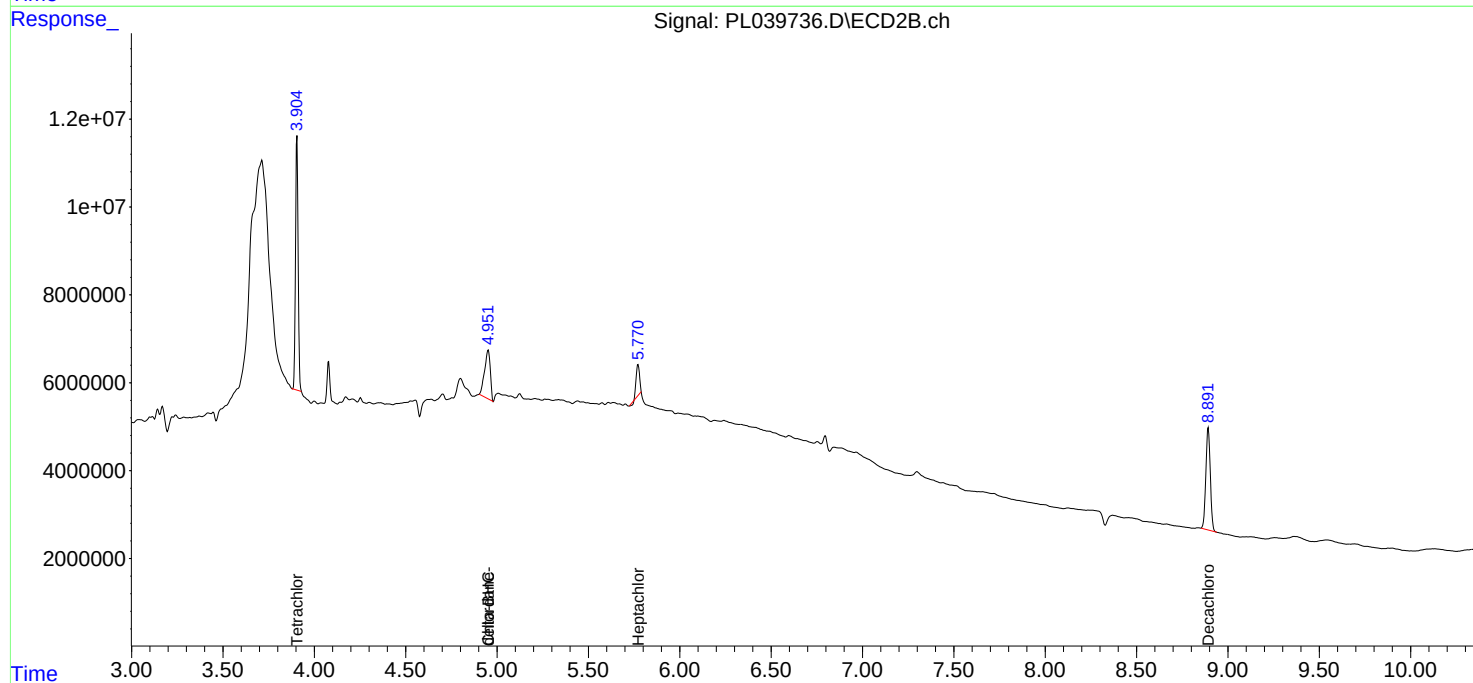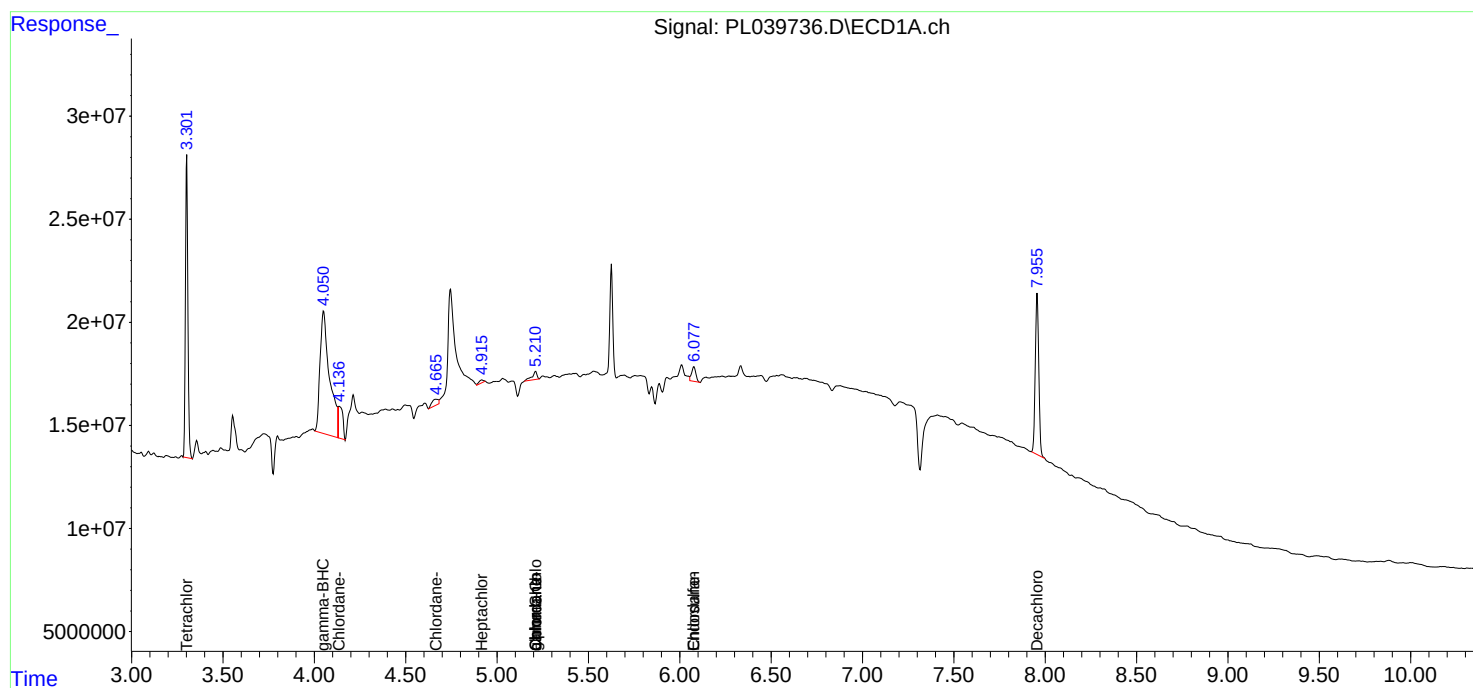


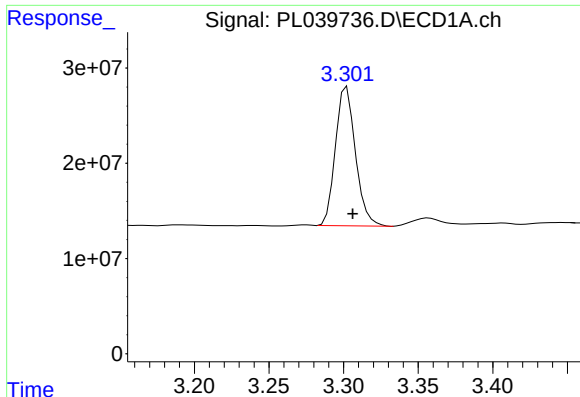

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: -0.004 min
Response: 136829404
Conc: 19.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

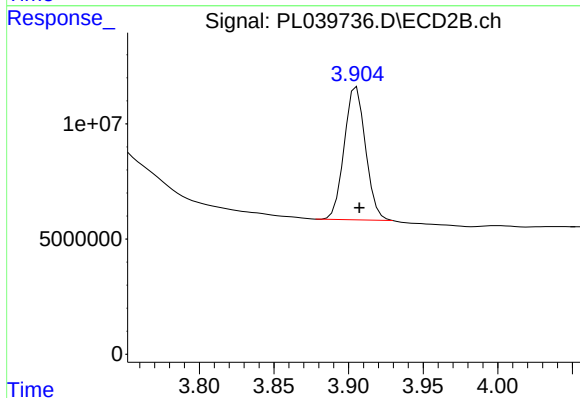


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 57451113
Conc: 21.43 ng/ml

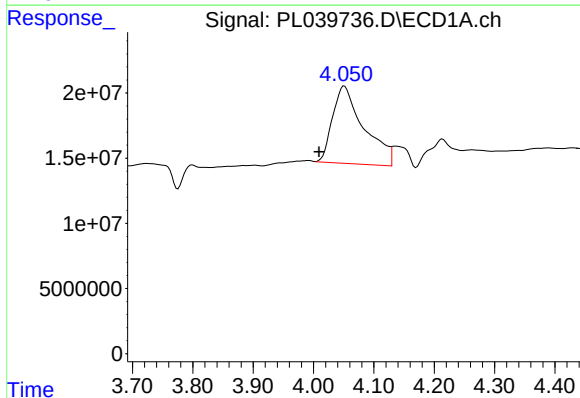


#3 gamma-BHC (Lindane)

R.T.: 4.051 min
Delta R.T.: 0.042 min
Response: 214685204
Conc: 20.24 ng/ml

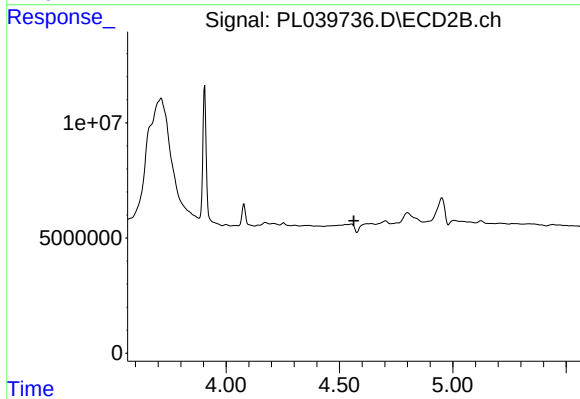

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

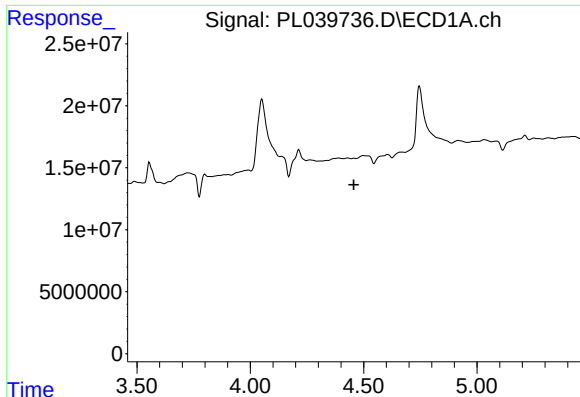

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

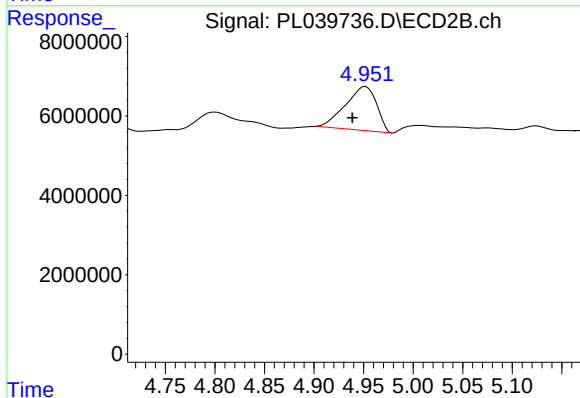


#7 delta-BHC

R.T.: 4.952 min
Delta R.T.: 0.013 min
Response: 23905983
Conc: 6.00 ng/ml

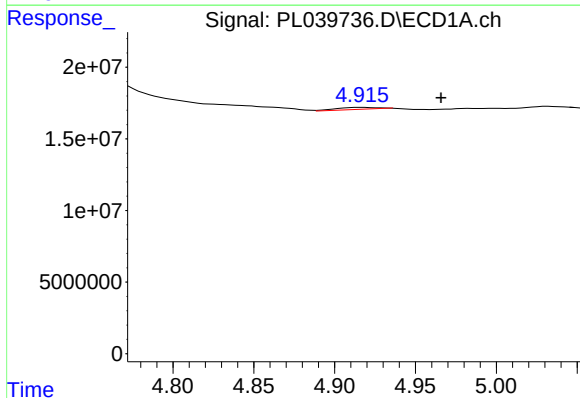


#8 Heptachlor epoxide

R.T.: 4.917 min
Delta R.T.: -0.049 min
Response: 3559700
Conc: 0.37 ng/ml

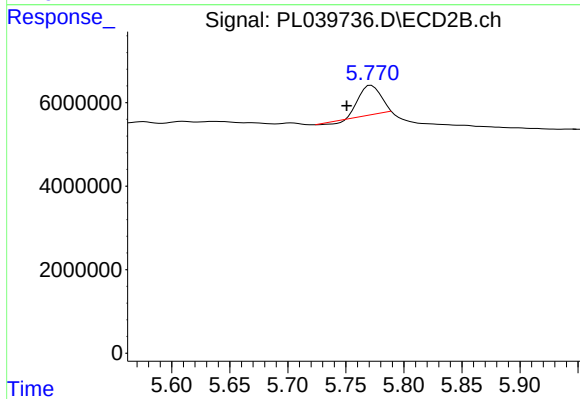

#8 Heptachlor epoxide


R.T.: 5.772 min
Delta R.T.: 0.021 min
Response: 9158616
Conc: 2.72 ng/ml

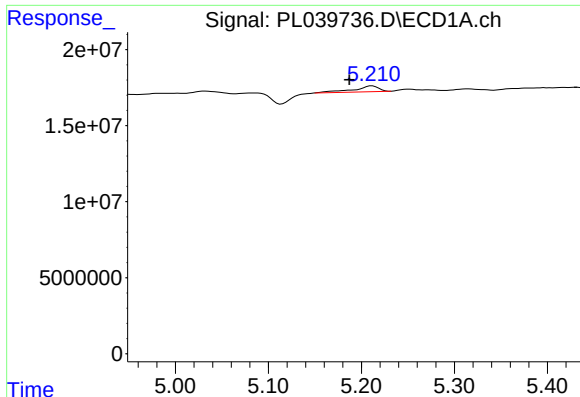

#10 gamma-Chlordane


R.T.: 5.212 min
Delta R.T.: 0.024 min
Response: 7386069
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

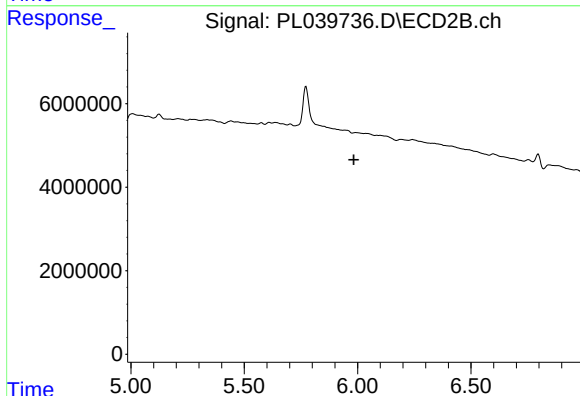


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

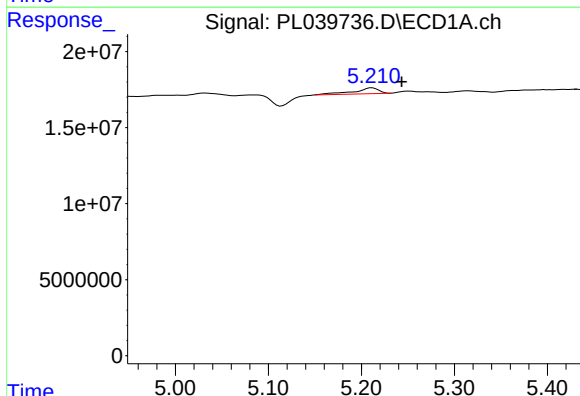


#11 alpha-Chlordane

R.T.: 5.212 min
Delta R.T.: -0.032 min
Response: 7386069
Conc: 0.77 ng/ml

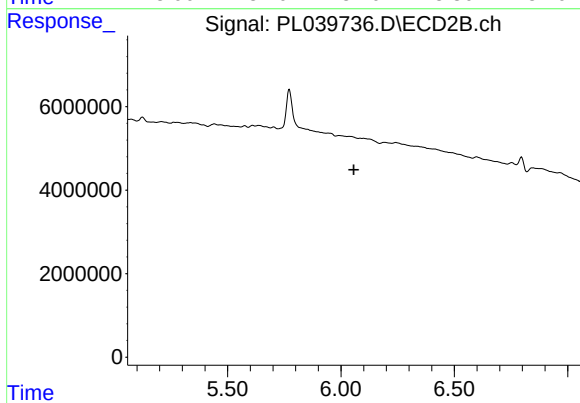

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

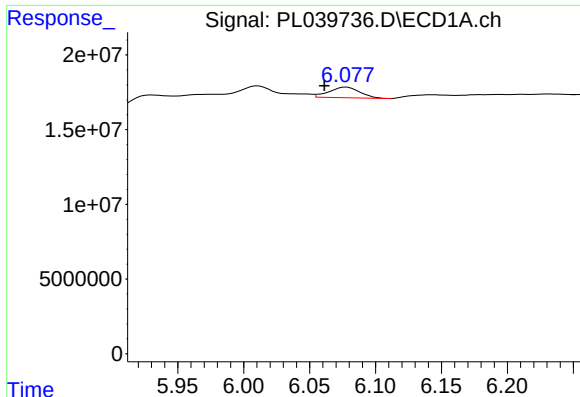

#15 Endosulfan II


R.T.: 6.078 min
Delta R.T.: 0.017 min
Response: 11593037
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

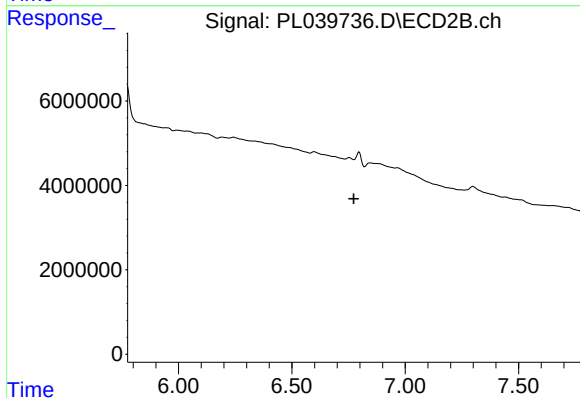


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

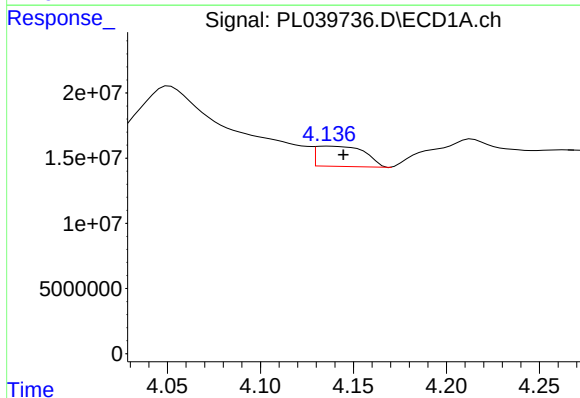


#23 Chlordane-1

R.T.: 4.137 min
Delta R.T.: -0.008 min
Response: 28285554
Conc: 89.35 ng/ml

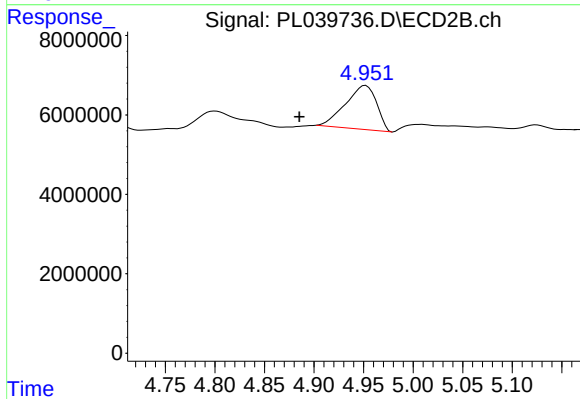

#23 Chlordane-1


R.T.: 4.952 min
Delta R.T.: 0.067 min
Response: 23905983
Conc: 191.35 ng/ml

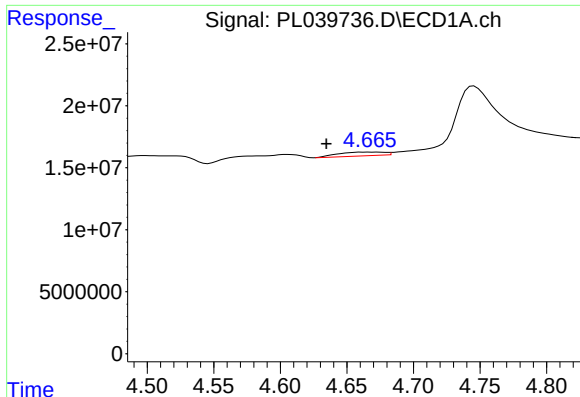

#24 Chlordane-2


R.T.: 4.666 min
Delta R.T.: 0.032 min
Response: 7366334
Conc: 21.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

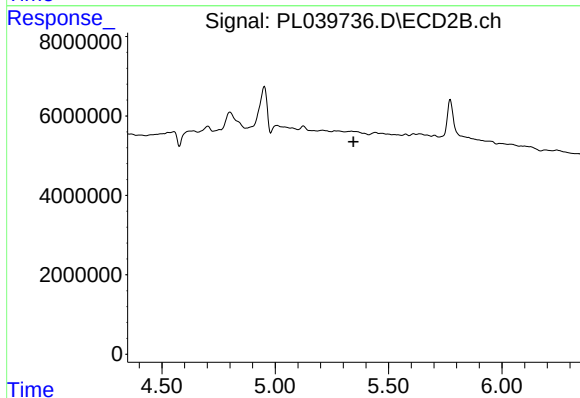


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

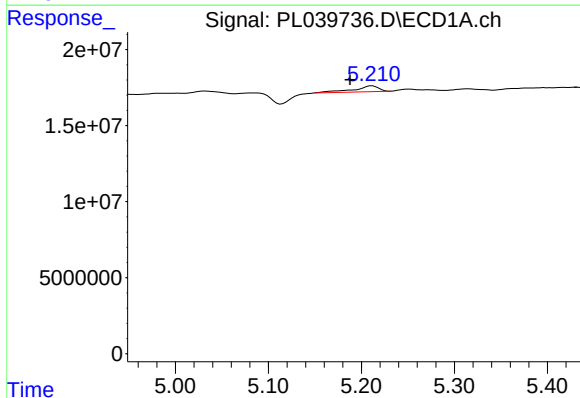


#25 Chlordane-3

R.T.: 5.212 min
Delta R.T.: 0.024 min
Response: 7386069
Conc: 6.76 ng/ml

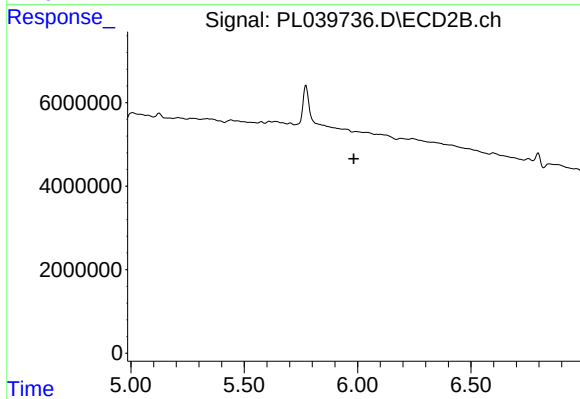

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

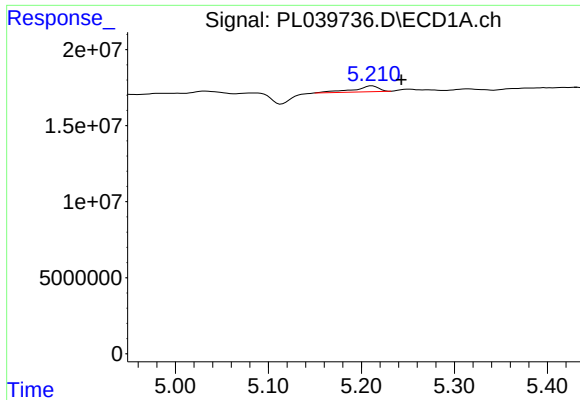

#26 Chlordane-4


R.T.: 5.212 min
Delta R.T.: -0.031 min
Response: 7386069
Conc: 7.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

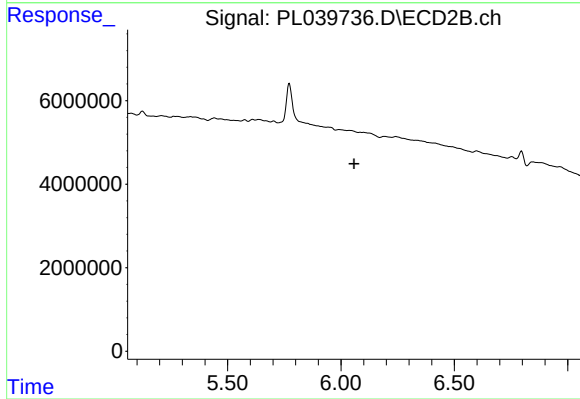


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

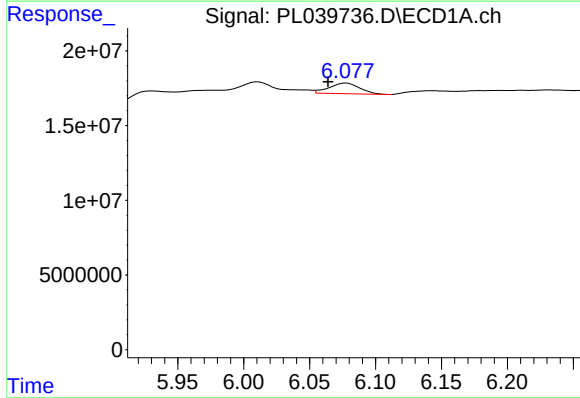


#27 Chlordane-5

R.T.: 6.078 min
Delta R.T.: 0.014 min
Response: 11593037
Conc: 35.74 ng/ml

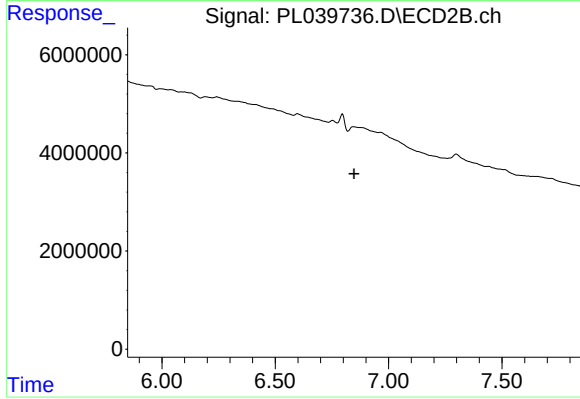

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

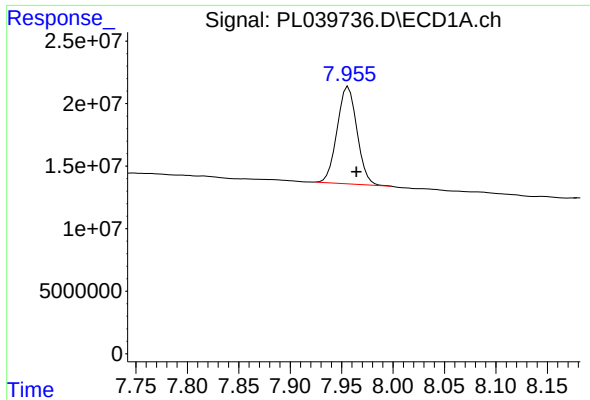

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.008 min
Response: 104060661
Conc: 14.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

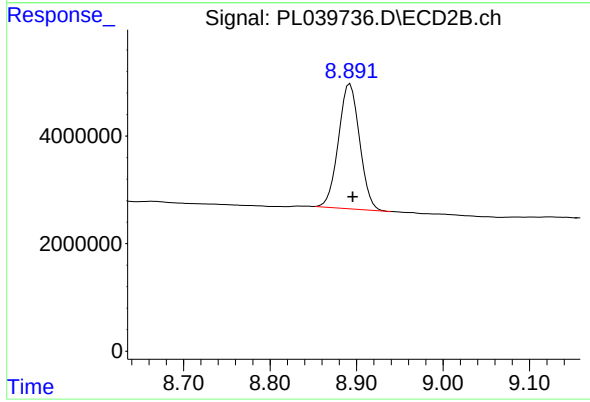

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 39156556
Conc: 16.87 ng/ml