

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
 Data File : PL039737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2018 19:26
 Operator : AJ\SJ
 Sample : J4801-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:13:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.906	131.4E6	57876475	18.801	21.588
28)	SA Decachlor...	7.957	8.893	137.4E6	51692236	19.563	22.275
Target Compounds							
2)	A alpha-BHC	3.689f	4.254f	917601	7091295	0.078	1.684 #
3)	MA gamma-BHC...	4.051f	0.000	104.7E6	0	9.870	N.D. #
7)	B delta-BHC	0.000	4.952	0	14855030	N.D.	3.731 #
8)	B Heptachlo...	4.926f	5.772	3008774	5850060	0.315	1.740 #
15)	B Endosulfa...	6.010f	0.000	7957476	0	0.915	N.D. #
20)	A Methoxychlor	6.696	0.000	7335714	0	1.793	N.D. #
23)	Chlordane-1	4.136	4.952	6421466	14855030	20.283	118.902 #
24)	Chlordane-2	4.677	0.000	18852080	0	53.926	N.D. #
27)	Chlordane-5	6.010	0.000	7957476	0	24.535	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
Data File : PL039737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2018 19:26
Operator : AJ\SJ
Sample : J4801-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:13:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

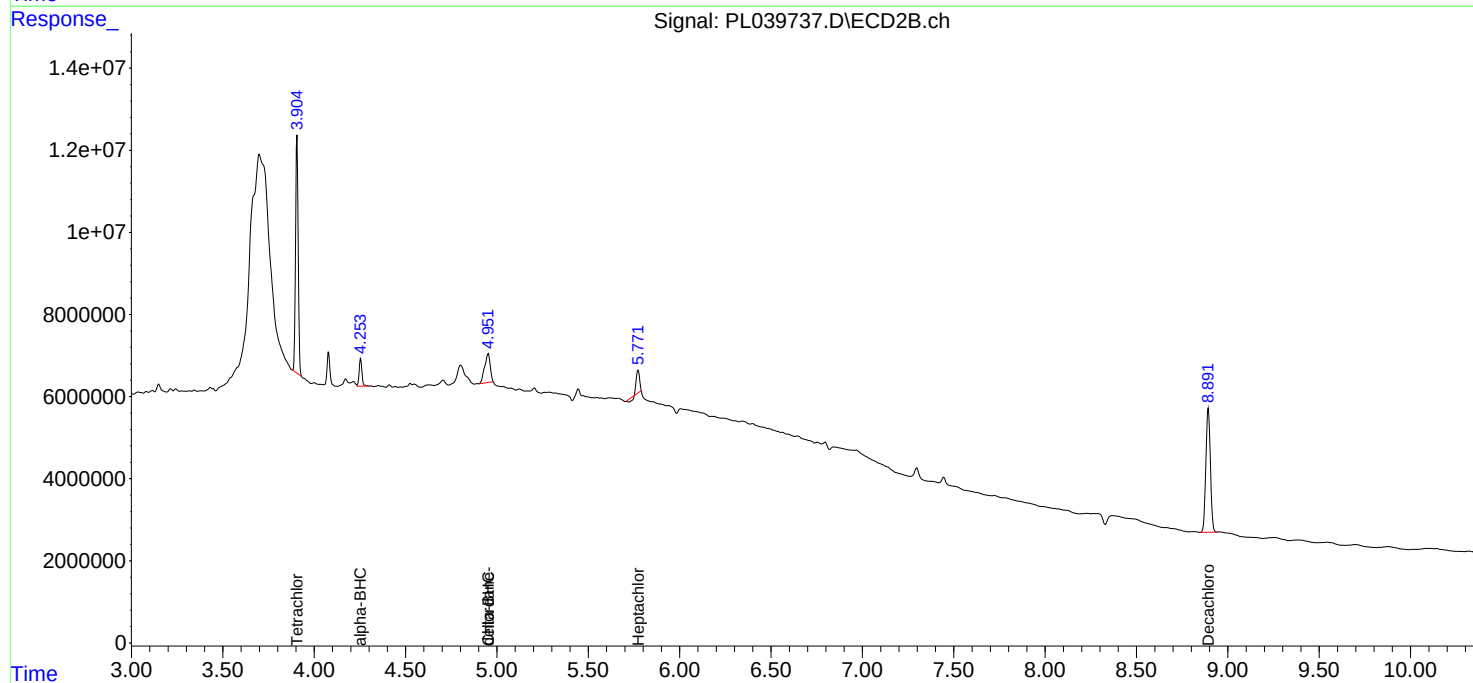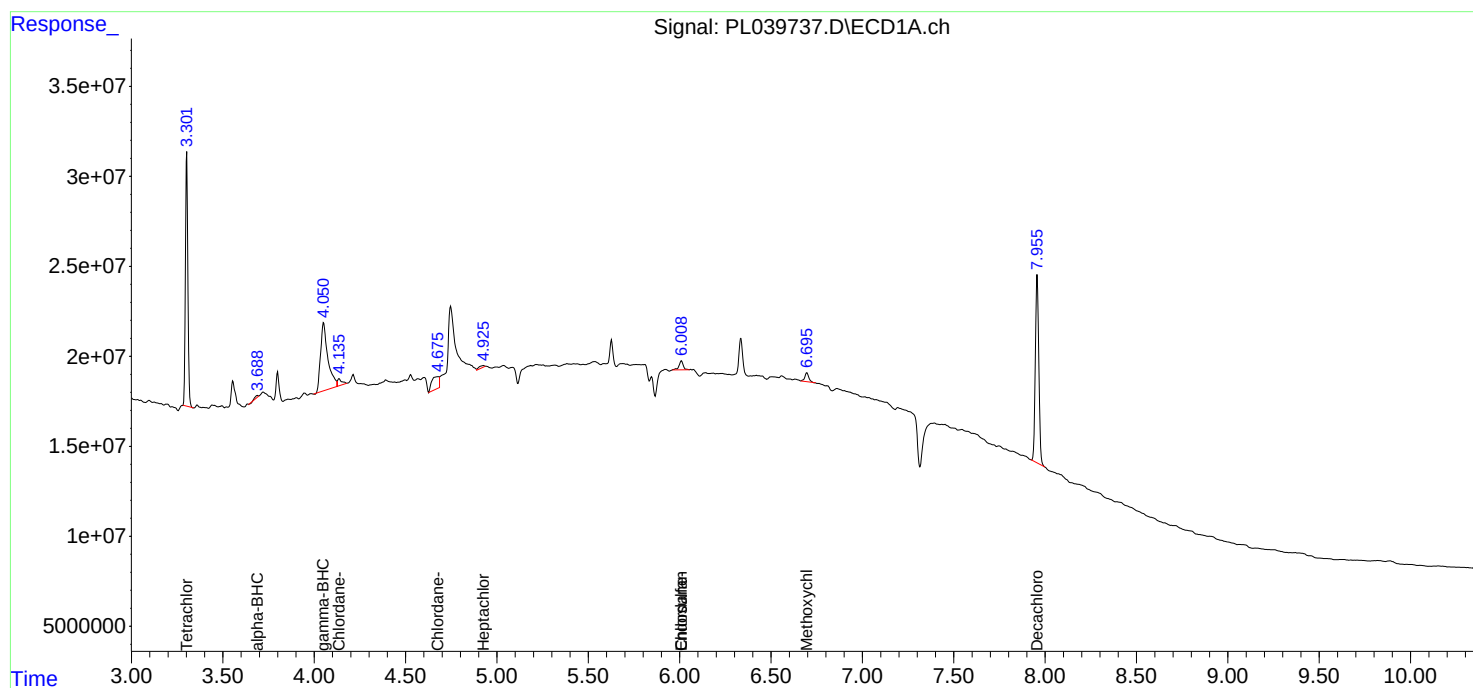


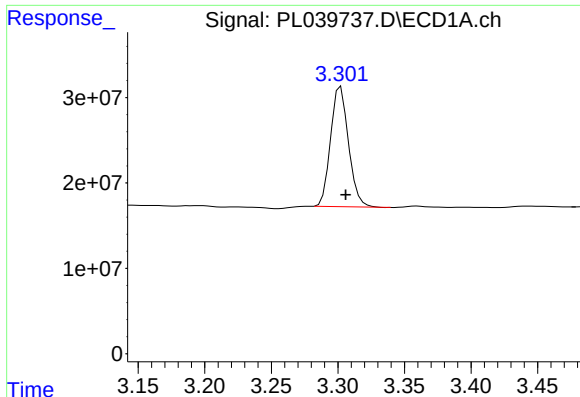

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: -0.004 min
Response: 131429382
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

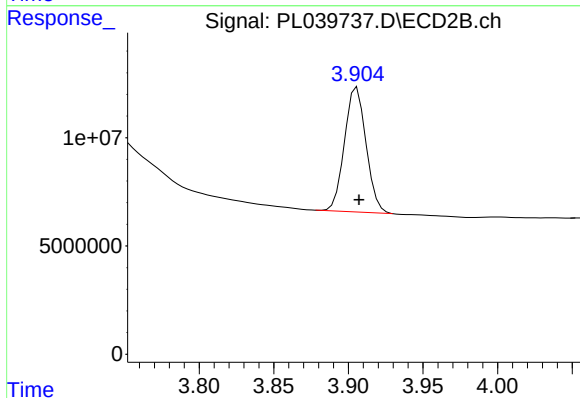


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 57876475
Conc: 21.59 ng/ml

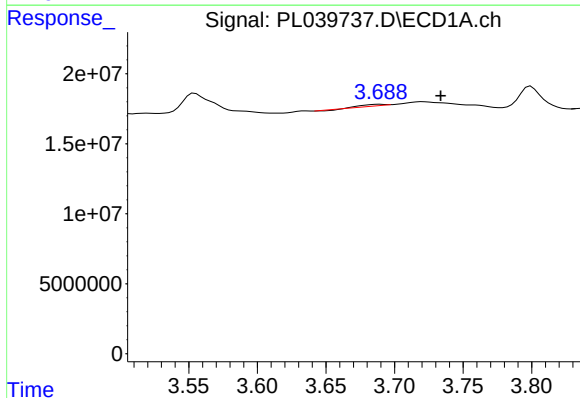


#2 alpha-BHC

R.T.: 3.689 min
Delta R.T.: -0.045 min
Response: 917601
Conc: 0.08 ng/ml

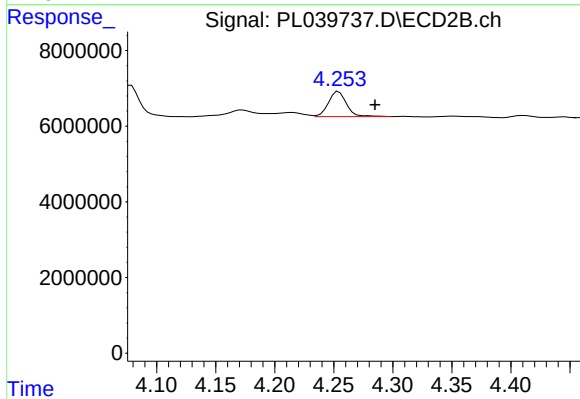

#2 alpha-BHC


R.T.: 4.254 min
Delta R.T.: -0.031 min
Response: 7091295
Conc: 1.68 ng/ml

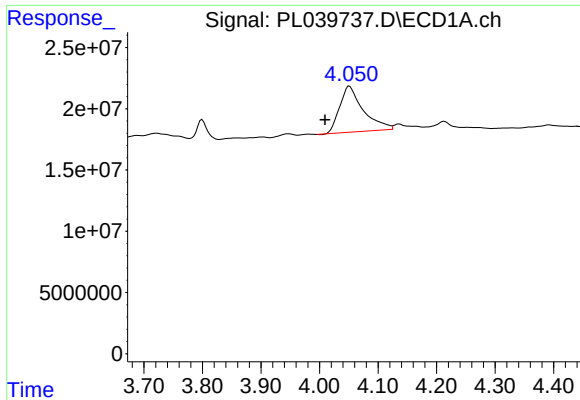

#3 gamma-BHC (Lindane)


R.T.: 4.051 min
Delta R.T.: 0.042 min
Response: 104682606
Conc: 9.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

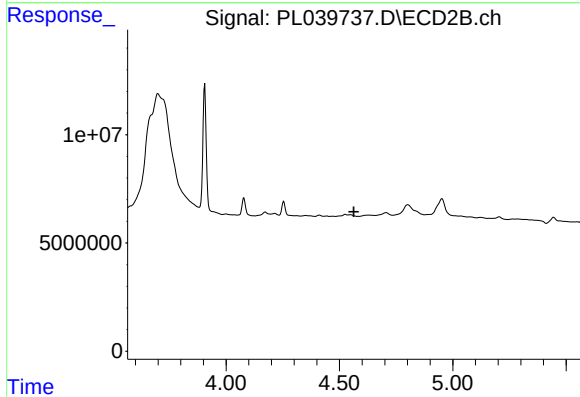


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

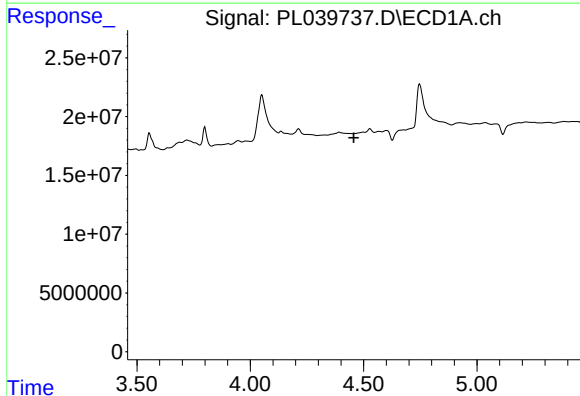


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

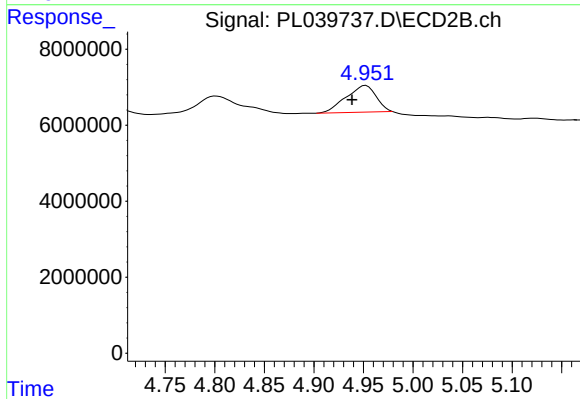

#7 delta-BHC


R.T.: 4.952 min
Delta R.T.: 0.014 min
Response: 14855030
Conc: 3.73 ng/ml

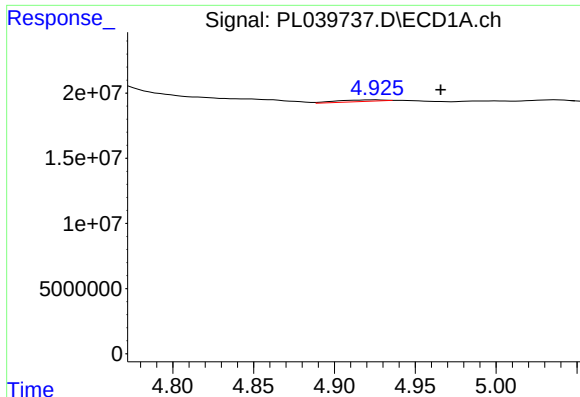

#8 Heptachlor epoxide


R.T.: 4.926 min
Delta R.T.: -0.040 min
Response: 3008774
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

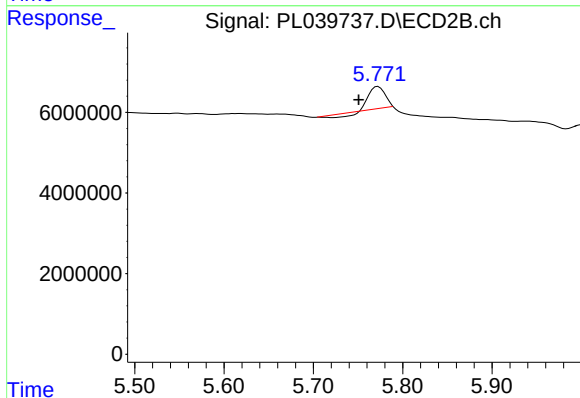


#8 Heptachlor epoxide

R.T.: 5.772 min
Delta R.T.: 0.022 min
Response: 5850060
Conc: 1.74 ng/ml

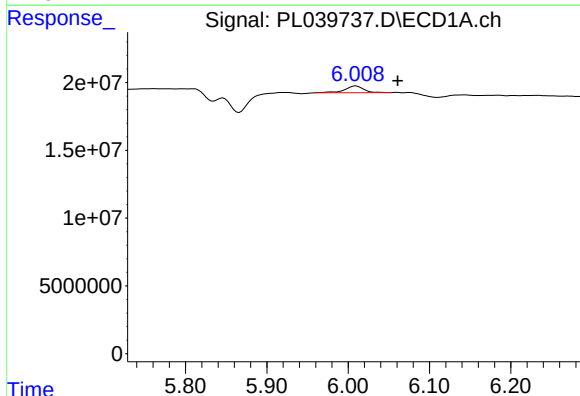


#15 Endosulfan II

R.T.: 6.010 min
Delta R.T.: -0.051 min
Response: 7957476
Conc: 0.92 ng/ml

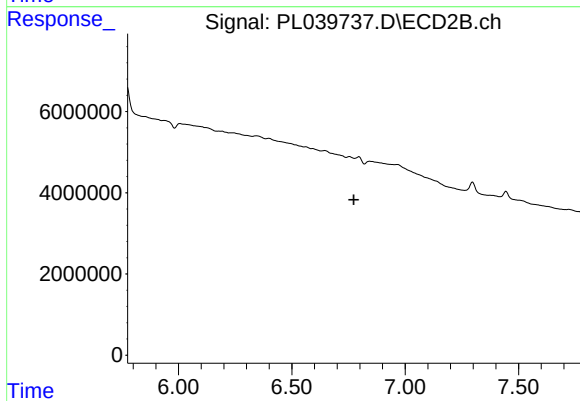

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.773 min
Response: 0
Conc: N.D.

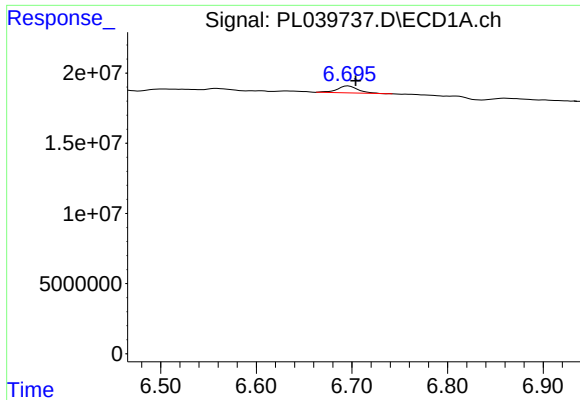

#20 Methoxychlor


R.T.: 6.696 min
Delta R.T.: -0.008 min
Response: 7335714
Conc: 1.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

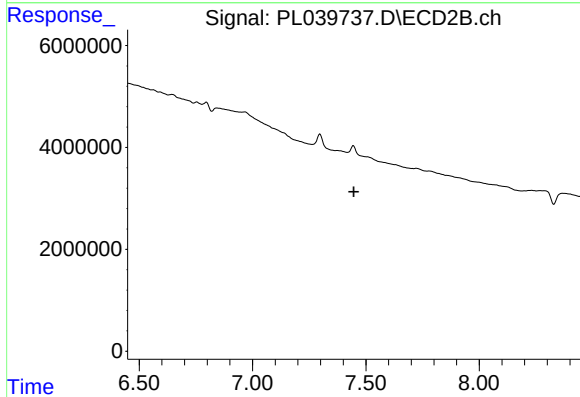


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

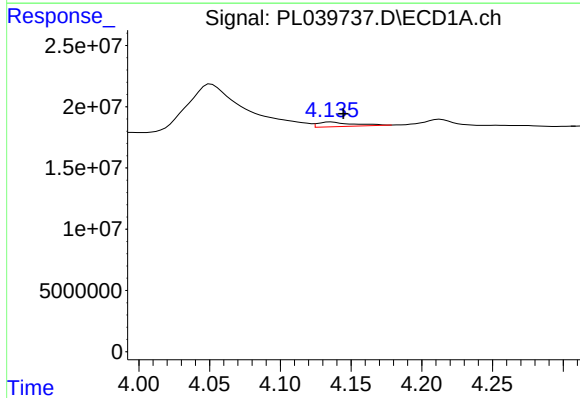


#23 Chlordane-1

R.T.: 4.136 min
Delta R.T.: -0.008 min
Response: 6421466
Conc: 20.28 ng/ml

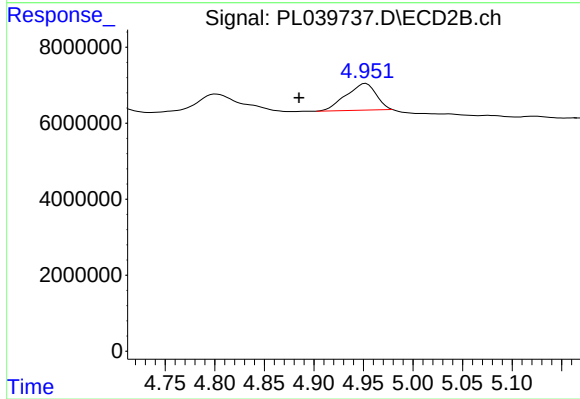

#23 Chlordane-1


R.T.: 4.952 min
Delta R.T.: 0.067 min
Response: 14855030
Conc: 118.90 ng/ml

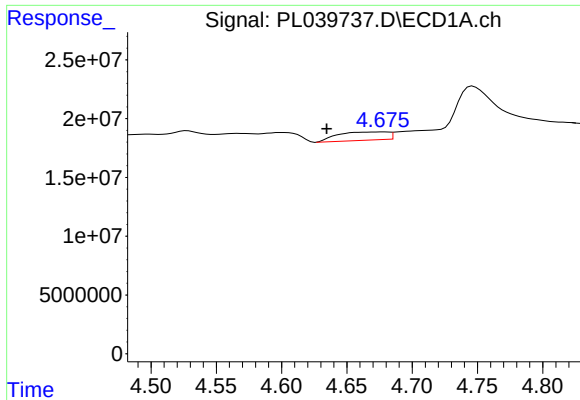

#24 Chlordane-2


R.T.: 4.677 min
Delta R.T.: 0.043 min
Response: 18852080
Conc: 53.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

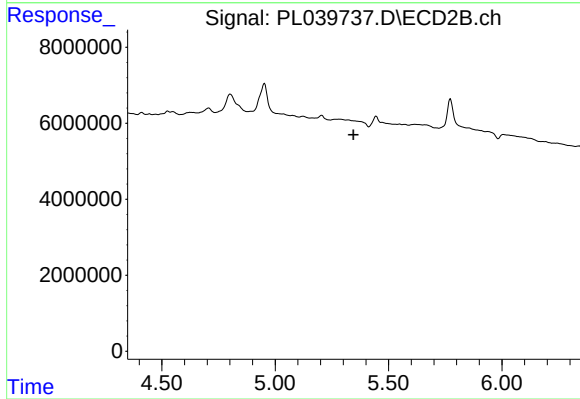


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

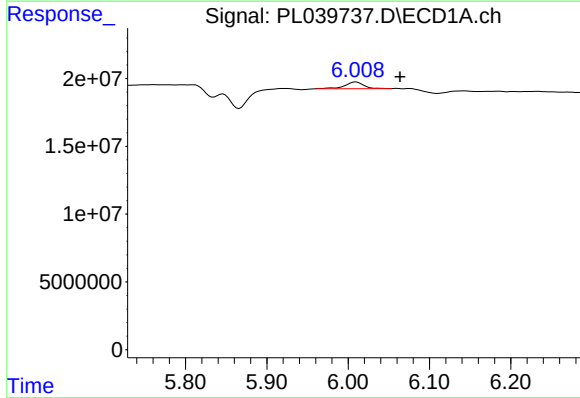


#27 Chlordane-5

R.T.: 6.010 min
Delta R.T.: -0.054 min
Response: 7957476
Conc: 24.54 ng/ml

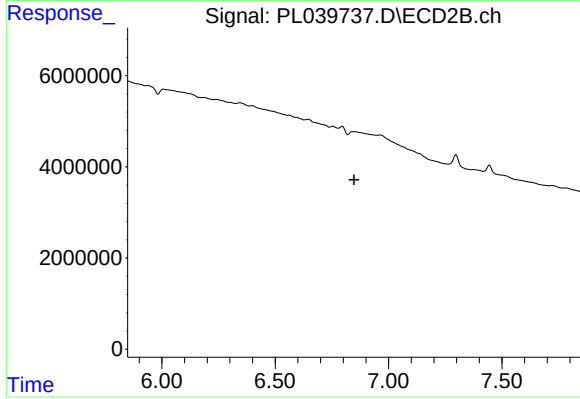

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

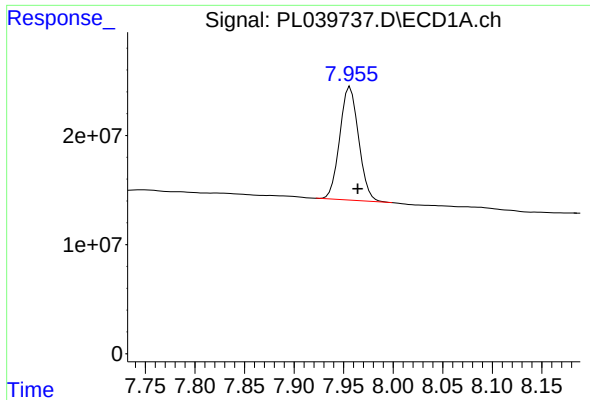

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.008 min
Response: 137398211
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

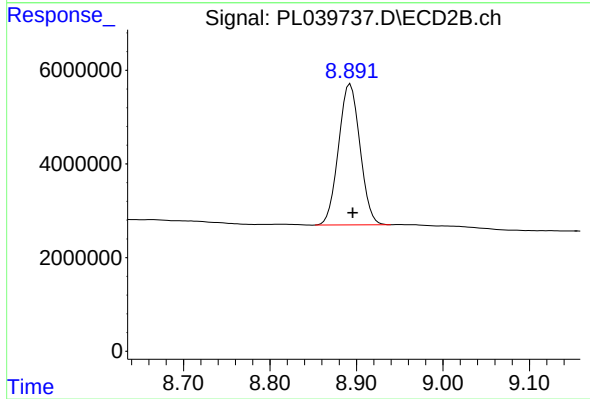

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.003 min
Response: 51692236
Conc: 22.28 ng/ml