

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
 Data File : PL039738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2018 19:40
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 04:13:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.906	128.1E6	53615192	18.322	19.999
28)	SA Decachlor...	7.956	8.892	130.8E6	48676887	18.628	20.976
Target Compounds							
3)	MA gamma-BHC...	4.052f	0.000	189.4E6	0	17.859	N.D. #
7)	B delta-BHC	0.000	4.950	0	17067157	N.D.	4.287 #
8)	B Heptachlo...	4.918f	5.772	3385050	8619485	0.354	2.563 #
15)	B Endosulfa...	6.009f	0.000	6925593	0	0.796	N.D. #
23)	Chlordane-1	4.170	4.950	7539775	17067157	23.816	136.609 #
27)	Chlordane-5	6.009	0.000	6925593	0	21.354	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090618\
Data File : PL039738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2018 19:40
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 04:13:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

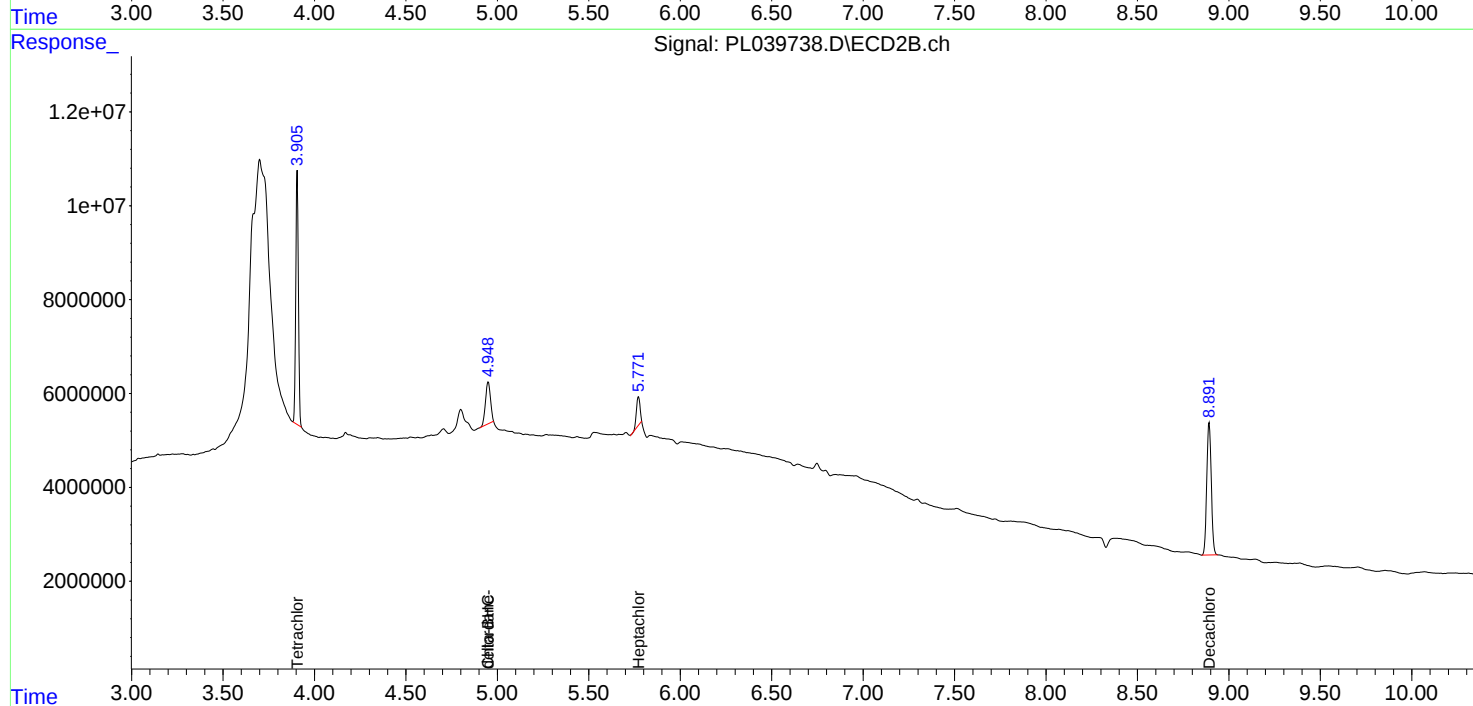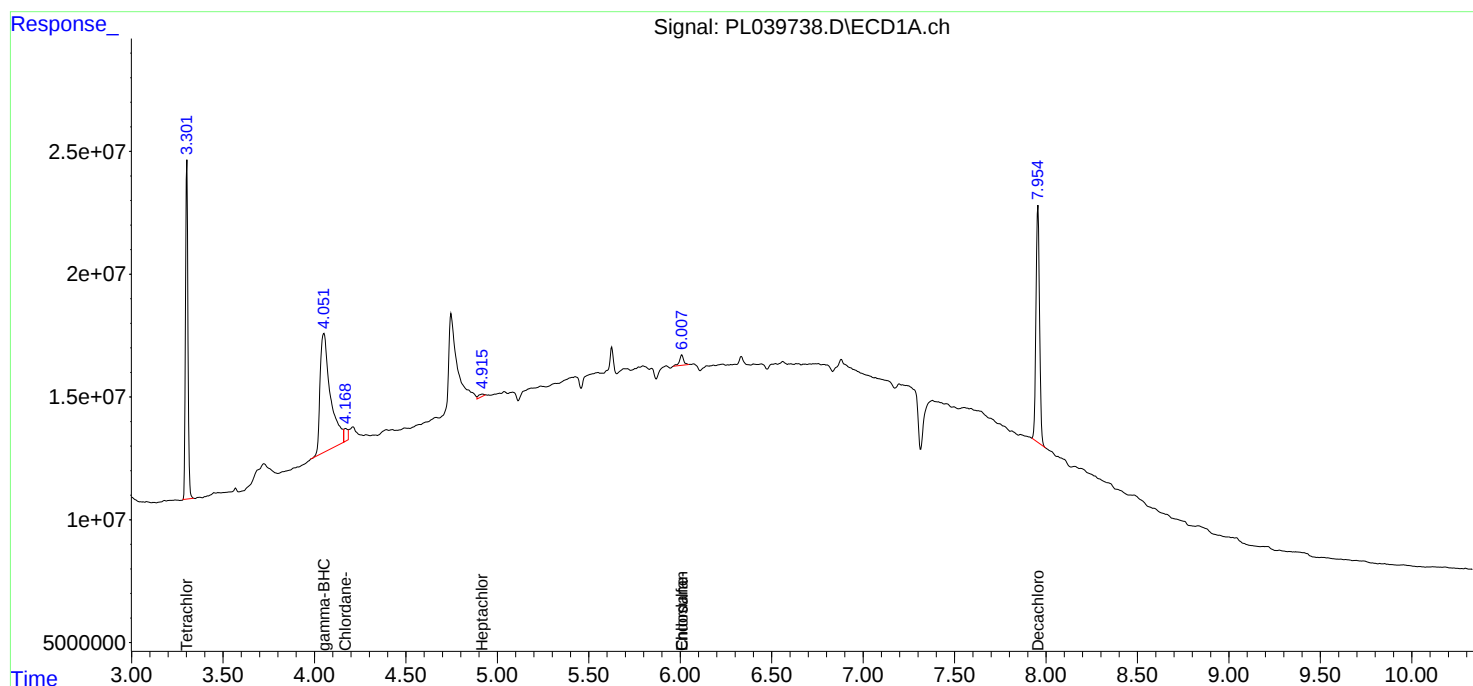


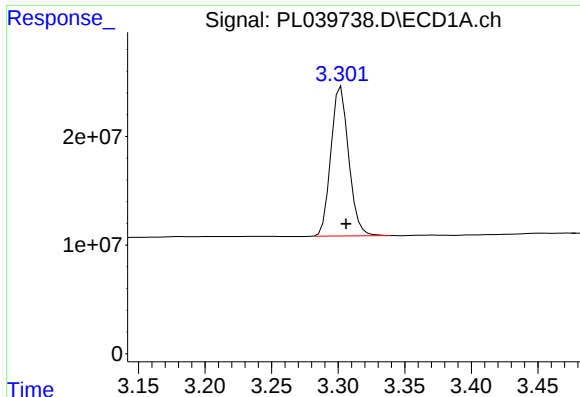

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: -0.004 min
Response: 128081218
Conc: 18.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

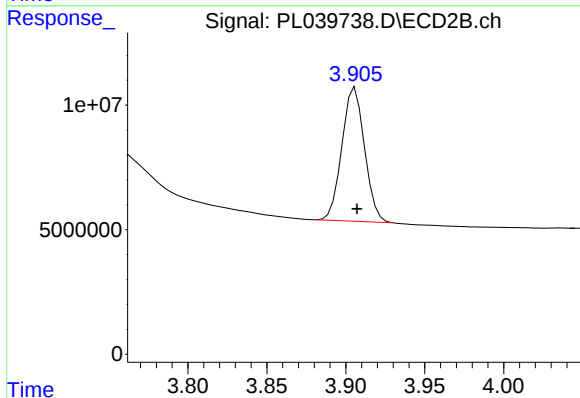


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 53615192
Conc: 20.00 ng/ml

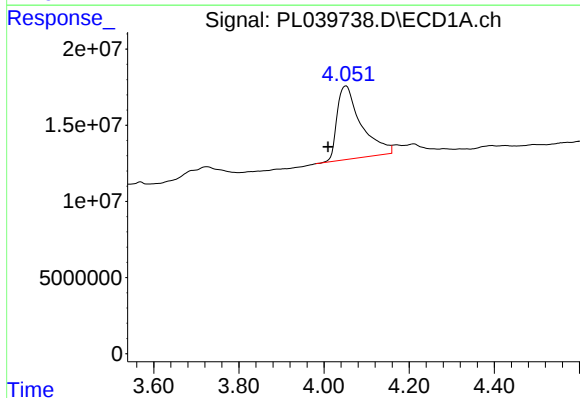


#3 gamma-BHC (Lindane)

R.T.: 4.052 min
Delta R.T.: 0.043 min
Response: 189419058
Conc: 17.86 ng/ml

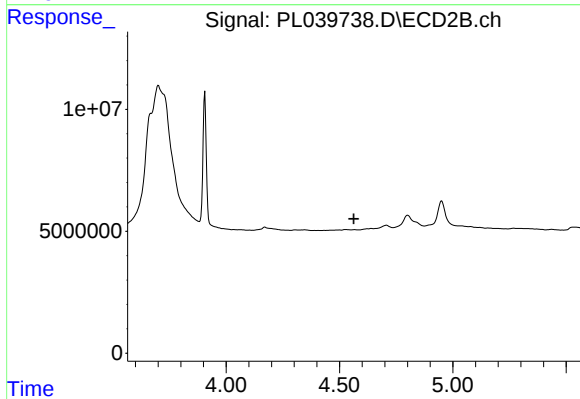

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

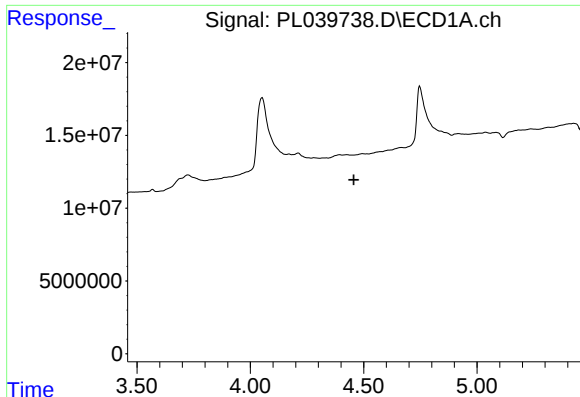

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

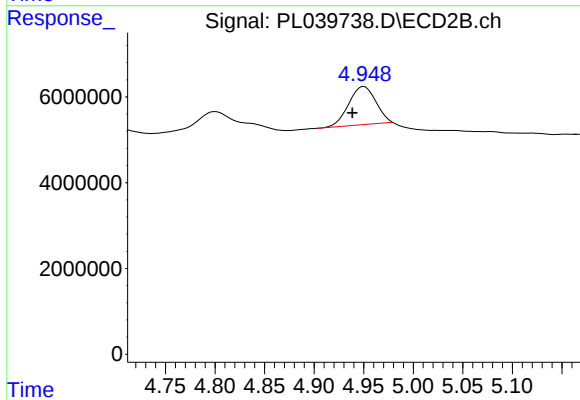


#7 delta-BHC

R.T.: 4.950 min
Delta R.T.: 0.012 min
Response: 17067157
Conc: 4.29 ng/ml

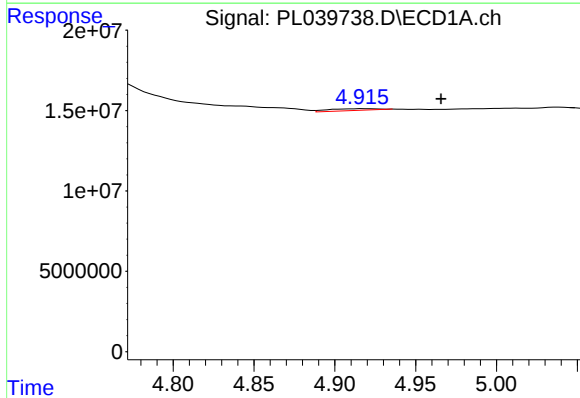


#8 Heptachlor epoxide

R.T.: 4.918 min
Delta R.T.: -0.047 min
Response: 3385050
Conc: 0.35 ng/ml

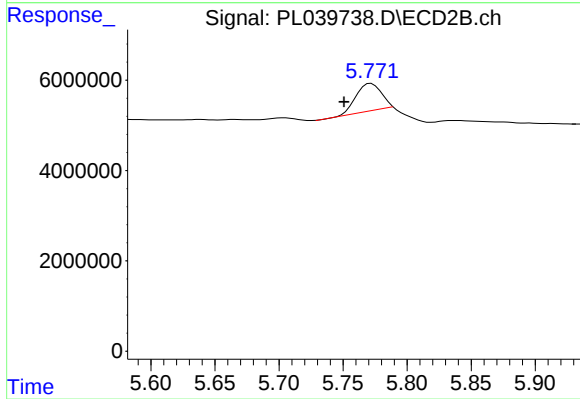

#8 Heptachlor epoxide


R.T.: 5.772 min
Delta R.T.: 0.021 min
Response: 8619485
Conc: 2.56 ng/ml

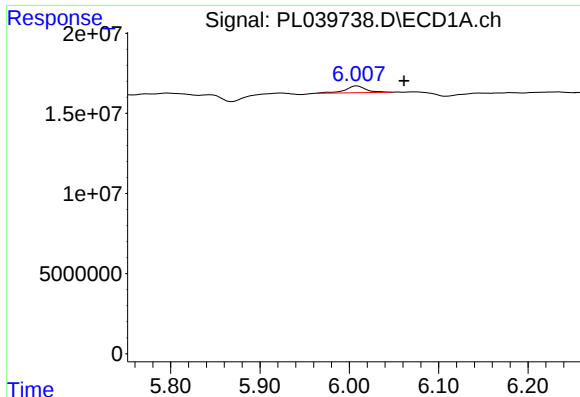

#15 Endosulfan II


R.T.: 6.009 min
Delta R.T.: -0.052 min
Response: 6925593
Conc: 0.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

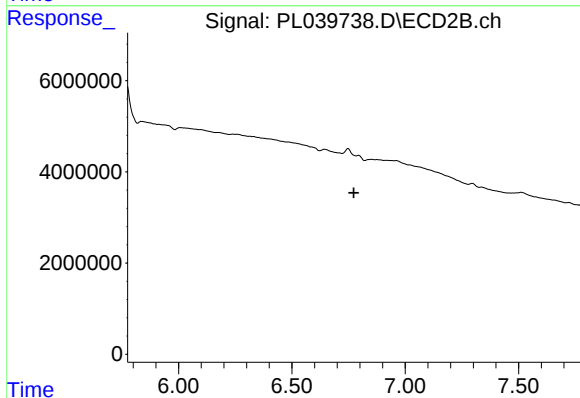


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

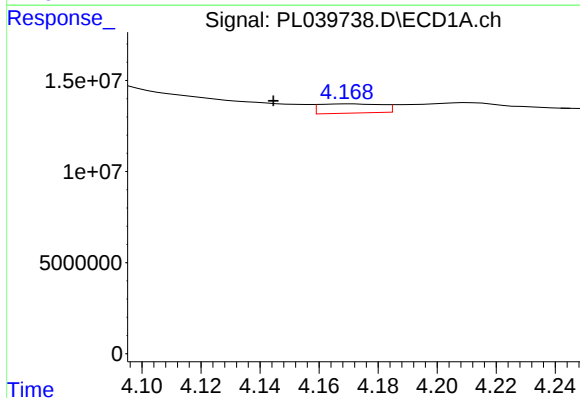


#23 Chlordane-1

R.T.: 4.170 min
Delta R.T.: 0.026 min
Response: 7539775
Conc: 23.82 ng/ml

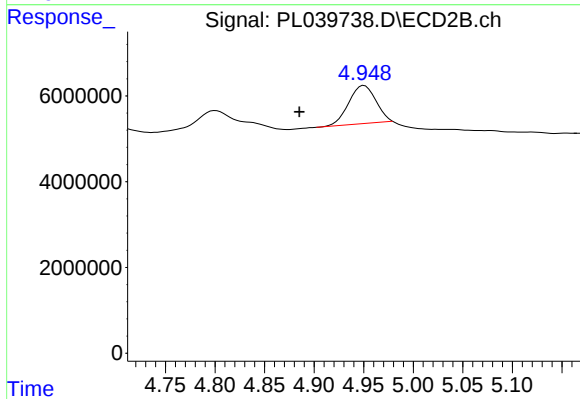

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.065 min
Response: 17067157
Conc: 136.61 ng/ml

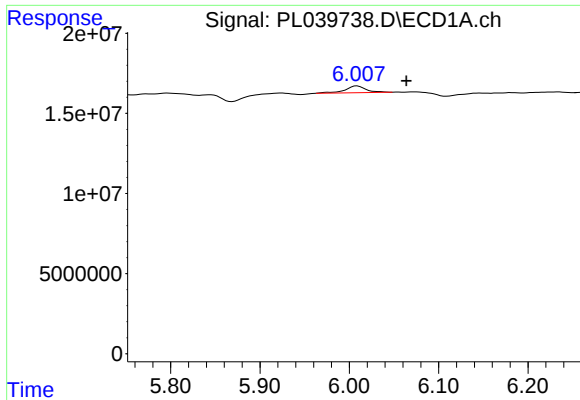

#27 Chlordane-5


R.T.: 6.009 min
Delta R.T.: -0.055 min
Response: 6925593
Conc: 21.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

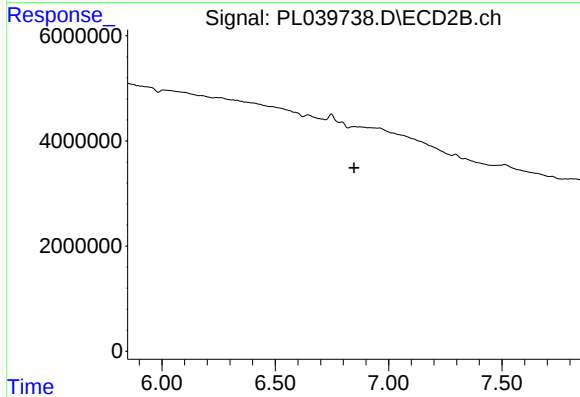


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.848 min
Response: 0
Conc: N.D.

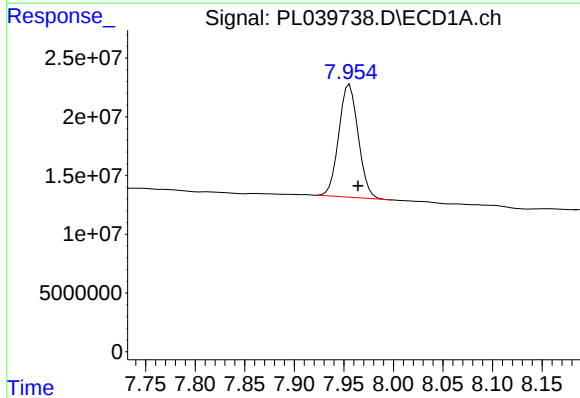

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.009 min
Response: 130829074
Conc: 18.63 ng/ml

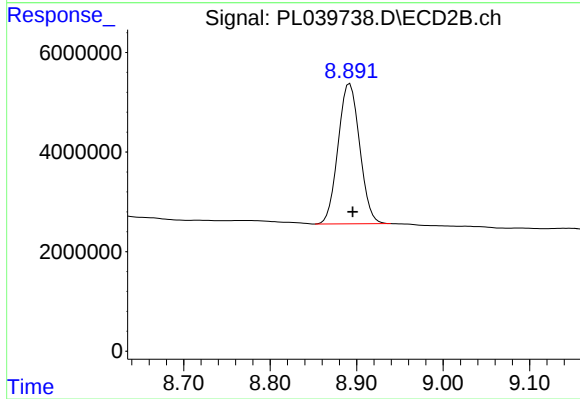

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 48676887
Conc: 20.98 ng/ml