

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
 Data File : PL052244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 09:01
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 22:55:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.924	251.6E6	58977439	29.394	26.994
28)	SA Decachlor...	7.974	8.949	314.8E6	70806839	25.935	23.262
Target Compounds							
8)	B Heptachlo...	0.000	5.784	0	8067863	N.D.	2.391 #
9)	A Endosulfan I	5.324f	0.000	11044073	0	0.822	N.D. #
15)	B Endosulfa...	6.082	0.000	11084674	0	0.797	N.D. #
17)	MA 4,4'-DDT	0.000	7.057f	0	622991	N.D.	0.213 #
18)	B Endrin al...	0.000	6.981f	0	191389	N.D.	0.068 #
19)	B Endosulfa...	0.000	7.175	0	3768857	N.D.	1.220 #
22)	Mirex	0.000	8.086	0	355435	N.D.	0.146 #
27)	Chlordane-5	6.082	6.918f	11084674	203809	22.589	2.067 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
Data File : PL052244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 09:01
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 22:55:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

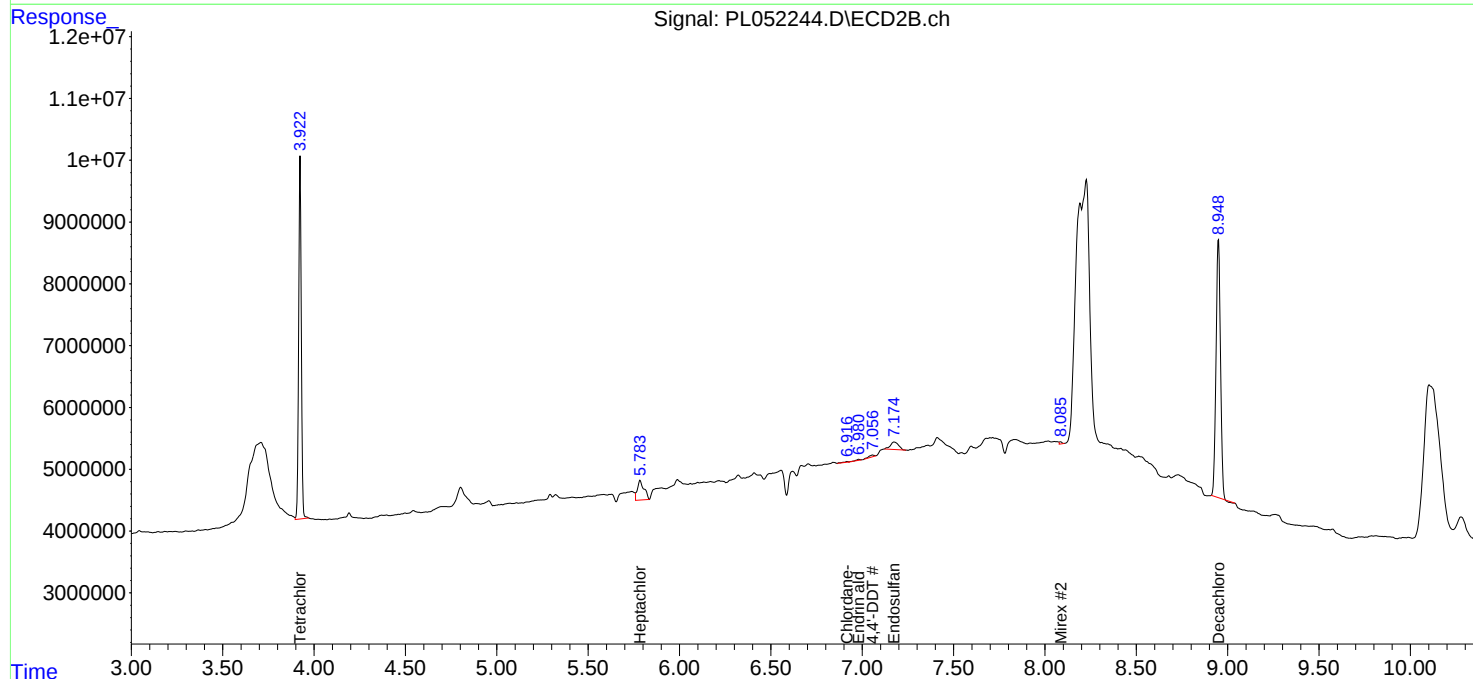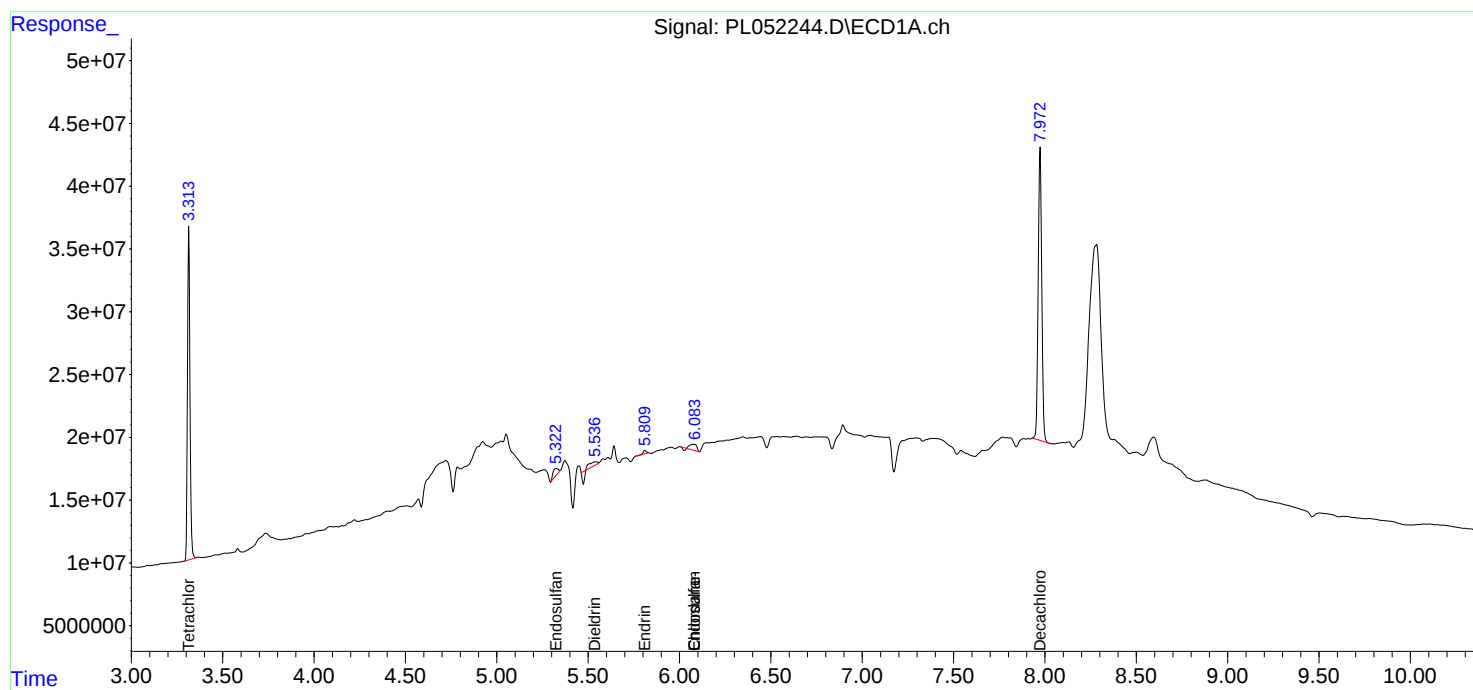


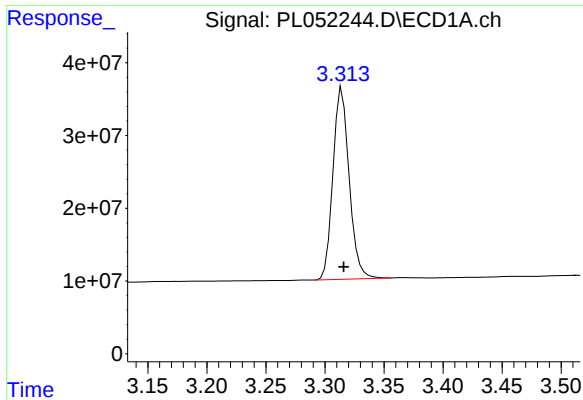

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.001 min
Response: 251575225
Conc: 29.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

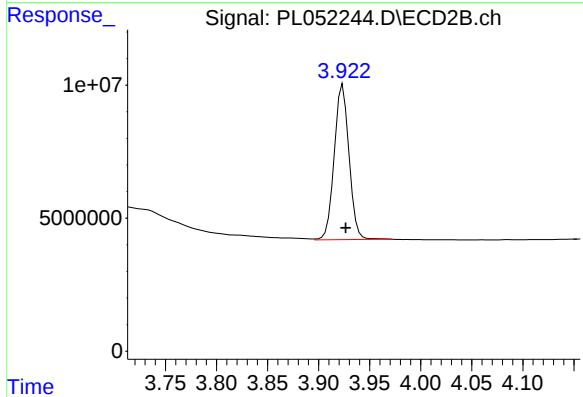


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 58977439
Conc: 26.99 ng/ml

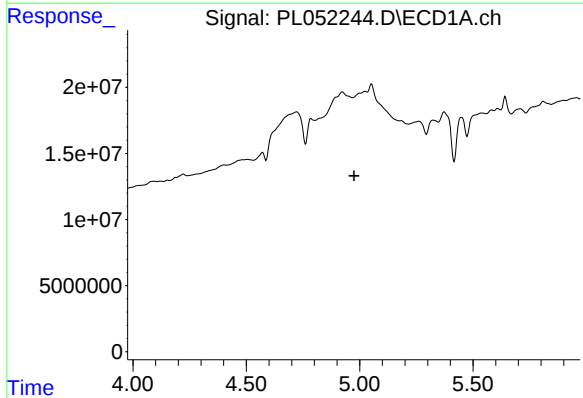


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

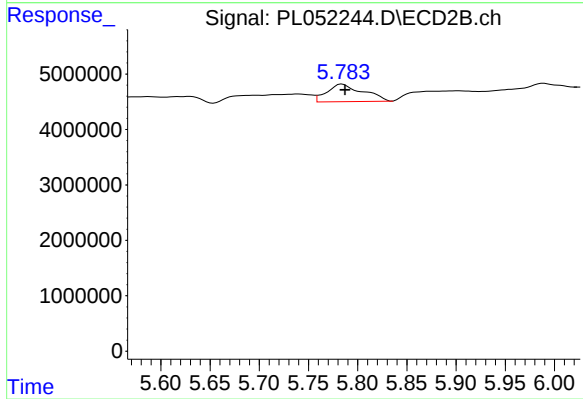

#8 Heptachlor epoxide


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 8067863
Conc: 2.39 ng/ml

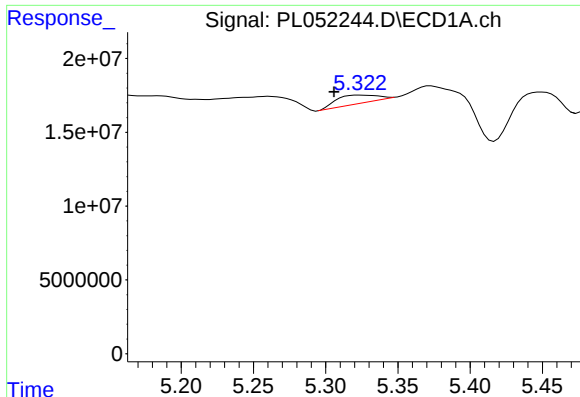

#9 Endosulfan I


R.T.: 5.324 min
Delta R.T.: 0.018 min
Response: 11044073
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

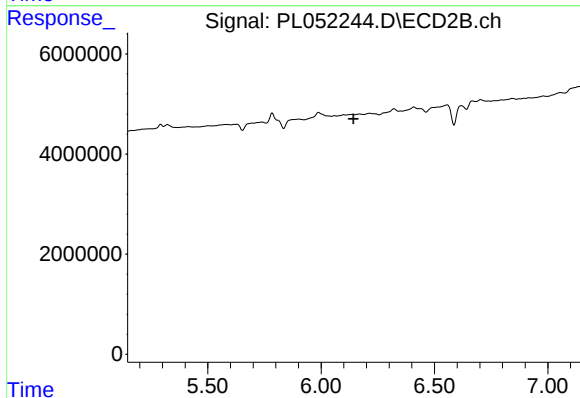


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

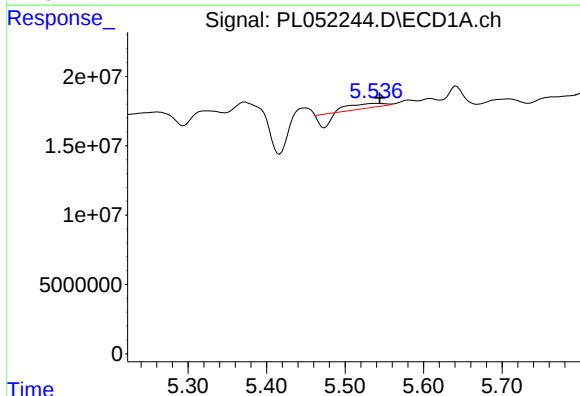


#13 Dieldrin

R.T.: 5.539 min
Delta R.T.: -0.005 min
Response: 1807181
Conc: 0.12 ng/ml

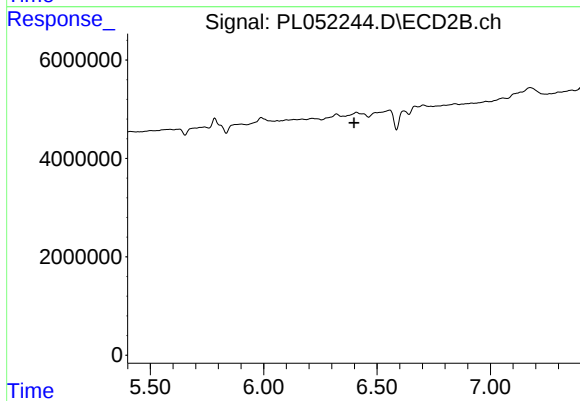

#13 Dieldrin


R.T.: 6.409 min
Delta R.T.: 0.010 min
Response: -985768
Conc: N.D.

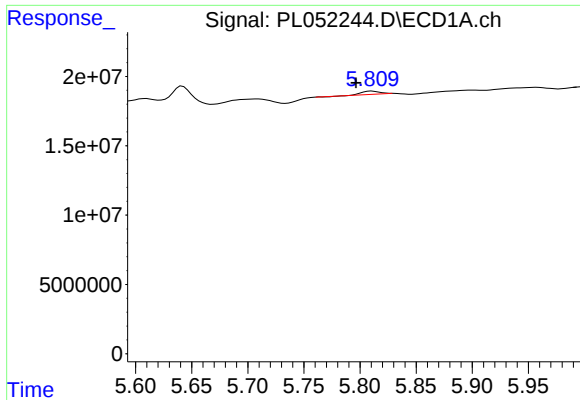

#14 Endrin


R.T.: 5.810 min
Delta R.T.: 0.014 min
Response: 3086531
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

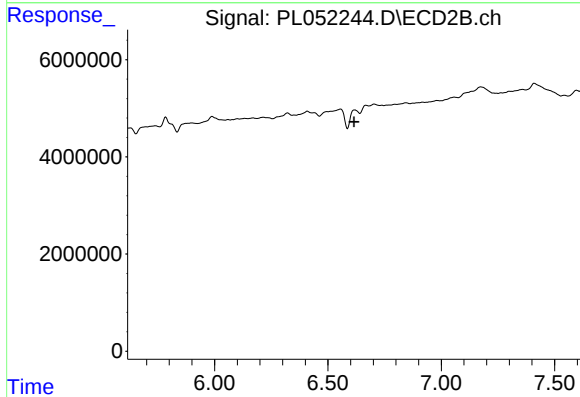


#14 Endrin

R.T.: 6.620 min
Delta R.T.: 0.004 min
Response: -921195
Conc: N.D.

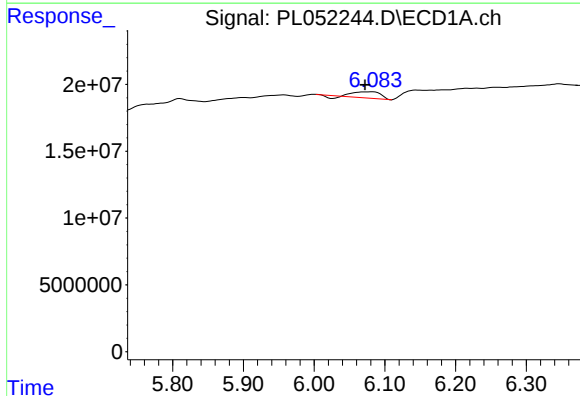


#15 Endosulfan II

R.T.: 6.082 min
Delta R.T.: 0.011 min
Response: 11084674
Conc: 0.80 ng/ml

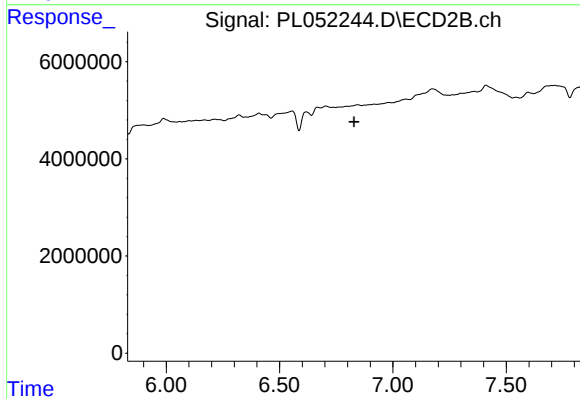

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.829 min
Response: 0
Conc: N.D.

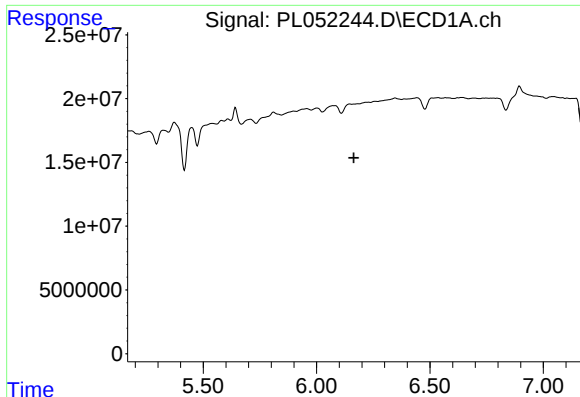

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

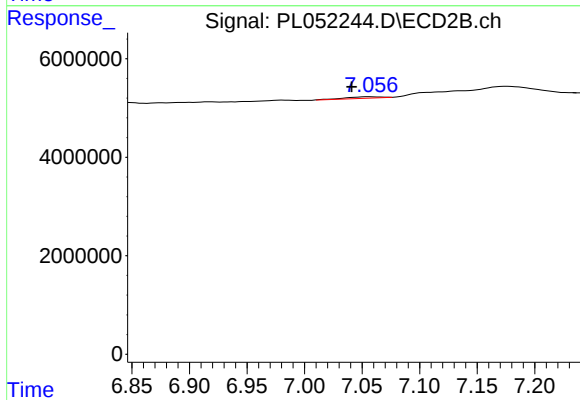


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.016 min
Response: 622991
Conc: 0.21 ng/ml

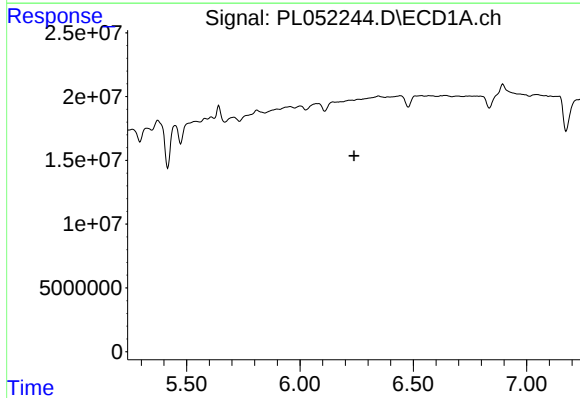


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

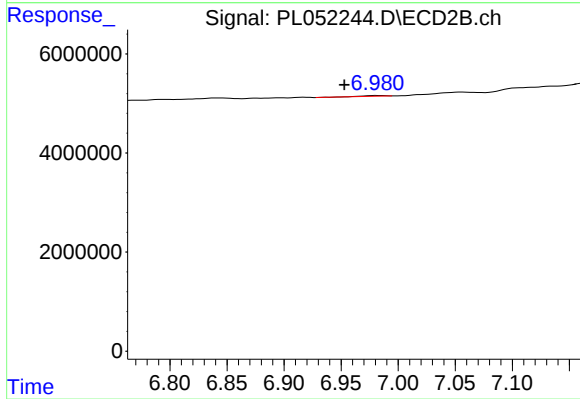

#18 Endrin aldehyde


R.T.: 6.981 min
Delta R.T.: 0.028 min
Response: 191389
Conc: 0.07 ng/ml

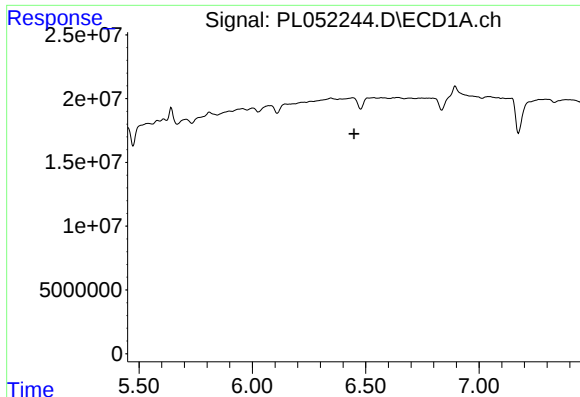

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

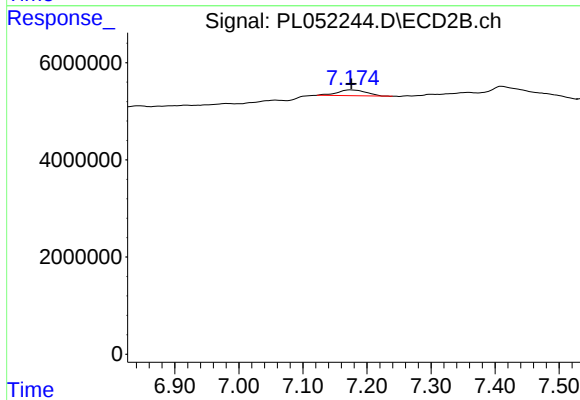


#19 Endosulfan Sulfate

R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 3768857
Conc: 1.22 ng/ml

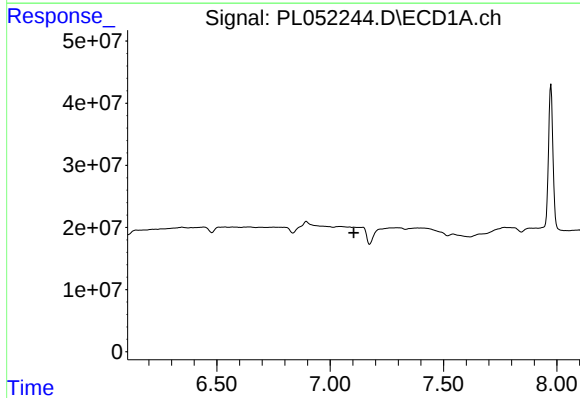


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.104 min
Response: 0
Conc: N.D.

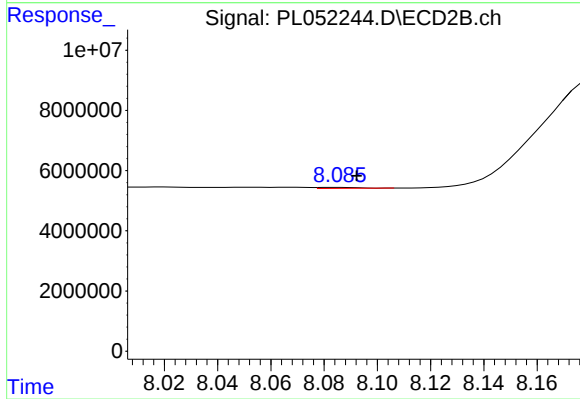

#22 Mirex


R.T.: 8.086 min
Delta R.T.: -0.006 min
Response: 355435
Conc: 0.15 ng/ml

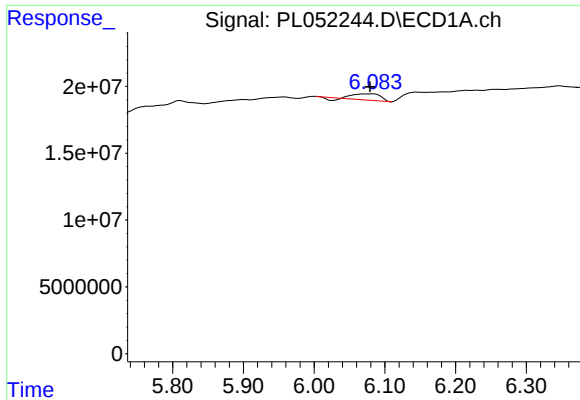

#27 Chlordane-5


R.T.: 6.082 min
Delta R.T.: 0.003 min
Response: 11084674
Conc: 22.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

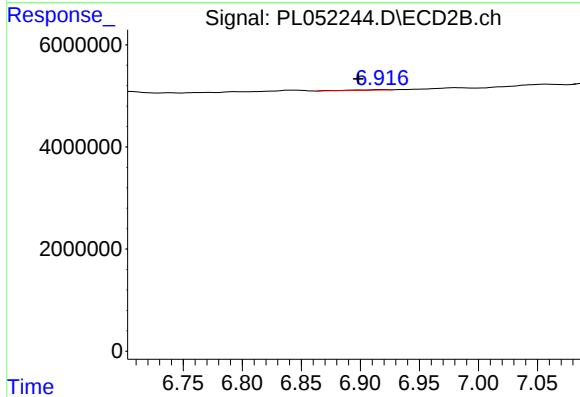


#27 Chlordane-5

R.T.: 6.918 min
Delta R.T.: 0.019 min
Response: 203809
Conc: 2.07 ng/ml

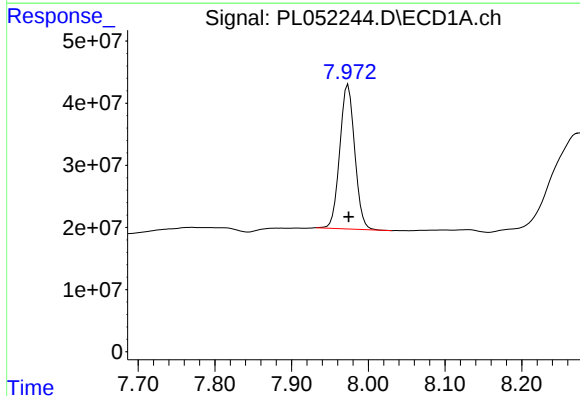

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: 0.000 min
Response: 314792858
Conc: 25.93 ng/ml

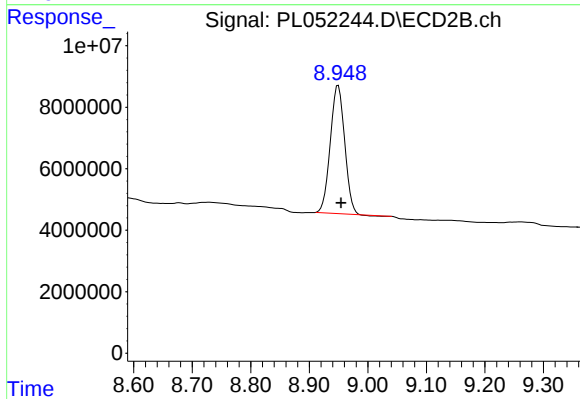

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.005 min
Response: 70806839
Conc: 23.26 ng/ml