

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
 Data File : PL052263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 13:52
 Operator : SG\AJ
 Sample : PB122845BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122845BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:00:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.924	193.9E6	48980418	22.656	22.419
28)	SA Decachlor...	7.980	8.953	283.4E6	61547739	23.348	20.220
Target Compounds							
5)	MB Aldrin	4.567f	0.000	2729880	0	0.189	N.D. #
8)	B Heptachlo...	0.000	5.807f	0	1961388	N.D.	0.581 #
9)	A Endosulfan I	5.332f	0.000	9050295	0	0.673	N.D. #
15)	B Endosulfa...	0.000	6.843	0	4675	N.D.	0.001 #
16)	A 4,4'-DDD	5.951f	0.000	4408615	0	0.360	N.D. #
17)	MA 4,4'-DDT	6.158	7.051	7687978	1118361	0.603	0.382 #
22)	Mirex	0.000	8.111f	0	1052269	N.D.	0.433 #
27)	Chlordane-5	0.000	6.884	0	55594	N.D.	0.564 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
Data File : PL052263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 13:52
Operator : SG\AJ
Sample : PB122845BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB122845BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:00:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

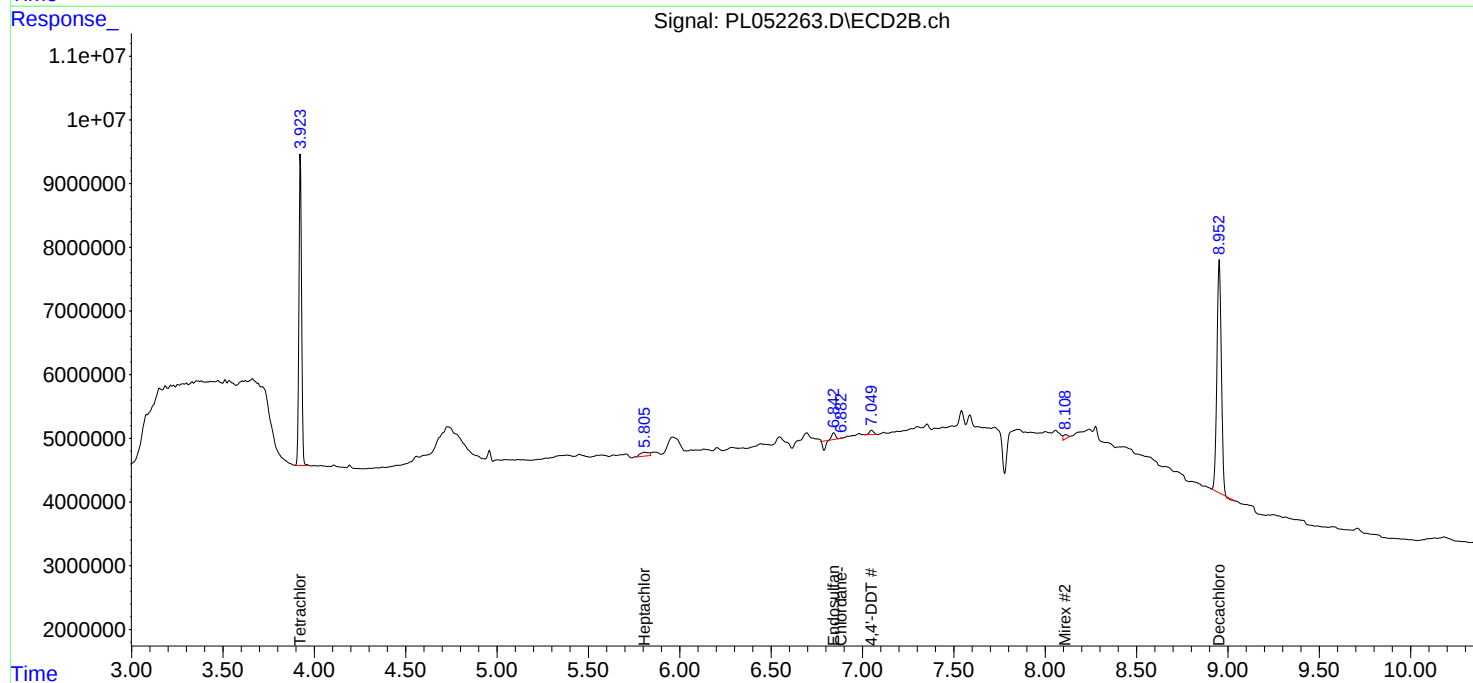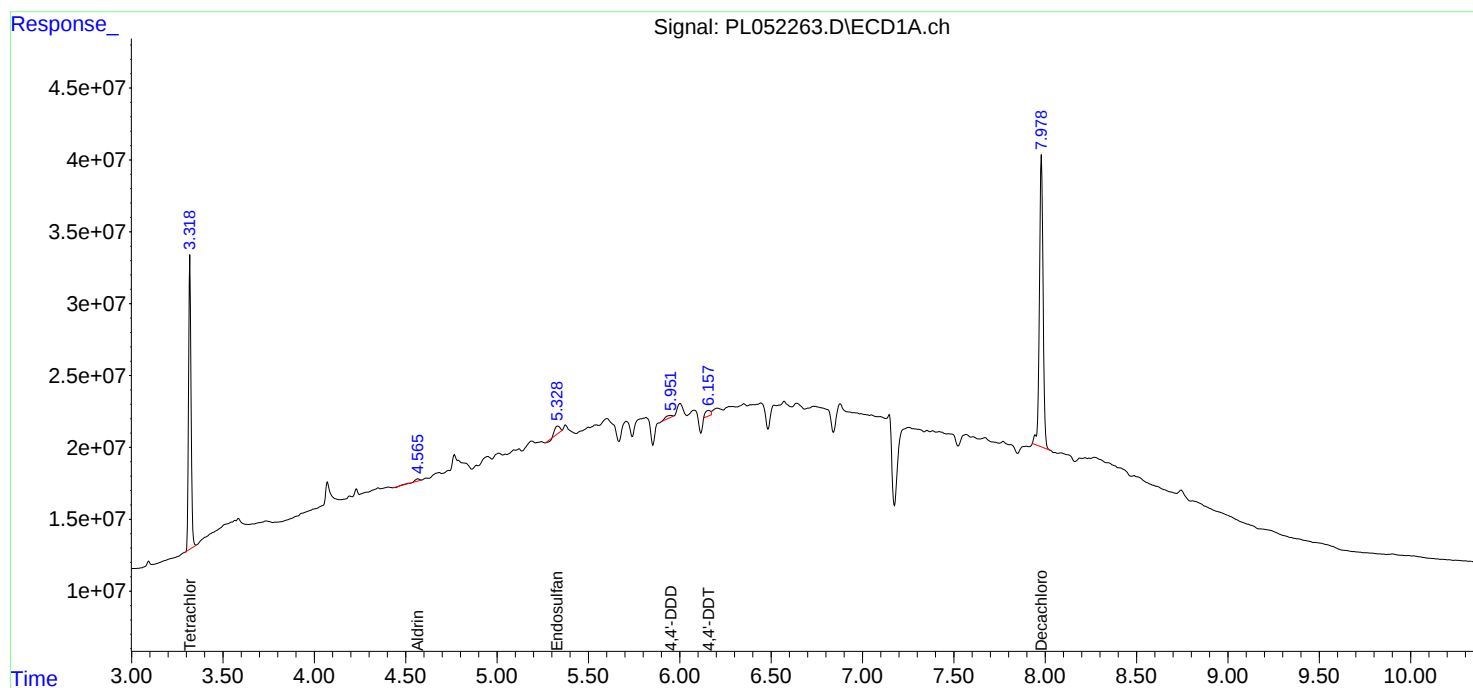


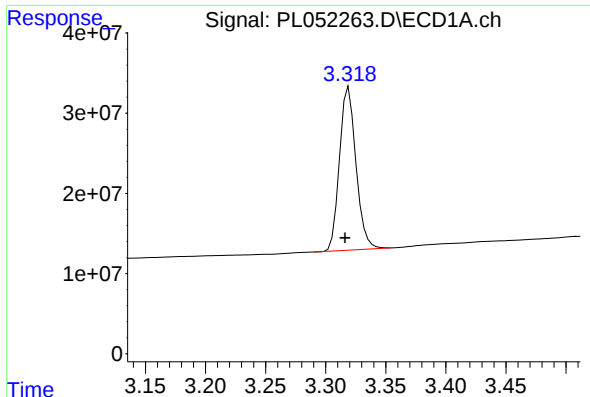

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.003 min
Response: 193902224
Conc: 22.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122845BL

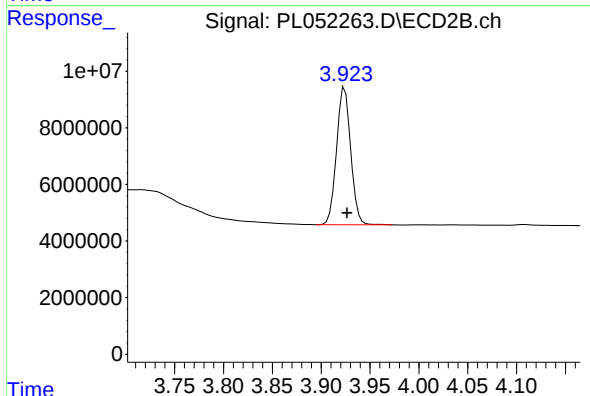


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 48980418
Conc: 22.42 ng/ml

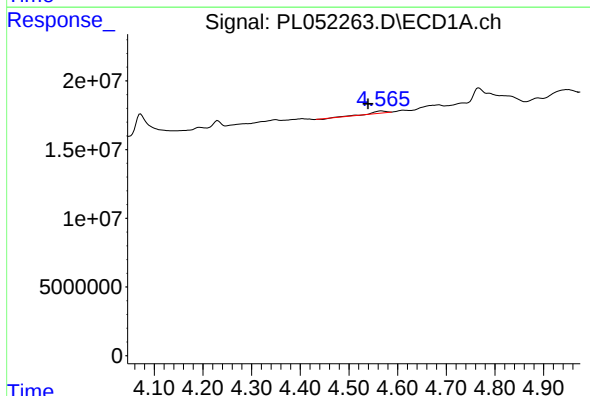


#5 Aldrin

R.T.: 4.567 min
Delta R.T.: 0.028 min
Response: 2729880
Conc: 0.19 ng/ml

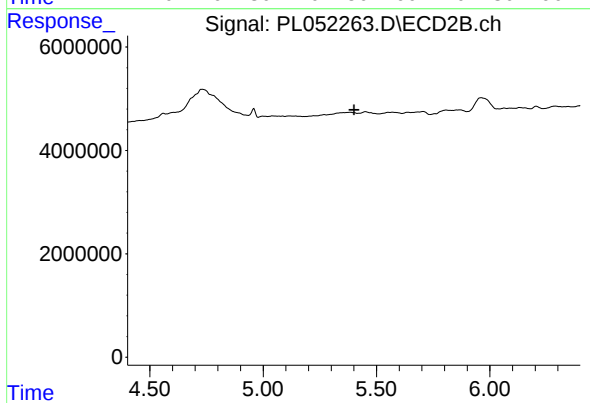

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.401 min
Response: 0
Conc: N.D.

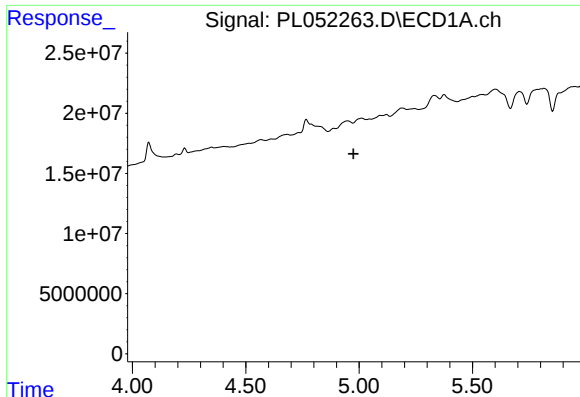

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122845BL

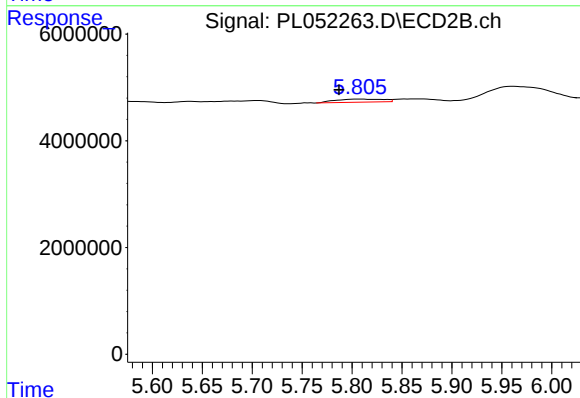


#8 Heptachlor epoxide

R.T.: 5.807 min
Delta R.T.: 0.020 min
Response: 1961388
Conc: 0.58 ng/ml

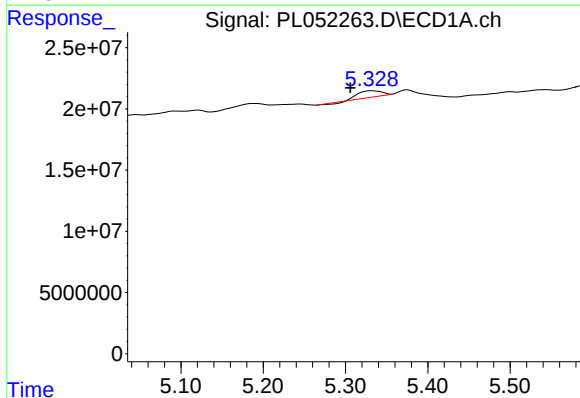


#9 Endosulfan I

R.T.: 5.332 min
Delta R.T.: 0.026 min
Response: 9050295
Conc: 0.67 ng/ml

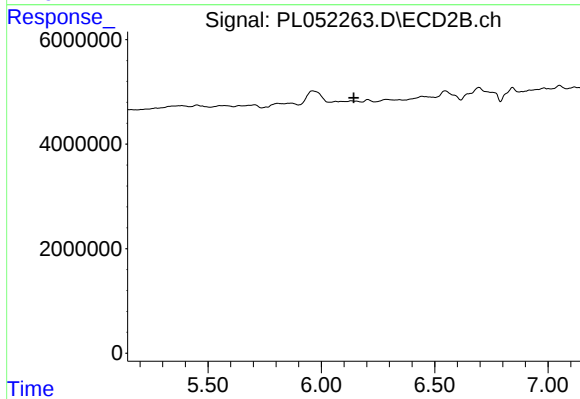

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

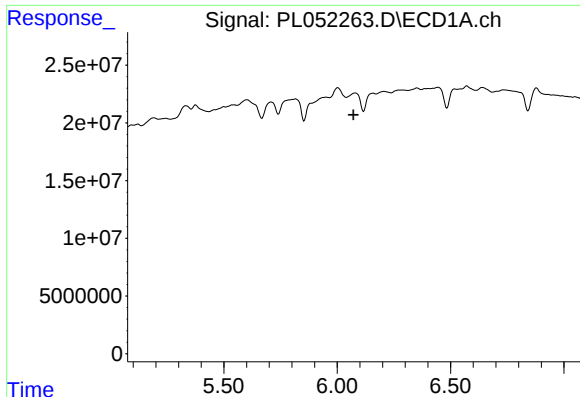

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122845BL

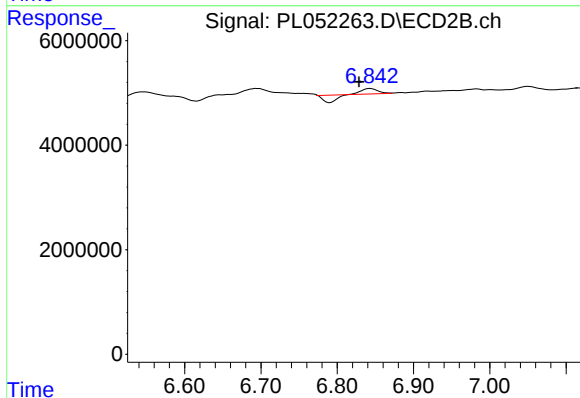


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.014 min
Response: 4675
Conc: 0.00 ng/ml

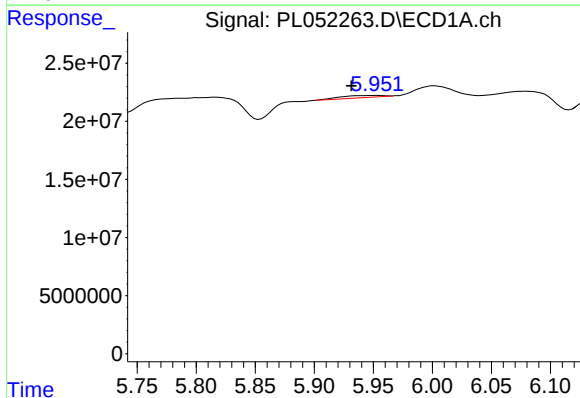


#16 4,4'-DDD

R.T.: 5.951 min
Delta R.T.: 0.020 min
Response: 4408615
Conc: 0.36 ng/ml

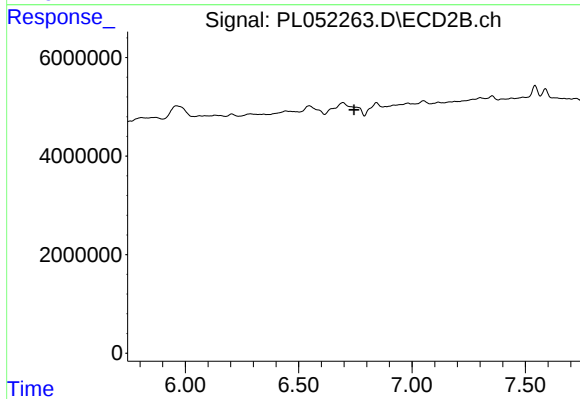

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.744 min
Response: 0
Conc: N.D.

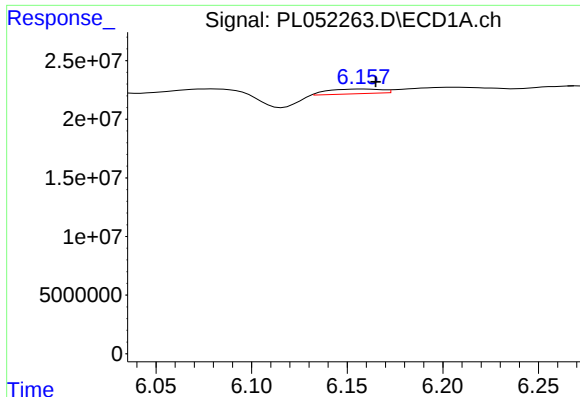

#17 4,4'-DDT


R.T.: 6.158 min
Delta R.T.: -0.007 min
Response: 7687978
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122845BL

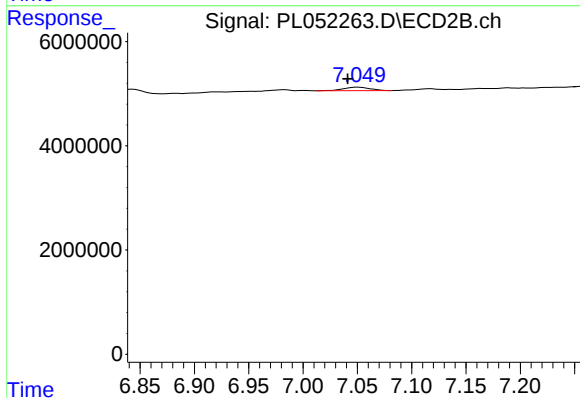


#17 4,4'-DDT

R.T.: 7.051 min
Delta R.T.: 0.010 min
Response: 1118361
Conc: 0.38 ng/ml

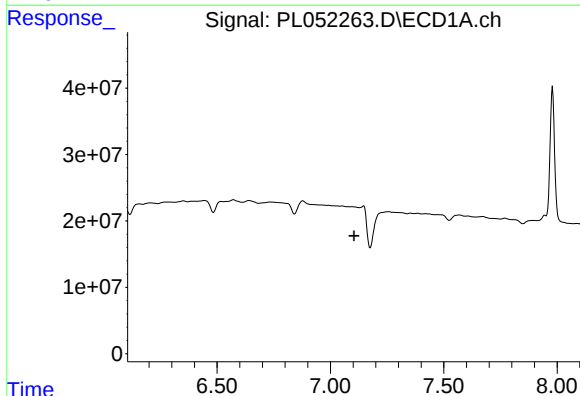


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.104 min
Response: 0
Conc: N.D.

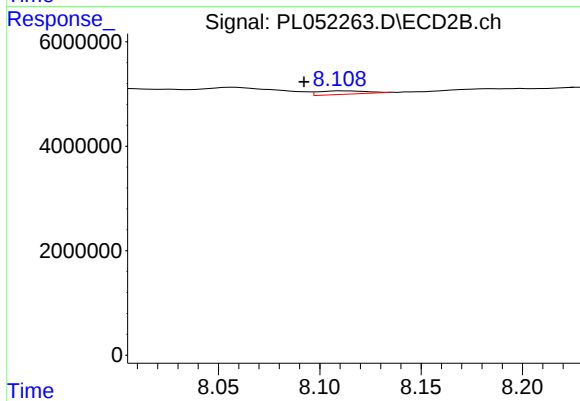

#22 Mirex


R.T.: 8.111 min
Delta R.T.: 0.019 min
Response: 1052269
Conc: 0.43 ng/ml

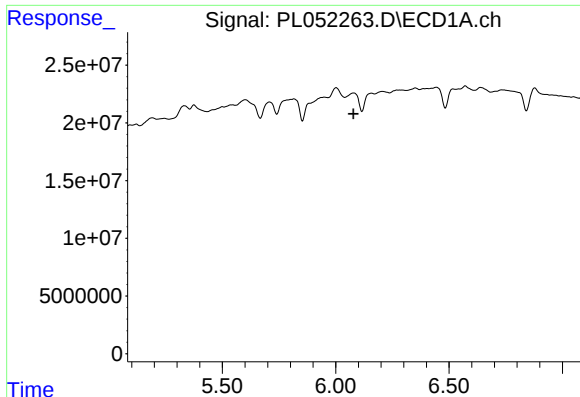

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122845BL

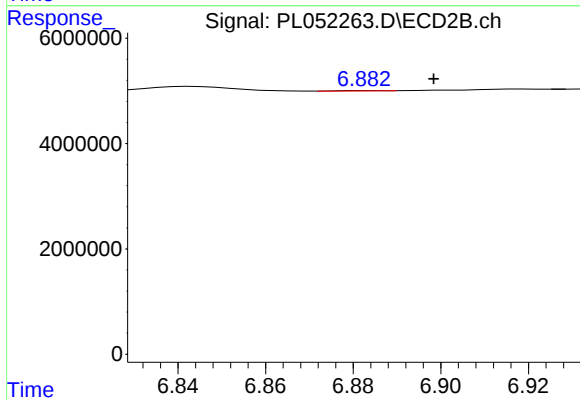


#27 Chlordane-5

R.T.: 6.884 min
Delta R.T.: -0.015 min
Response: 55594
Conc: 0.56 ng/ml

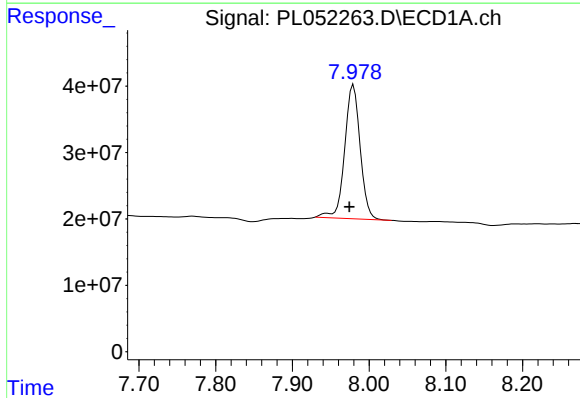

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.005 min
Response: 283394511
Conc: 23.35 ng/ml

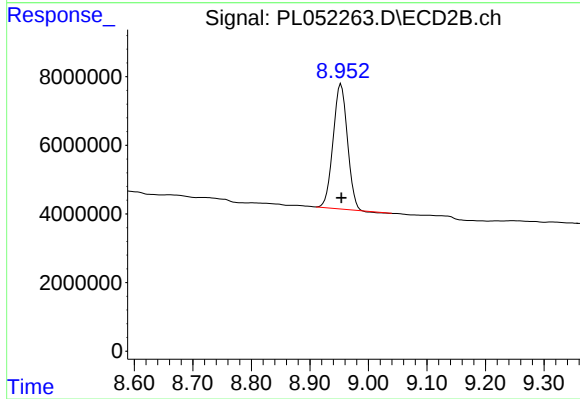

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.000 min
Response: 61547739
Conc: 20.22 ng/ml