

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
 Data File : PL052279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 19:15
 Operator : SG\AJ
 Sample : K4716-03 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-20-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:03:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	23534714	9036816	2.750	4.136 #
28)	SA Decachlor...	7.972	8.951	15836178	5923734	1.305	1.946 #
Target Compounds							
3)	MA gamma-BHC...	0.000	4.579f	0	779017	N.D.	0.247 #
6)	B beta-BHC	0.000	4.800f	0	1740619	N.D.	1.194 #
8)	B Heptachlo...	0.000	5.801	0	1175542	N.D.	0.348 #
9)	A Endosulfan I	5.335f	0.000	739828	0	0.055	N.D. #
10)	B gamma-Chl...	0.000	6.014	0	769325	N.D.	0.211 #
11)	B alpha-Chl...	0.000	6.091	0	1216257	N.D.	0.352 #
15)	B Endosulfa...	6.086	6.845f	1246395	2327533	0.090	0.706 #
18)	B Endrin al...	0.000	6.962	0	467628	N.D.	0.165 #
25)	Chlordane-3	0.000	6.014	0	769325	N.D.	1.727 #
26)	Chlordane-4	0.000	6.091	0	1216257	N.D.	2.239 #
27)	Chlordane-5	6.086	6.912	1246395	1089813	2.540	11.055 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
Data File : PL052279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 19:15
Operator : SG\AJ
Sample : K4716-03 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-20-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:03:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

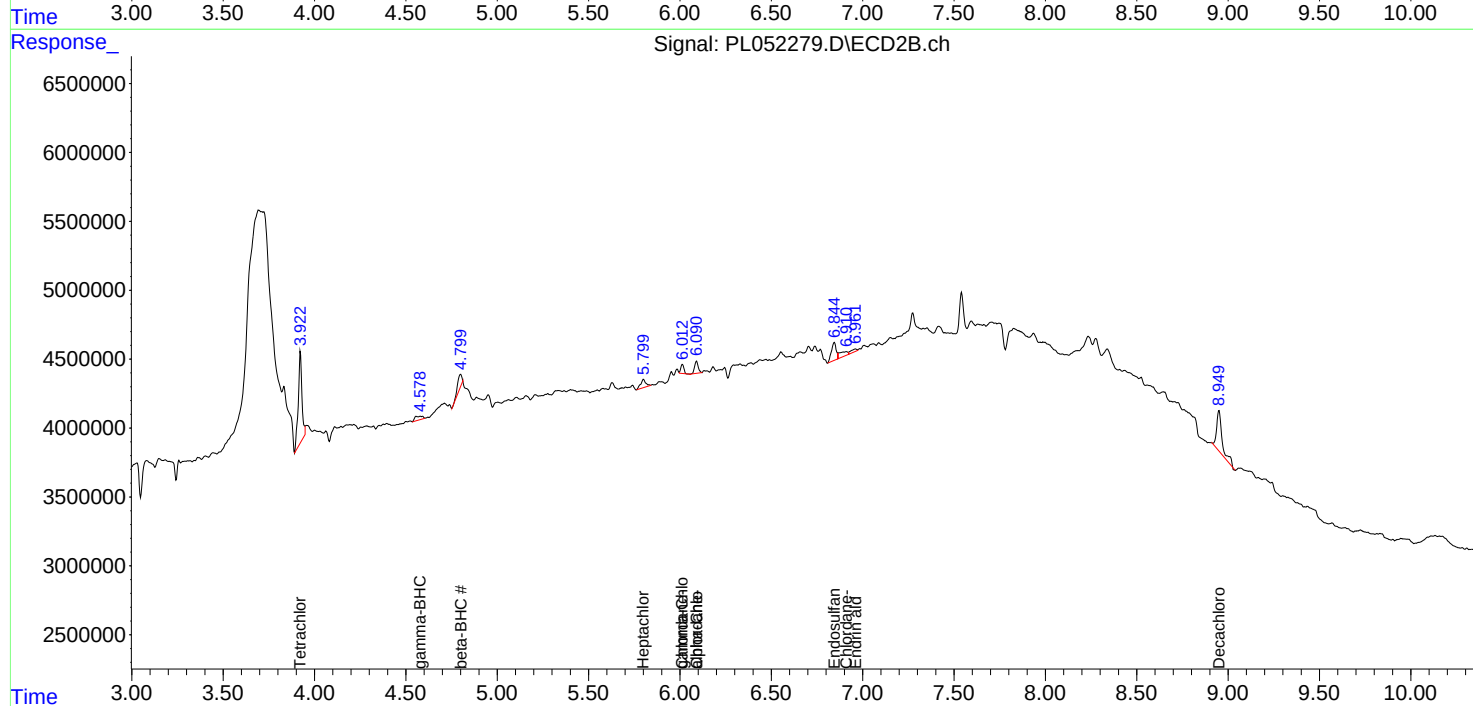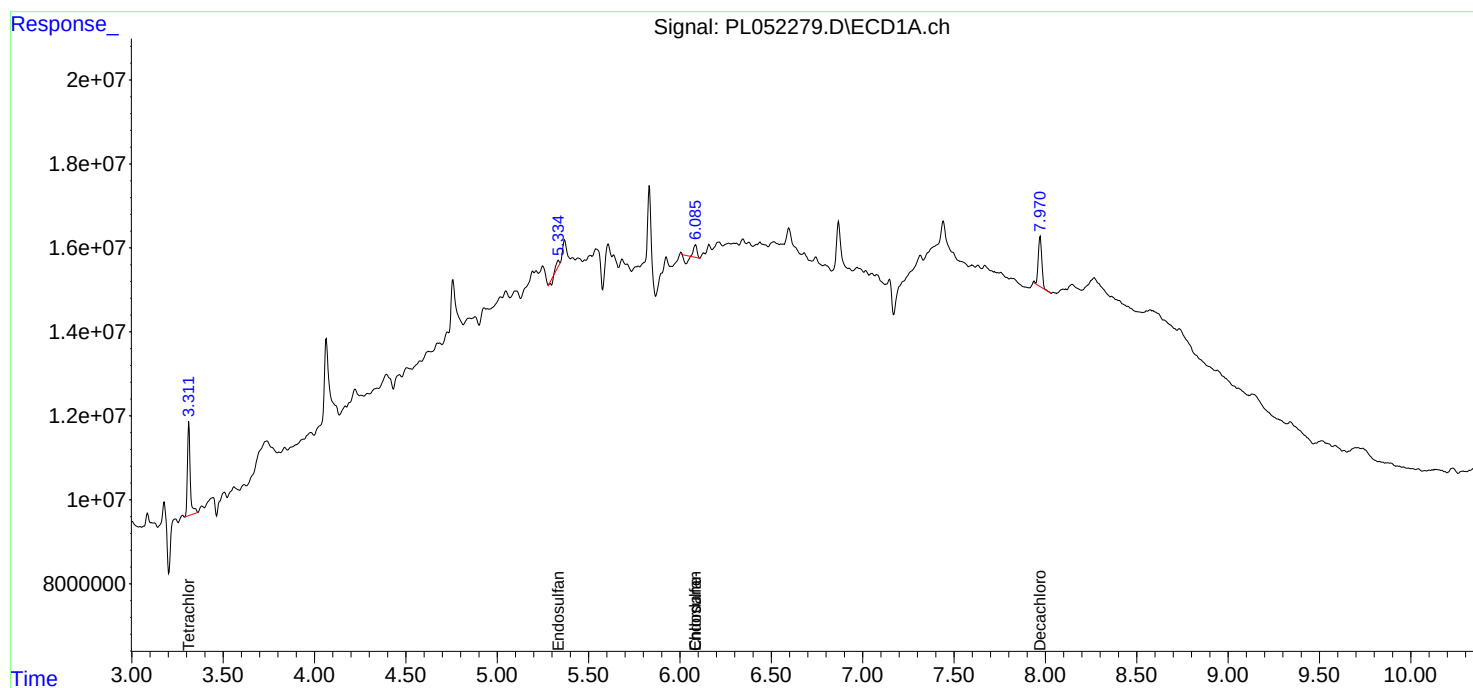


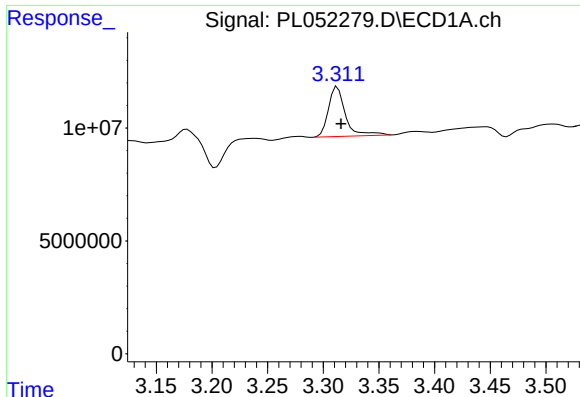

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 23534714
Conc: 2.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-20-S

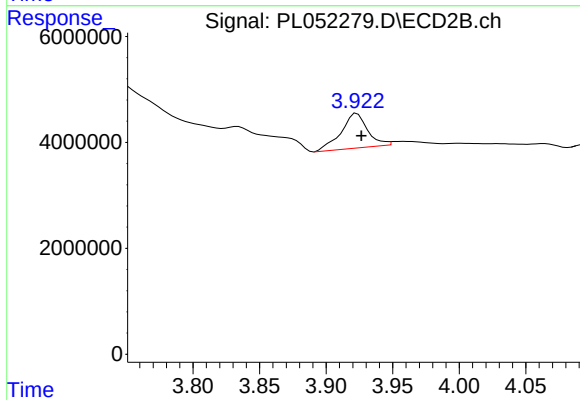


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 9036816
Conc: 4.14 ng/ml

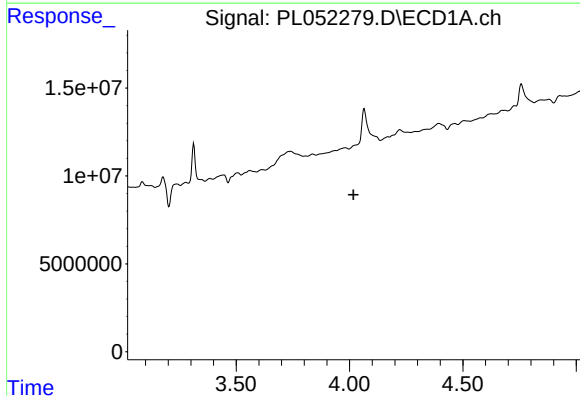


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.018 min
Response: 0
Conc: N.D.

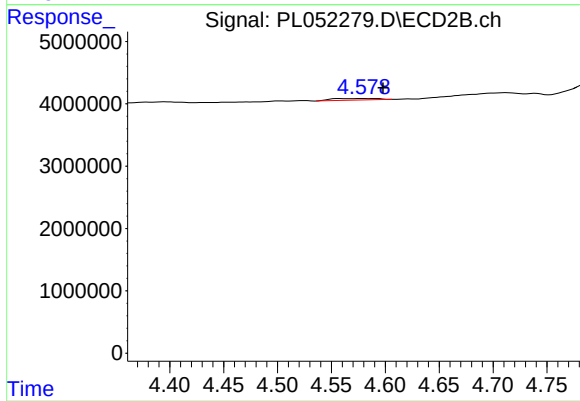

#3 gamma-BHC (Lindane)


R.T.: 4.579 min
Delta R.T.: -0.019 min
Response: 779017
Conc: 0.25 ng/ml

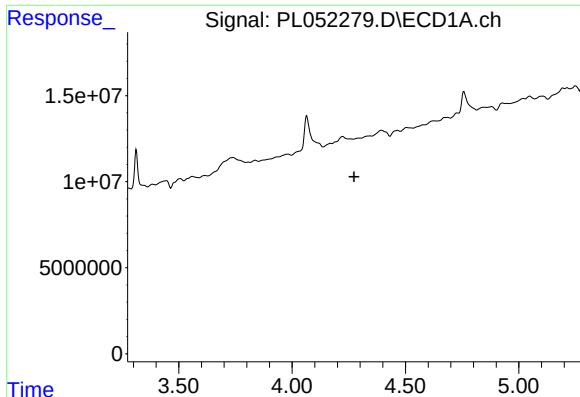

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20-S

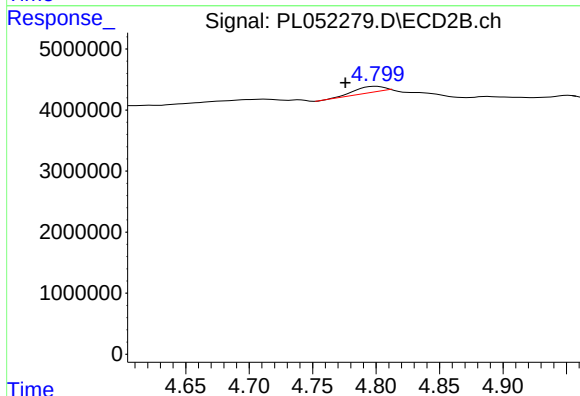


#6 beta-BHC

R.T.: 4.800 min
Delta R.T.: 0.024 min
Response: 1740619
Conc: 1.19 ng/ml

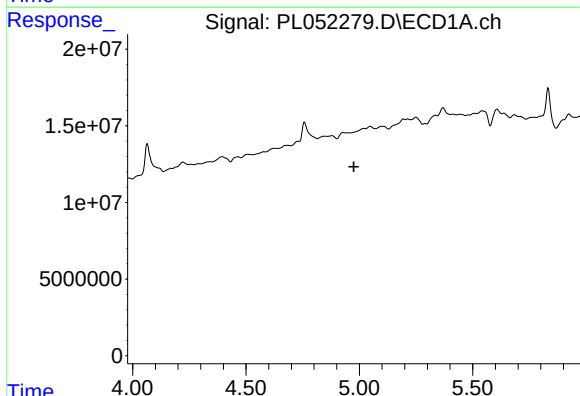


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

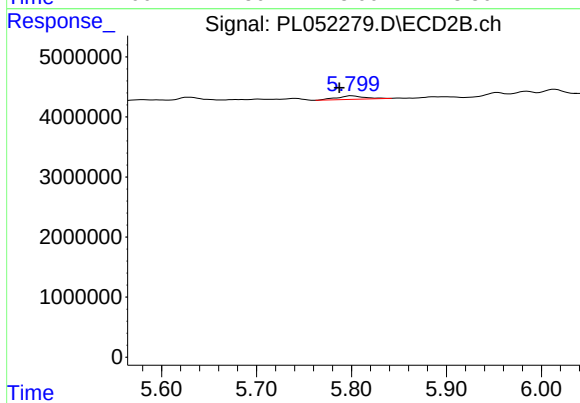

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.014 min
Response: 1175542
Conc: 0.35 ng/ml

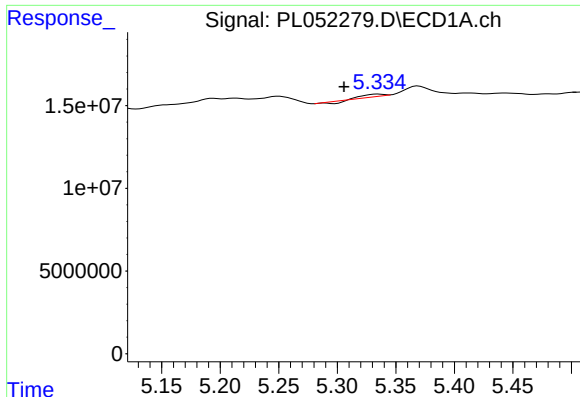

#9 Endosulfan I


R.T.: 5.335 min
Delta R.T.: 0.029 min
Response: 739828
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-20-S

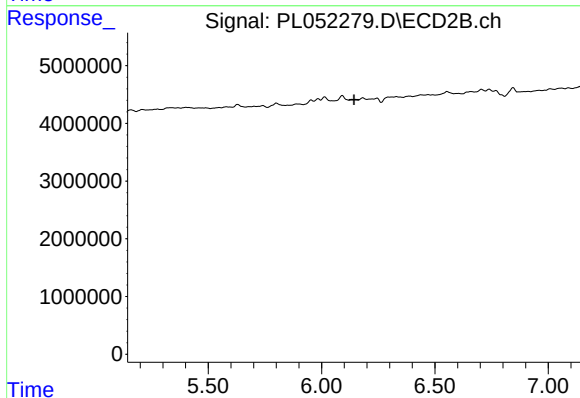


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

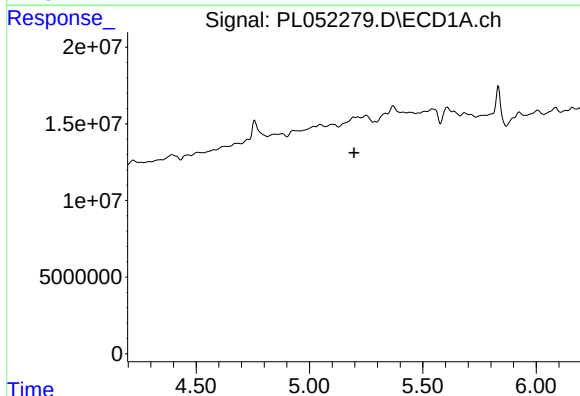


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

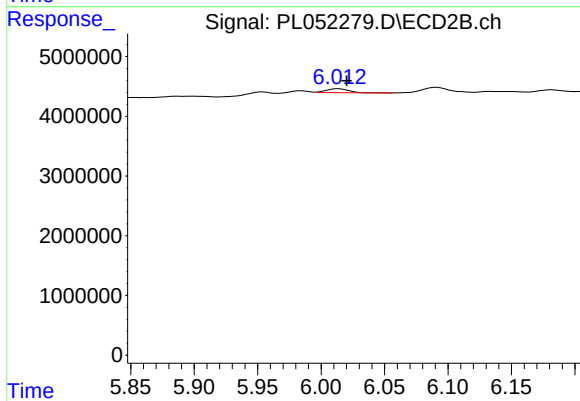

#10 gamma-Chlordane


R.T.: 6.014 min
Delta R.T.: -0.006 min
Response: 769325
Conc: 0.21 ng/ml

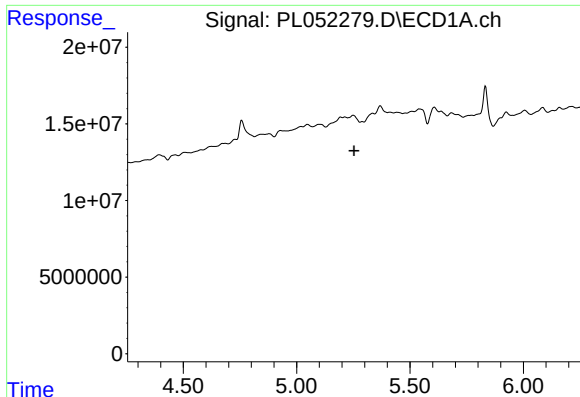

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20-S

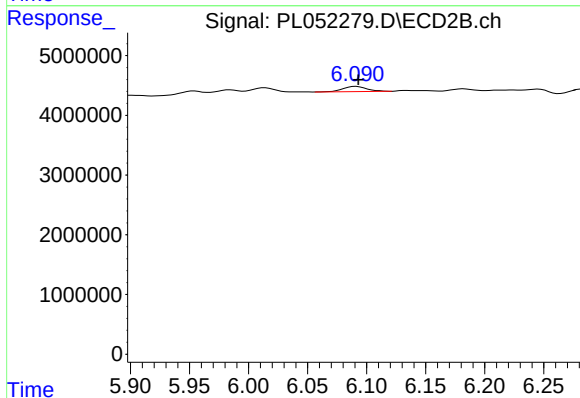


#11 alpha-Chlordane

R.T.: 6.091 min
Delta R.T.: -0.002 min
Response: 1216257
Conc: 0.35 ng/ml

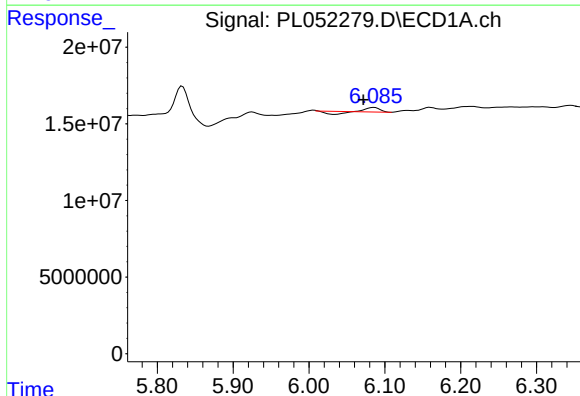


#15 Endosulfan II

R.T.: 6.086 min
Delta R.T.: 0.014 min
Response: 1246395
Conc: 0.09 ng/ml

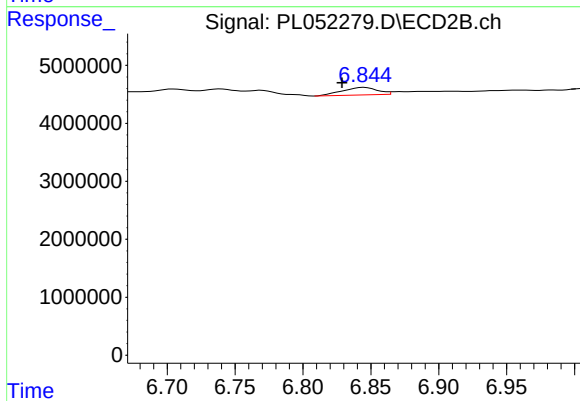

#15 Endosulfan II


R.T.: 6.845 min
Delta R.T.: 0.017 min
Response: 2327533
Conc: 0.71 ng/ml

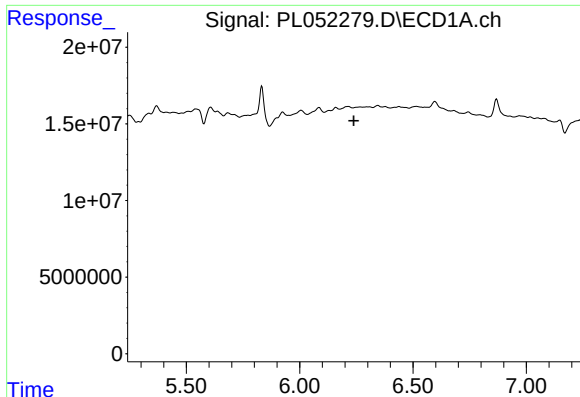

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20-S

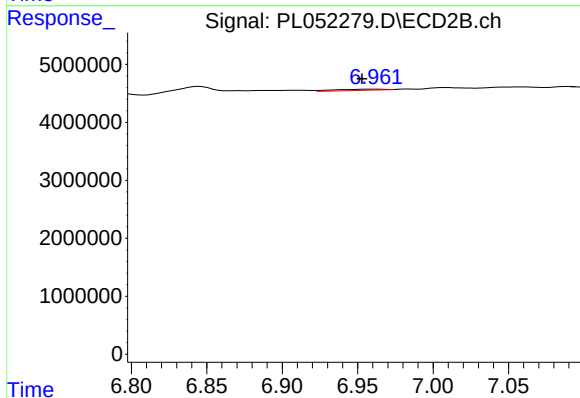


#18 Endrin aldehyde

R.T.: 6.962 min
Delta R.T.: 0.009 min
Response: 467628
Conc: 0.17 ng/ml

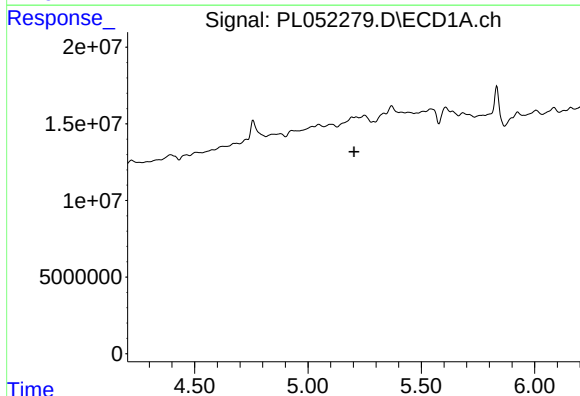


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

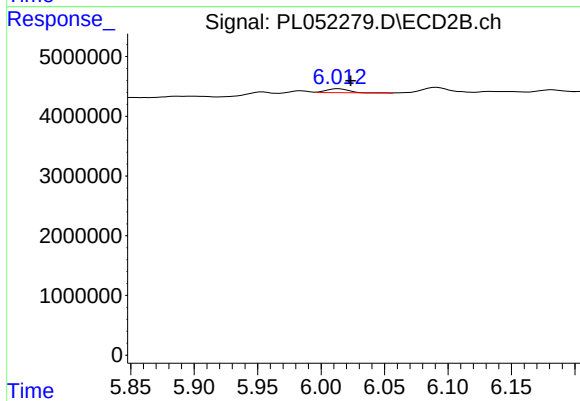

#25 Chlordane-3


R.T.: 6.014 min
Delta R.T.: -0.010 min
Response: 769325
Conc: 1.73 ng/ml

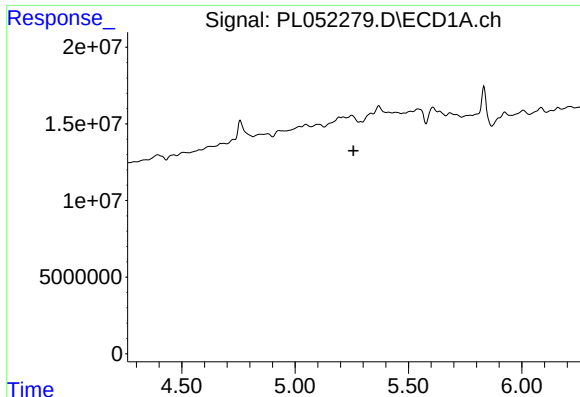

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20-S

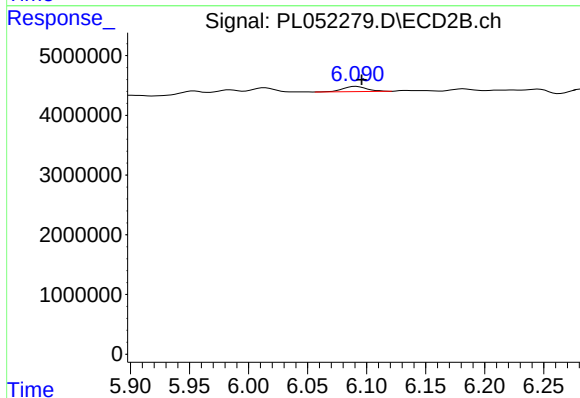


#26 Chlordane-4

R.T.: 6.091 min
Delta R.T.: -0.005 min
Response: 1216257
Conc: 2.24 ng/ml

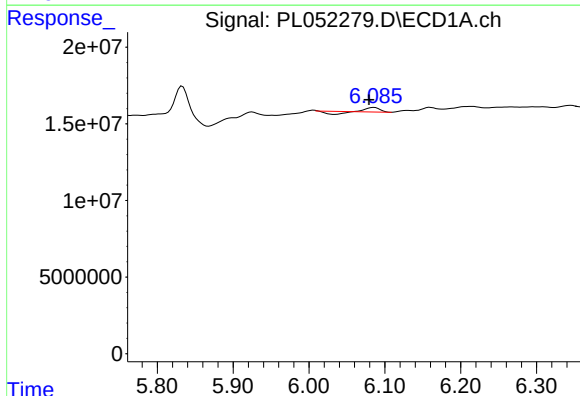


#27 Chlordane-5

R.T.: 6.086 min
Delta R.T.: 0.007 min
Response: 1246395
Conc: 2.54 ng/ml

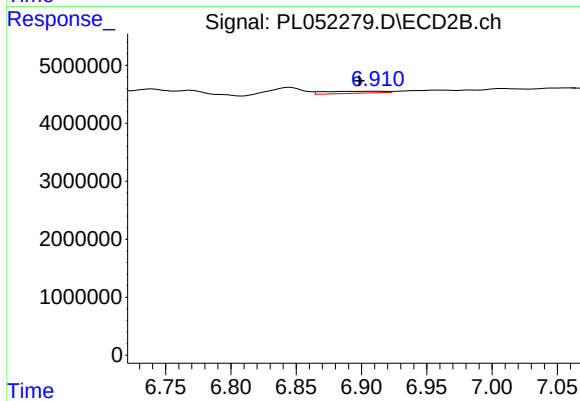

#27 Chlordane-5


R.T.: 6.912 min
Delta R.T.: 0.013 min
Response: 1089813
Conc: 11.05 ng/ml

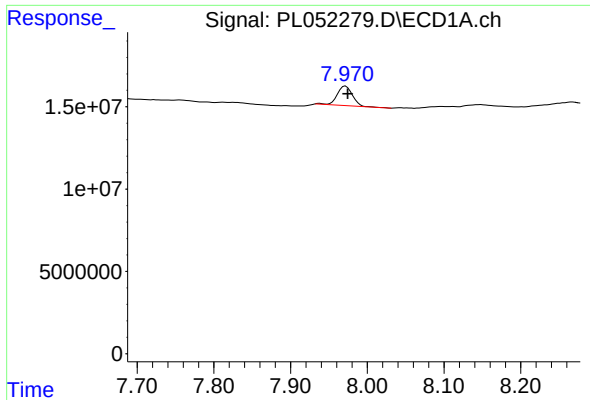

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 15836178
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-20-S

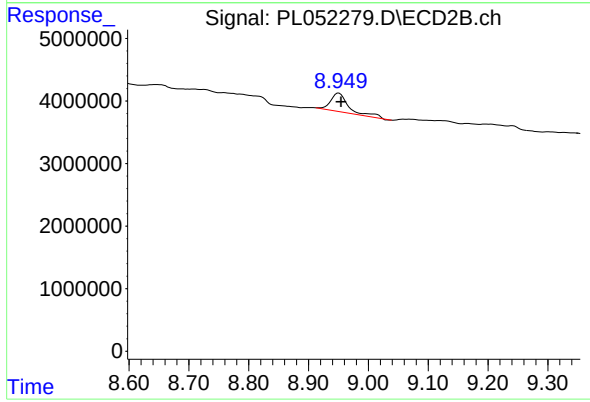

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.004 min
Response: 5923734
Conc: 1.95 ng/ml