

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
 Data File : PL052250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 10:33
 Operator : SG\AJ
 Sample : K4650-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 9/9/2019 3:06:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 22:57:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.923	193.8E6	46805065	22.646	21.423
28)	SA Decachlor...	7.970	8.947	195.6E6	51002165	16.118	16.756m
Target Compounds							
14)	MA Endrin	5.794	6.606	10449952	3955580	0.716m	1.308m#
16)	A 4,4'-DDD	5.920	6.740	11693725	8946663	0.955m	3.305m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
Data File : PL052250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 10:33
Operator : SG\AJ
Sample : K4650-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
9/9/2019 3:06:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 22:57:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

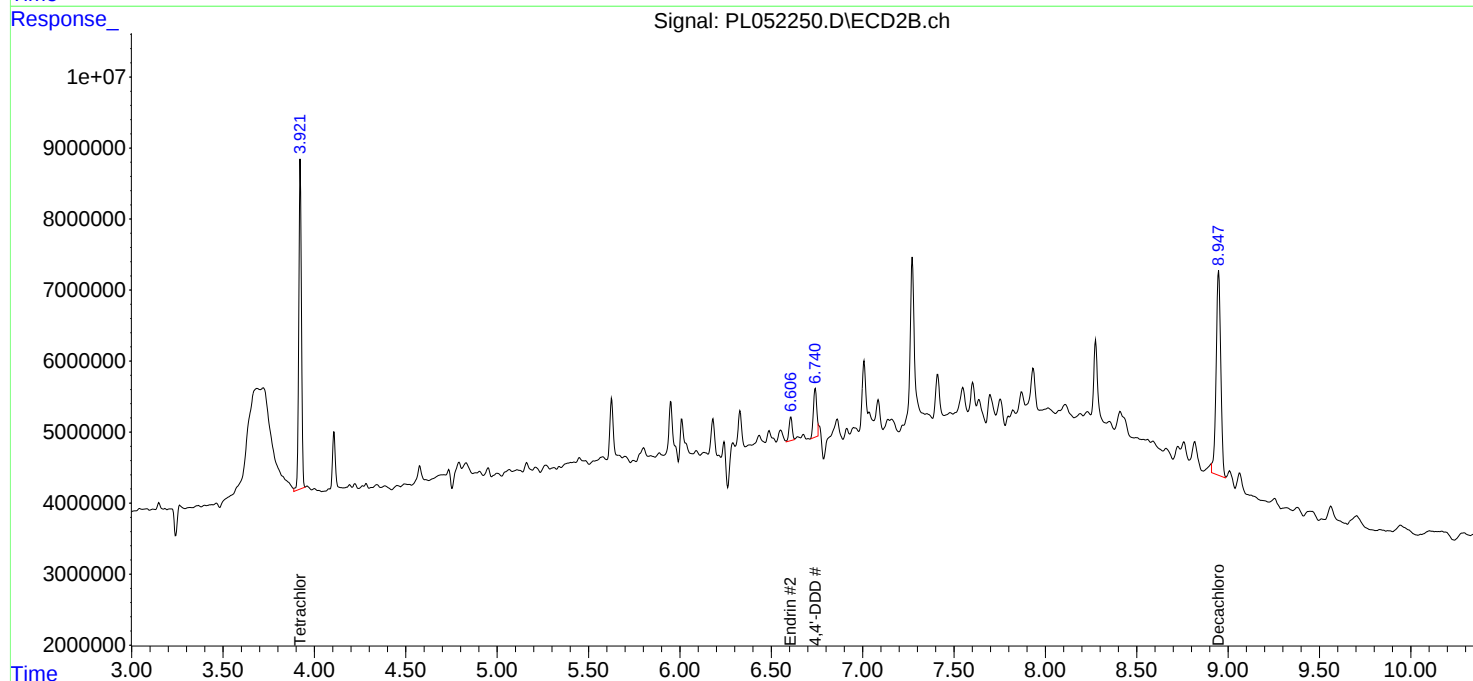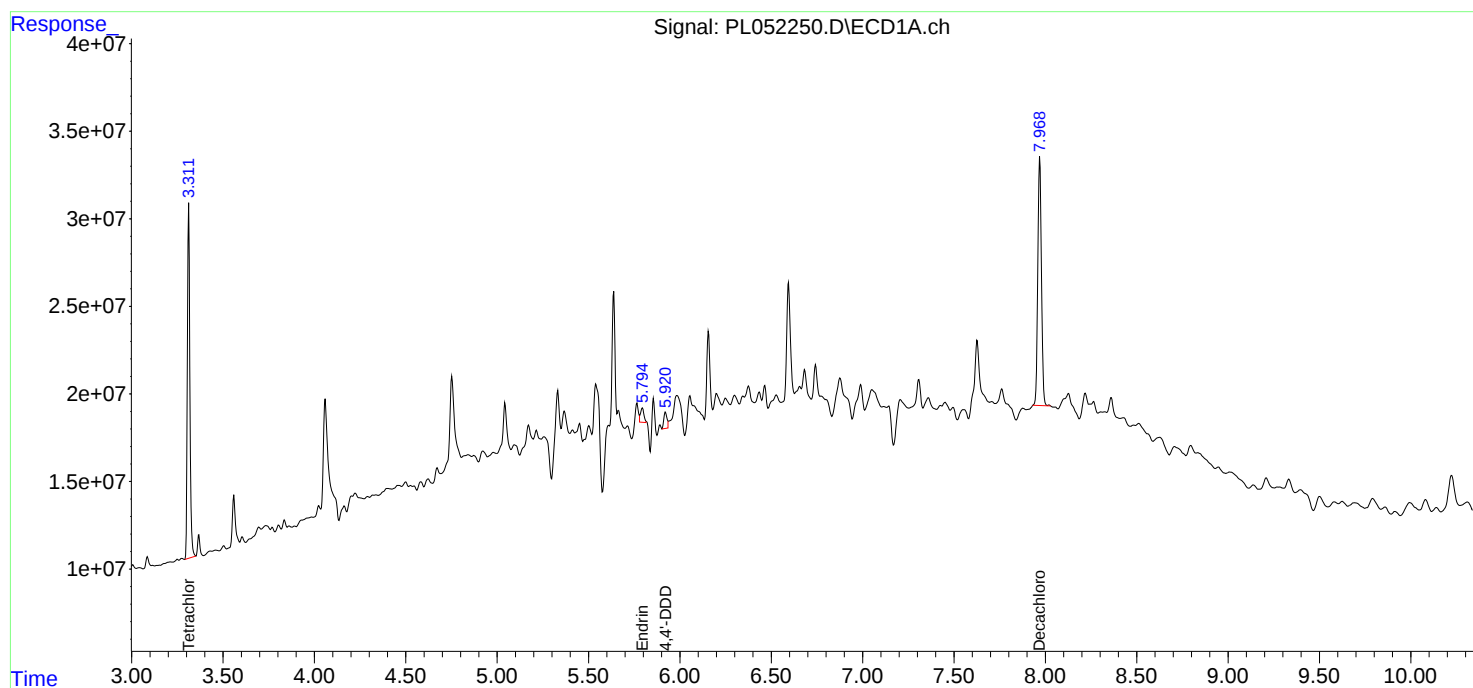

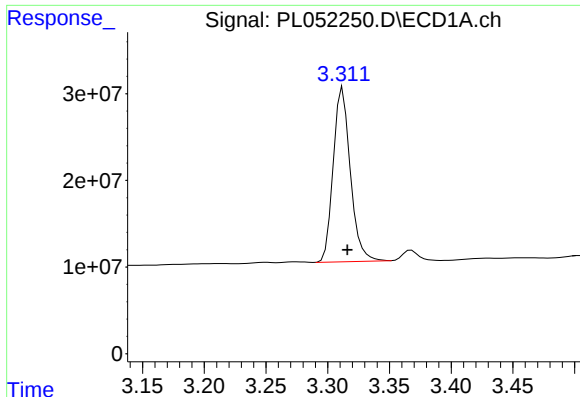


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 193814269
Conc: 22.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/9/2019 3:06:45 PM

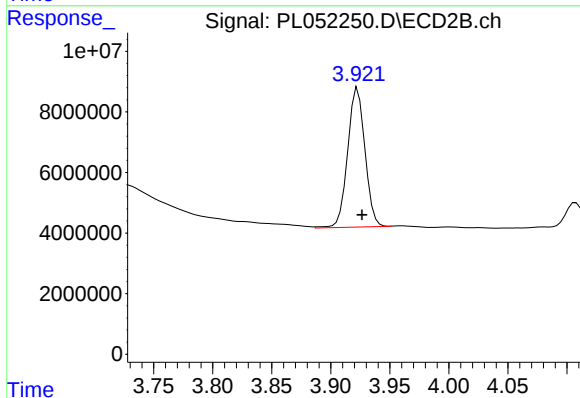


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.004 min
Response: 46805065
Conc: 21.42 ng/ml

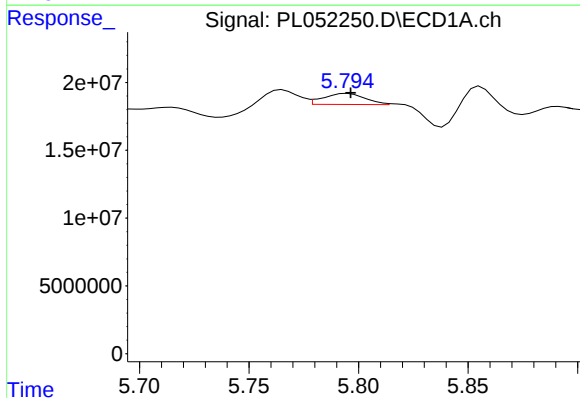


#14 Endrin

R.T.: 5.794 min
Delta R.T.: -0.003 min
Response: 10449952
Conc: 0.72 ng/ml m

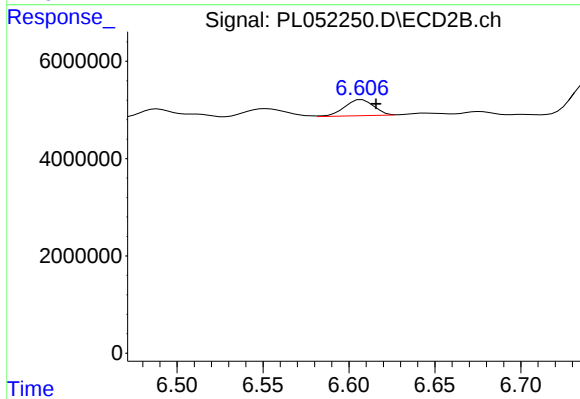

#14 Endrin

R.T.: 6.606 min
Delta R.T.: -0.010 min
Response: 3955580
Conc: 1.31 ng/ml m

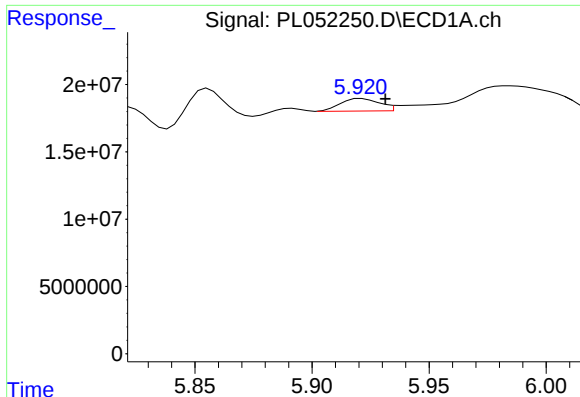


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: -0.012 min
Response: 11693725
Conc: 0.95 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
9/9/2019 3:06:45 PM

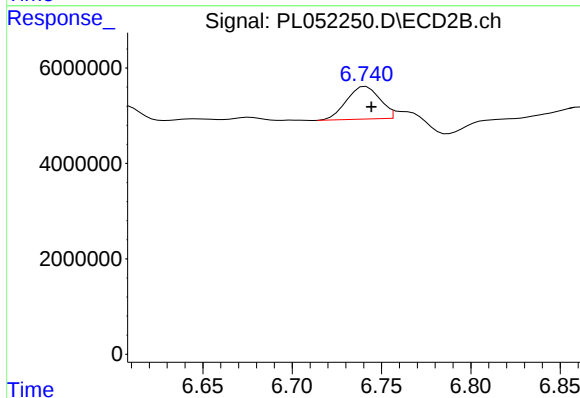


#16 4,4'-DDD

R.T.: 6.740 min
Delta R.T.: -0.004 min
Response: 8946663
Conc: 3.30 ng/ml m

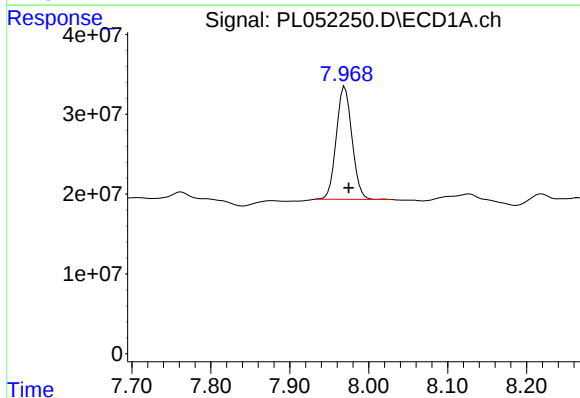

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.005 min
Response: 195637458
Conc: 16.12 ng/ml

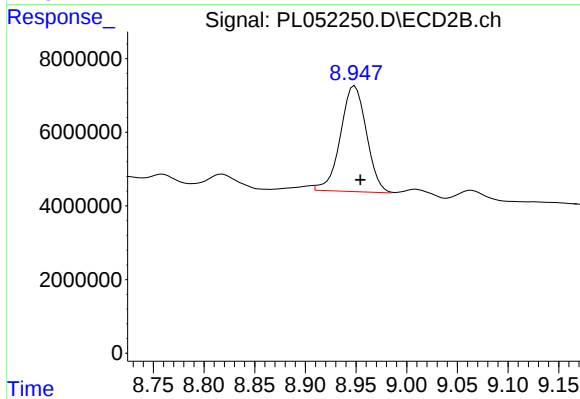

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.007 min
Response: 51002165
Conc: 16.76 ng/ml m