

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
 Data File : PL052268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2019 16:40
 Operator : SG\AJ
 Sample : K4669-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-090519

Manual Integrations
 APPROVED

Ankita
 9/9/2019 3:07:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 23:01:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	144.1E6	34020535	16.836	15.571
28)	SA Decachlor...	7.972	8.950	115.1E6	29151787	9.481	9.577
Target Compounds							
10)	B gamma-Chl...	5.188	6.017	26883236	3002562	1.800m	0.822m#
11)	B alpha-Chl...	5.250	6.089	17362012	6328690	1.200	1.834m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090619\
Data File : PL052268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2019 16:40
Operator : SG\AJ
Sample : K4669-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-05-090519


Manual Integrations
APPROVED

Ankita
9/9/2019 3:07:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 23:01:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

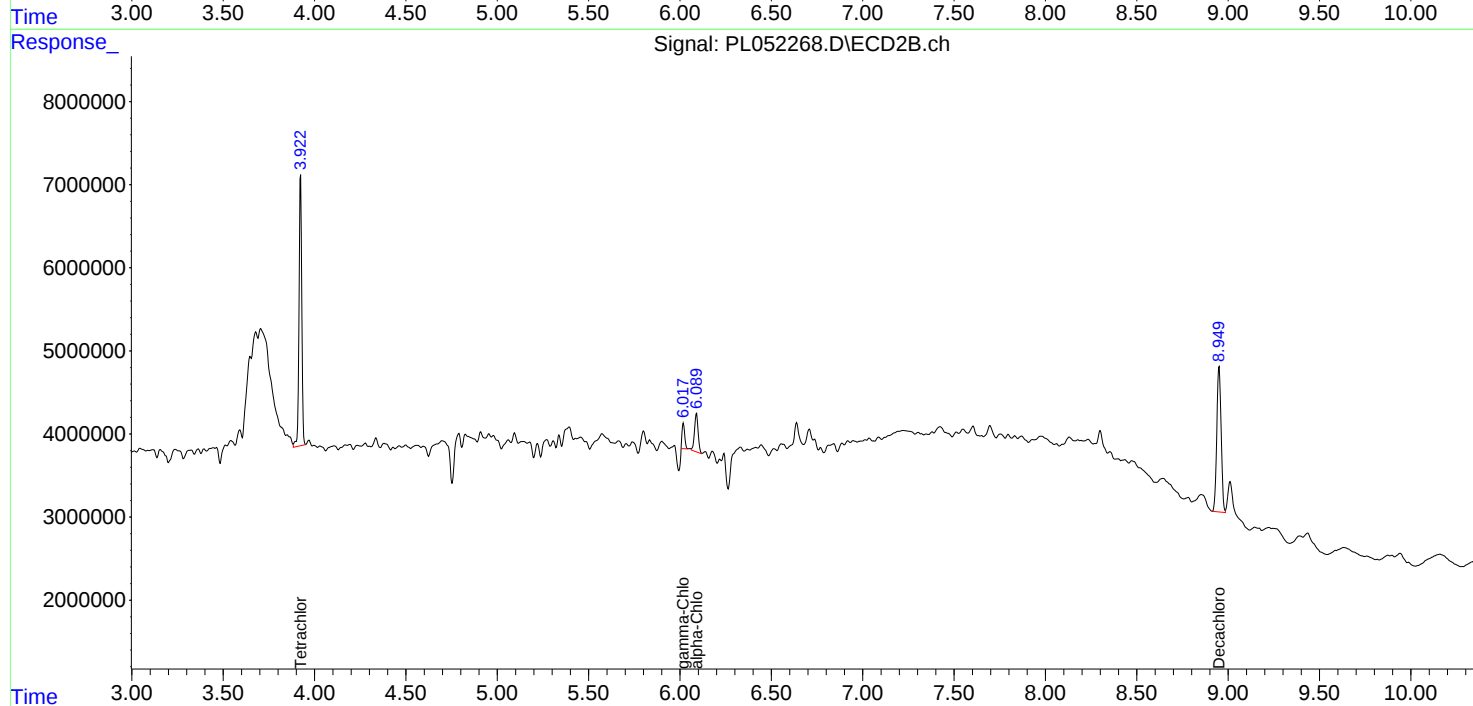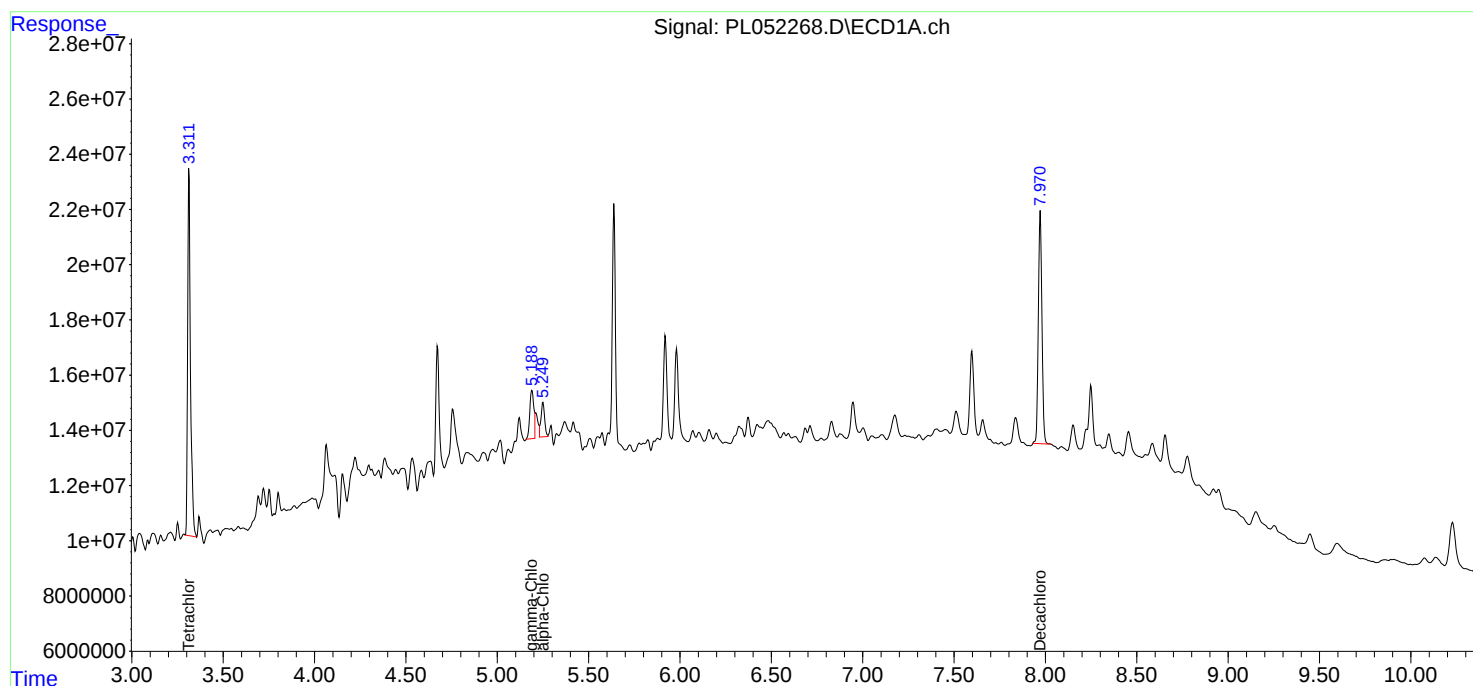

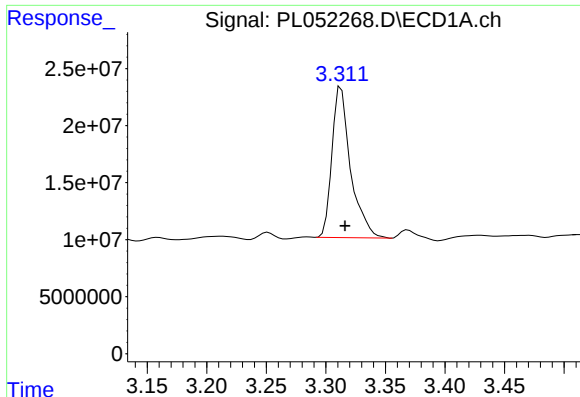


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 144089670
Conc: 16.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-090519


Manual Integrations
APPROVED

Ankita
9/9/2019 3:07:03 PM

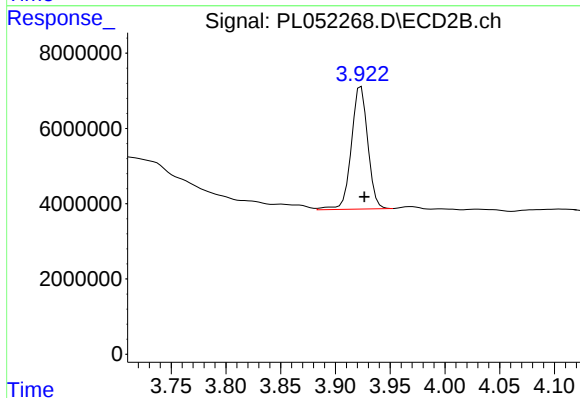


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 34020535
Conc: 15.57 ng/ml

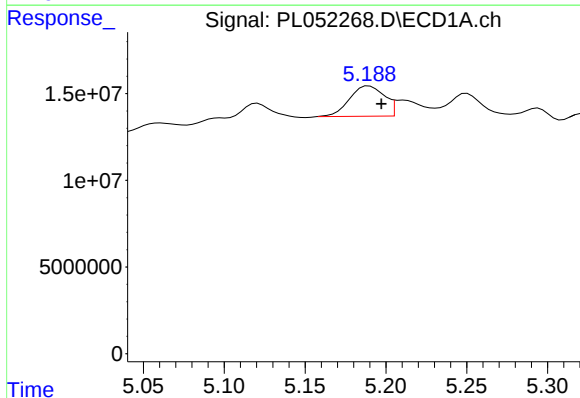


#10 gamma-Chlordane

R.T.: 5.188 min
Delta R.T.: -0.009 min
Response: 26883236
Conc: 1.80 ng/ml m

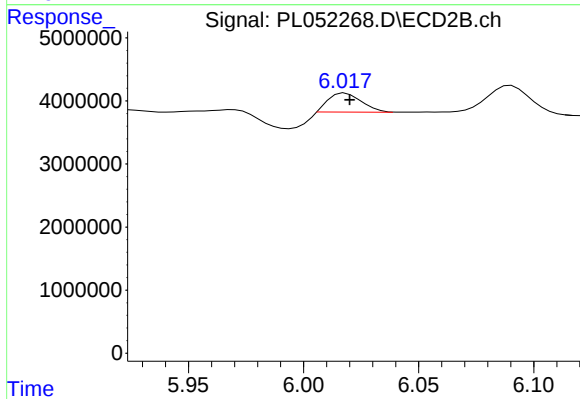

#10 gamma-Chlordane

R.T.: 6.017 min
Delta R.T.: -0.003 min
Response: 3002562
Conc: 0.82 ng/ml m

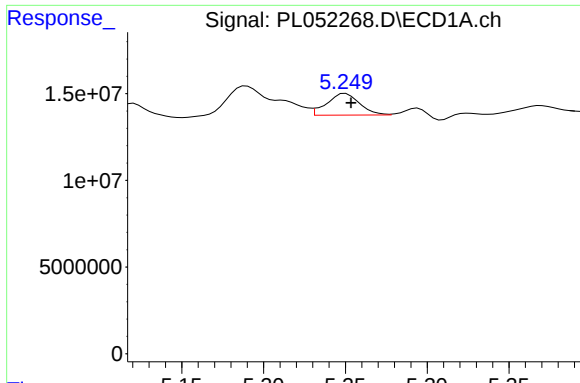


#11 alpha-Chlordane

R.T.: 5.250 min
Delta R.T.: -0.003 min
Response: 17362012
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-090519


Manual Integrations
APPROVED

Ankita
9/9/2019 3:07:03 PM

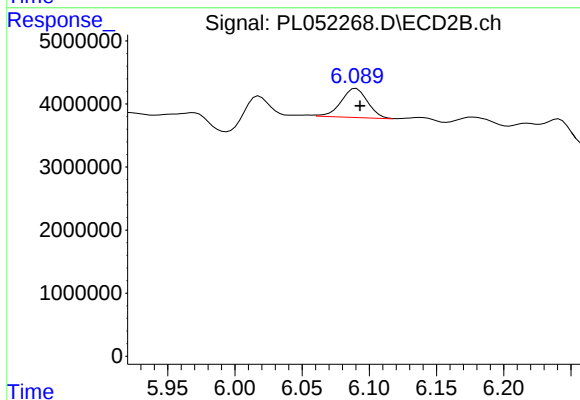


#11 alpha-Chlordane

R.T.: 6.089 min
Delta R.T.: -0.004 min
Response: 6328690
Conc: 1.83 ng/ml m

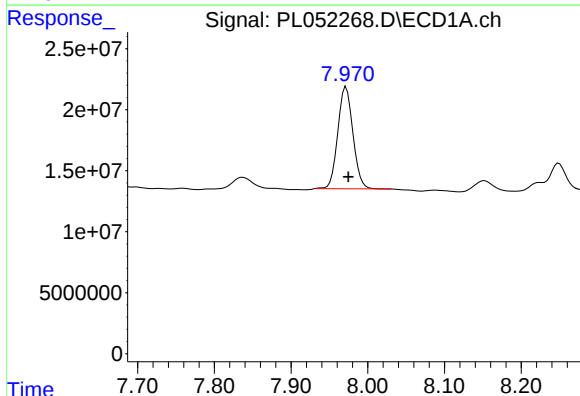

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 115084142
Conc: 9.48 ng/ml

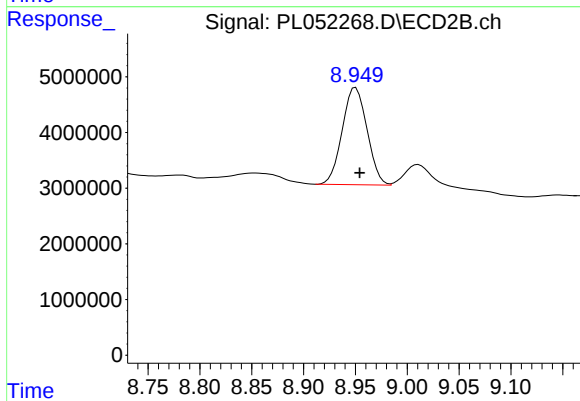

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 29151787
Conc: 9.58 ng/ml