

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090622\
 Data File : PL077522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2022 15:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 18:50:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 05:19:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.631	31415156	53476994	22.823	20.101
28)	SA Decachlor...	8.907	7.730	25149579	37339882	21.973	15.823 #
Target Compounds							
2)	A alpha-BHC	0.000	3.108f	0	333010	N.D.	0.083 #
5)	MB Aldrin	0.000	4.069	0	1097285	N.D.	0.333 #
8)	B Heptachlo...	5.572	0.000	1751044	0	1.308	N.D. #
10)	B gamma-Chl...	0.000	4.796	0	262650	N.D.	0.086 #
13)	MA Dieldrin	0.000	5.174	0	4179686	N.D.	1.455 #
14)	MA Endrin	0.000	5.476f	0	1100164	N.D.	0.484 #
15)	B Endosulfa...	6.709f	0.000	709227	0	0.631	N.D. #
17)	MA 4,4'-DDT	6.901	0.000	574300	0	0.489	N.D. #
21)	B Endrin ke...	7.538	0.000	97215	0	0.078	N.D. #
25)	Chlordane-3	0.000	4.796	0	262650	N.D.	0.873 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090622\
Data File : PL077522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2022 15:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 18:50:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 05:19:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

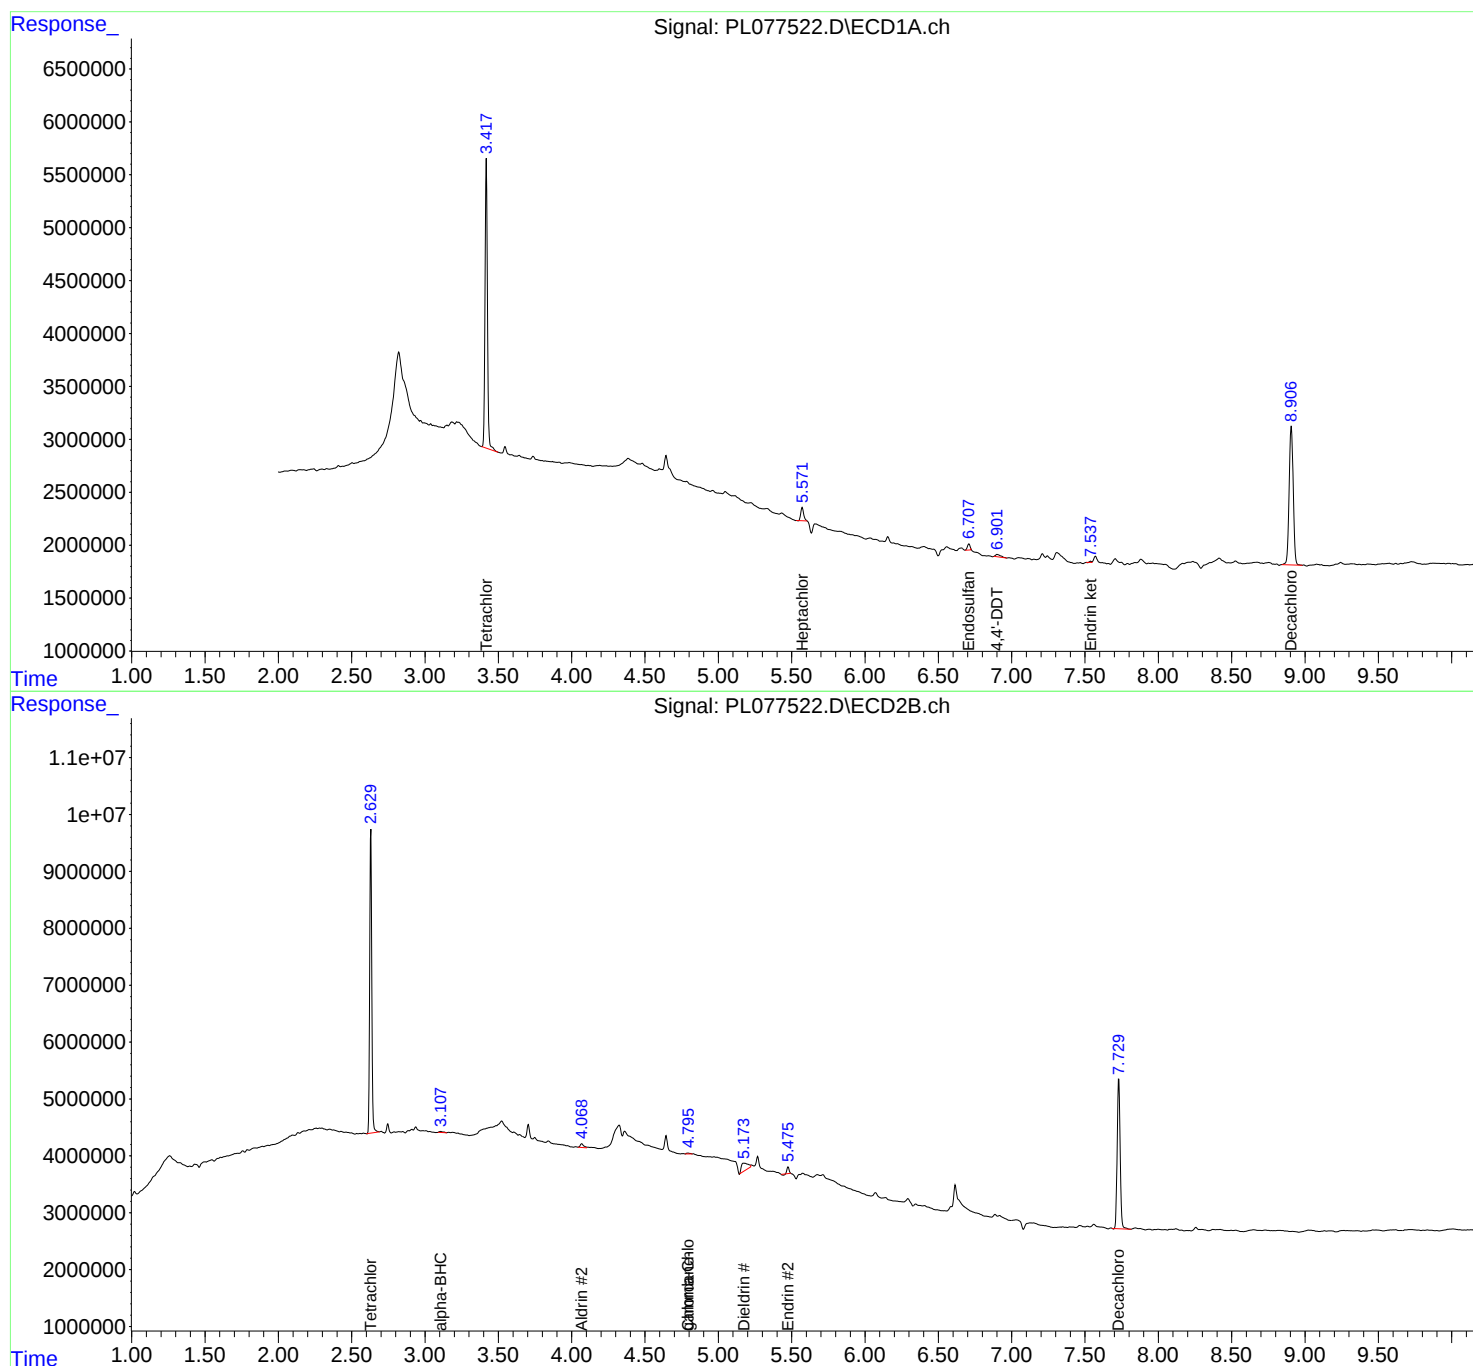


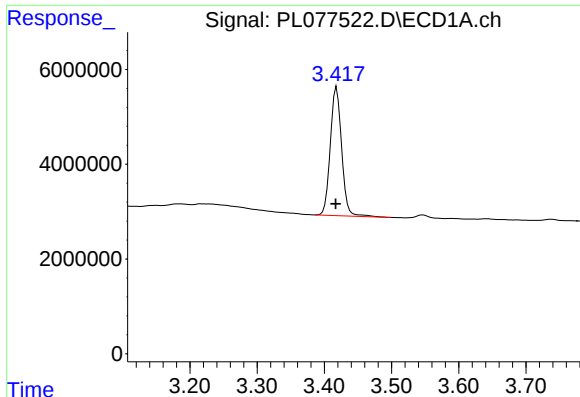

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.001 min
Response: 31415156
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

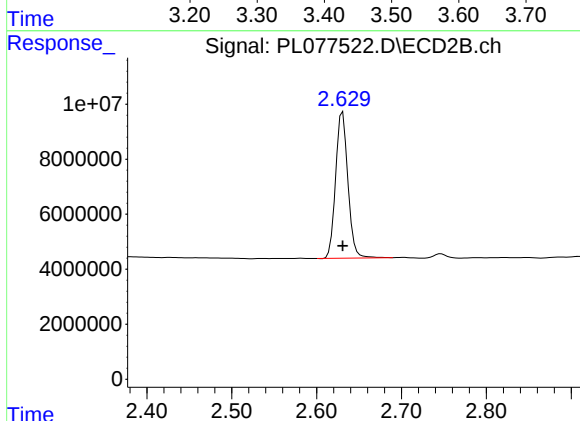


#1 Tetrachloro-m-xylene

R.T.: 2.631 min
Delta R.T.: 0.000 min
Response: 53476994
Conc: 20.10 ng/ml

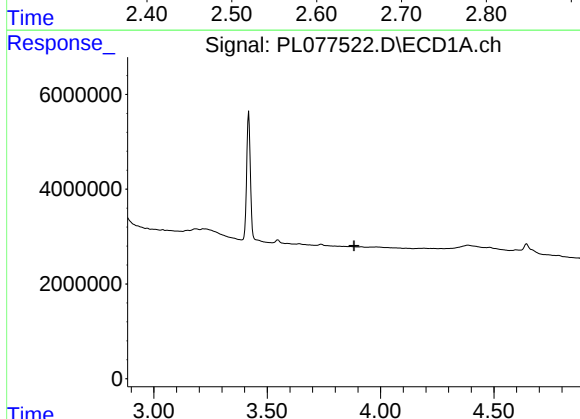


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.883 min
Response: 0
Conc: N.D.

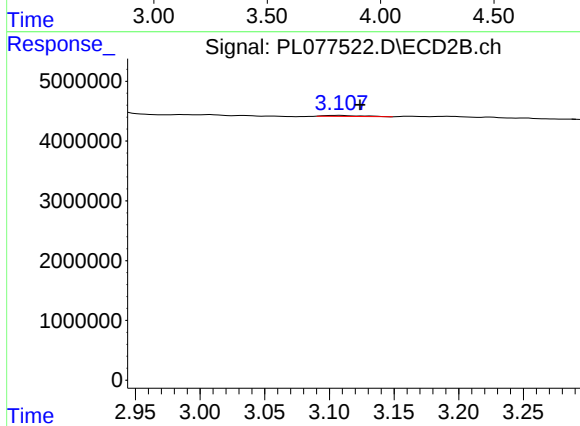

#2 alpha-BHC


R.T.: 3.108 min
Delta R.T.: -0.015 min
Response: 333010
Conc: 0.08 ng/ml

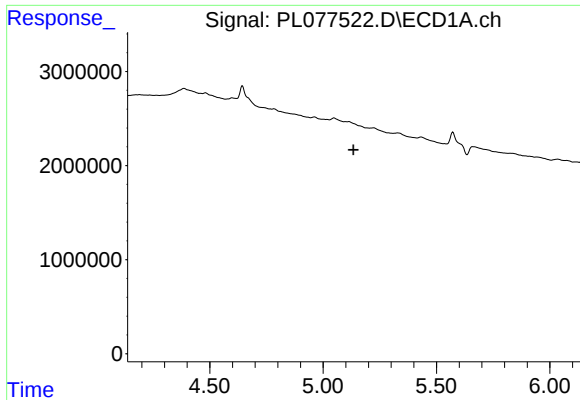

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.134 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

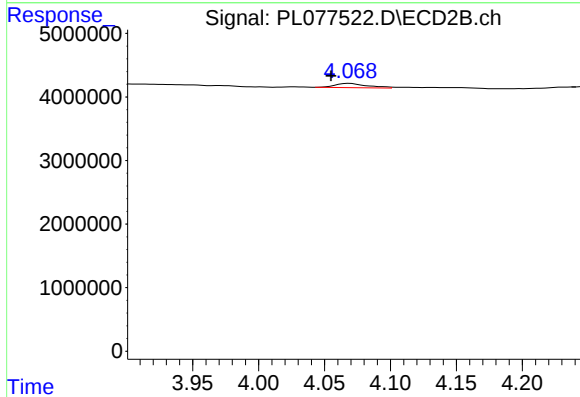


#5 Aldrin

R.T.: 4.069 min
Delta R.T.: 0.014 min
Response: 1097285
Conc: 0.33 ng/ml

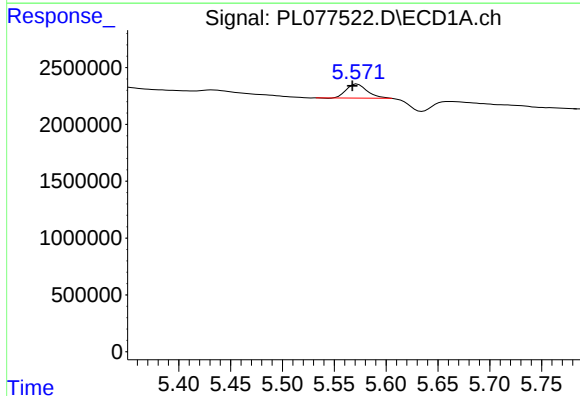


#8 Heptachlor epoxide

R.T.: 5.572 min
Delta R.T.: 0.004 min
Response: 1751044
Conc: 1.31 ng/ml

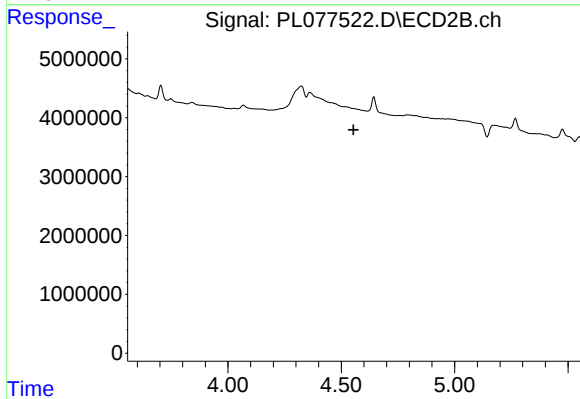

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.554 min
Response: 0
Conc: N.D.

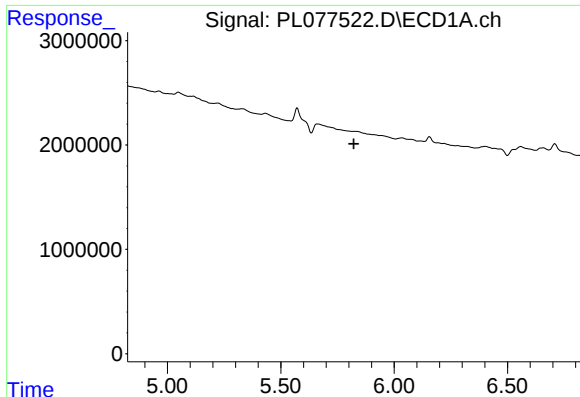

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.822 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

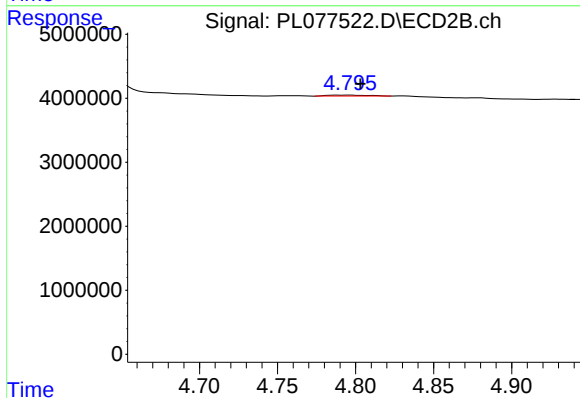


#10 gamma-Chlordane

R.T.: 4.796 min
Delta R.T.: -0.007 min
Response: 262650
Conc: 0.09 ng/ml

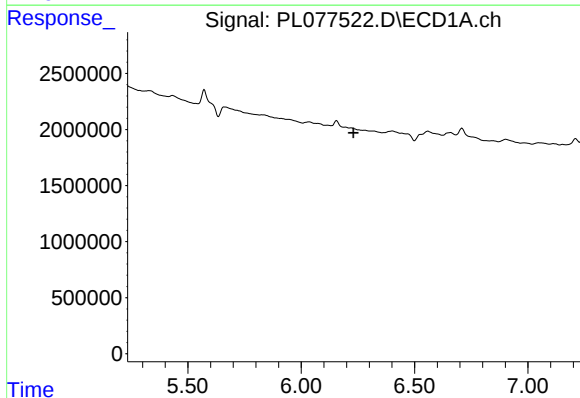


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

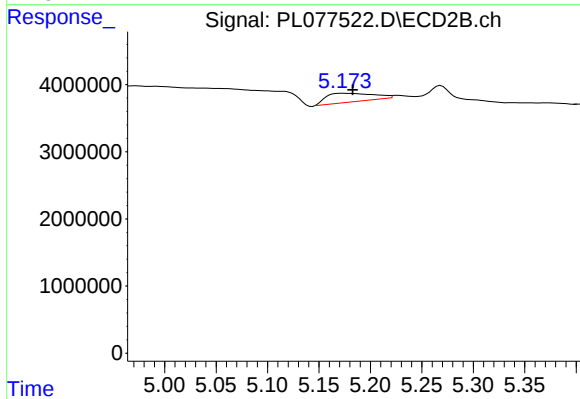

#13 Dieldrin


R.T.: 5.174 min
Delta R.T.: -0.009 min
Response: 4179686
Conc: 1.45 ng/ml

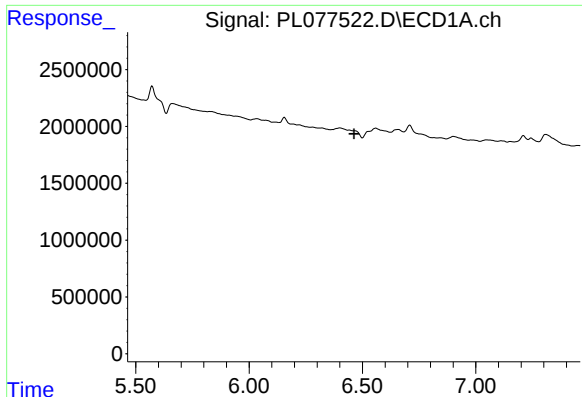

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

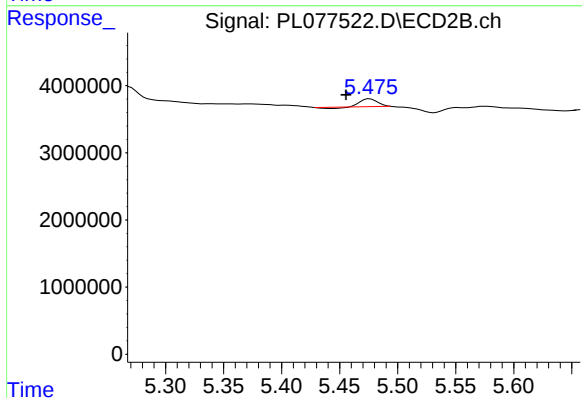


#14 Endrin

R.T.: 5.476 min
Delta R.T.: 0.021 min
Response: 1100164
Conc: 0.48 ng/ml

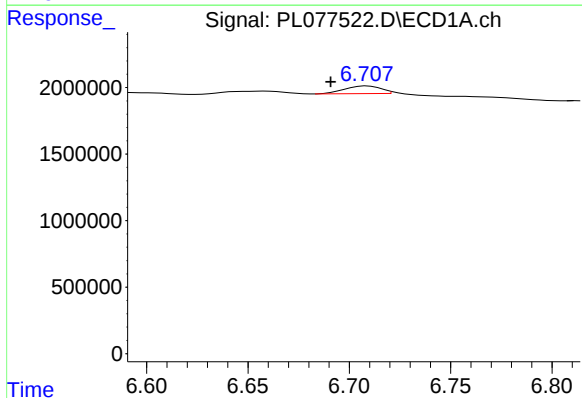


#15 Endosulfan II

R.T.: 6.709 min
Delta R.T.: 0.018 min
Response: 709227
Conc: 0.63 ng/ml

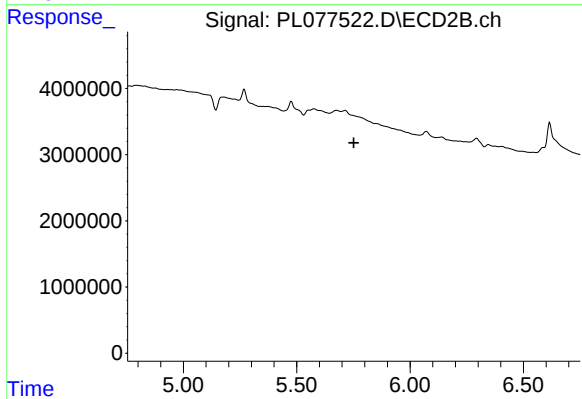

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.751 min
Response: 0
Conc: N.D.

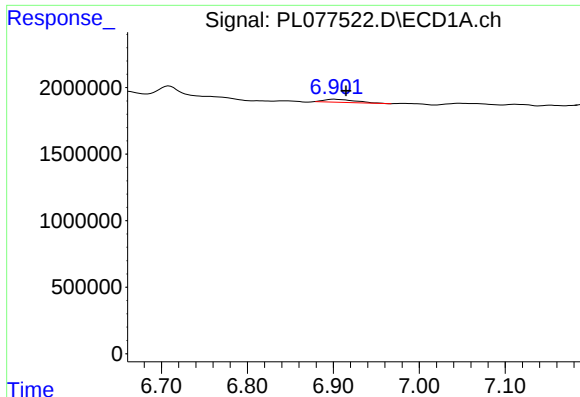

#17 4,4'-DDT


R.T.: 6.901 min
Delta R.T.: -0.014 min
Response: 574300
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

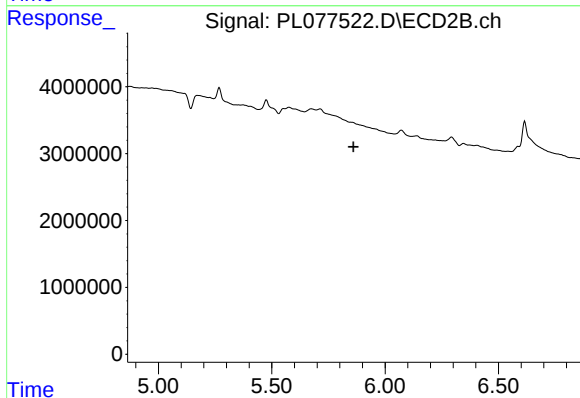


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.861 min
Response: 0
Conc: N.D.

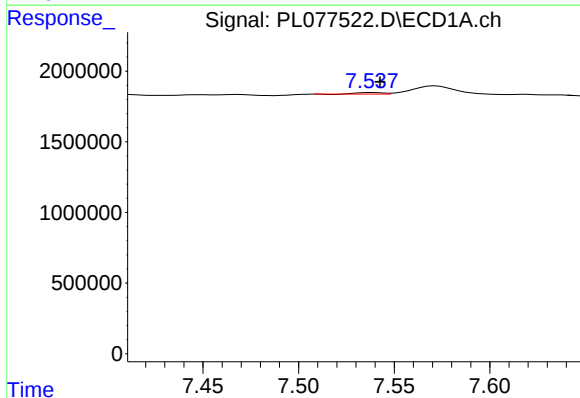


#21 Endrin ketone

R.T.: 7.538 min
Delta R.T.: -0.004 min
Response: 97215
Conc: 0.08 ng/ml

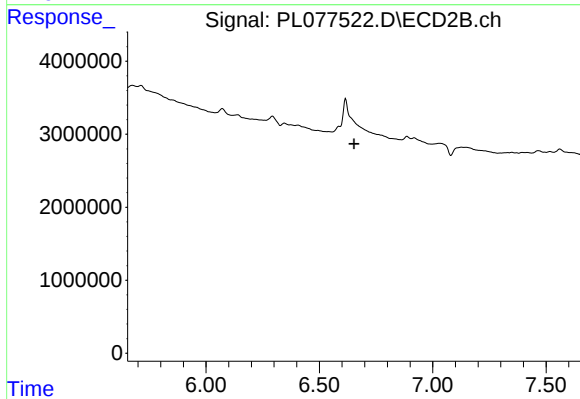

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.653 min
Response: 0
Conc: N.D.

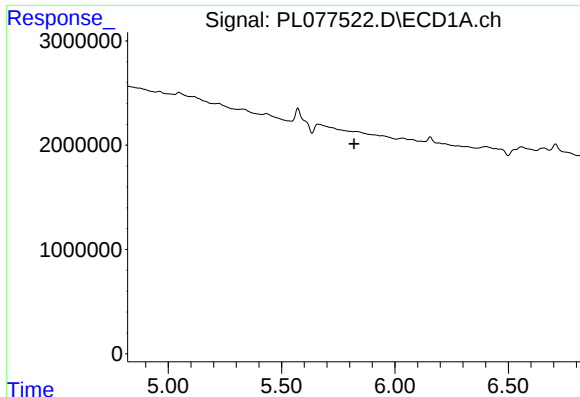

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

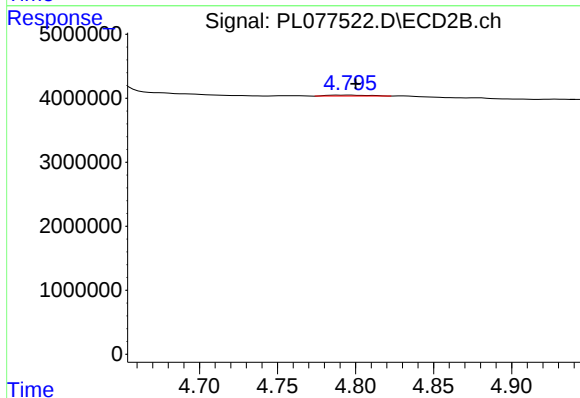


#25 Chlordane-3

R.T.: 4.796 min
Delta R.T.: -0.004 min
Response: 262650
Conc: 0.87 ng/ml

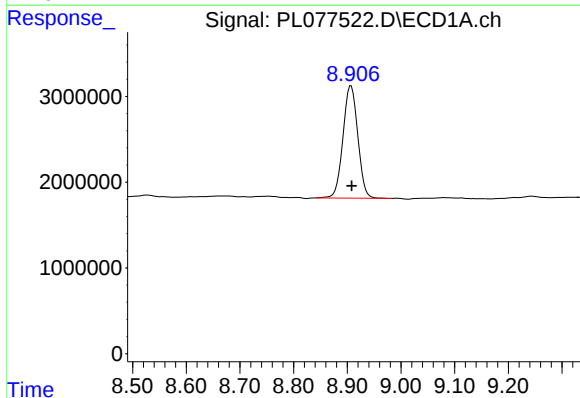

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.001 min
Response: 25149579
Conc: 21.97 ng/ml

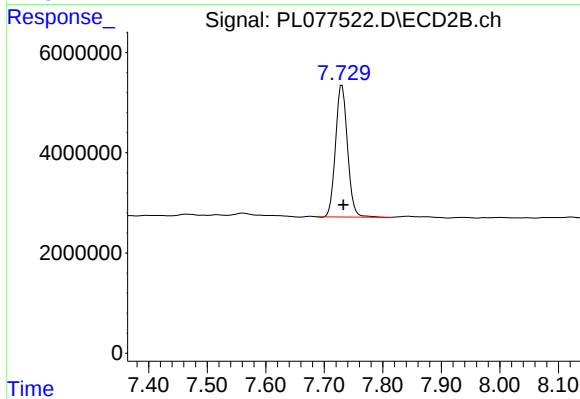

#28 Decachlorobiphenyl

R.T.: 7.730 min
Delta R.T.: -0.002 min
Response: 37339882
Conc: 15.82 ng/ml