

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090622\
 Data File : PL077512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2022 08:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/07/2022
 Supervised By : Ankita Jodhani 09/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 14:16:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 03 05:19:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.632	35620008	56522576	25.878	21.246
28)	SA Decachlor...	8.910	7.731	23997118	34059406	20.966	14.433m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090622\
Data File : PL077512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2022 08:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/07/2022
Supervised By : Ankita Jodhani 09/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 14:16:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090222.M
Quant Title : GC Extractables
QLast Update : Sat Sep 03 05:19:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

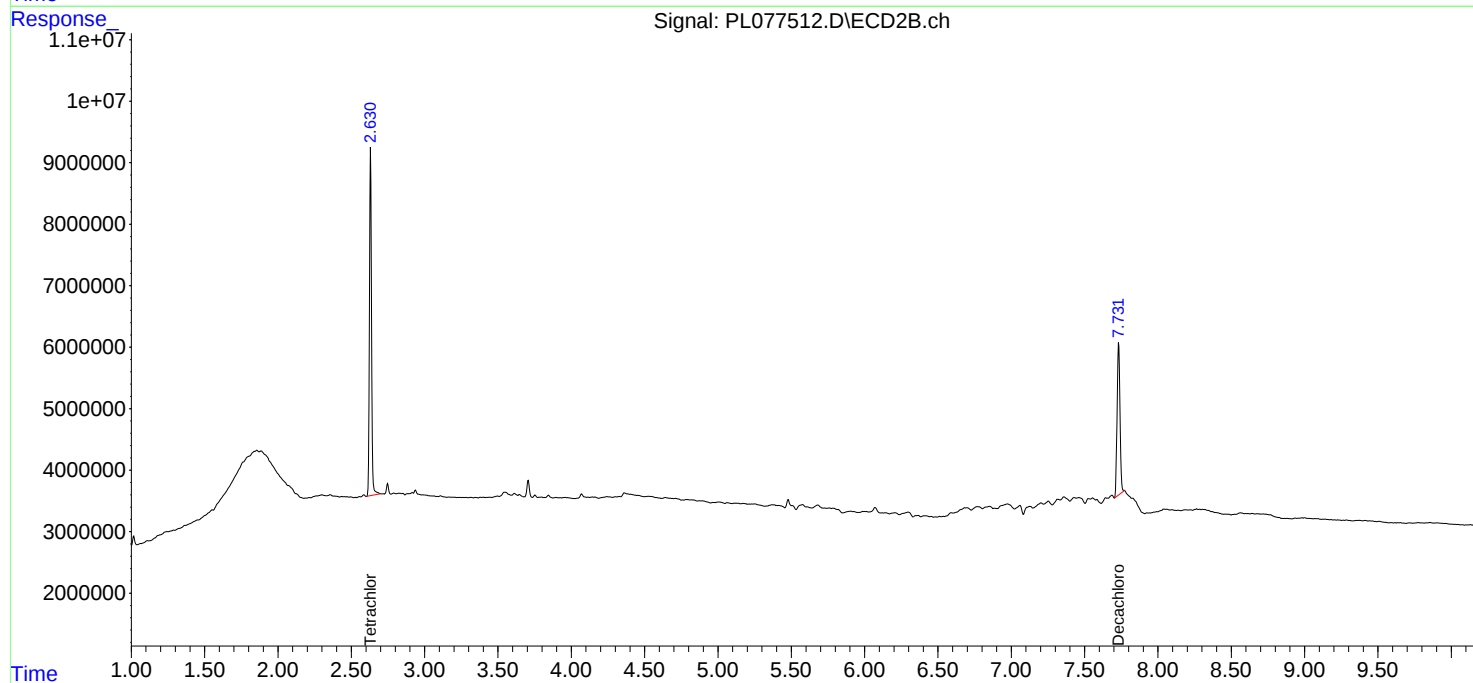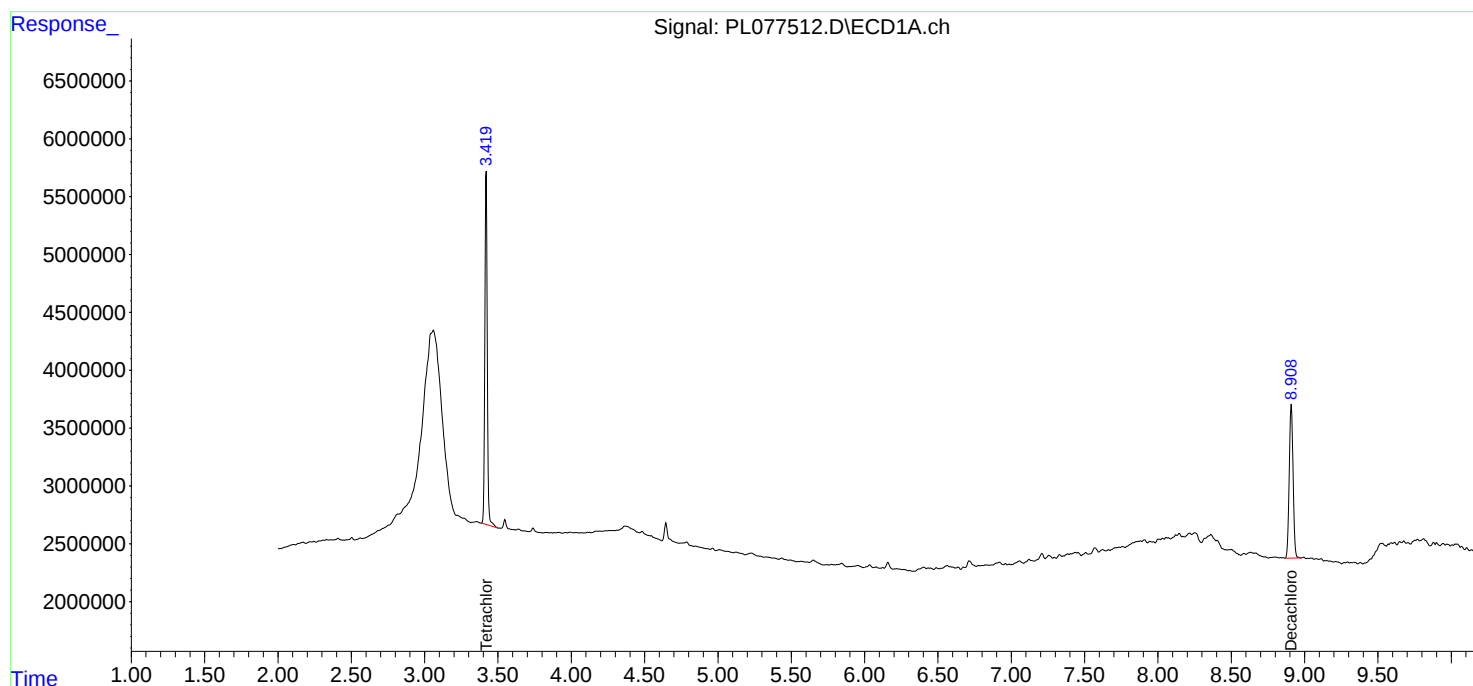

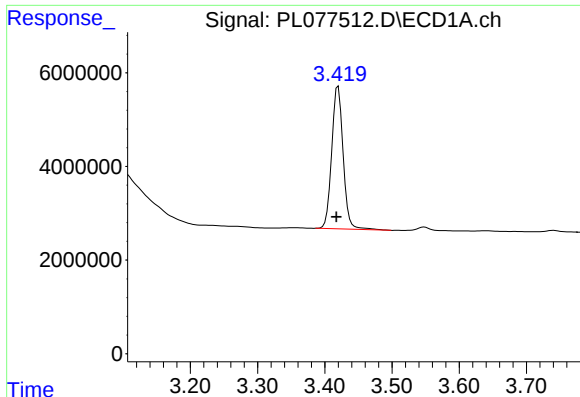


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.003 min
Response: 35620008
Conc: 25.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/07/2022
Supervised By :Ankita Jodhani 09/07/2022

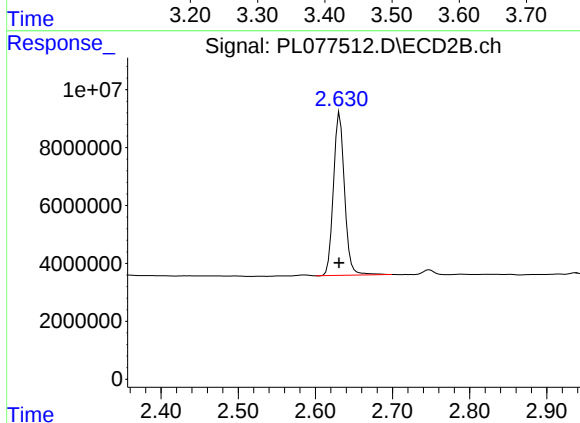


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: 0.000 min
Response: 56522576
Conc: 21.25 ng/ml

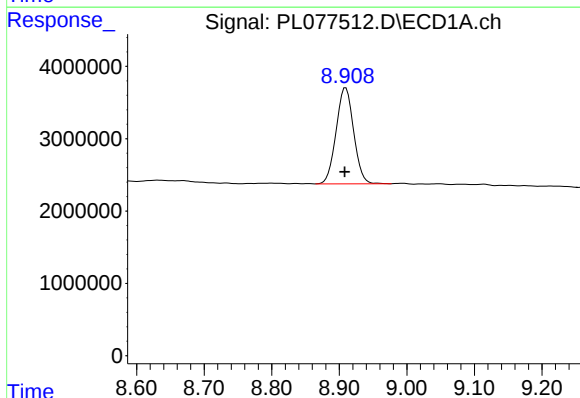

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.001 min
Response: 23997118
Conc: 20.97 ng/ml

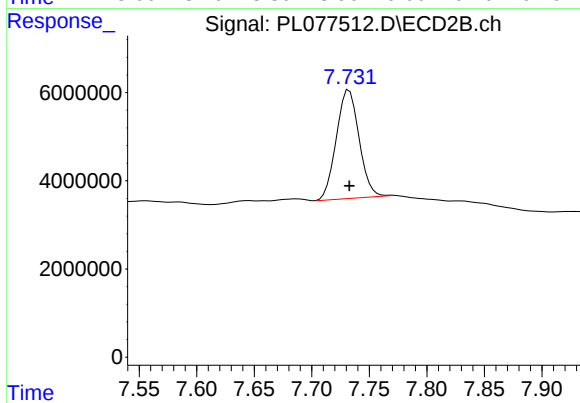

#28 Decachlorobiphenyl

R.T.: 7.731 min
Delta R.T.: -0.002 min
Response: 34059406
Conc: 14.43 ng/ml m