

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090623\
 Data File : PL085139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 12:22
 Operator : AR\AJ
 Sample : 04238-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 20:52:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.479	2.685	34762018	16597126	14.212	14.608
28) SA Decachlor...	9.030	7.865	40304934	21213761	25.064	15.937 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090623\
Data File : PL085139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 12:22
Operator : AR\AJ
Sample : 04238-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 20:52:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

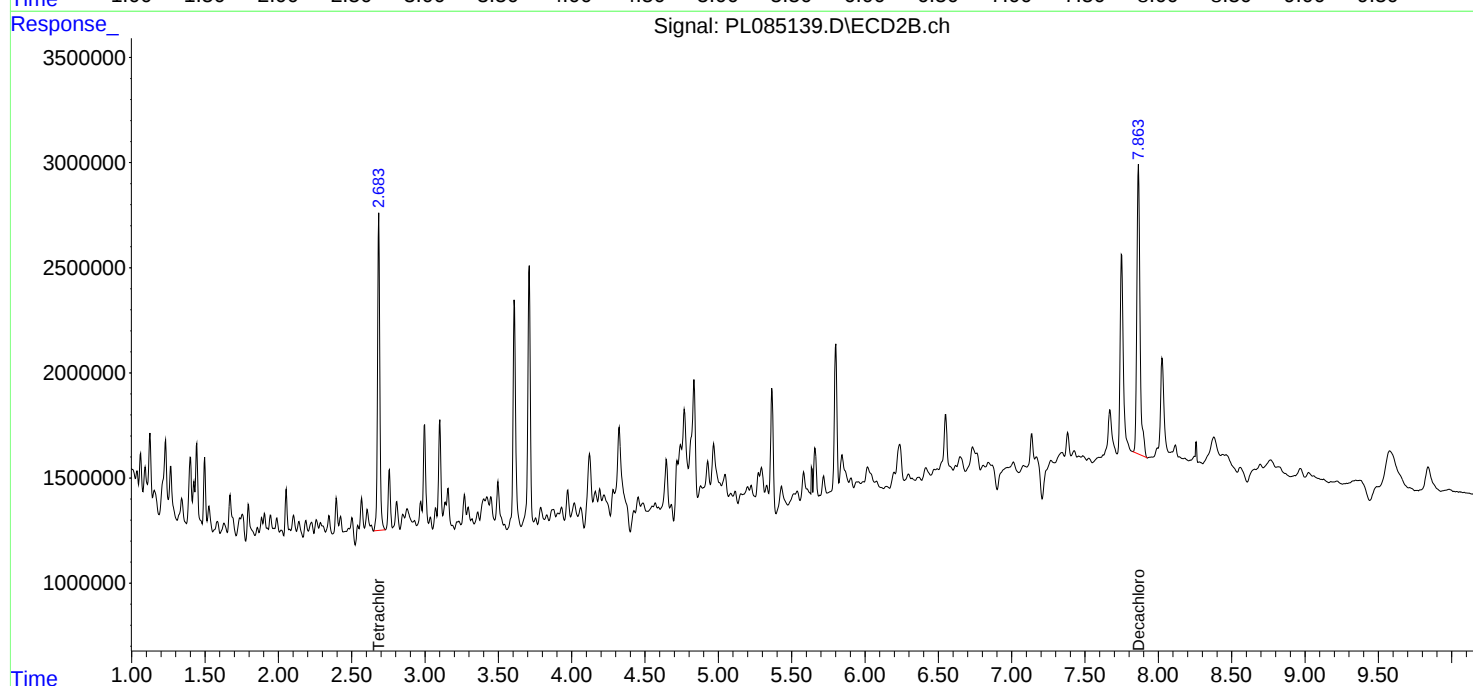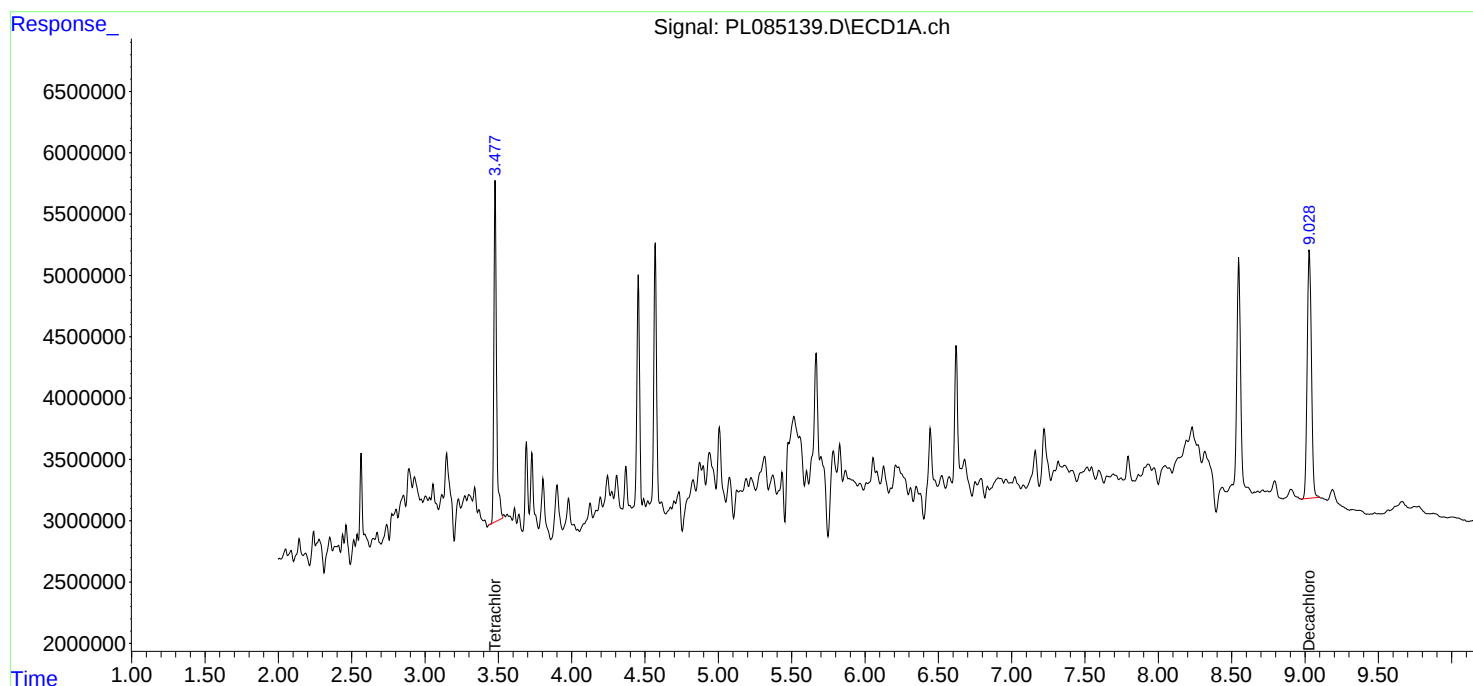


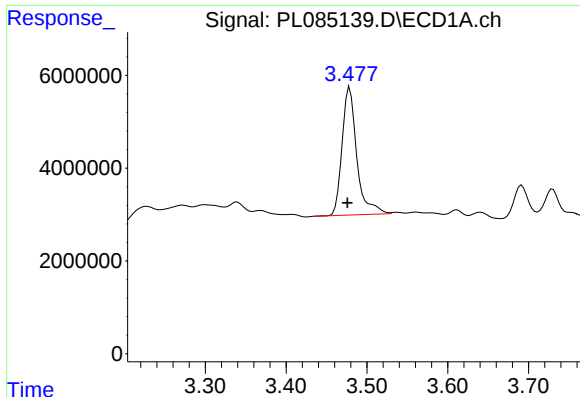

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.003 min
Response: 34762018
Conc: 14.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT

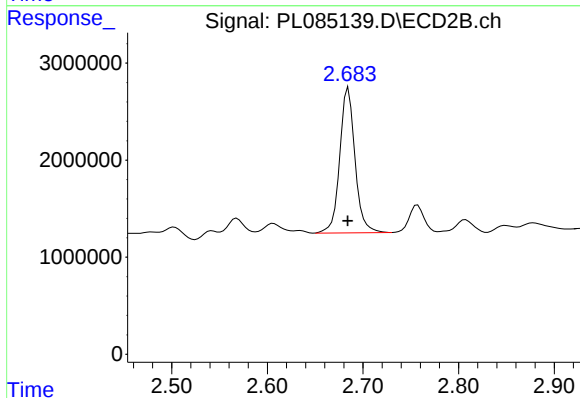


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 16597126
Conc: 14.61 ng/ml

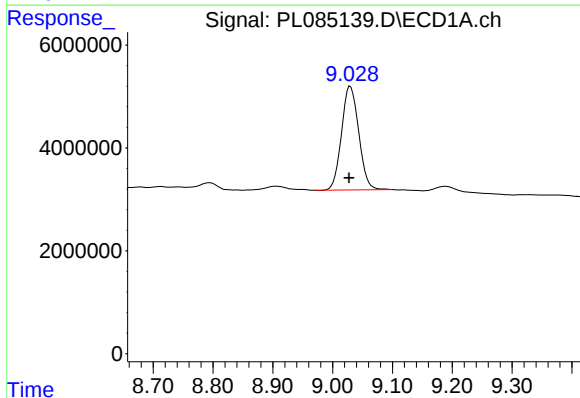

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: 0.003 min
Response: 40304934
Conc: 25.06 ng/ml

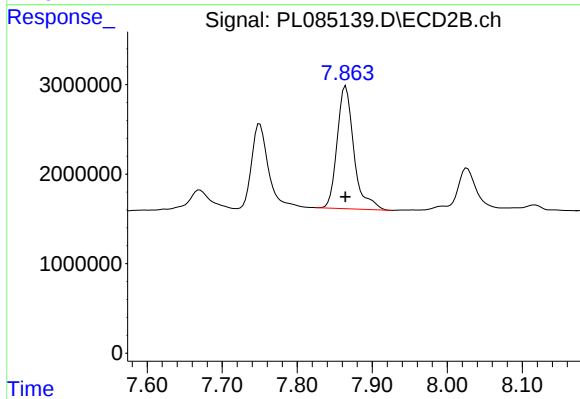

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 21213761
Conc: 15.94 ng/ml