

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090718\
 Data File : PL039740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2018 13:06
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 04:26:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
3)	MA	gamma-BHC...	3.969f	0.000	2114068	0	0.199	N.D.	#
8)	B	Heptachlo...	4.922f	5.740	24365571	26912542	2.552	8.002	#
9)	A	Endosulfan I	5.300	0.000	15638261	0	1.786	N.D.	#
11)	B	alpha-Chl...	5.300f	0.000	15638261	0	1.628	N.D.	#
14)	MA	Endrin	5.796	0.000	10715374	0	1.197	N.D.	#
15)	B	Endosulfa...	6.076	0.000	39975544	0	4.597	N.D.	#
17)	MA	4,4'-DDT	6.133	0.000	27238066	0	3.593	N.D.	#
21)	B	Endrin ke...	6.877f	0.000	115.5E6	0	13.415	N.D.	#
23)		Chlordane-1	4.108	0.000	12346482	0	38.999	N.D.	#
26)		Chlordane-4	5.300	0.000	15638261	0	15.648	N.D.	#
27)		Chlordane-5	6.076	0.000	39975544	0	123.256	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090718\
Data File : PL039740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2018 13:06
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 04:26:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

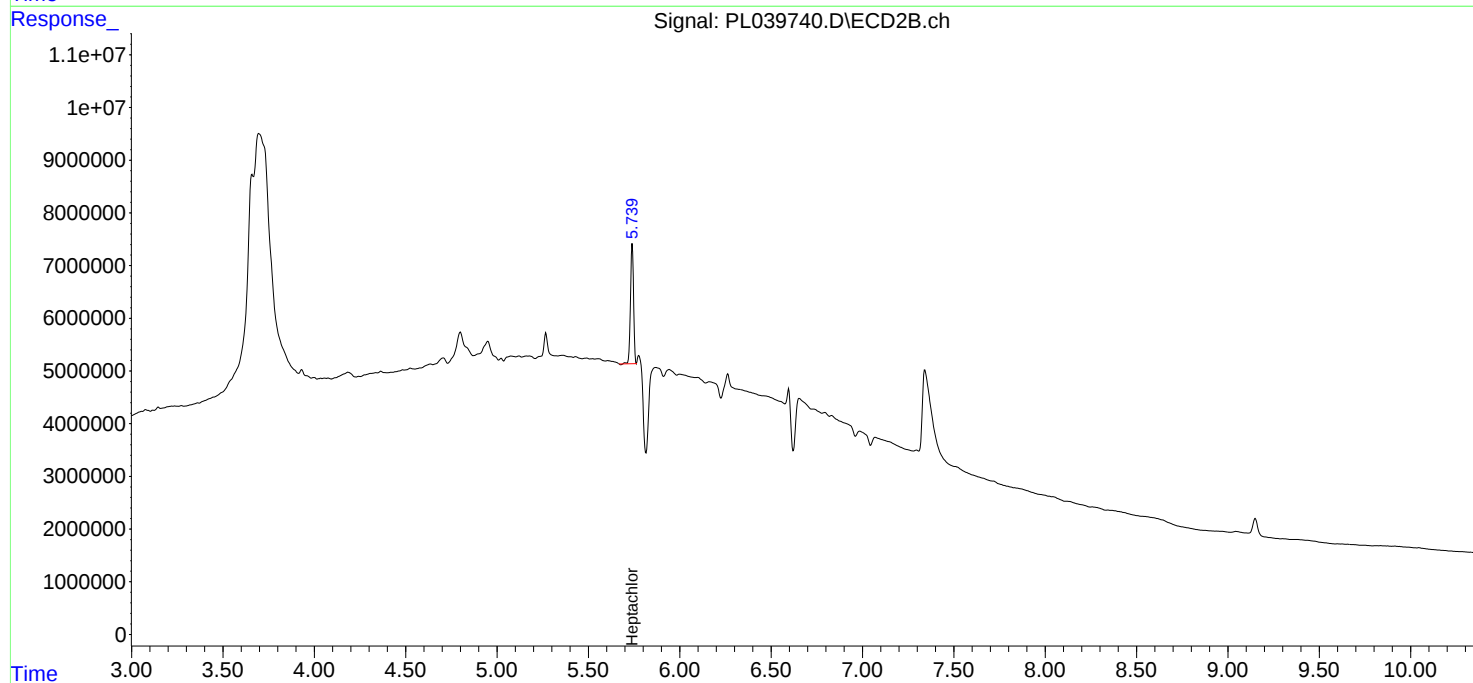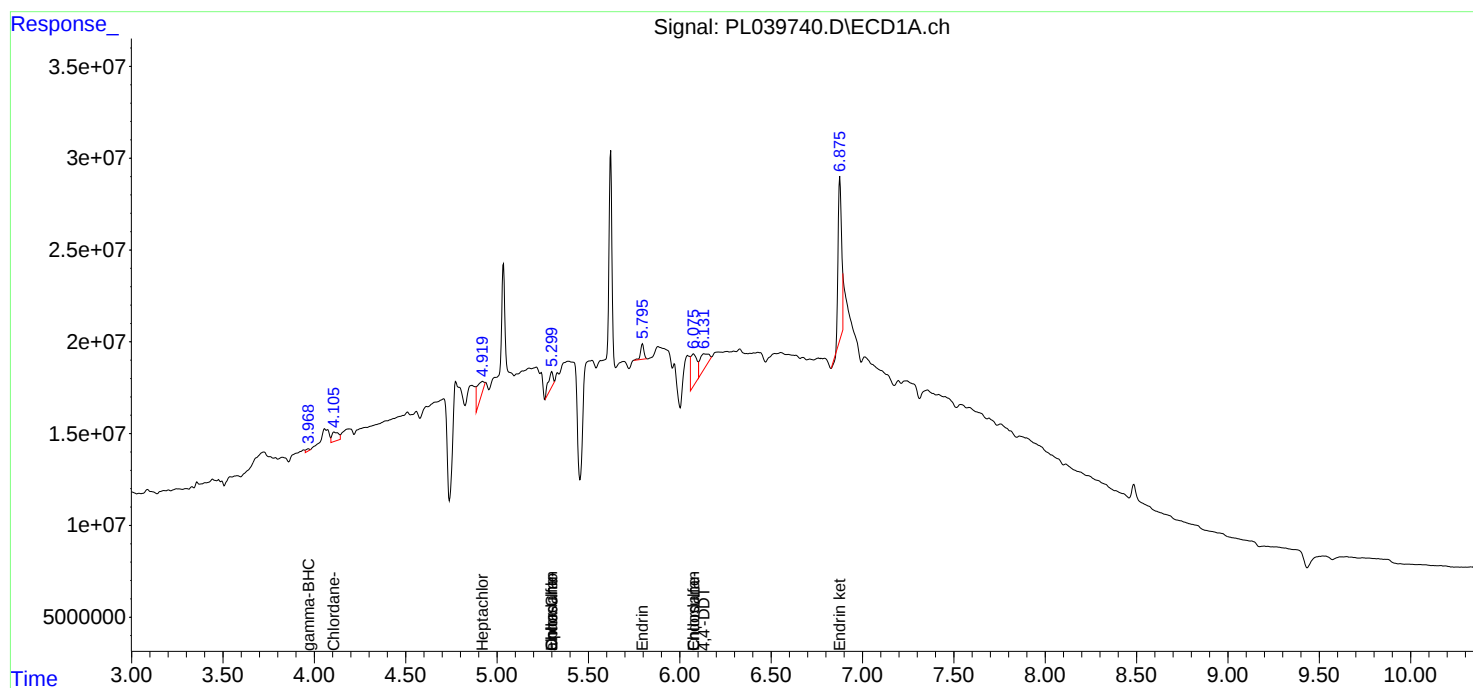


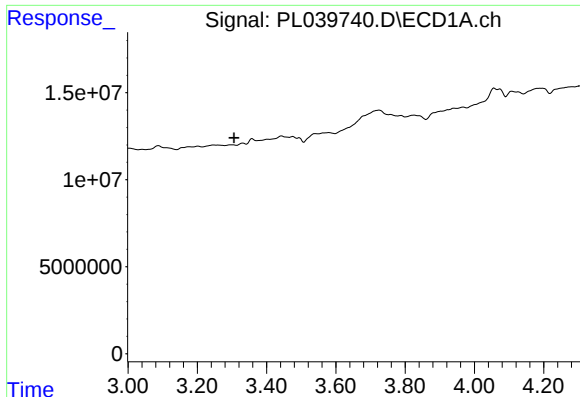

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

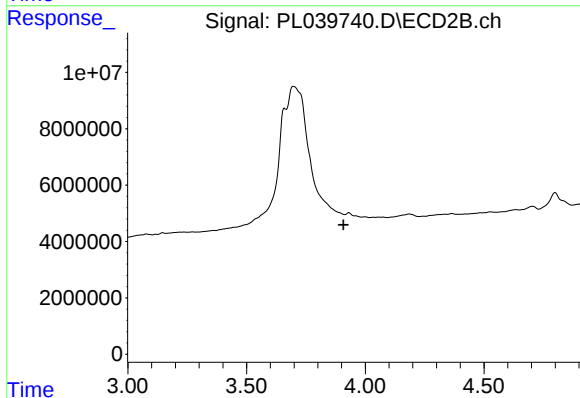


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.

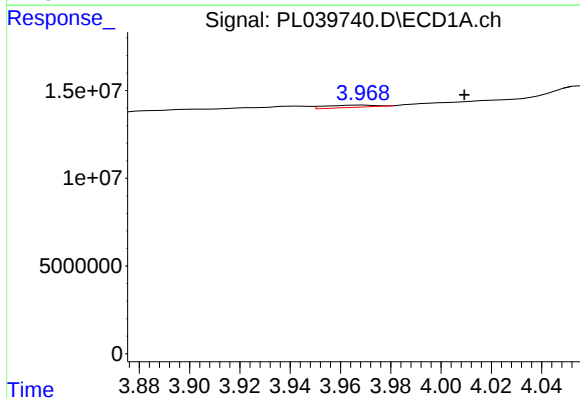


#3 gamma-BHC (Lindane)

R.T.: 3.969 min
Delta R.T.: -0.040 min
Response: 2114068
Conc: 0.20 ng/ml

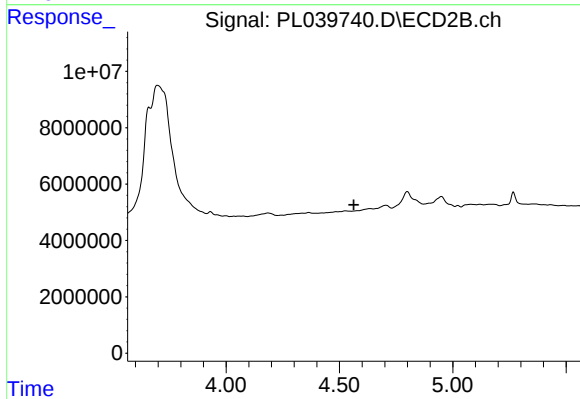

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

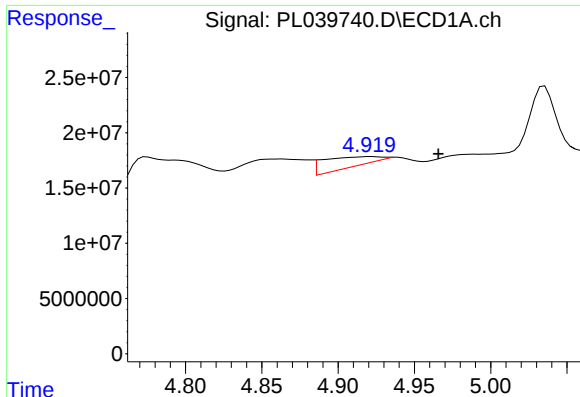

#8 Heptachlor epoxide


R.T.: 4.922 min
Delta R.T.: -0.044 min
Response: 24365571
Conc: 2.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

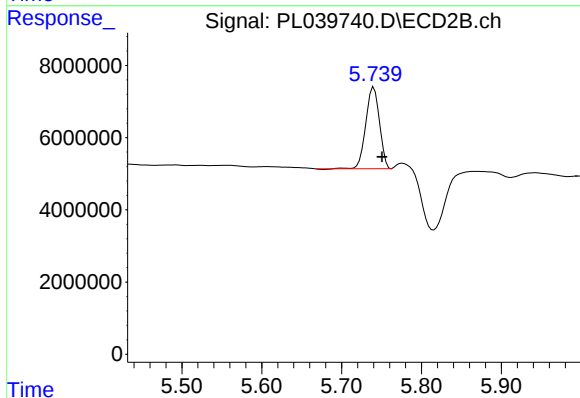


#8 Heptachlor epoxide

R.T.: 5.740 min
Delta R.T.: -0.011 min
Response: 26912542
Conc: 8.00 ng/ml

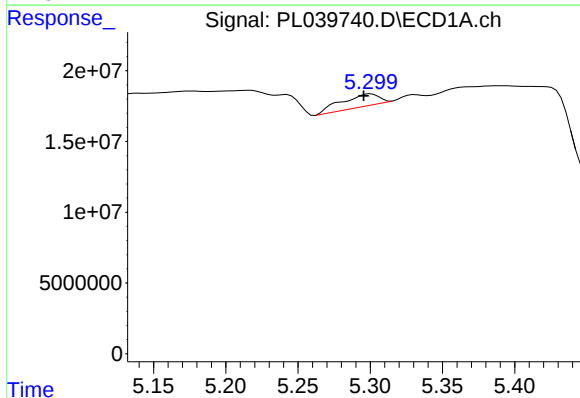


#9 Endosulfan I

R.T.: 5.300 min
Delta R.T.: 0.005 min
Response: 15638261
Conc: 1.79 ng/ml

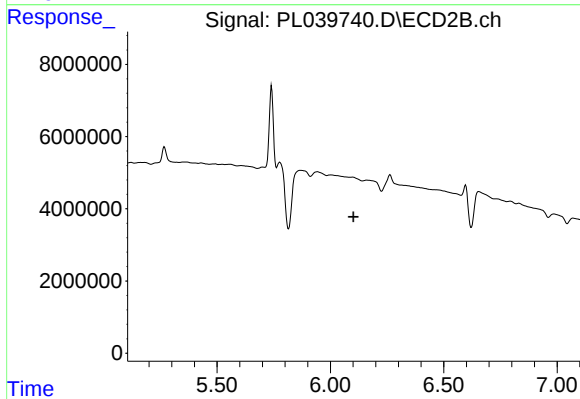

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.102 min
Response: 0
Conc: N.D.

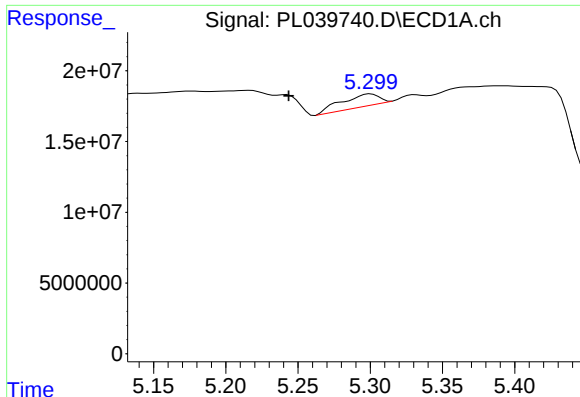

#11 alpha-Chlordane


R.T.: 5.300 min
Delta R.T.: 0.057 min
Response: 15638261
Conc: 1.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

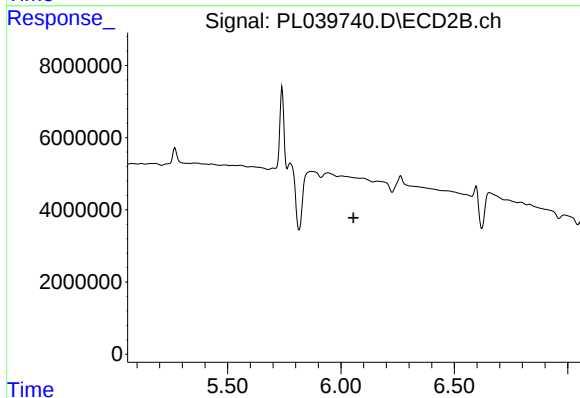


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

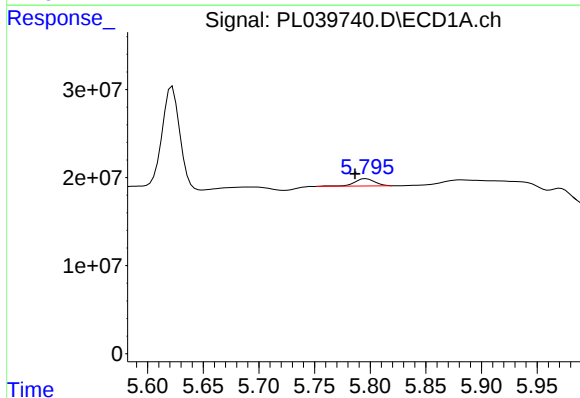


#14 Endrin

R.T.: 5.796 min
Delta R.T.: 0.010 min
Response: 10715374
Conc: 1.20 ng/ml

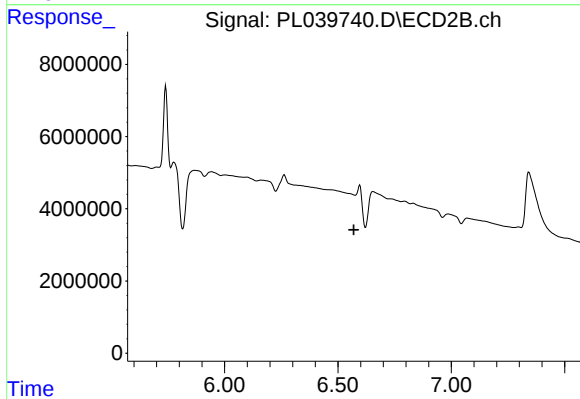

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

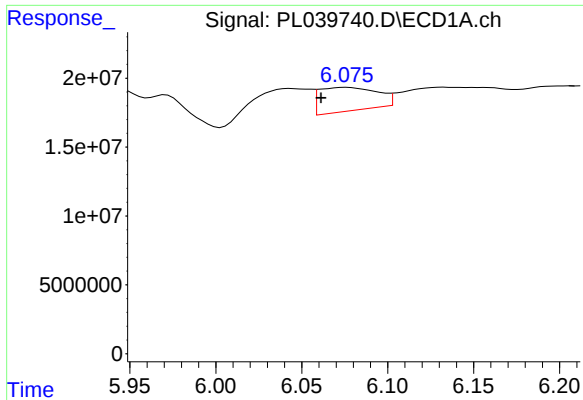

#15 Endosulfan II


R.T.: 6.076 min
Delta R.T.: 0.015 min
Response: 39975544
Conc: 4.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

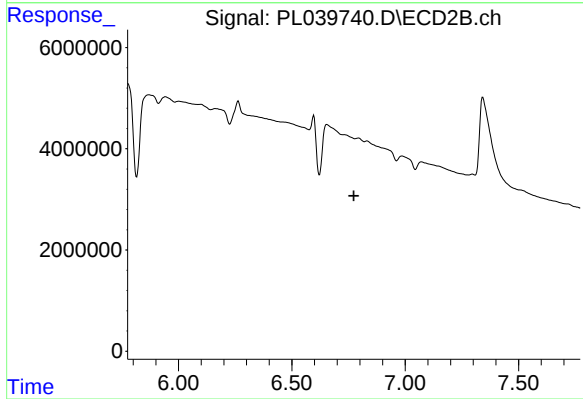


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

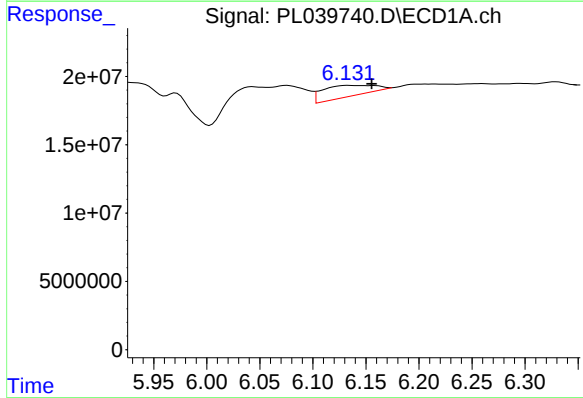


#17 4,4'-DDT

R.T.: 6.133 min
Delta R.T.: -0.023 min
Response: 27238066
Conc: 3.59 ng/ml

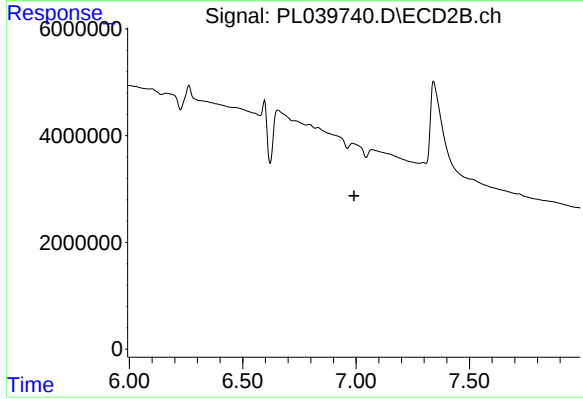

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

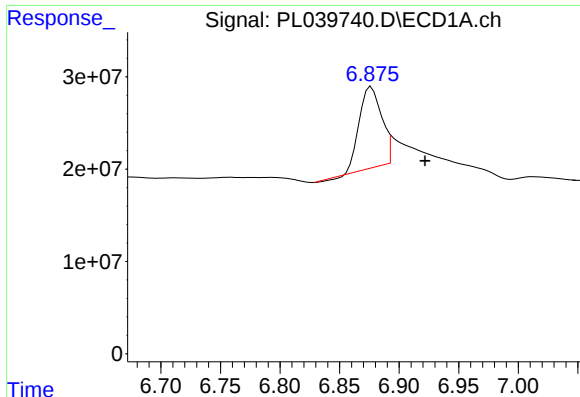

#21 Endrin ketone


R.T.: 6.877 min
Delta R.T.: -0.045 min
Response: 115456848
Conc: 13.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

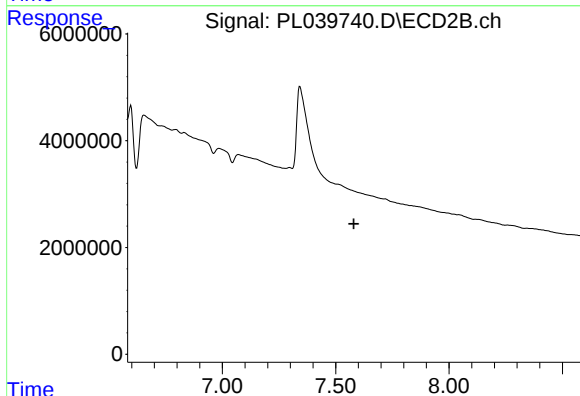


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.580 min
Response: 0
Conc: N.D.

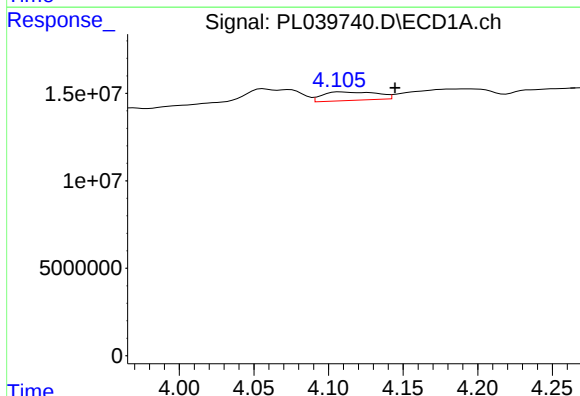


#23 Chlordane-1

R.T.: 4.108 min
Delta R.T.: -0.037 min
Response: 12346482
Conc: 39.00 ng/ml

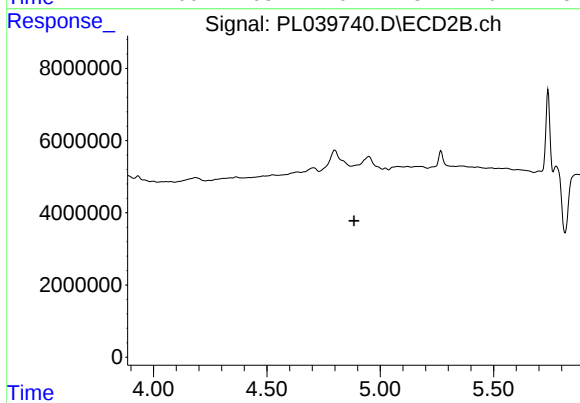

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

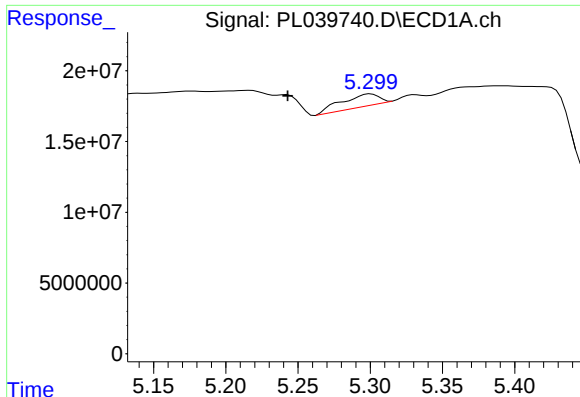

#26 Chlordane-4


R.T.: 5.300 min
Delta R.T.: 0.057 min
Response: 15638261
Conc: 15.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

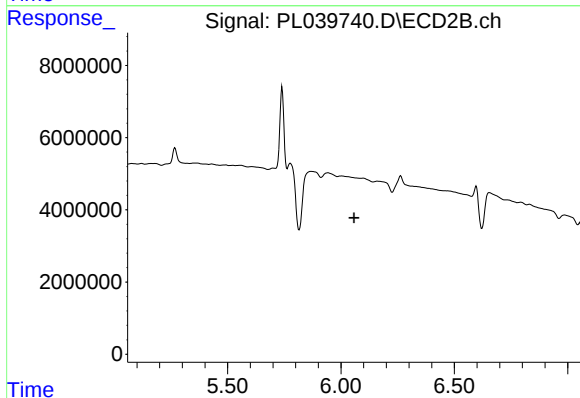


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

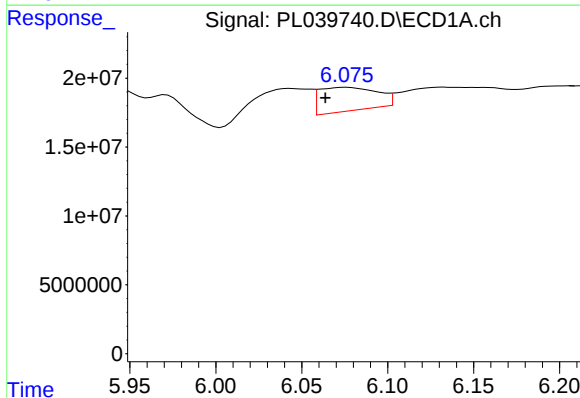


#27 Chlordane-5

R.T.: 6.076 min
Delta R.T.: 0.012 min
Response: 39975544
Conc: 123.26 ng/ml

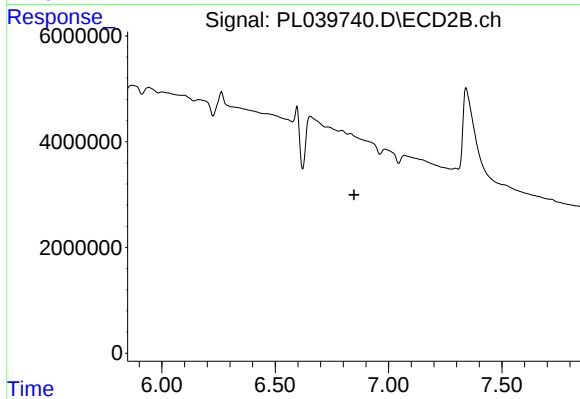

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

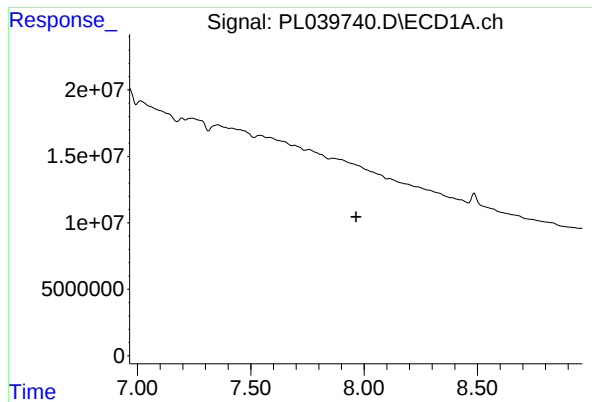

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

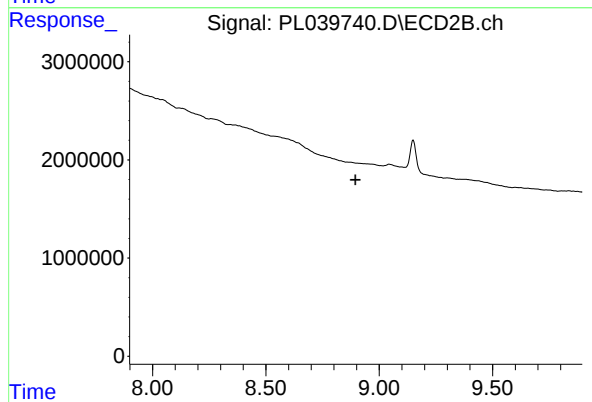

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.