

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090721\
 Data File : PL069743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2021 18:59
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 10:16:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 08 10:15:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.630	5.565	4368463	13613054	10.283	9.858
27)	SA Decachlor...	10.397	11.486	16310607	24109014	21.335	20.191
Target Compounds							
2)	A alpha-BHC	5.336	6.146	5714781	17515167	10.271	9.625
3)	MA gamma-BHC...	5.759	6.542	5648007	16963784	9.955	9.683
4)	MA Heptachlor	6.169	7.191	6681215	16967641	9.975	9.706
9)	A Endosulfan I	7.473	8.435	6207450	13598144	10.079	9.967
13)	MA Dieldrin	7.760	8.725	12858051	28718482	19.297	19.523
14)	MA Endrin	8.051	8.964	12192849	23930831	19.552	19.465
16)	A 4,4'-DDD	8.217	9.106	10257918	22895251	19.001	19.625
17)	MA 4,4'-DDT	8.477	9.424	12156761	24101971	19.492	19.830
20)	A Methoxychlor	9.071	9.910	38750290	64267978	102.544	100.724


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090721\
Data File : PL069743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2021 18:59
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 10:16:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 08 10:15:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

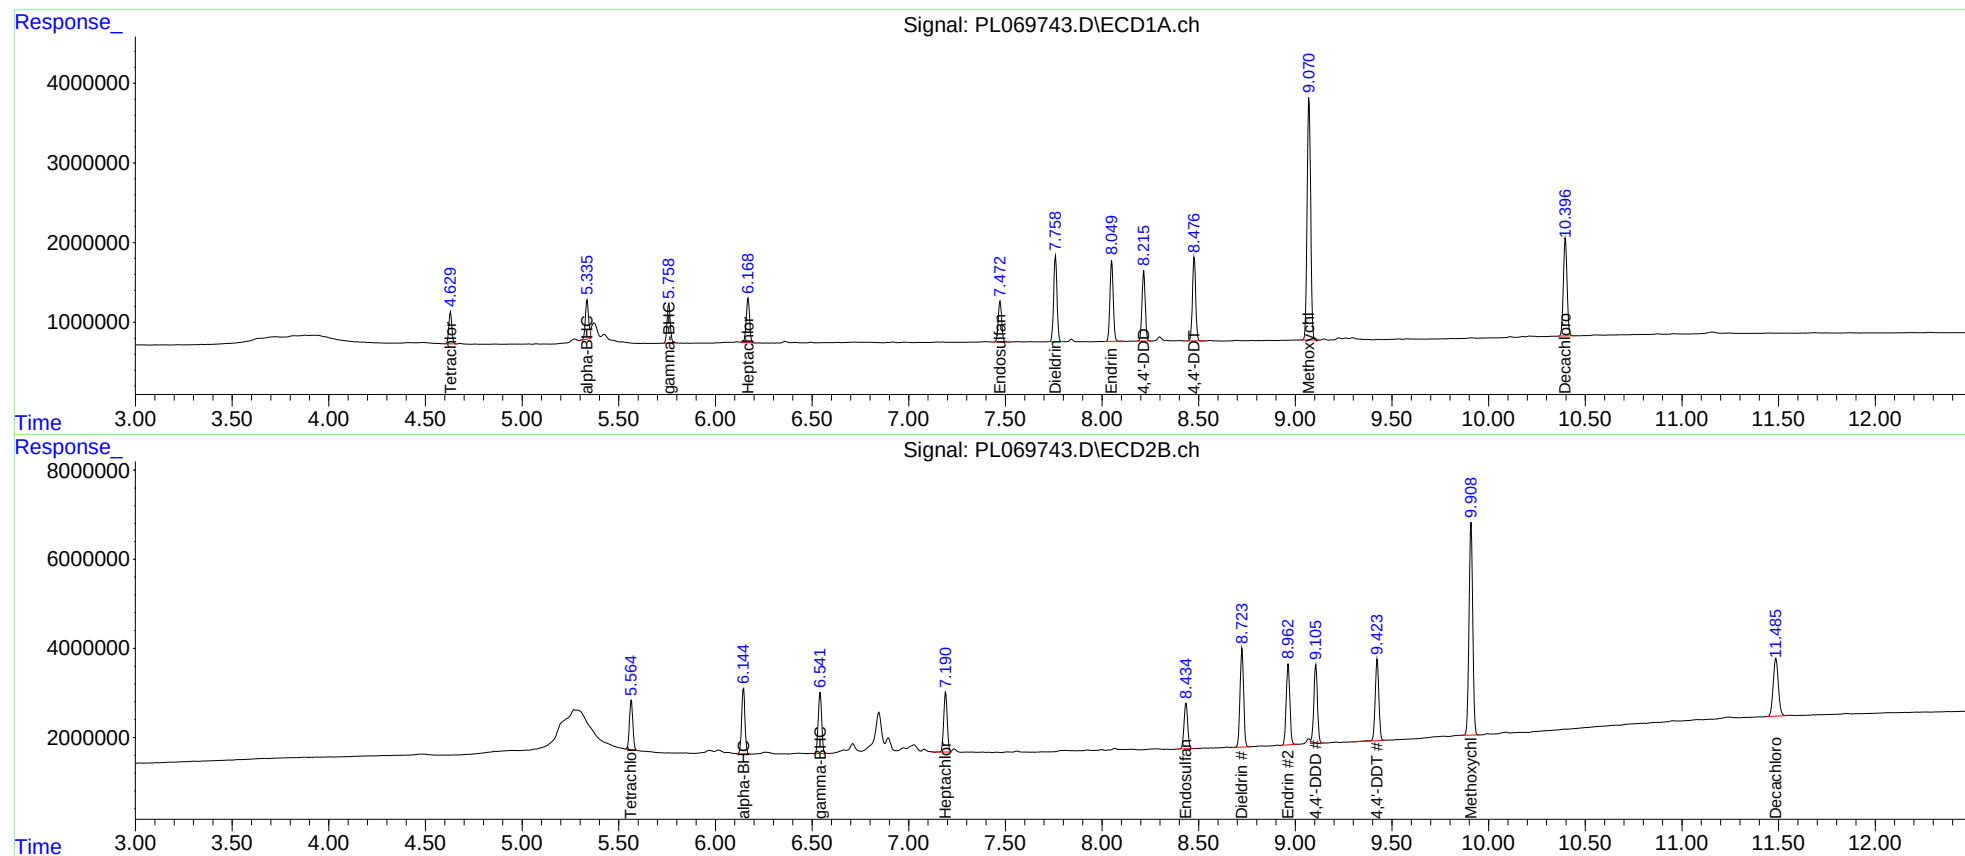

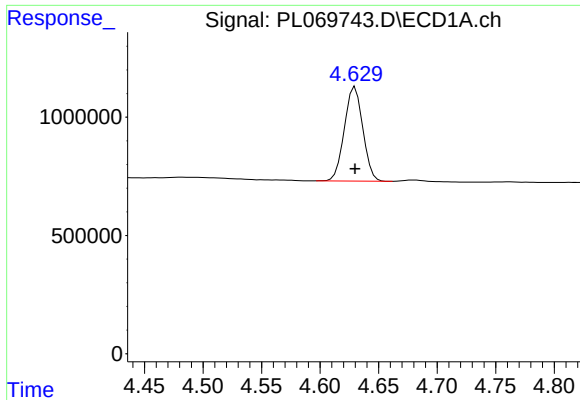


#1 Tetrachloro-m-xylene

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 4368463
Conc: 10.28 ng/ml

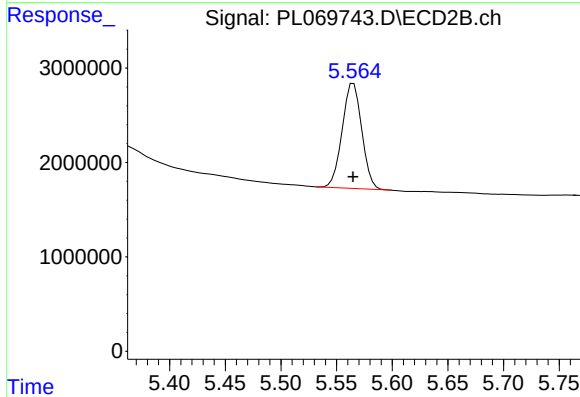


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 13613054
Conc: 9.86 ng/ml

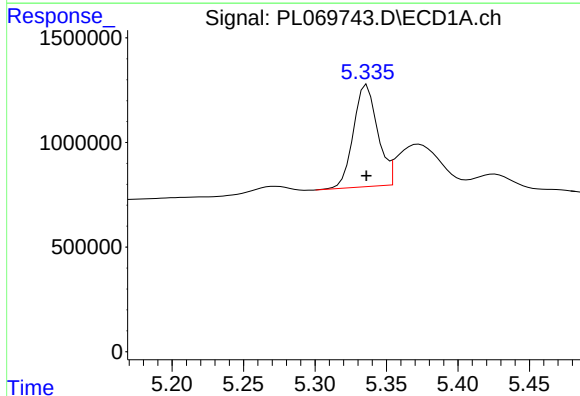


#2 alpha-BHC

R.T.: 5.336 min
Delta R.T.: 0.000 min
Response: 5714781
Conc: 10.27 ng/ml

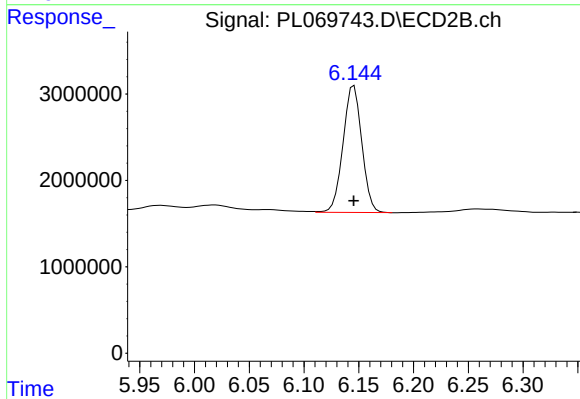


#2 alpha-BHC

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 17515167
Conc: 9.63 ng/ml

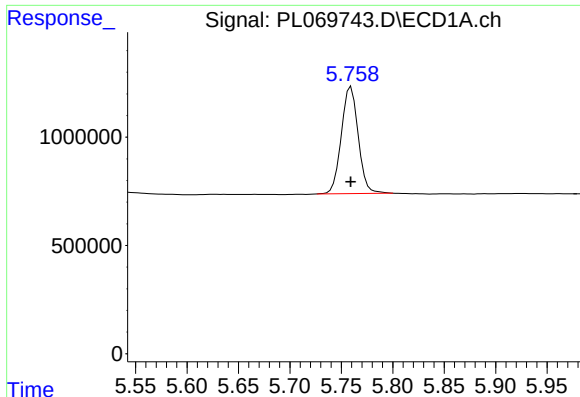


#3 gamma-BHC (Lindane)

R.T.: 5.759 min
Delta R.T.: 0.000 min
Response: 5648007
Conc: 9.96 ng/ml

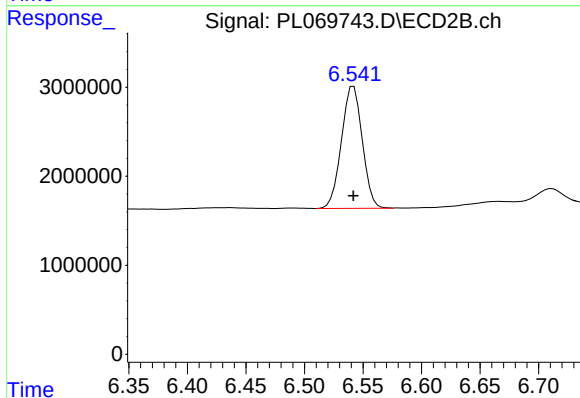


#3 gamma-BHC (Lindane)

R.T.: 6.542 min
Delta R.T.: 0.000 min
Response: 16963784
Conc: 9.68 ng/ml

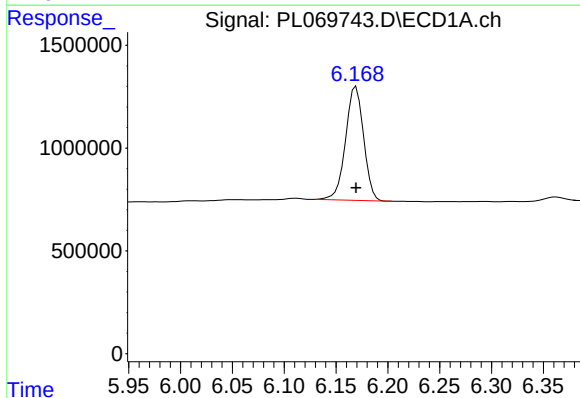


#4 Heptachlor

R.T.: 6.169 min
Delta R.T.: 0.000 min
Response: 6681215
Conc: 9.98 ng/ml

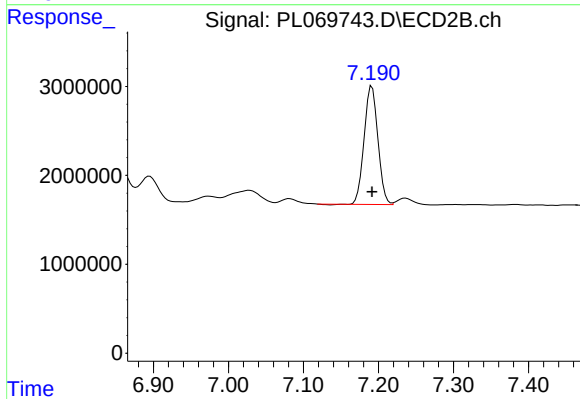


#4 Heptachlor

R.T.: 7.191 min
Delta R.T.: 0.000 min
Response: 16967641
Conc: 9.71 ng/ml

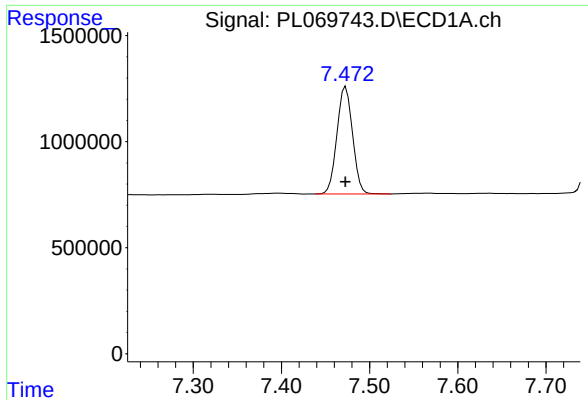


#9 Endosulfan I

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 6207450
Conc: 10.08 ng/ml

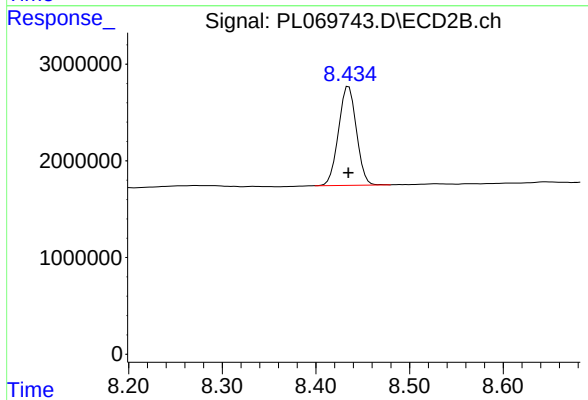


#9 Endosulfan I

R.T.: 8.435 min
Delta R.T.: 0.000 min
Response: 13598144
Conc: 9.97 ng/ml

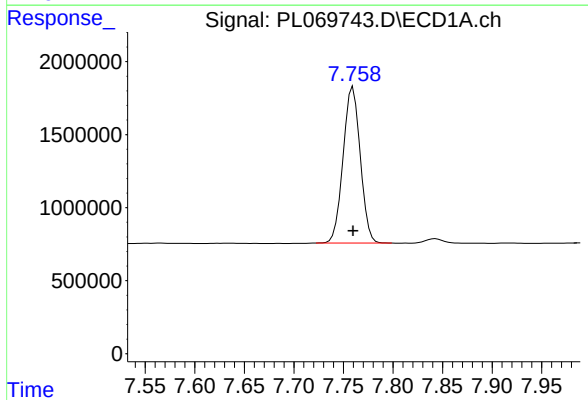


#13 Dieldrin

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 12858051
Conc: 19.30 ng/ml

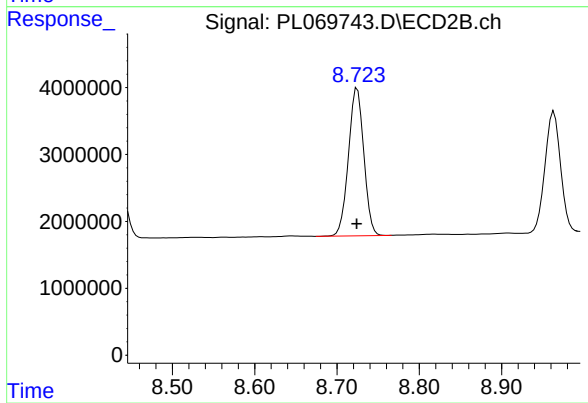


#13 Dieldrin

R.T.: 8.725 min
Delta R.T.: 0.000 min
Response: 28718482
Conc: 19.52 ng/ml

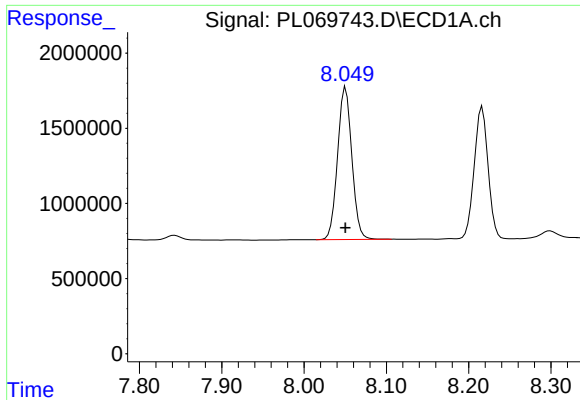


#14 Endrin

R.T.: 8.051 min
Delta R.T.: 0.000 min
Response: 12192849
Conc: 19.55 ng/ml

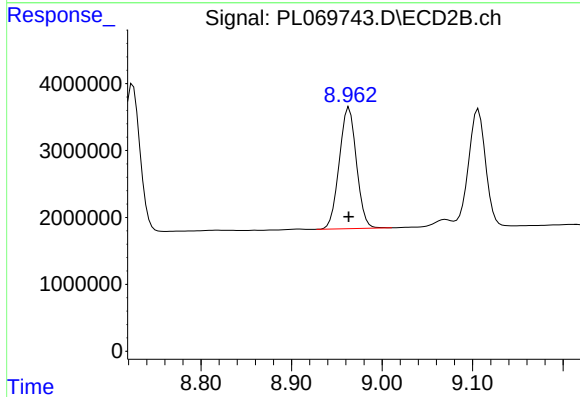


#14 Endrin

R.T.: 8.964 min
Delta R.T.: 0.000 min
Response: 23930831
Conc: 19.46 ng/ml

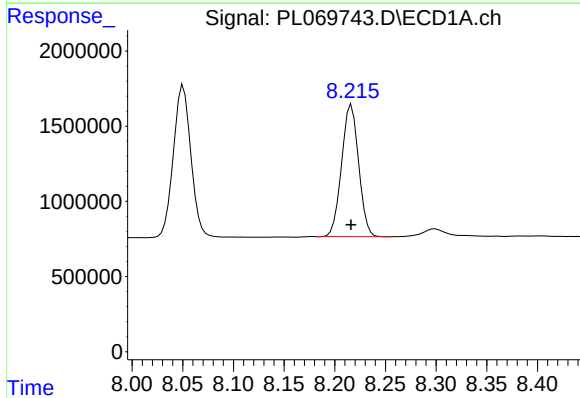


#16 4,4'-DDD

R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 10257918
Conc: 19.00 ng/ml

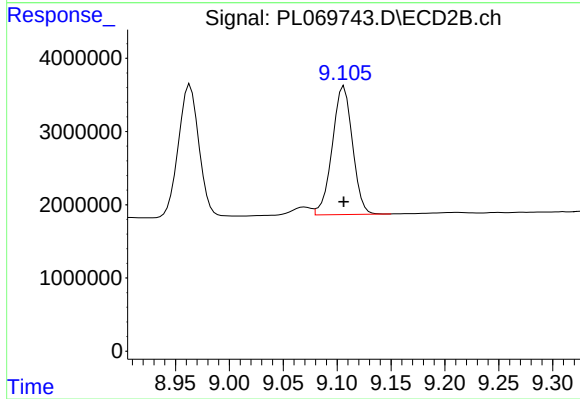


#16 4,4'-DDD

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 22895251
Conc: 19.62 ng/ml

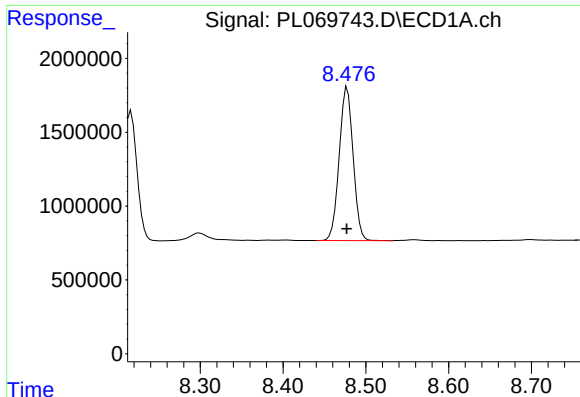


#17 4,4'-DDT

R.T.: 8.477 min
Delta R.T.: 0.000 min
Response: 12156761
Conc: 19.49 ng/ml

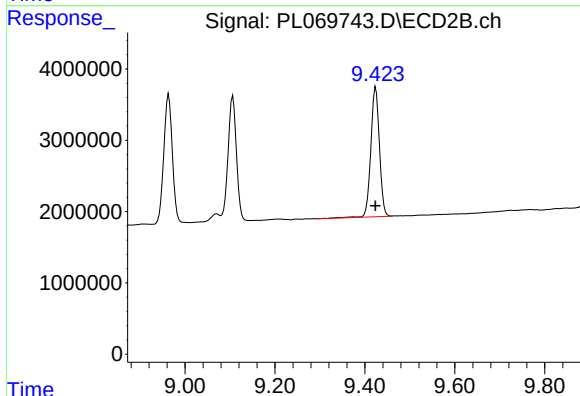


#17 4,4'-DDT

R.T.: 9.424 min
Delta R.T.: 0.000 min
Response: 24101971
Conc: 19.83 ng/ml

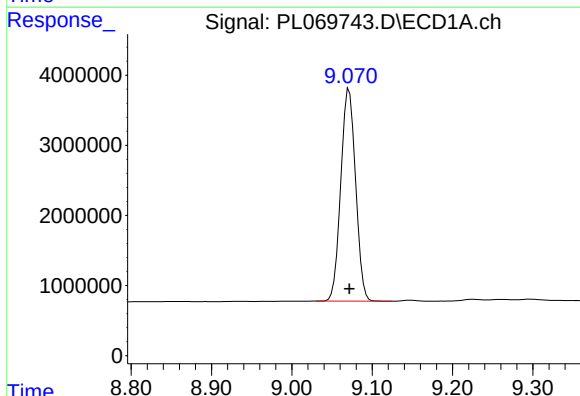


#20 Methoxychlor

R.T.: 9.071 min
Delta R.T.: 0.000 min
Response: 38750290
Conc: 102.54 ng/ml

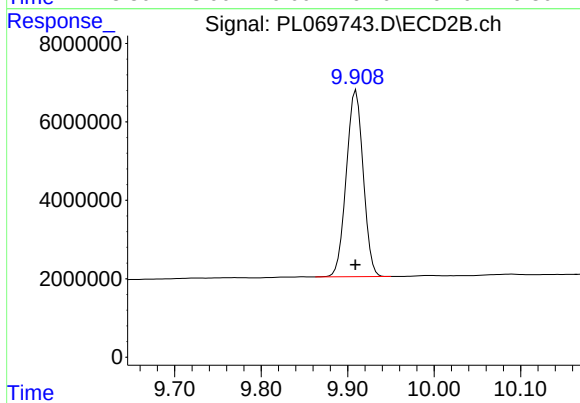


#20 Methoxychlor

R.T.: 9.910 min
Delta R.T.: 0.000 min
Response: 64267978
Conc: 100.72 ng/ml

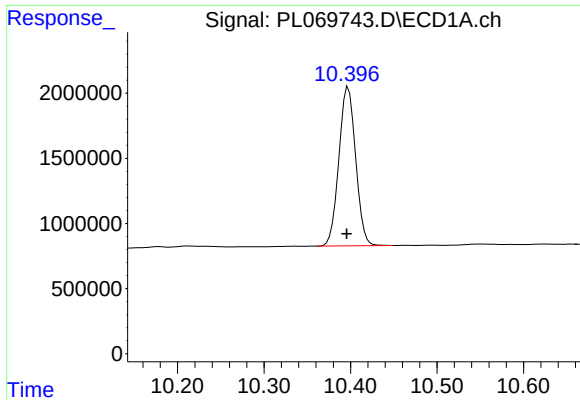

#27 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: 0.002 min
Response: 16310607
Conc: 21.34 ng/ml

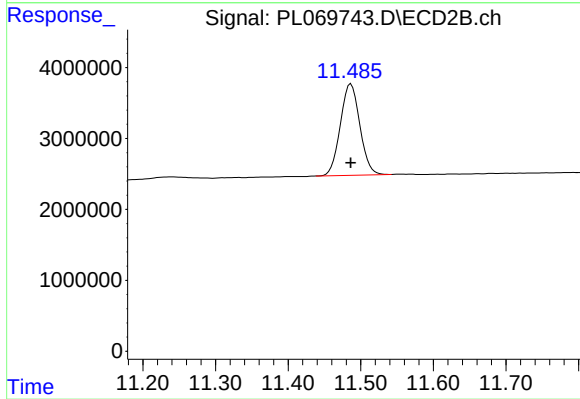

#27 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: 0.000 min
Response: 24109014
Conc: 20.19 ng/ml