

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090721\
 Data File : PL069745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2021 19:32
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 10:16:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 08 10:15:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.630	5.565	8496707	27618227	20.000	20.000
27)	SA Decachlor...	10.396	11.486	30579403	47762717	40.000	40.000
Target Compounds							
2)	A alpha-BHC	5.336	6.146	11128426	36393480	20.000	20.000
3)	MA gamma-BHC...	5.759	6.542	11346802	35037599	20.000	20.000
4)	MA Heptachlor	6.169	7.191	13395580	34962041	20.000	20.000
9)	A Endosulfan I	7.473	8.434	12317146	27286009	20.000	20.000
13)	MA Dieldrin	7.760	8.724	26652852	58840972	40.000	40.000
14)	MA Endrin	8.050	8.963	24944054	49177682	40.000	40.000
16)	A 4,4'-DDD	8.216	9.106	21594959	46666179	40.000	40.000
17)	MA 4,4'-DDT	8.477	9.423	24947385	48617502	40.000	40.000
20)	A Methoxychlor	9.072	9.909	75577859	127.6E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090721\
Data File : PL069745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2021 19:32
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 10:16:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 08 10:15:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

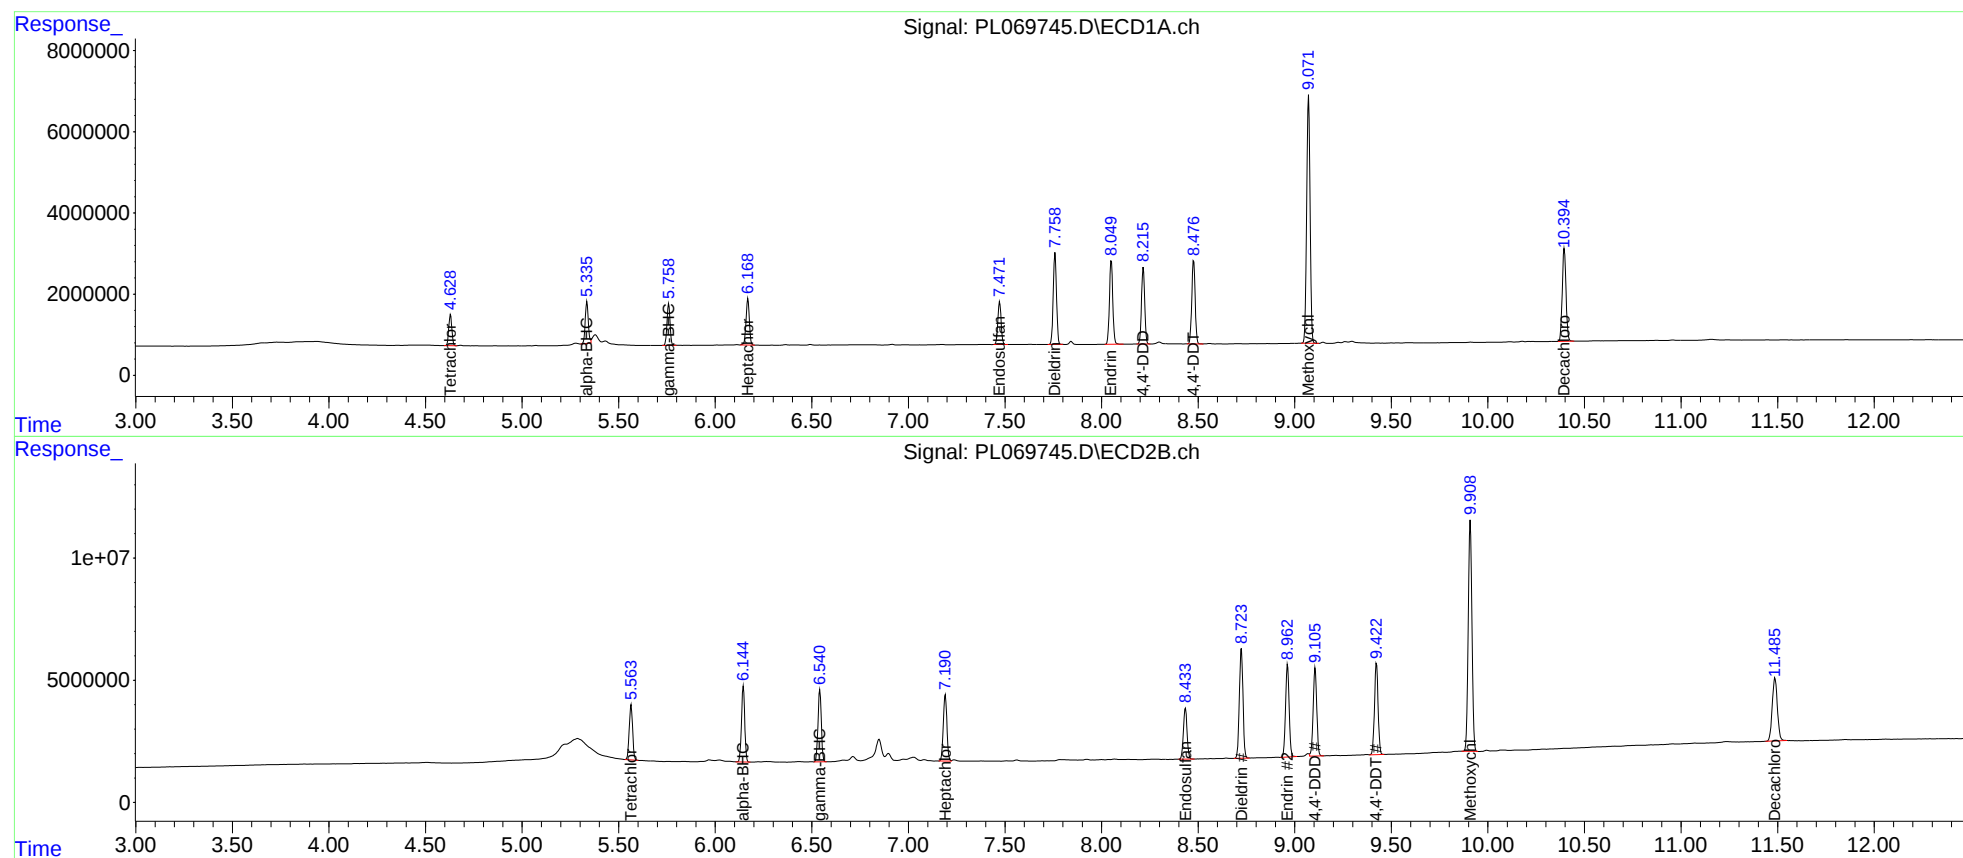

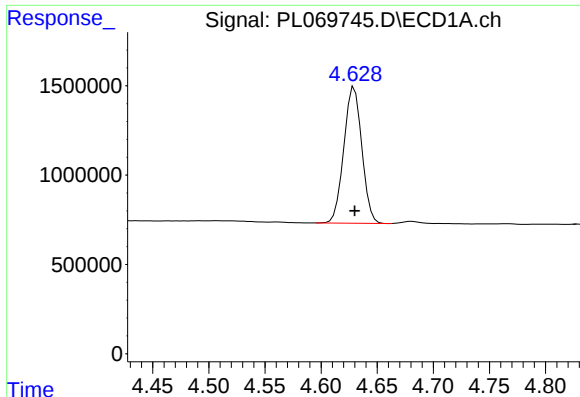


#1 Tetrachloro-m-xylene

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 8496707
Conc: 20.00 ng/ml

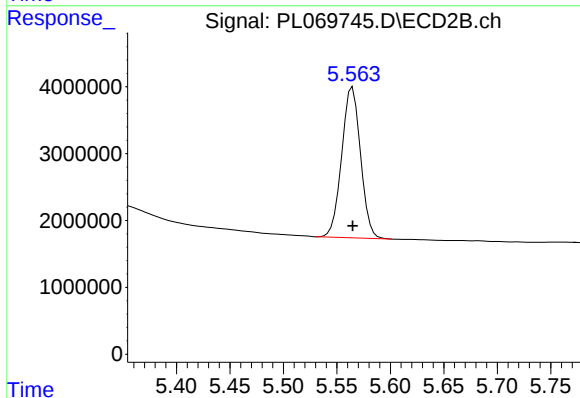


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 27618227
Conc: 20.00 ng/ml

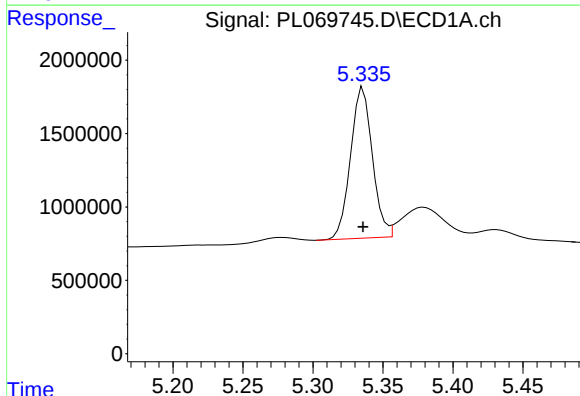


#2 alpha-BHC

R.T.: 5.336 min
Delta R.T.: 0.000 min
Response: 11128426
Conc: 20.00 ng/ml

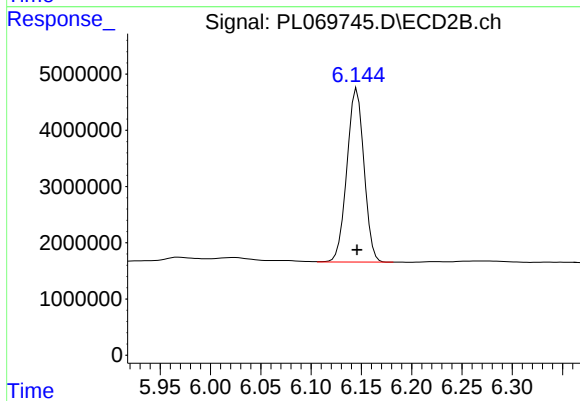


#2 alpha-BHC

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 36393480
Conc: 20.00 ng/ml

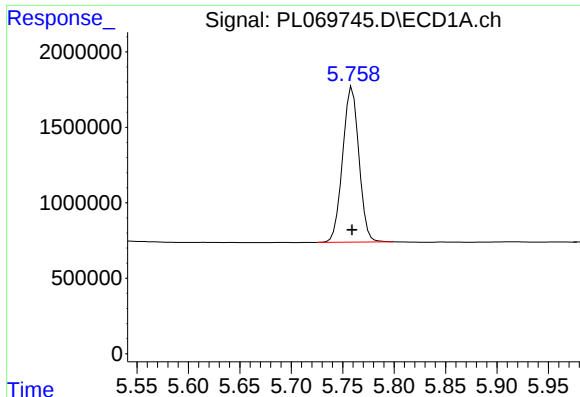


#3 gamma-BHC (Lindane)

R.T.: 5.759 min
Delta R.T.: 0.000 min
Response: 11346802
Conc: 20.00 ng/ml

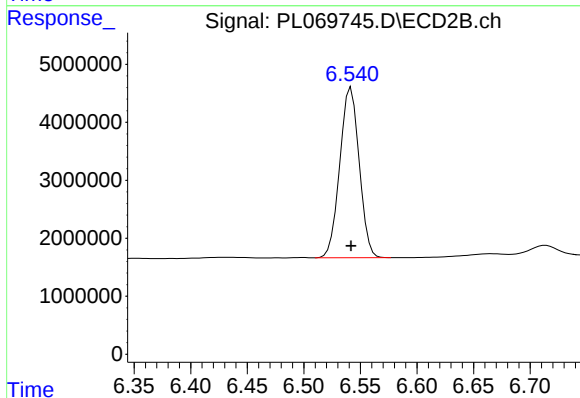


#3 gamma-BHC (Lindane)

R.T.: 6.542 min
Delta R.T.: 0.000 min
Response: 35037599
Conc: 20.00 ng/ml

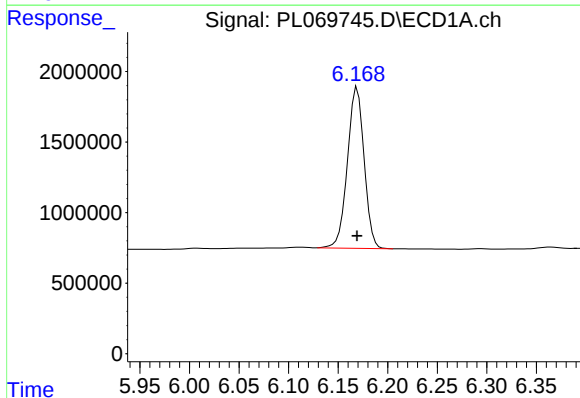


#4 Heptachlor

R.T.: 6.169 min
Delta R.T.: 0.000 min
Response: 13395580
Conc: 20.00 ng/ml

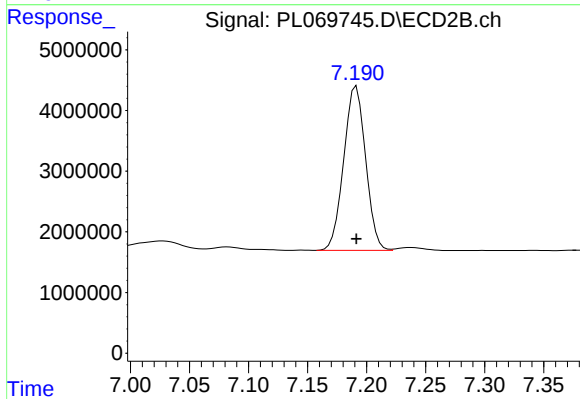


#4 Heptachlor

R.T.: 7.191 min
Delta R.T.: 0.000 min
Response: 34962041
Conc: 20.00 ng/ml

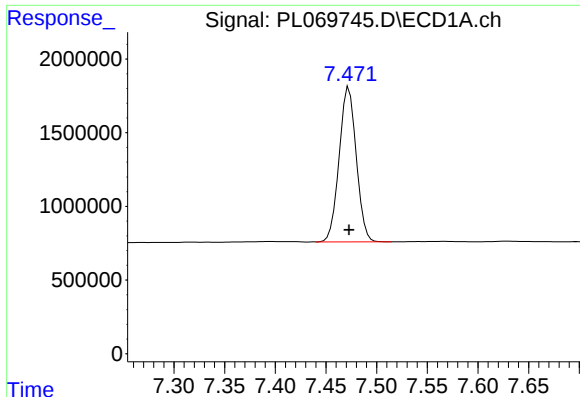


#9 Endosulfan I

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 12317146
Conc: 20.00 ng/ml

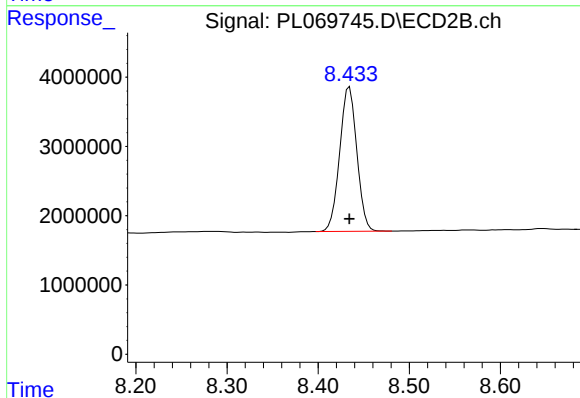


#9 Endosulfan I

R.T.: 8.434 min
Delta R.T.: 0.000 min
Response: 27286009
Conc: 20.00 ng/ml

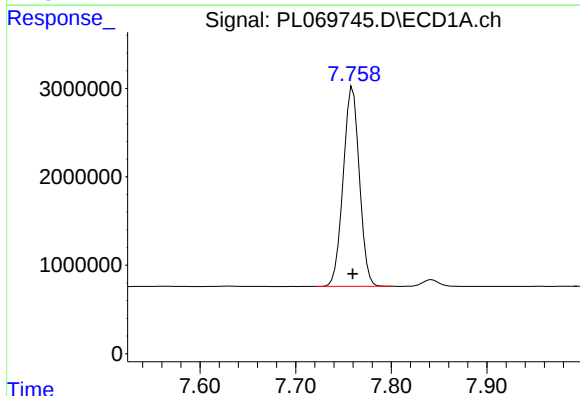


#13 Dieldrin

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 26652852
Conc: 40.00 ng/ml

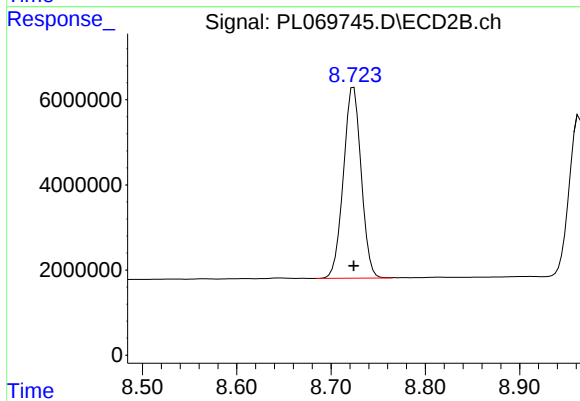


#13 Dieldrin

R.T.: 8.724 min
Delta R.T.: 0.000 min
Response: 58840972
Conc: 40.00 ng/ml

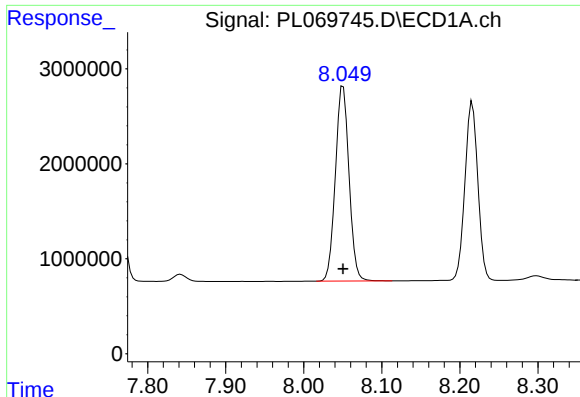


#14 Endrin

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 24944054
Conc: 40.00 ng/ml

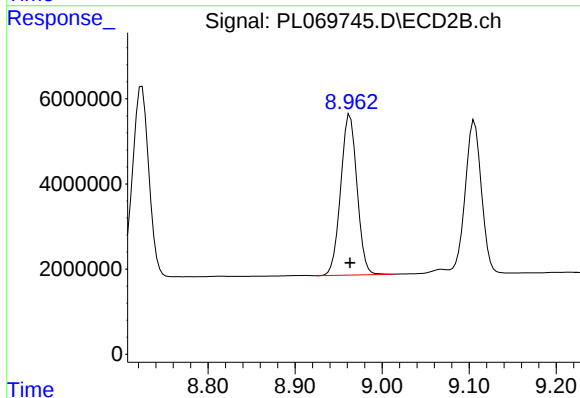


#14 Endrin

R.T.: 8.963 min
Delta R.T.: 0.000 min
Response: 49177682
Conc: 40.00 ng/ml

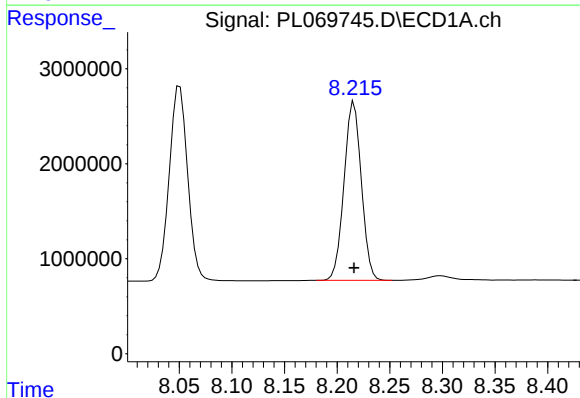


#16 4,4'-DDD

R.T.: 8.216 min
Delta R.T.: 0.000 min
Response: 21594959
Conc: 40.00 ng/ml

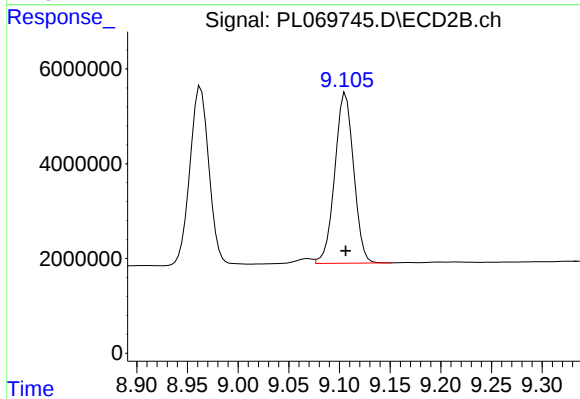


#16 4,4'-DDD

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 46666179
Conc: 40.00 ng/ml

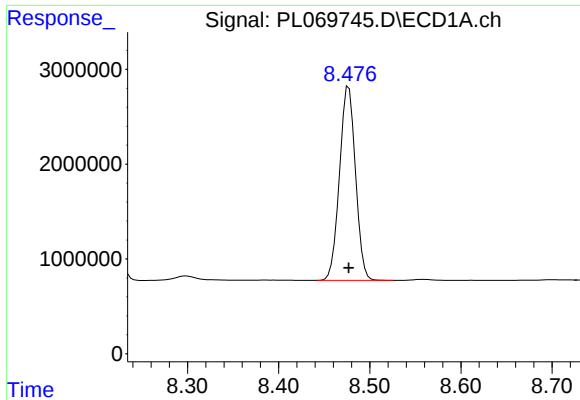


#17 4,4'-DDT

R.T.: 8.477 min
Delta R.T.: 0.000 min
Response: 24947385
Conc: 40.00 ng/ml

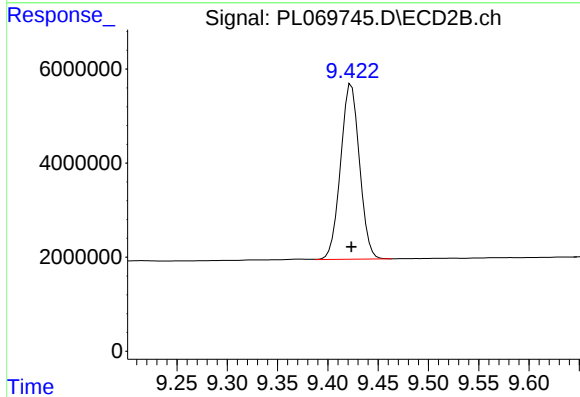


#17 4,4'-DDT

R.T.: 9.423 min
Delta R.T.: 0.000 min
Response: 48617502
Conc: 40.00 ng/ml

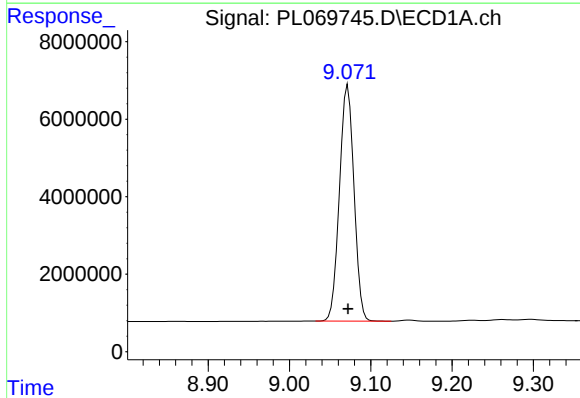


#20 Methoxychlor

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 75577859
Conc: 200.00 ng/ml

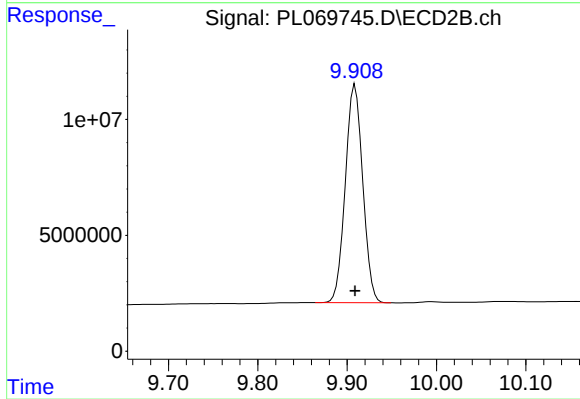


#20 Methoxychlor

R.T.: 9.909 min
Delta R.T.: 0.000 min
Response: 127612595
Conc: 200.00 ng/ml

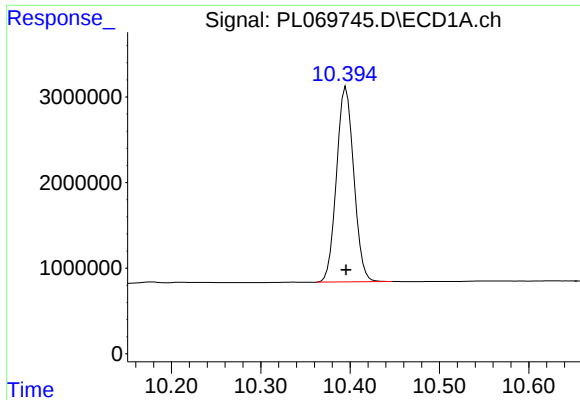

#27 Decachlorobiphenyl

R.T.: 10.396 min
Delta R.T.: 0.000 min
Response: 30579403
Conc: 40.00 ng/ml

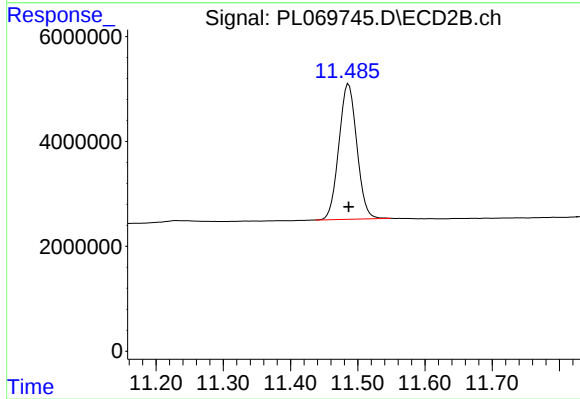

#27 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: 0.000 min
Response: 47762717
Conc: 40.00 ng/ml