

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090721\
 Data File : PL069749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2021 20:39
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 10:17:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 08 10:15:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.630	5.565	32780664	108.2E6	77.161	78.390
27)	SA Decachlor...	10.397	11.486	106.2E6	176.9E6	138.892	148.157
Target Compounds							
2)	A alpha-BHC	5.337	6.146	49095359	157.4E6	88.234	86.490
3)	MA gamma-BHC...	5.759	6.542	48550858	147.9E6	85.576	84.395
4)	MA Heptachlor	6.170	7.192	54056489	144.1E6	80.708	82.426
9)	A Endosulfan I	7.474	8.435	49271872	110.6E6	80.005	81.059
13)	MA Dieldrin	7.760	8.724	113.5E6	244.9E6	170.413	166.460
14)	MA Endrin	8.051	8.964	103.3E6	202.7E6	165.653	164.856
16)	A 4,4'-DDD	8.216	9.107	92185674	192.8E6	170.754	165.283
17)	MA 4,4'-DDT	8.477	9.424	103.9E6	200.3E6	166.584	164.788
20)	A Methoxychlor	9.072	9.909	274.0E6	475.0E6	725.102	744.411


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090721\
Data File : PL069749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2021 20:39
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 10:17:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 08 10:15:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

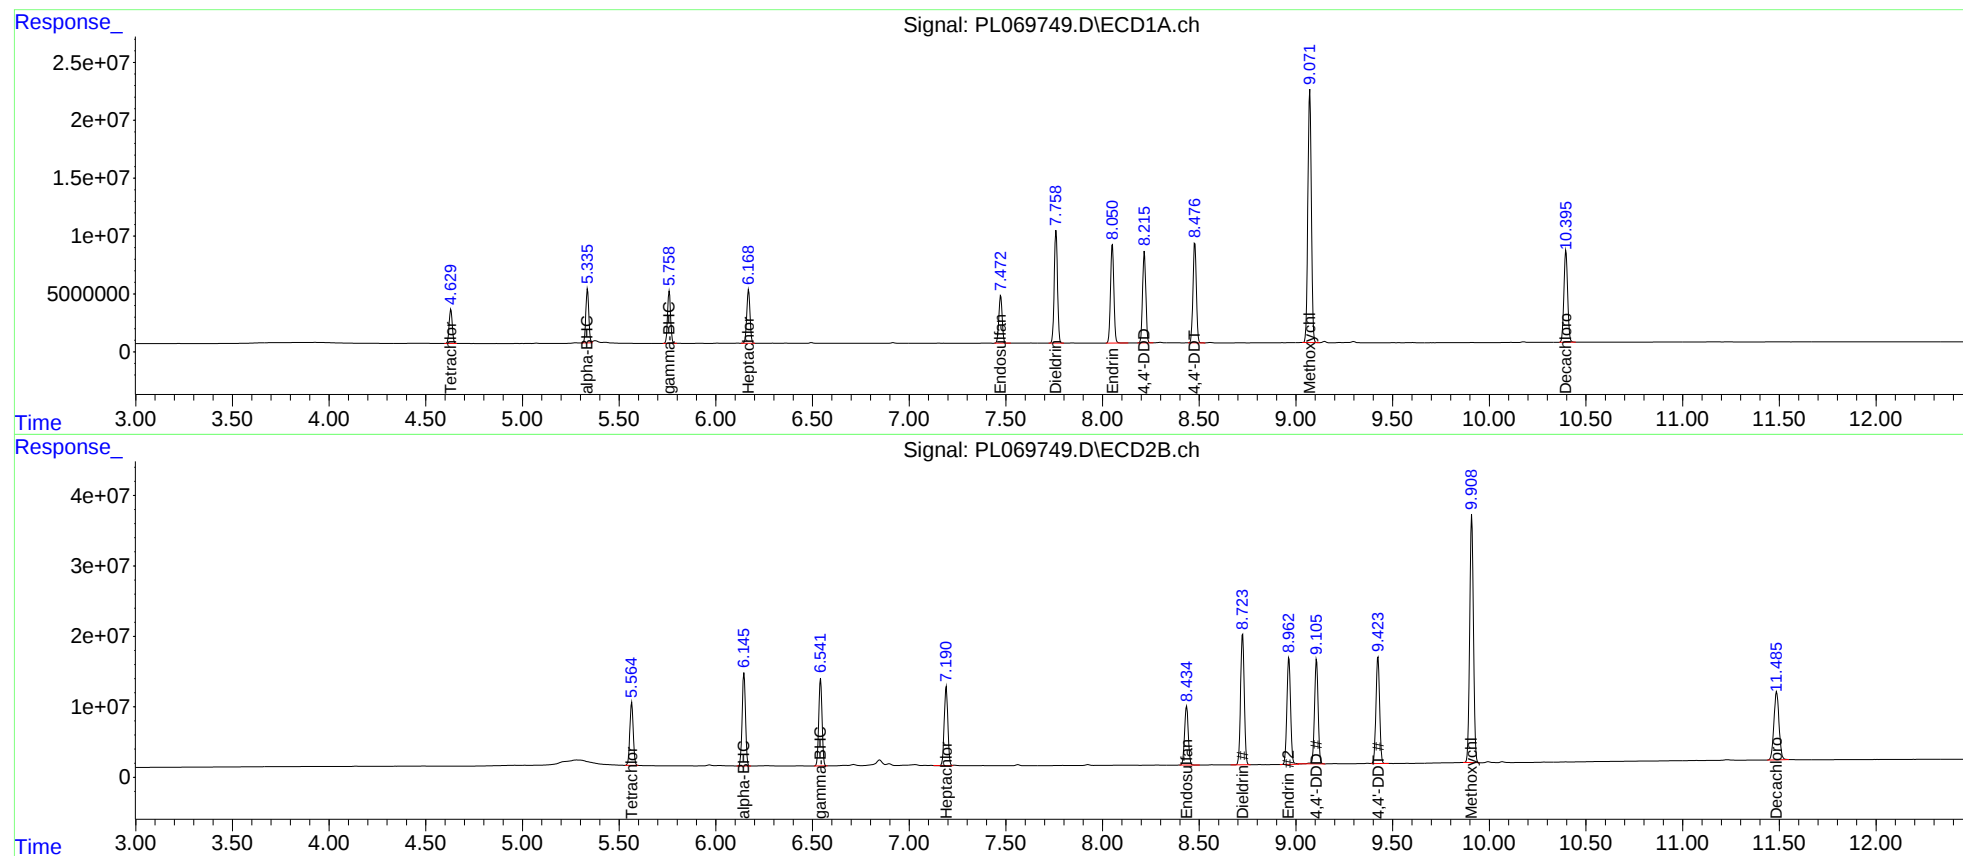

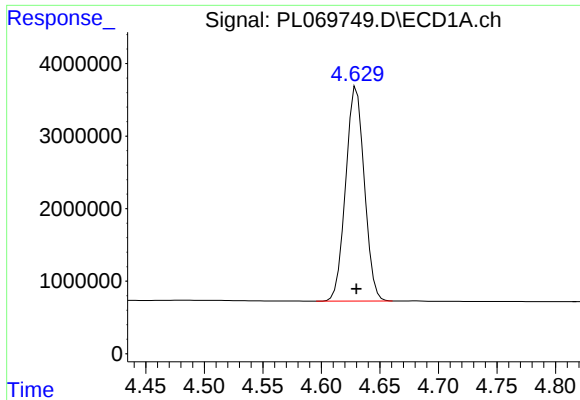


#1 Tetrachloro-m-xylene

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 32780664
Conc: 77.16 ng/ml

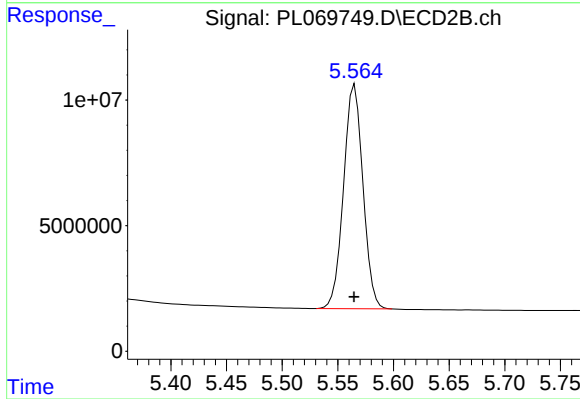


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 108249775
Conc: 78.39 ng/ml

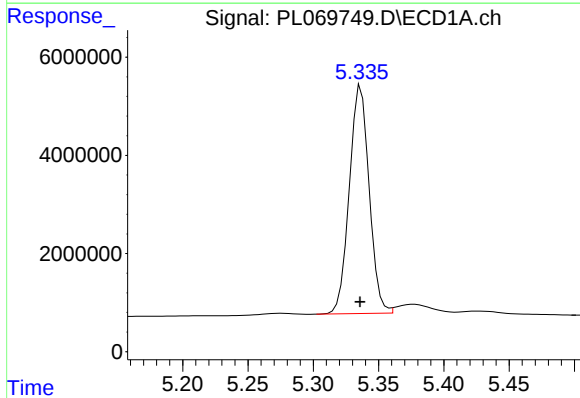


#2 alpha-BHC

R.T.: 5.337 min
Delta R.T.: 0.000 min
Response: 49095359
Conc: 88.23 ng/ml

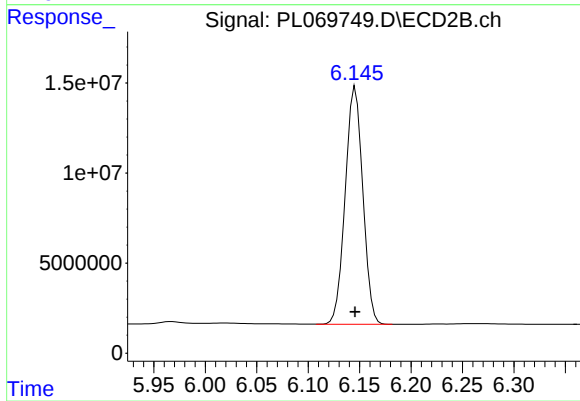


#2 alpha-BHC

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 157382981
Conc: 86.49 ng/ml

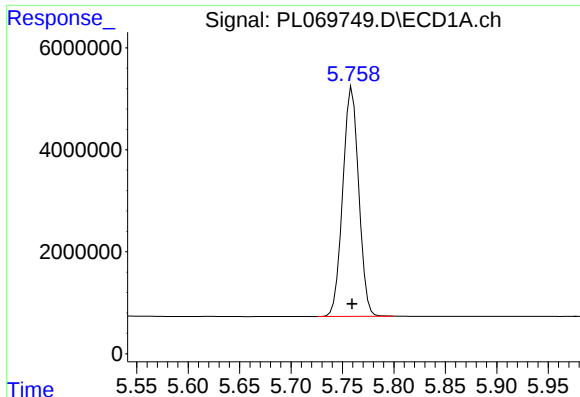


#3 gamma-BHC (Lindane)

R.T.: 5.759 min
Delta R.T.: 0.000 min
Response: 48550858
Conc: 85.58 ng/ml

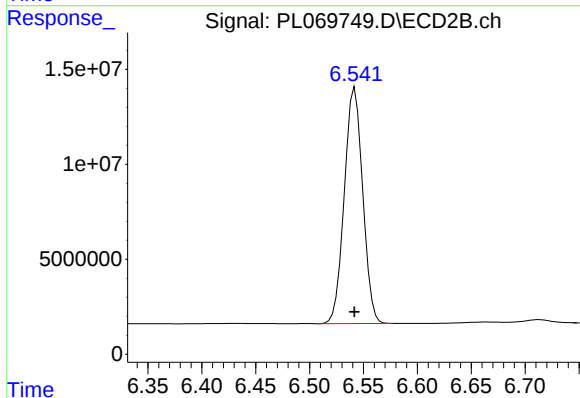


#3 gamma-BHC (Lindane)

R.T.: 6.542 min
Delta R.T.: 0.000 min
Response: 147850611
Conc: 84.40 ng/ml

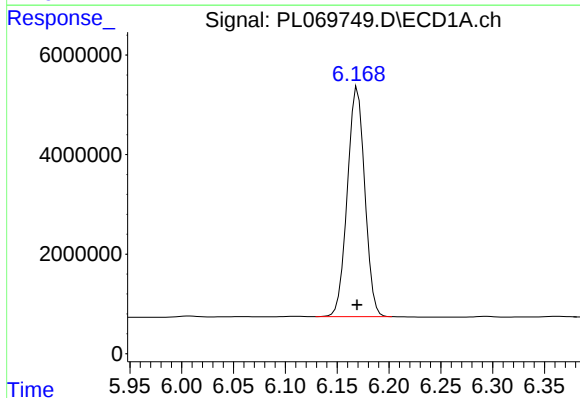


#4 Heptachlor

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 54056489
Conc: 80.71 ng/ml

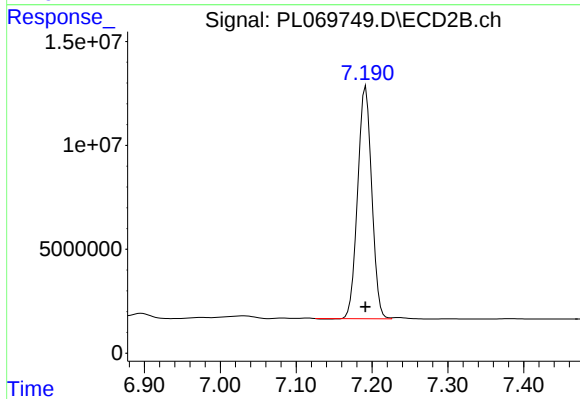


#4 Heptachlor

R.T.: 7.192 min
Delta R.T.: 0.000 min
Response: 144088210
Conc: 82.43 ng/ml

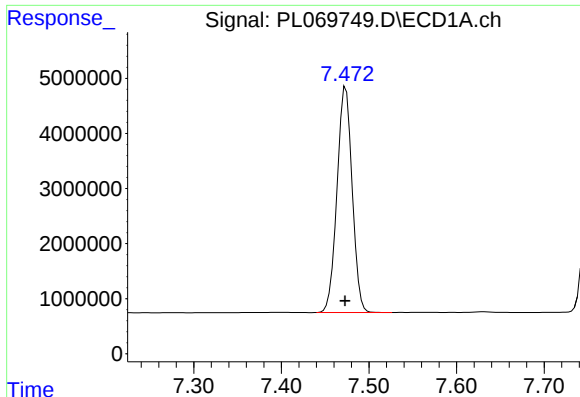


#9 Endosulfan I

R.T.: 7.474 min
Delta R.T.: 0.000 min
Response: 49271872
Conc: 80.01 ng/ml

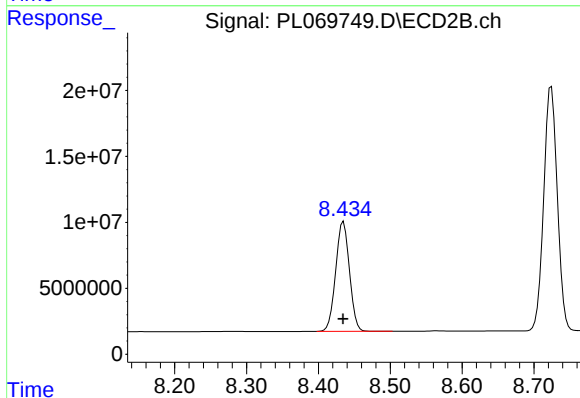


#9 Endosulfan I

R.T.: 8.435 min
Delta R.T.: 0.000 min
Response: 110589061
Conc: 81.06 ng/ml

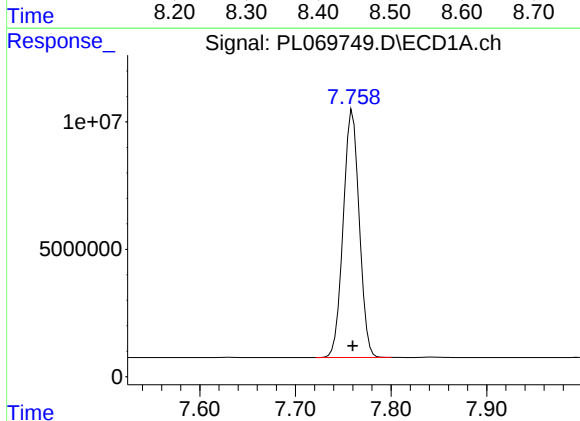


#13 Dieldrin

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 113549742
Conc: 170.41 ng/ml

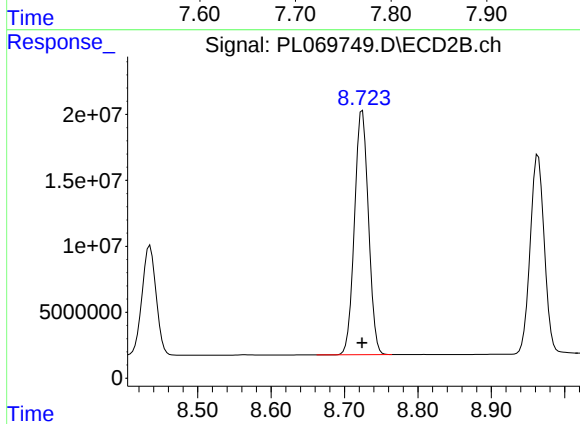


#13 Dieldrin

R.T.: 8.724 min
Delta R.T.: 0.000 min
Response: 244866283
Conc: 166.46 ng/ml

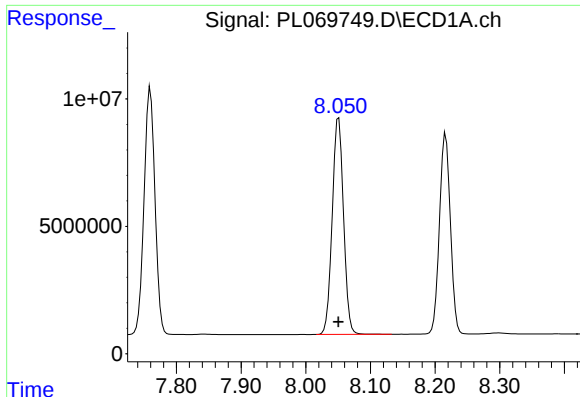


#14 Endrin

R.T.: 8.051 min
Delta R.T.: 0.000 min
Response: 103301294
Conc: 165.65 ng/ml

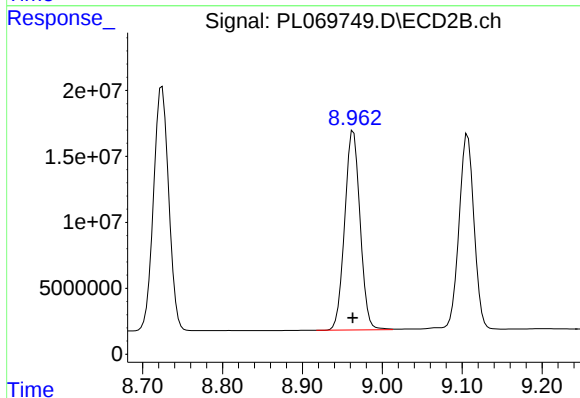


#14 Endrin

R.T.: 8.964 min
Delta R.T.: 0.000 min
Response: 202680965
Conc: 164.86 ng/ml

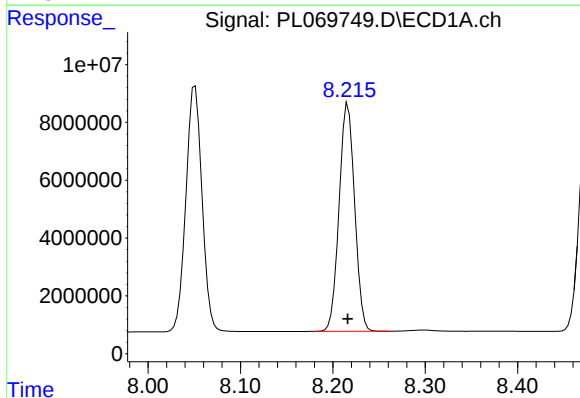


#16 4,4'-DDD

R.T.: 8.216 min
Delta R.T.: 0.000 min
Response: 92185674
Conc: 170.75 ng/ml

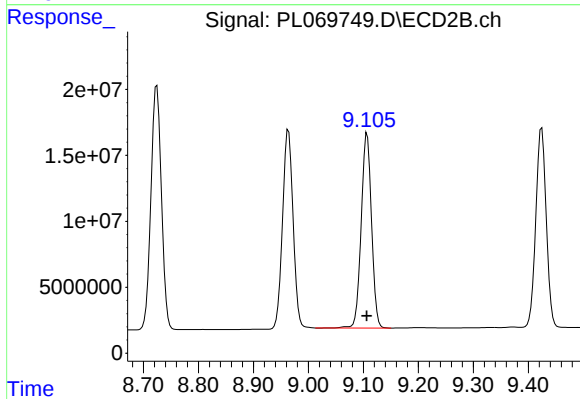


#16 4,4'-DDD

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 192827725
Conc: 165.28 ng/ml

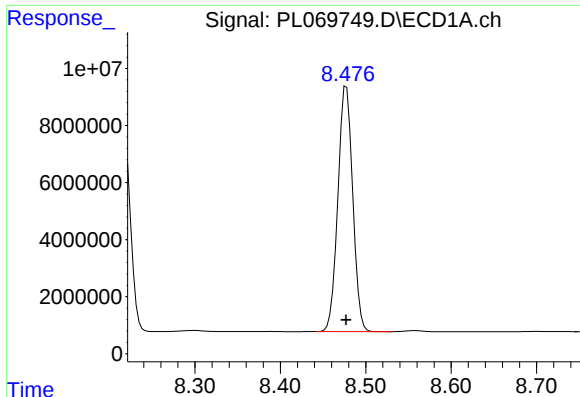


#17 4,4'-DDT

R.T.: 8.477 min
Delta R.T.: 0.000 min
Response: 103895855
Conc: 166.58 ng/ml

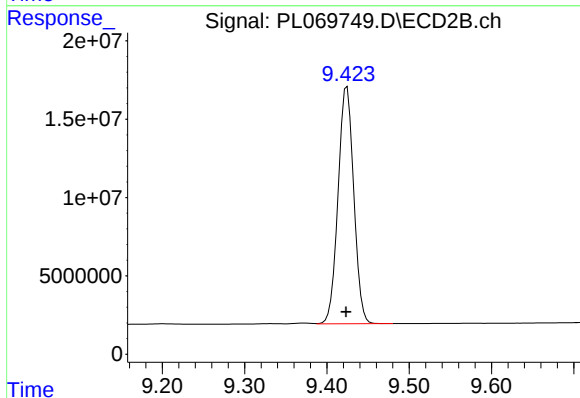


#17 4,4'-DDT

R.T.: 9.424 min
Delta R.T.: 0.000 min
Response: 200289018
Conc: 164.79 ng/ml

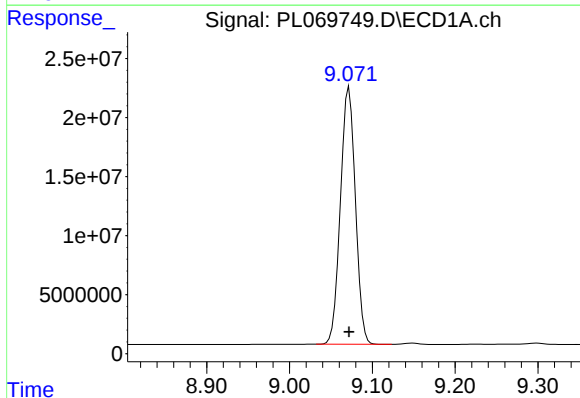


#20 Methoxychlor

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 274008353
Conc: 725.10 ng/ml

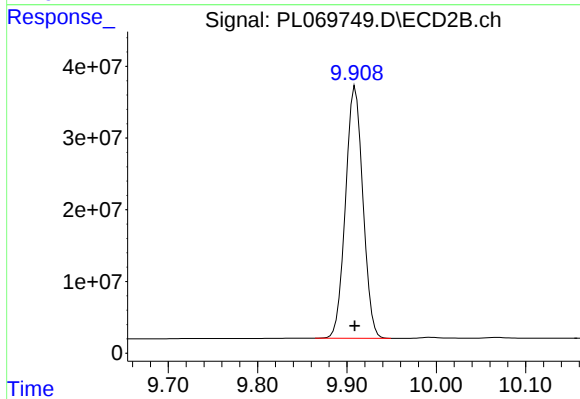


#20 Methoxychlor

R.T.: 9.909 min
Delta R.T.: 0.000 min
Response: 474980962
Conc: 744.41 ng/ml

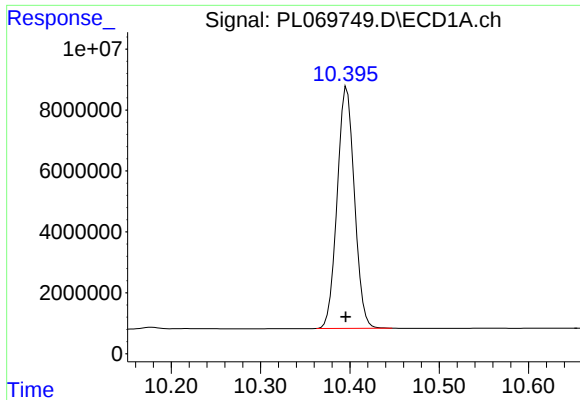

#27 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: 0.001 min
Response: 106180641
Conc: 138.89 ng/ml

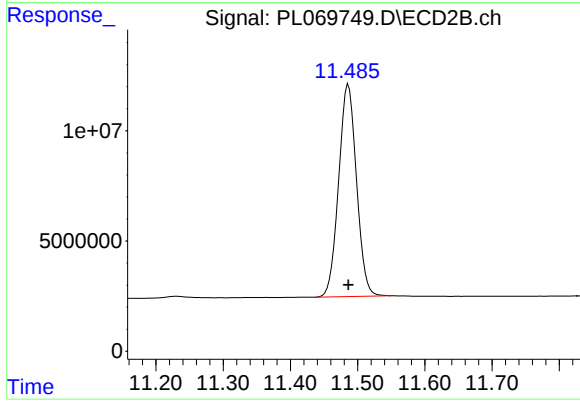

#27 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: 0.000 min
Response: 176910112
Conc: 148.16 ng/ml