

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 12:15
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 12:37:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 12:26:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.629	8352607	16573812	4.778	5.254
28)	SA Decachlor...	8.907	7.730	8604818	10904256	5.765	5.568
Target Compounds							
23)	Chlordane-1	4.577	3.606	3174050	3612837	47.216	40.519
24)	Chlordane-2	5.111	4.177	4422579	5316609	58.936	53.629
25)	Chlordane-3	5.822	4.801	12741431	15548591	45.317	54.295
26)	Chlordane-4	5.901	4.862	16015494	15457566	46.092	51.423
27)	Chlordane-5	6.759	5.526	3164953	3517302	51.885	50.053



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 12:15
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 12:37:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 12:26:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

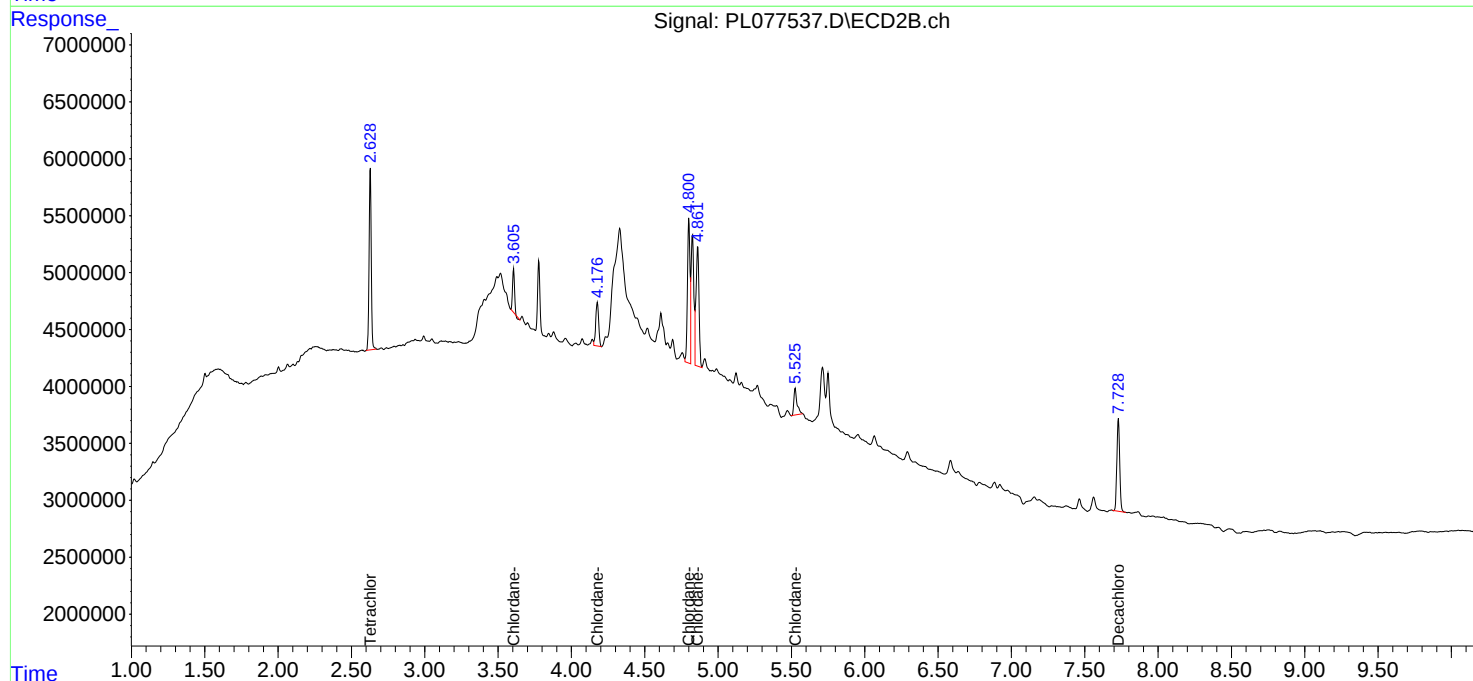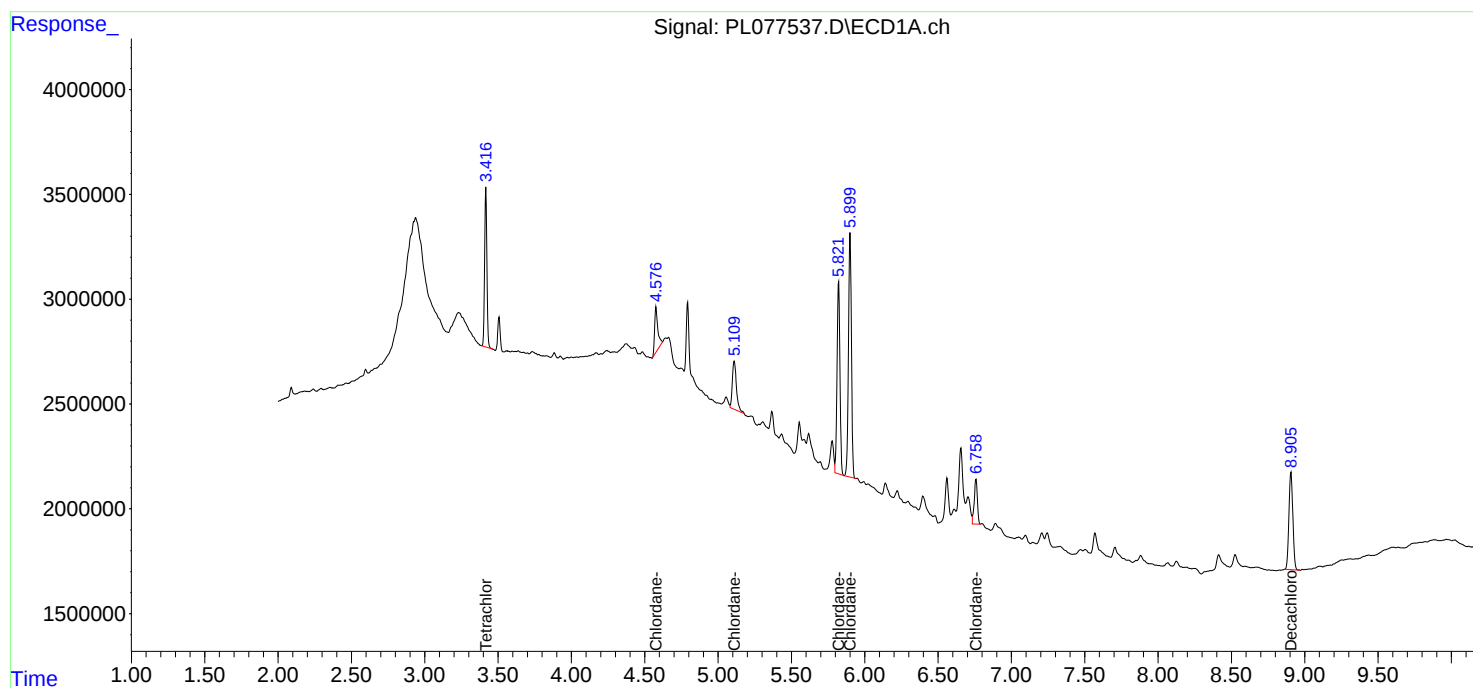


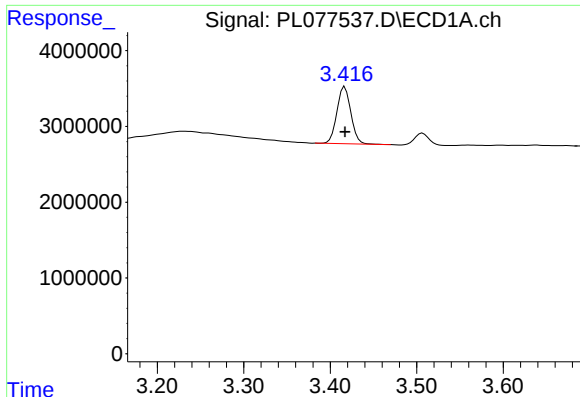

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 8352607
Conc: 4.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

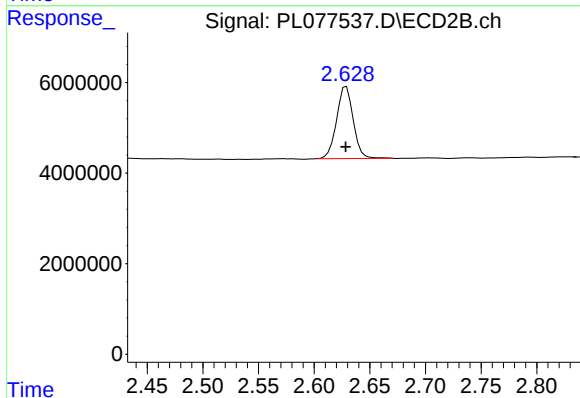


#1 Tetrachloro-m-xylene

R.T.: 2.629 min
Delta R.T.: 0.000 min
Response: 16573812
Conc: 5.25 ng/ml

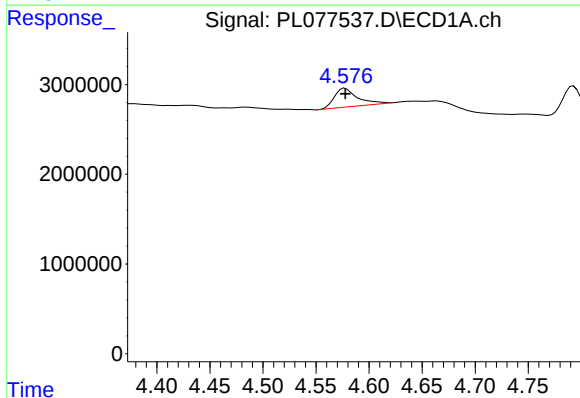


#23 Chlordane-1

R.T.: 4.577 min
Delta R.T.: 0.000 min
Response: 3174050
Conc: 47.22 ng/ml

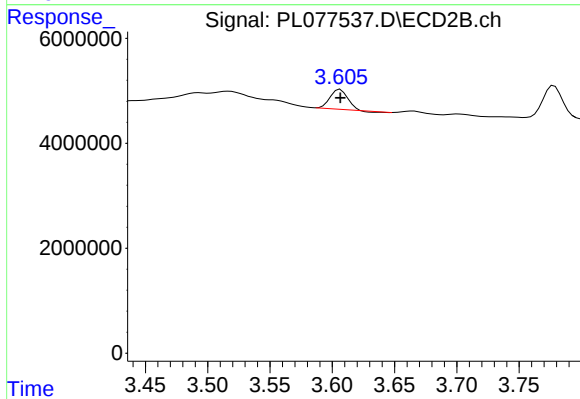

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 3612837
Conc: 40.52 ng/ml

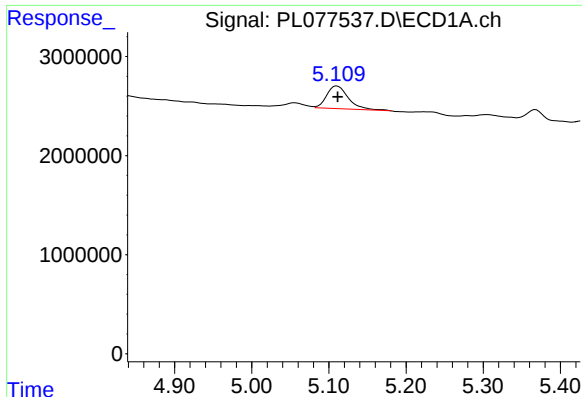

#24 Chlordane-2


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 4422579
Conc: 58.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

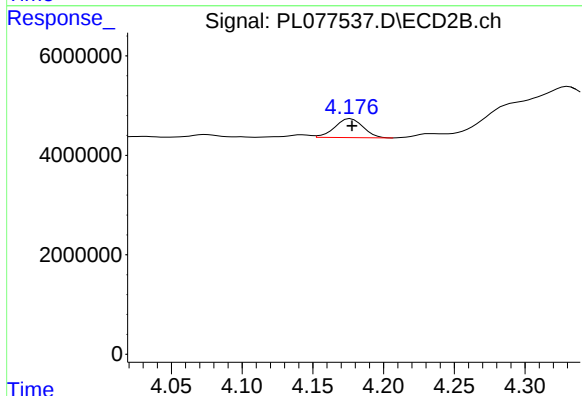


#24 Chlordane-2

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 5316609
Conc: 53.63 ng/ml

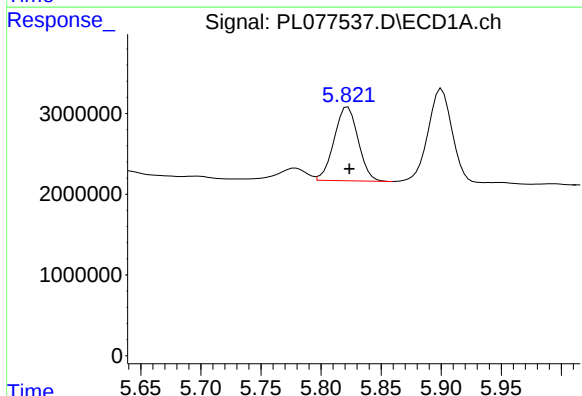


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: -0.001 min
Response: 12741431
Conc: 45.32 ng/ml

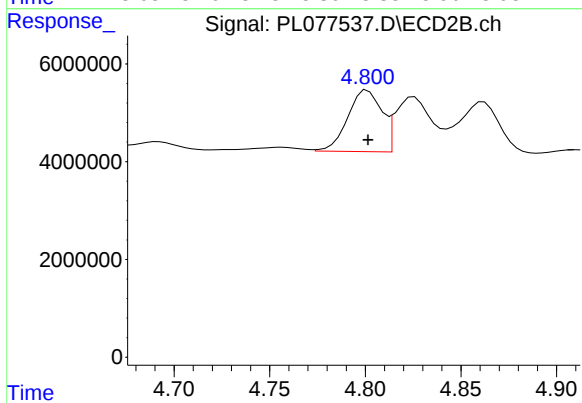

#25 Chlordane-3


R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 15548591
Conc: 54.30 ng/ml

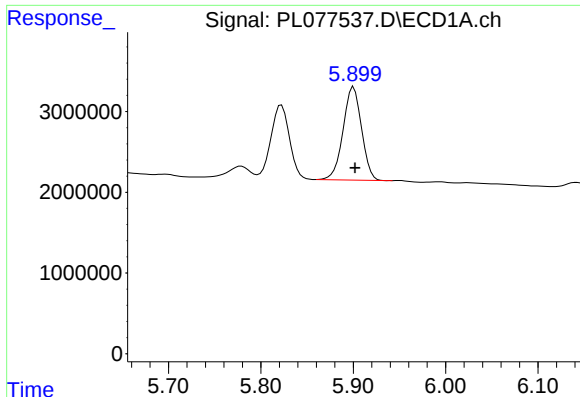

#26 Chlordane-4


R.T.: 5.901 min
Delta R.T.: -0.001 min
Response: 16015494
Conc: 46.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

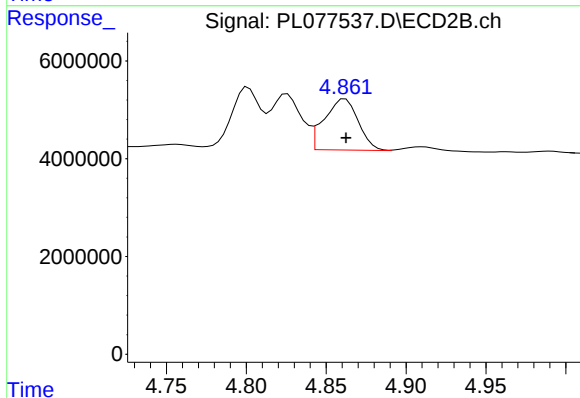


#26 Chlordane-4

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 15457566
Conc: 51.42 ng/ml

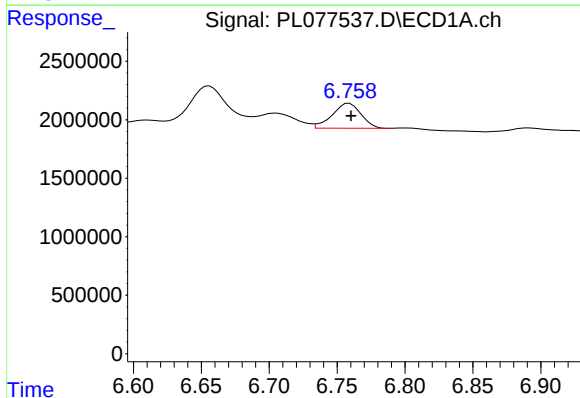


#27 Chlordane-5

R.T.: 6.759 min
Delta R.T.: -0.001 min
Response: 3164953
Conc: 51.88 ng/ml

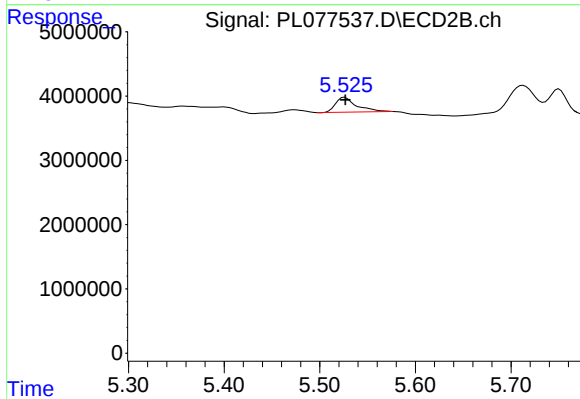

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 3517302
Conc: 50.05 ng/ml

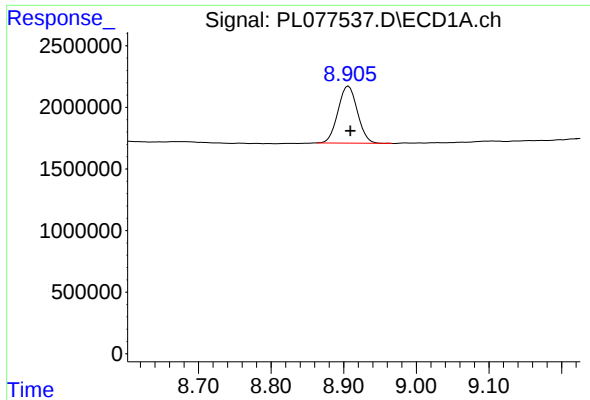

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.003 min
Response: 8604818
Conc: 5.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

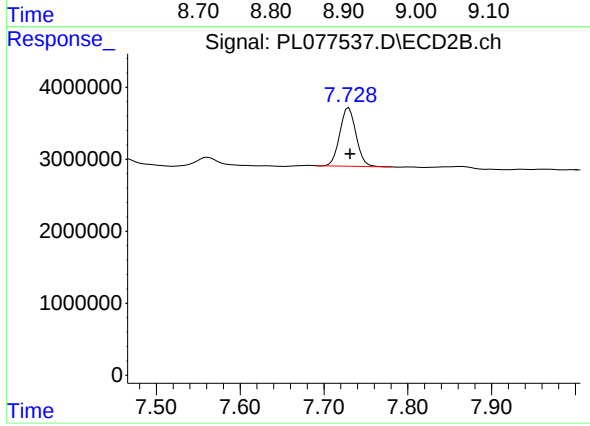

#28 Decachlorobiphenyl

R.T.: 7.730 min
Delta R.T.: -0.002 min
Response: 10904256
Conc: 5.57 ng/ml