

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 20:34
 Operator : AR\AJ
 Sample : PB147514BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB147514BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 04:47:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:34:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.628	32237228	50374708	18.855	19.037
28)	SA Decachlor...	8.905	7.726	25137244	36214728	16.759	18.364
Target Compounds							
3)	MA gamma-BHC...	4.236f	0.000	121940	0	0.051	N.D. #
5)	MB Aldrin	0.000	4.080f	0	129367	N.D.	0.041 #
7)	B delta-BHC	4.668	0.000	1087939	0	0.578	N.D. #
8)	B Heptachlo...	5.585f	0.000	816944	0	0.511	N.D. #
14)	MA Endrin	0.000	5.472f	0	2128082	N.D.	1.032 #
15)	B Endosulfa...	6.707f	0.000	1944959	0	1.200	N.D. #
21)	B Endrin ke...	7.569f	0.000	2042174	0	1.323	N.D. #
23)	Chlordane-1	4.593f	0.000	32357	0	0.500	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 20:34
Operator : AR\AJ
Sample : PB147514BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB147514BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 04:47:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:34:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

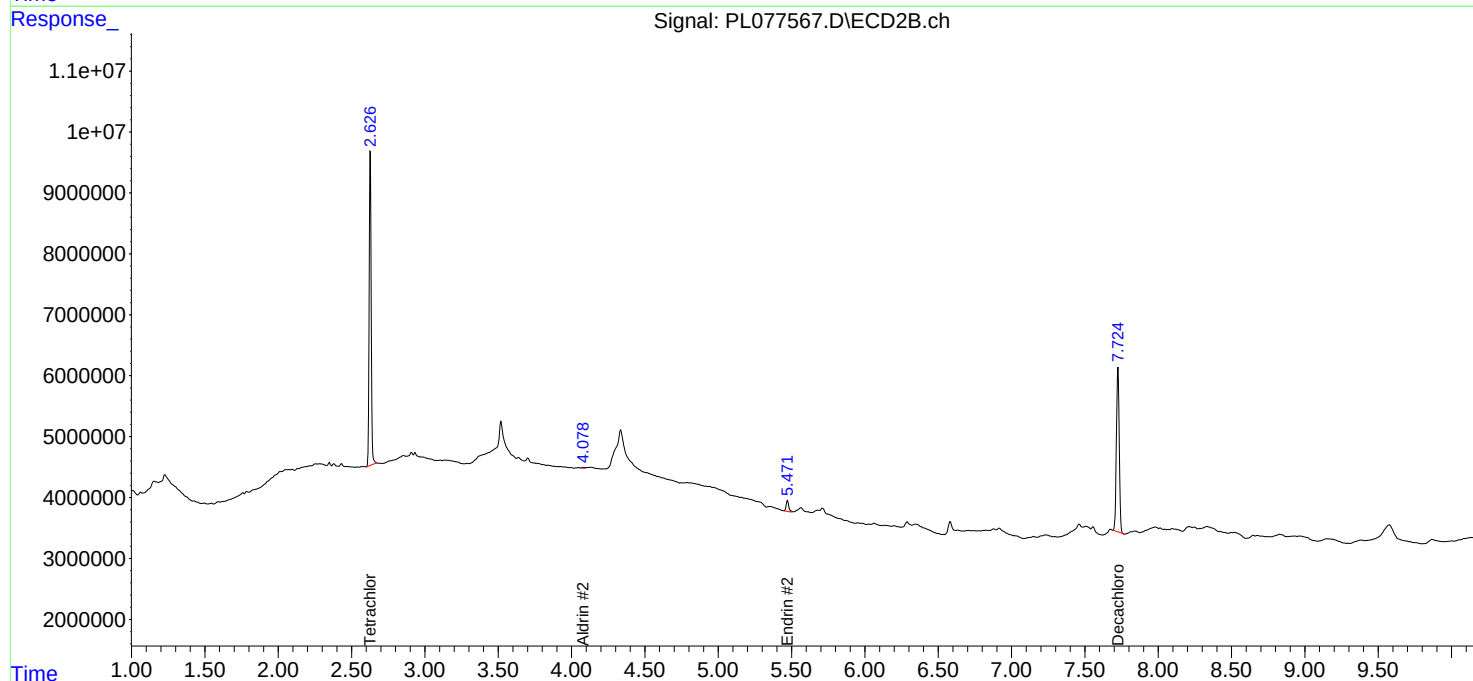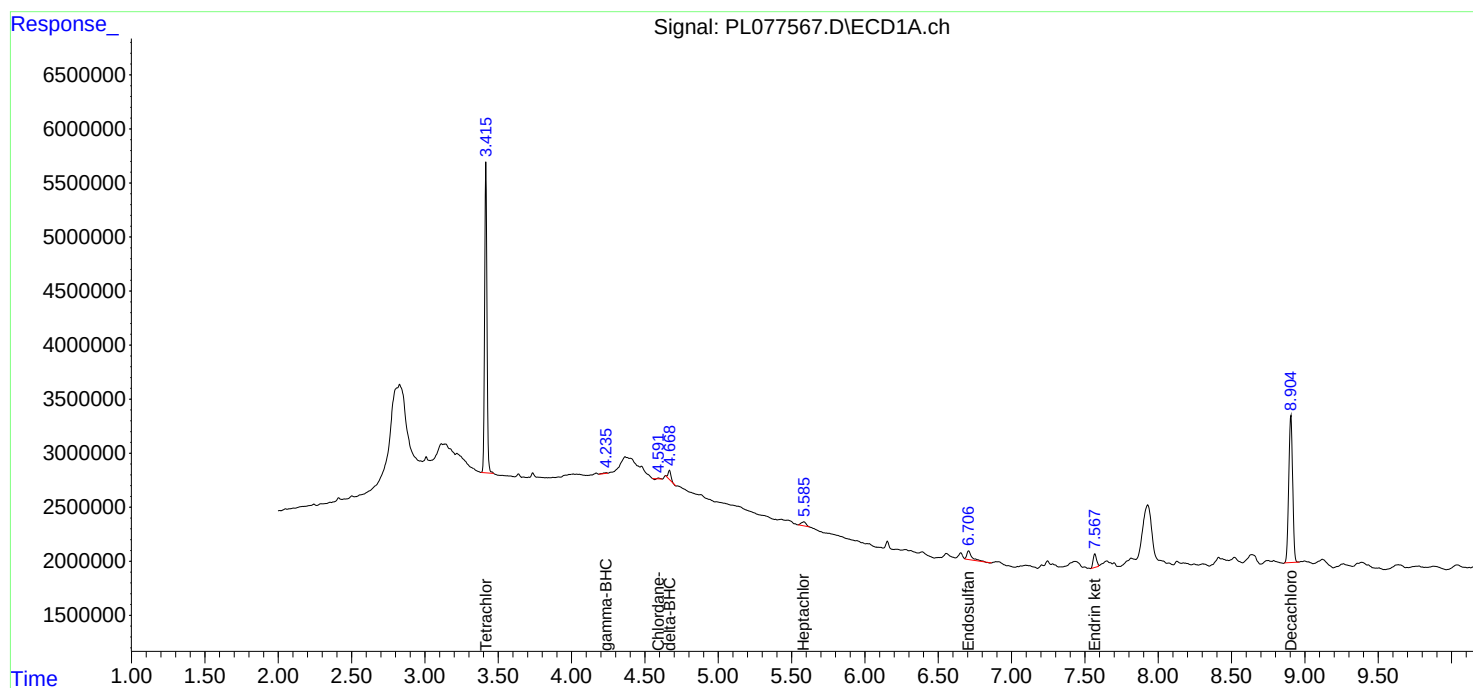


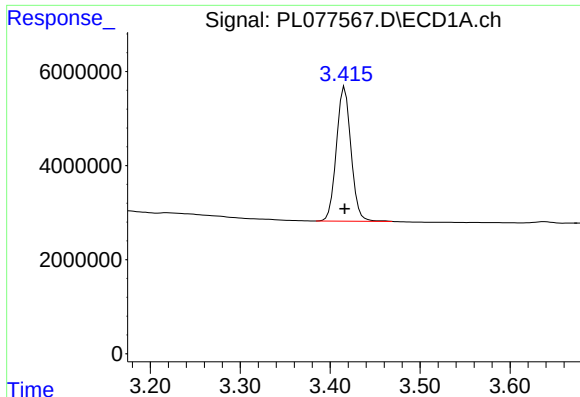

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 32237228
Conc: 18.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147514BL

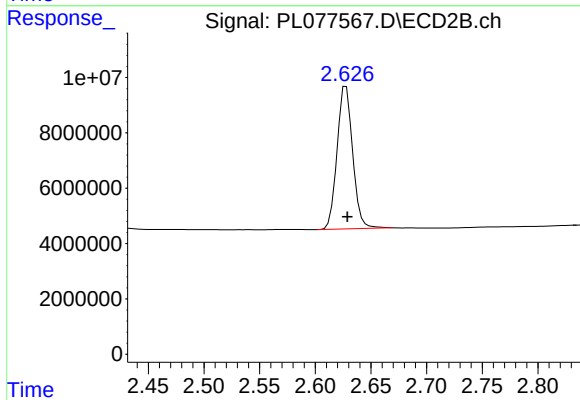


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: -0.001 min
Response: 50374708
Conc: 19.04 ng/ml

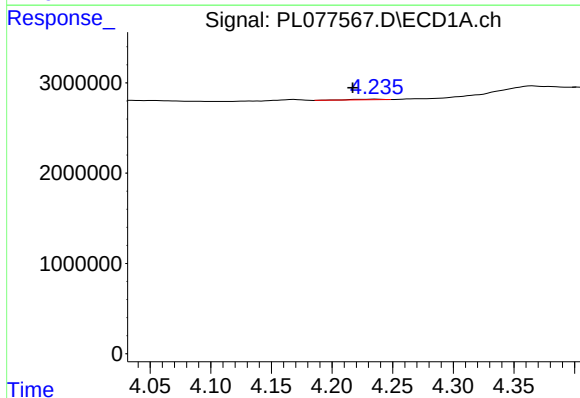


#3 gamma-BHC (Lindane)

R.T.: 4.236 min
Delta R.T.: 0.019 min
Response: 121940
Conc: 0.05 ng/ml

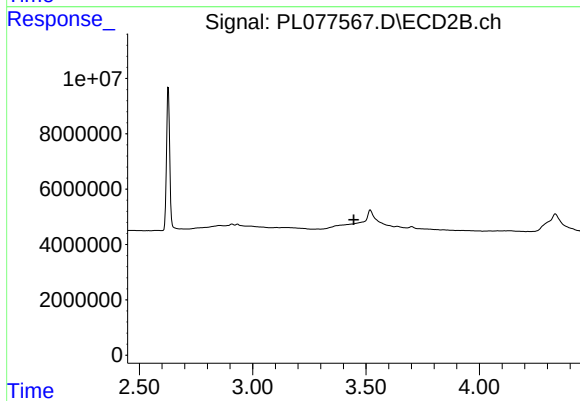

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.446 min
Response: 0
Conc: N.D.

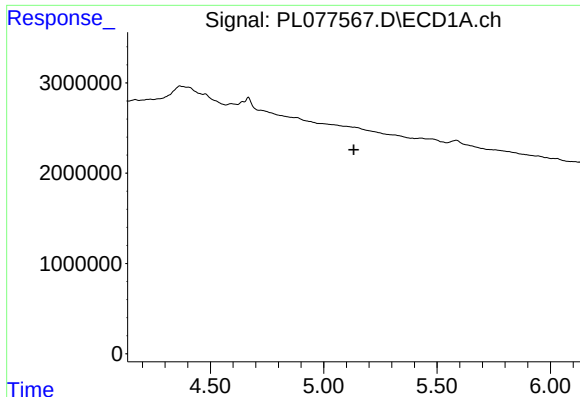

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB147514BL

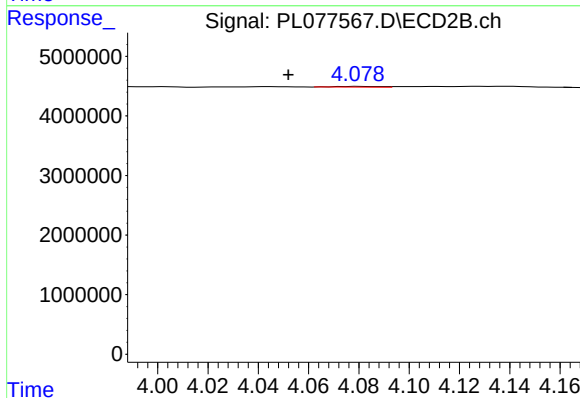


#5 Aldrin

R.T.: 4.080 min
Delta R.T.: 0.028 min
Response: 129367
Conc: 0.04 ng/ml

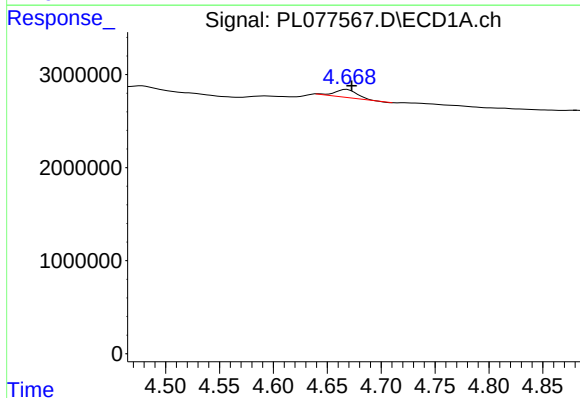


#7 delta-BHC

R.T.: 4.668 min
Delta R.T.: -0.004 min
Response: 1087939
Conc: 0.58 ng/ml

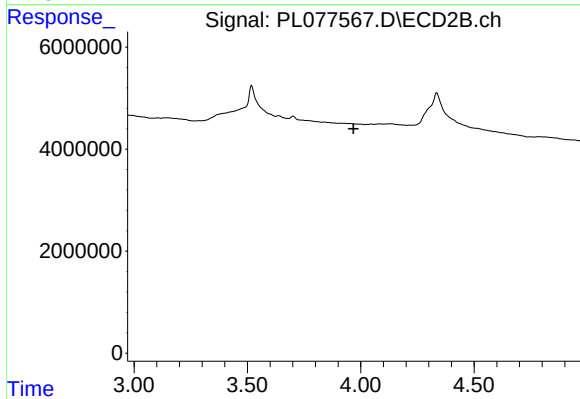

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 3.968 min
Response: 0
Conc: N.D.

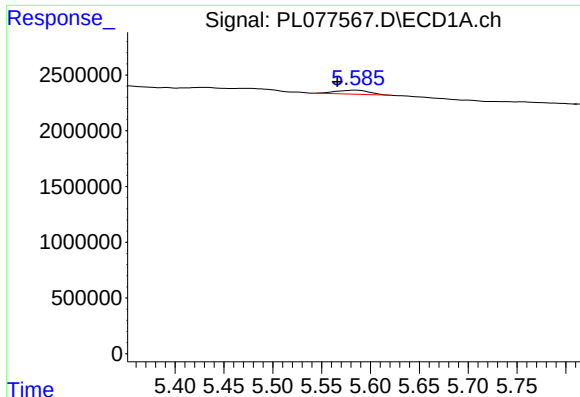

#8 Heptachlor epoxide


R.T.: 5.585 min
Delta R.T.: 0.018 min
Response: 816944
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147514BL

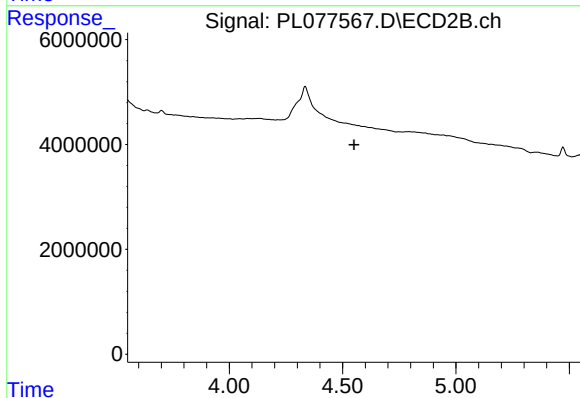


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

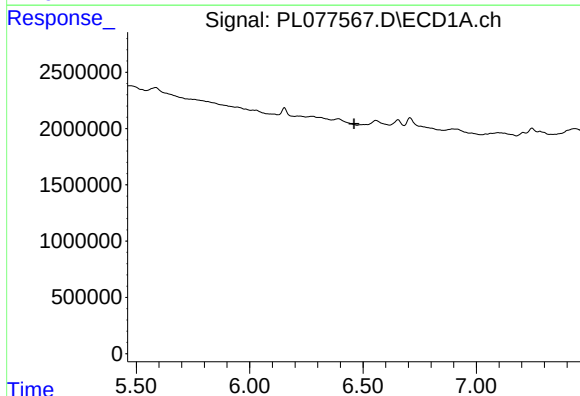


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

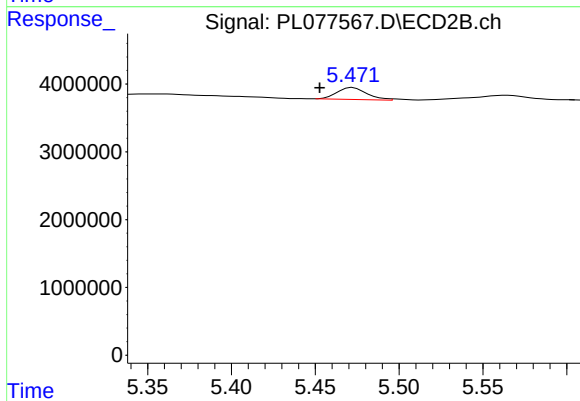

#14 Endrin


R.T.: 5.472 min
Delta R.T.: 0.020 min
Response: 2128082
Conc: 1.03 ng/ml

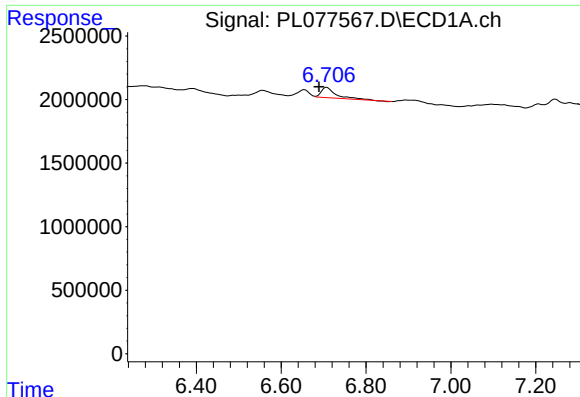

#15 Endosulfan II


R.T.: 6.707 min
Delta R.T.: 0.018 min
Response: 1944959
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147514BL

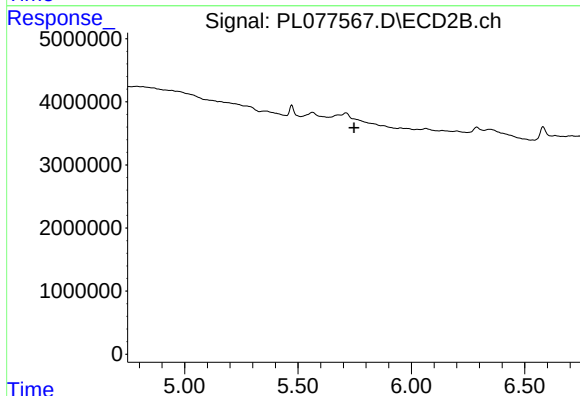


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.748 min
Response: 0
Conc: N.D.

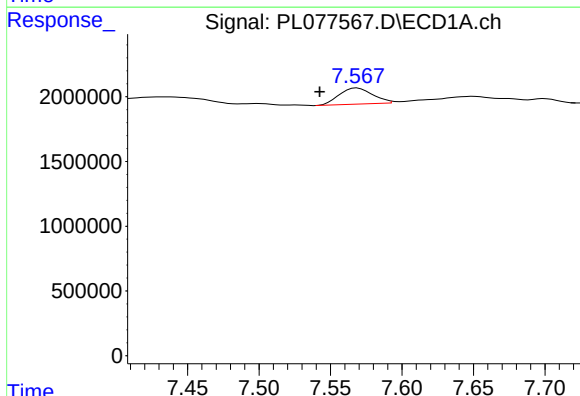


#21 Endrin ketone

R.T.: 7.569 min
Delta R.T.: 0.026 min
Response: 2042174
Conc: 1.32 ng/ml

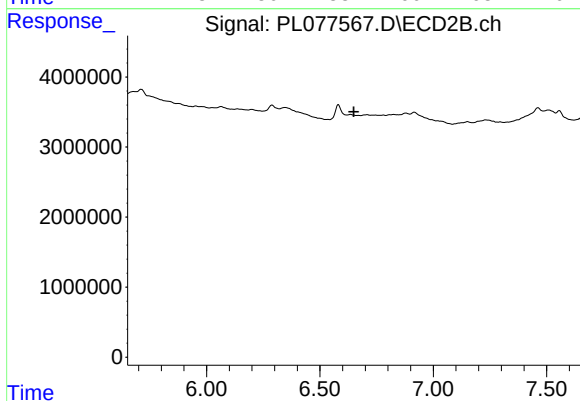

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.650 min
Response: 0
Conc: N.D.

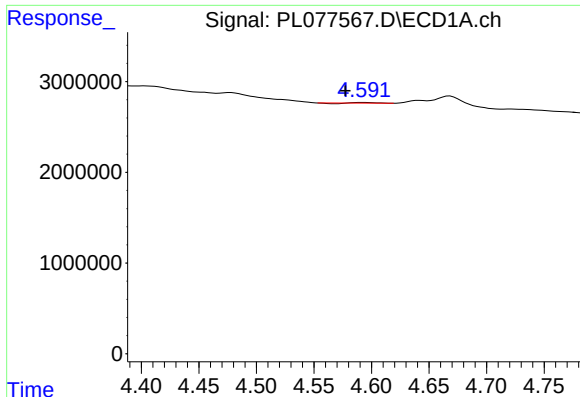

#23 Chlordane-1


R.T.: 4.593 min
Delta R.T.: 0.015 min
Response: 32357
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147514BL

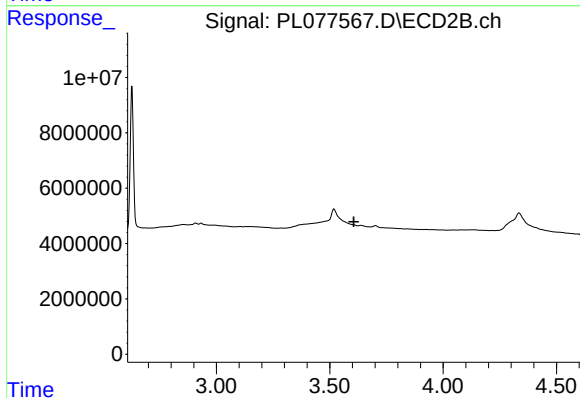


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 3.606 min
Response: 0
Conc: N.D.

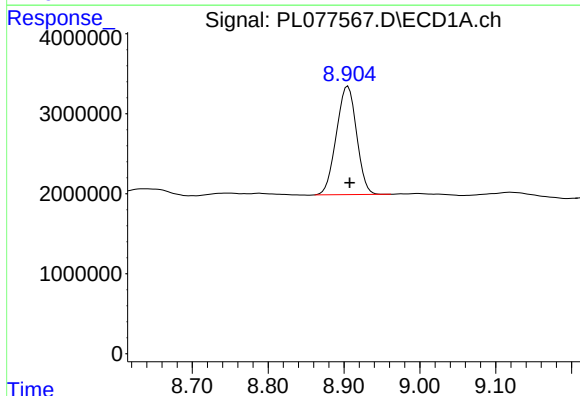

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: -0.003 min
Response: 25137244
Conc: 16.76 ng/ml

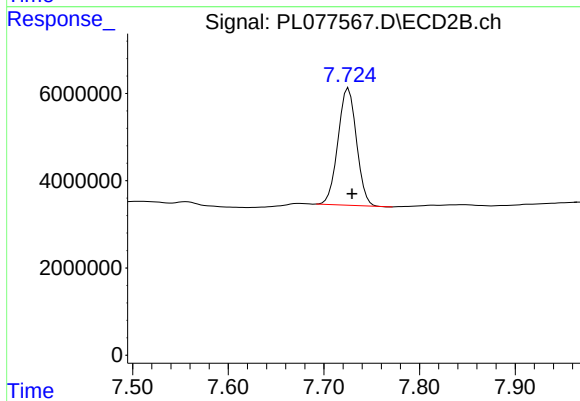

#28 Decachlorobiphenyl

R.T.: 7.726 min
Delta R.T.: -0.004 min
Response: 36214728
Conc: 18.36 ng/ml