

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 22:25
 Operator : AR\AJ
 Sample : N4502-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SLUDGE-DRUM-1-4-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 04:49:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:34:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.416	2.628	28588235	43309823	16.720	16.367
28) SA Decachlor...	8.905	7.726	25599051	37084250	17.067	18.805
Target Compounds						
14) MA Endrin	0.000	5.473f	0	2777640	N.D.	1.347 #
15) B Endosulfa...	6.708f	0.000	1823425	0	1.125	N.D. #
21) B Endrin ke...	7.569f	0.000	1304349	0	0.845	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 22:25
Operator : AR\AJ
Sample : N4502-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SLUDGE-DRUM-1-4-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 04:49:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:34:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

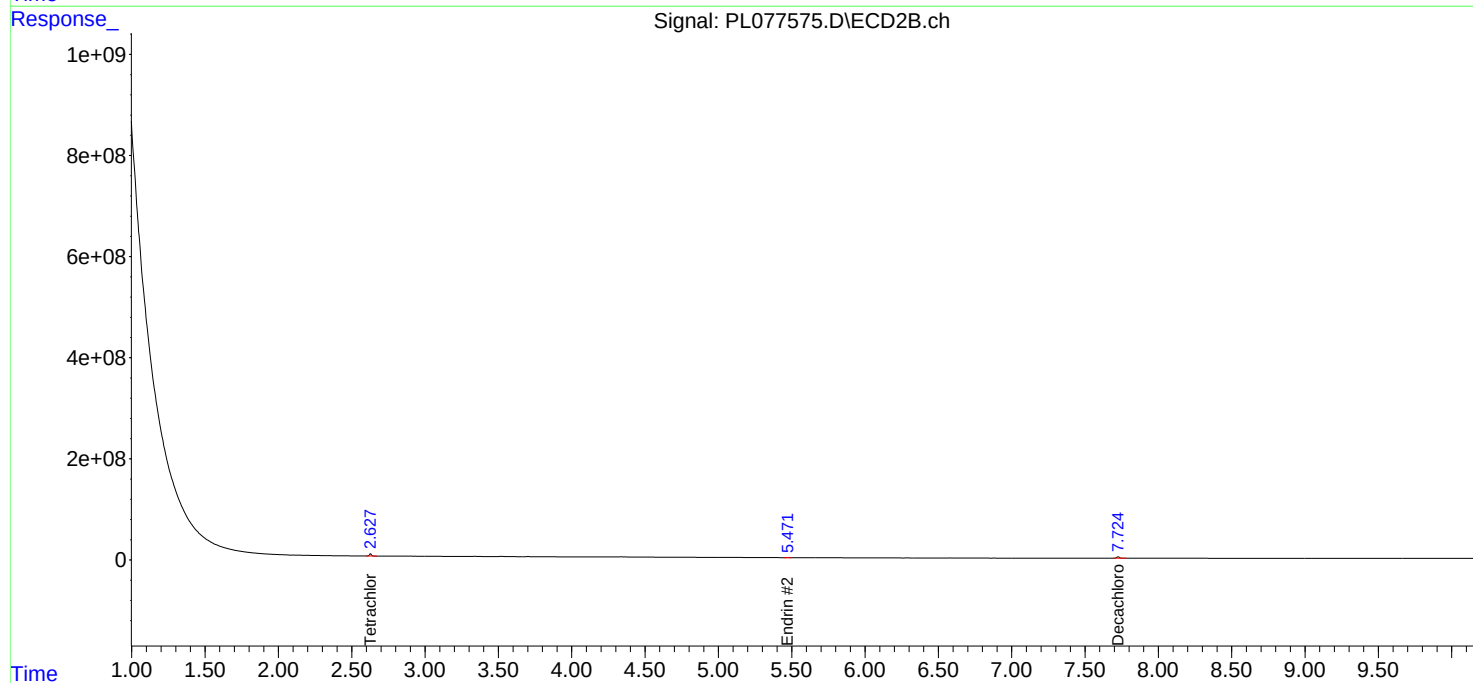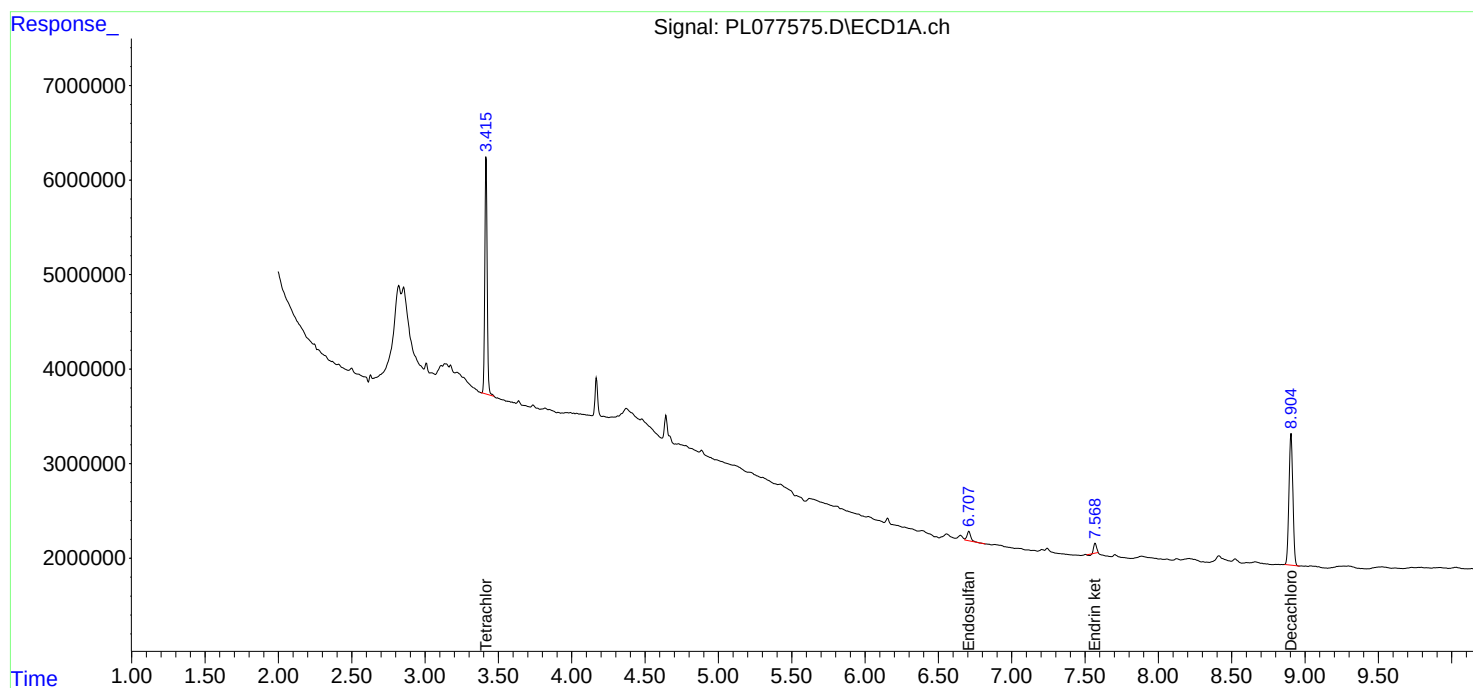


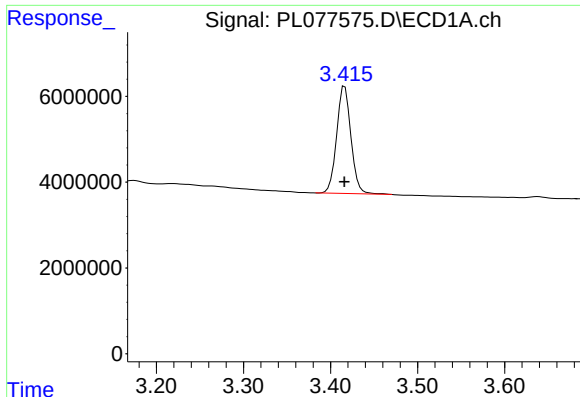

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 28588235
Conc: 16.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
SLUDGE-DRUM-1-4-COMP

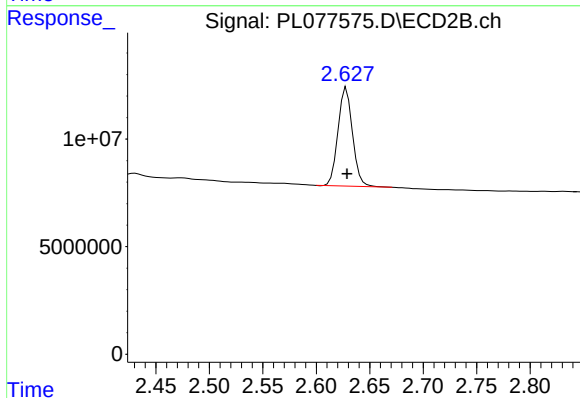


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 43309823
Conc: 16.37 ng/ml

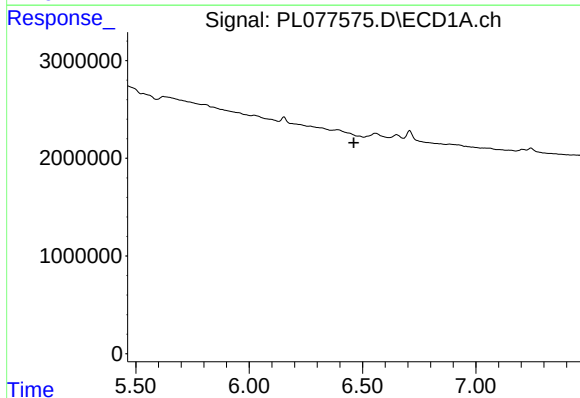


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

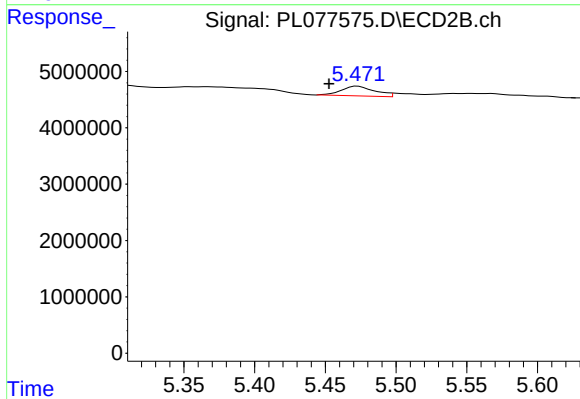

#14 Endrin


R.T.: 5.473 min
Delta R.T.: 0.020 min
Response: 2777640
Conc: 1.35 ng/ml

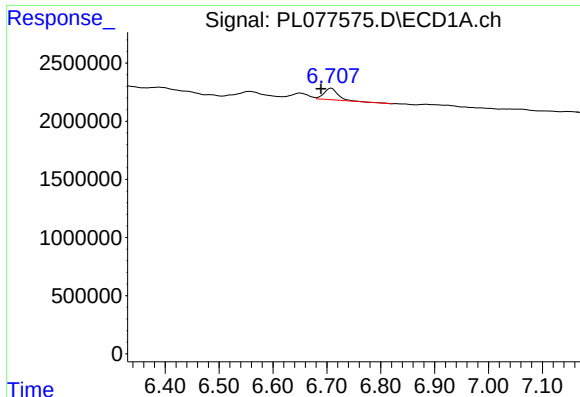

#15 Endosulfan II


R.T.: 6.708 min
Delta R.T.: 0.019 min
Response: 1823425
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
SLUDGE-DRUM-1-4-COMP

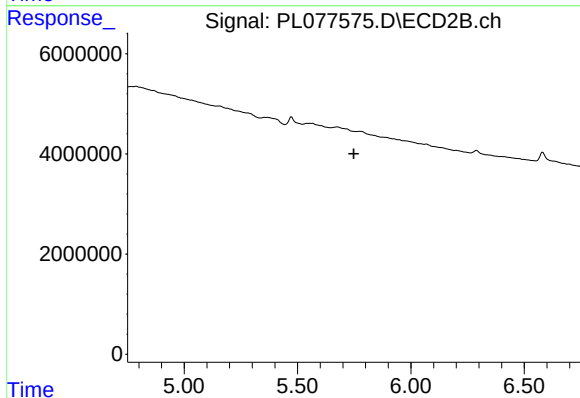


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.748 min
Response: 0
Conc: N.D.

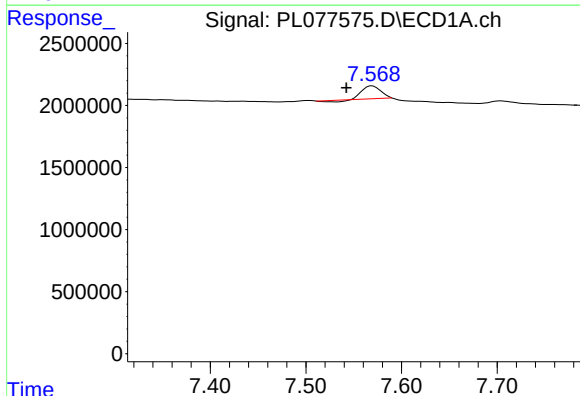


#21 Endrin ketone

R.T.: 7.569 min
Delta R.T.: 0.027 min
Response: 1304349
Conc: 0.84 ng/ml

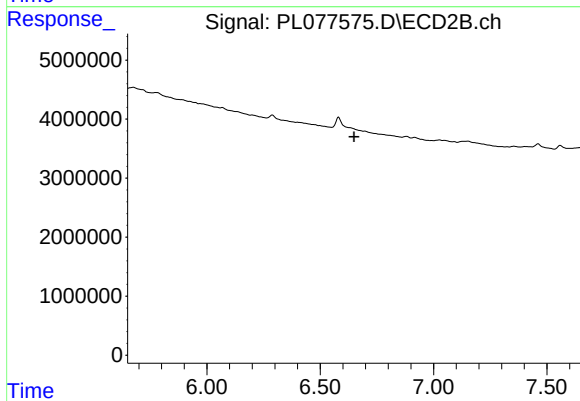

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.650 min
Response: 0
Conc: N.D.

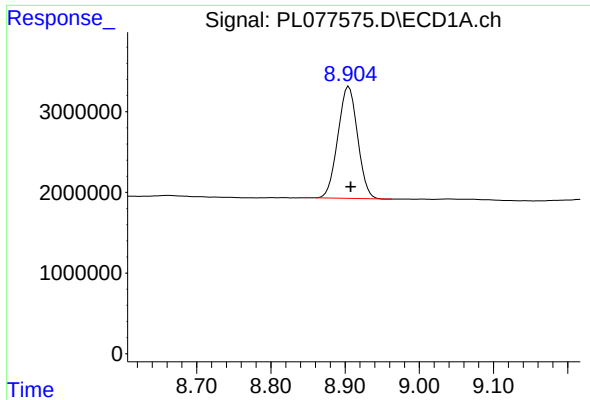

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: -0.003 min
Response: 25599051
Conc: 17.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
SLUDGE-DRUM-1-4-COMP

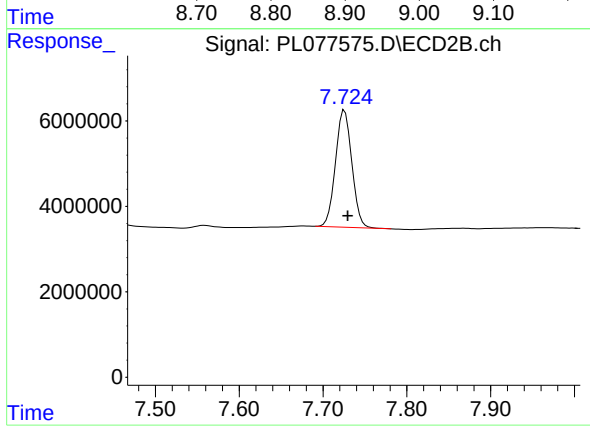

#28 Decachlorobiphenyl

R.T.: 7.726 min
Delta R.T.: -0.004 min
Response: 37084250
Conc: 18.80 ng/ml