

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 22:39
 Operator : AR\AJ
 Sample : N4502-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DEACON-WATER-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 04:49:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 14:34:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.628	36197347	54851313	21.171	20.729
28)	SA Decachlor...	8.905	7.727	15504897	22660623	10.337	11.491
Target Compounds							
7)	B delta-BHC	4.670	0.000	359480	0	0.191	N.D. #
14)	MA Endrin	0.000	5.474f	0	1503361	N.D.	0.729 #
15)	B Endosulfa...	6.709f	0.000	1746013	0	1.077	N.D. #
21)	B Endrin ke...	7.570f	0.000	1455494	0	0.943	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 22:39
Operator : AR\AJ
Sample : N4502-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DEACON-WATER-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 04:49:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 14:34:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

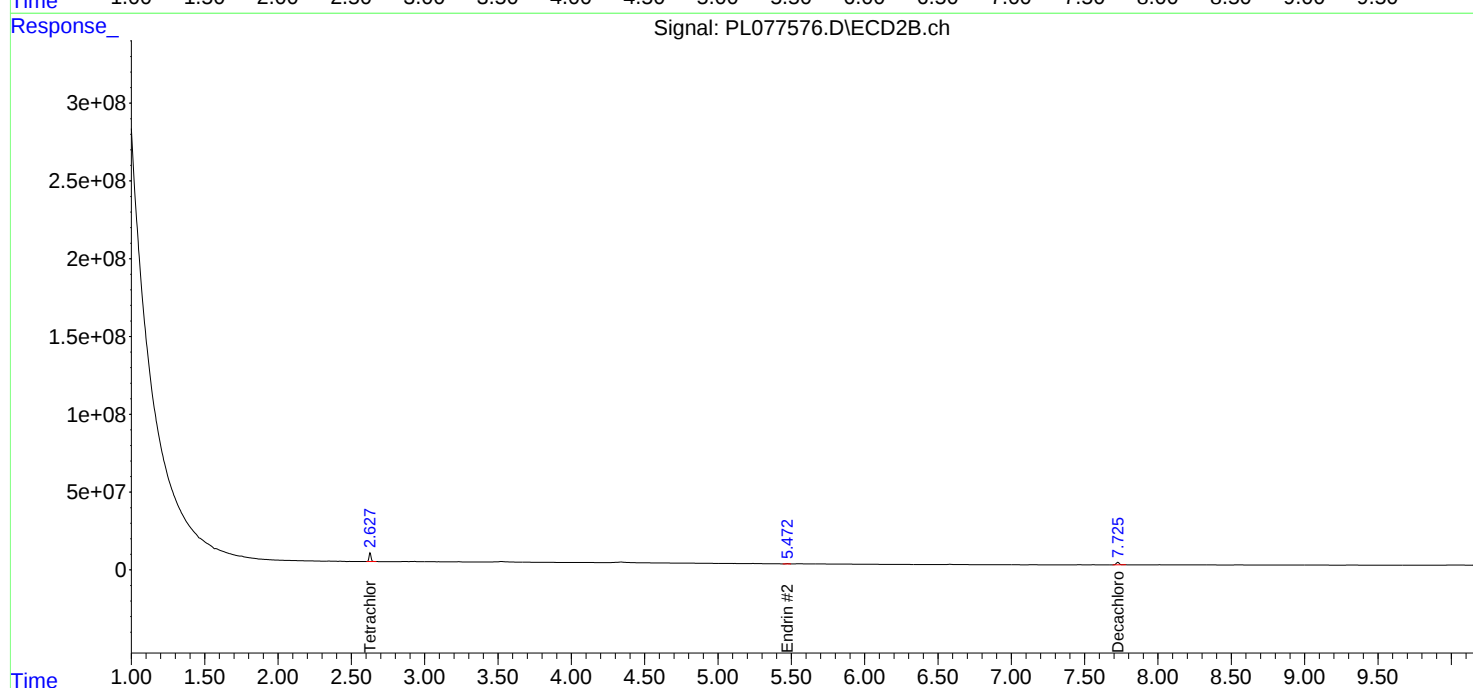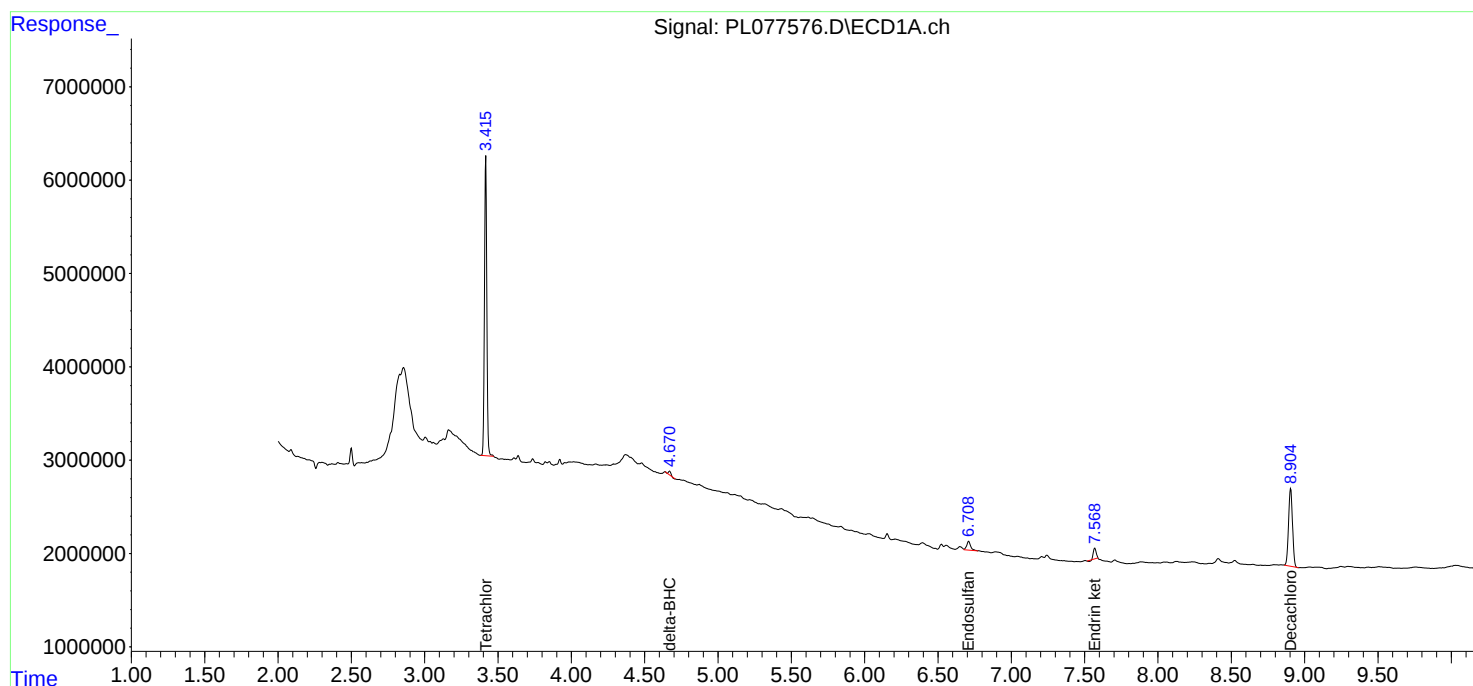


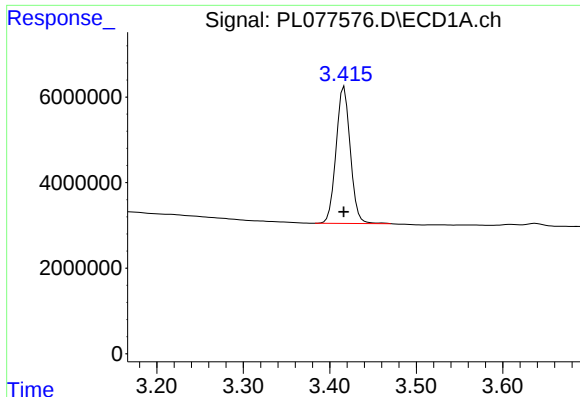

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 36197347
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
DEACON-WATER-COMP

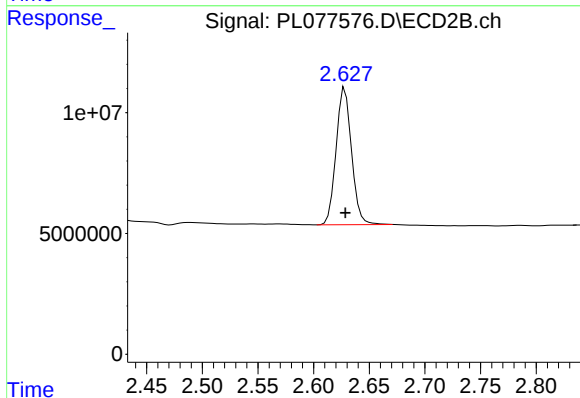


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 54851313
Conc: 20.73 ng/ml

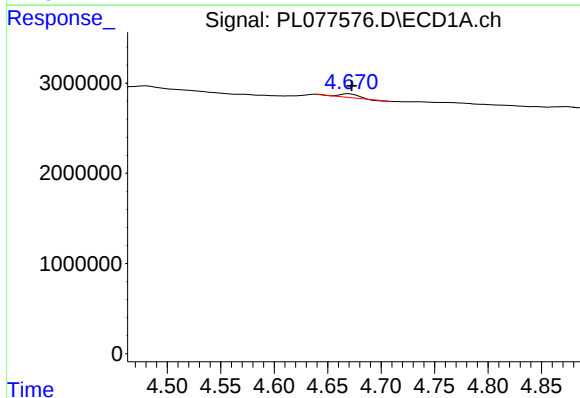


#7 delta-BHC

R.T.: 4.670 min
Delta R.T.: -0.003 min
Response: 359480
Conc: 0.19 ng/ml

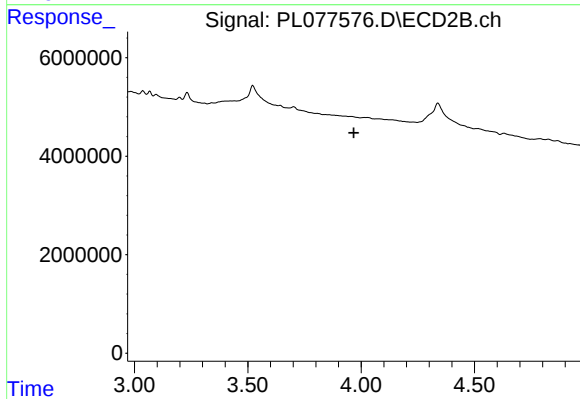

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 3.968 min
Response: 0
Conc: N.D.

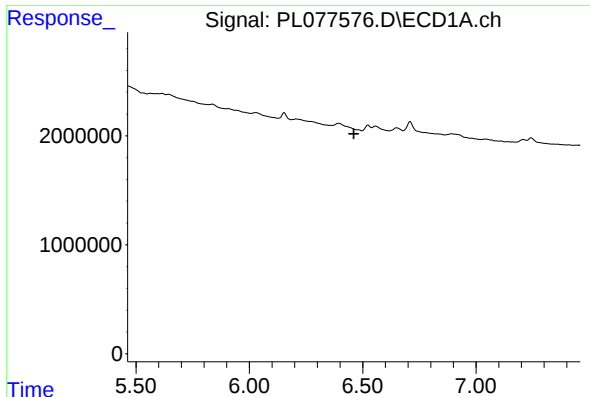

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DEACON-WATER-COMP

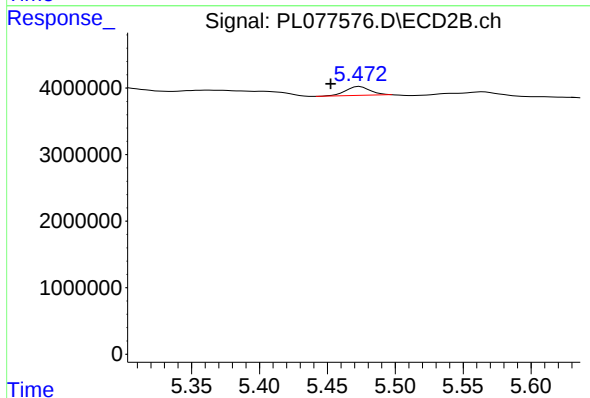


#14 Endrin

R.T.: 5.474 min
Delta R.T.: 0.021 min
Response: 1503361
Conc: 0.73 ng/ml

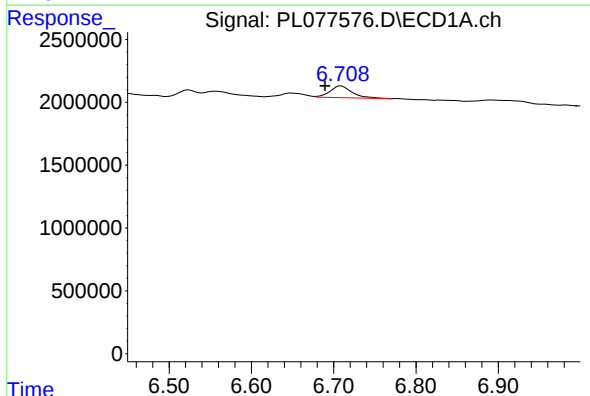


#15 Endosulfan II

R.T.: 6.709 min
Delta R.T.: 0.019 min
Response: 1746013
Conc: 1.08 ng/ml

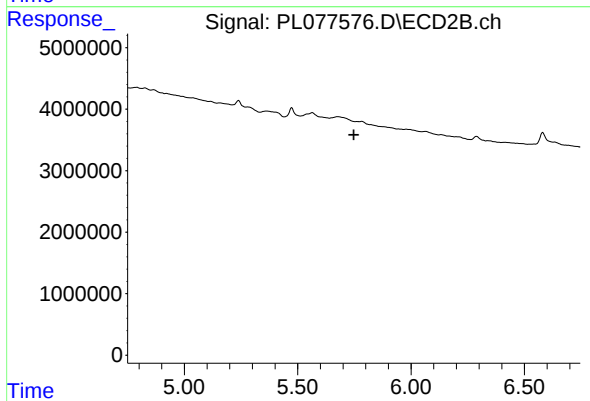

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.748 min
Response: 0
Conc: N.D.

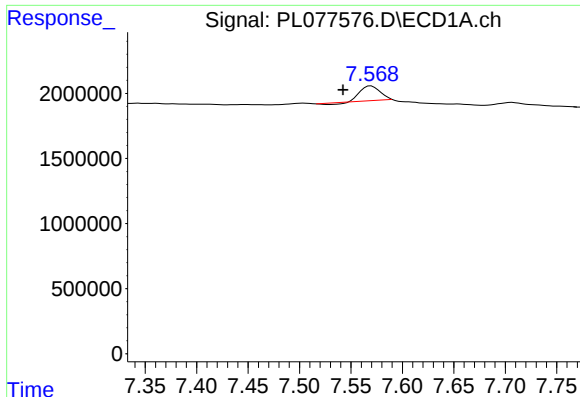

#21 Endrin ketone


R.T.: 7.570 min
Delta R.T.: 0.027 min
Response: 1455494
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
DEACON-WATER-COMP

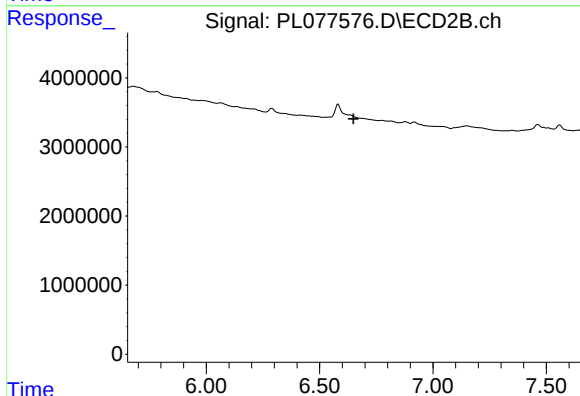


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.650 min
Response: 0
Conc: N.D.

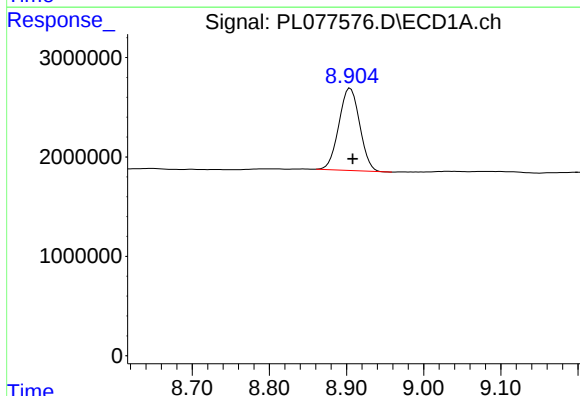

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: -0.003 min
Response: 15504897
Conc: 10.34 ng/ml

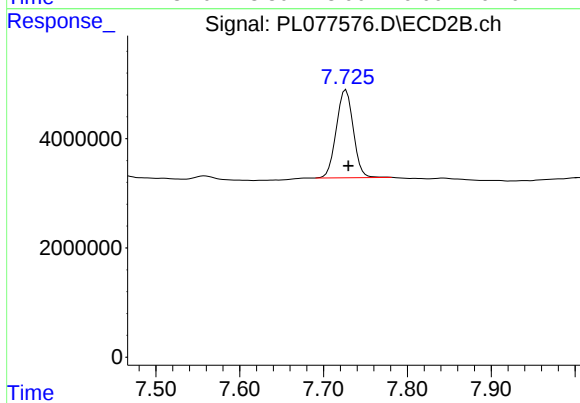

#28 Decachlorobiphenyl

R.T.: 7.727 min
Delta R.T.: -0.003 min
Response: 22660623
Conc: 11.49 ng/ml