

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
 Data File : PL077533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2022 11:20
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 12:27:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 07 12:26:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.628	176.9E6	310.1E6	101.201	98.292
28)	SA Decachlor...	8.908	7.730	140.8E6	187.6E6	94.299	95.815
Target Compounds							
23)	Chlordane-1	4.577	3.607	66373615	87332733	987.341	979.464
24)	Chlordane-2	5.112	4.177	72376499	95303462	964.506	961.334
25)	Chlordane-3	5.823	4.801	289.2E6	278.7E6	1028.514	973.051
26)	Chlordane-4	5.901	4.862	352.2E6	294.0E6	1013.692	978.152
27)	Chlordane-5	6.760	5.526	59508806	68475768	975.561	974.445



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090722\
Data File : PL077533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2022 11:20
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 12:27:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090722.M
Quant Title : GC Extractables
QLast Update : Wed Sep 07 12:26:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

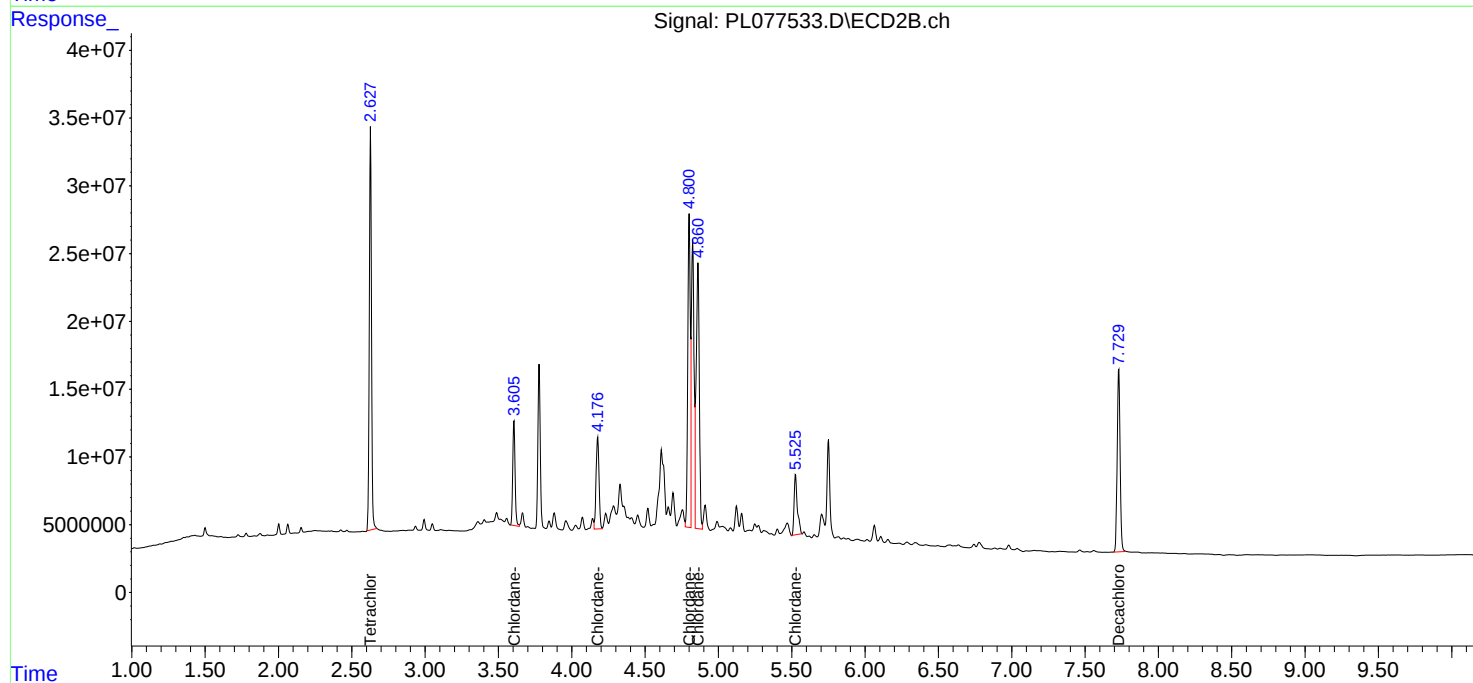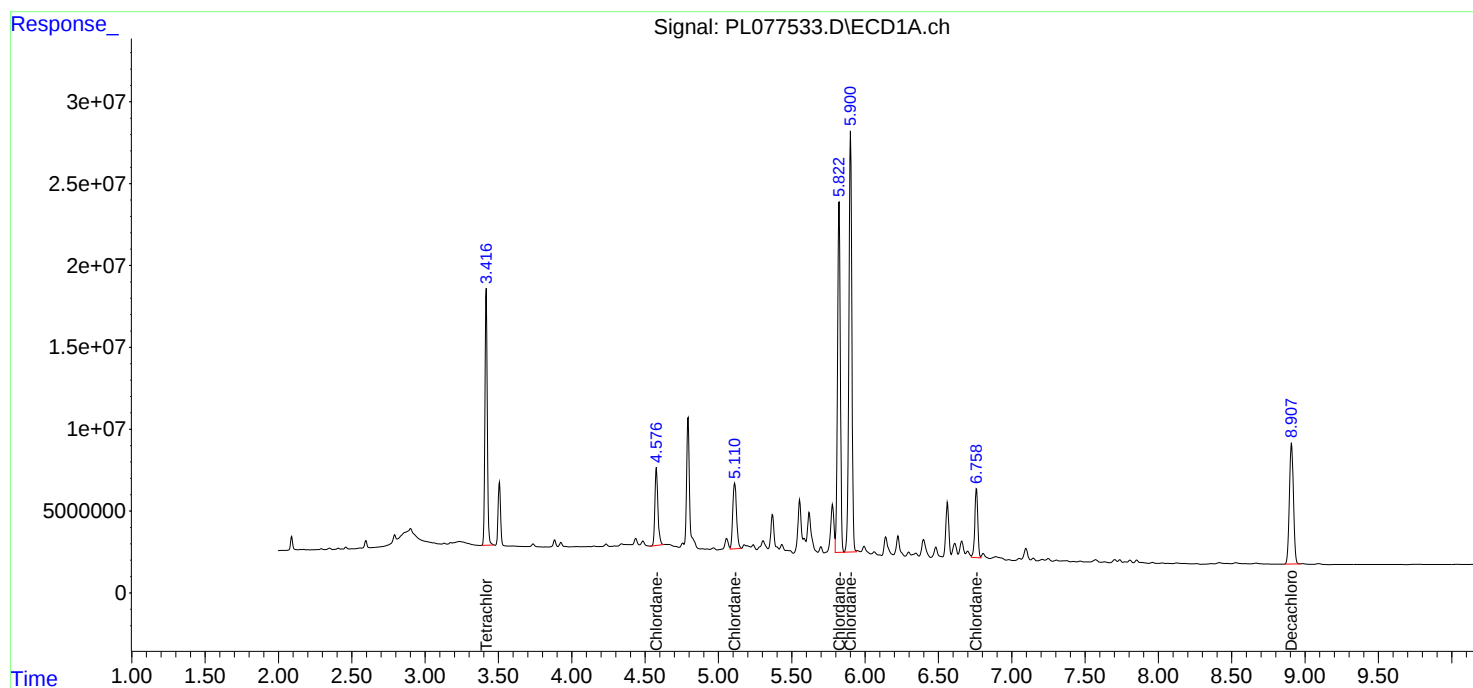


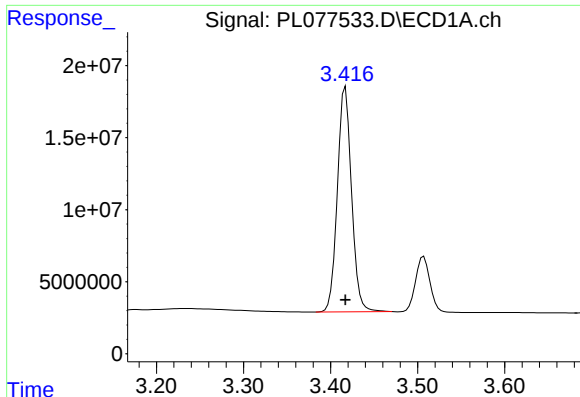

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 176917307
Conc: 101.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

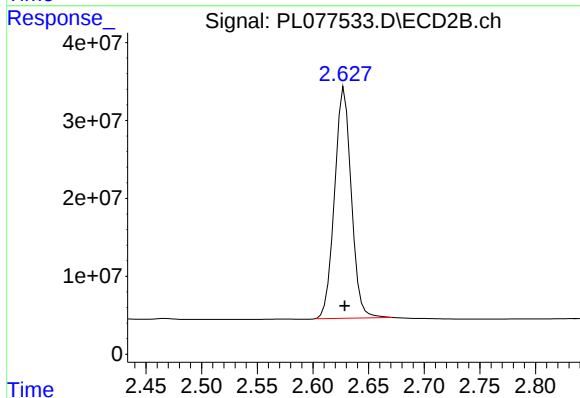


#1 Tetrachloro-m-xylene

R.T.: 2.628 min
Delta R.T.: 0.000 min
Response: 310082061
Conc: 98.29 ng/ml

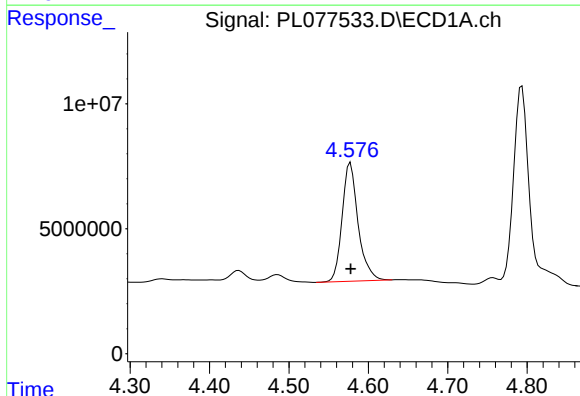


#23 Chlordane-1

R.T.: 4.577 min
Delta R.T.: 0.000 min
Response: 66373615
Conc: 987.34 ng/ml

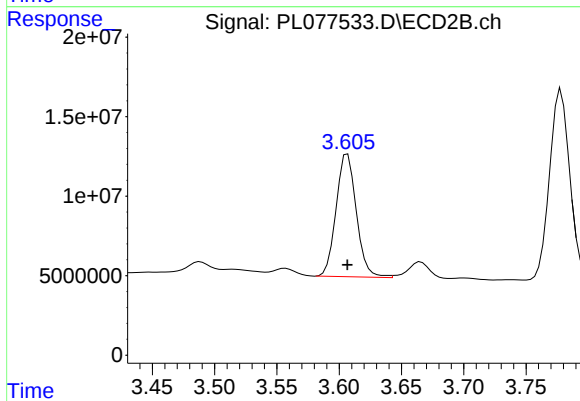

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 87332733
Conc: 979.46 ng/ml

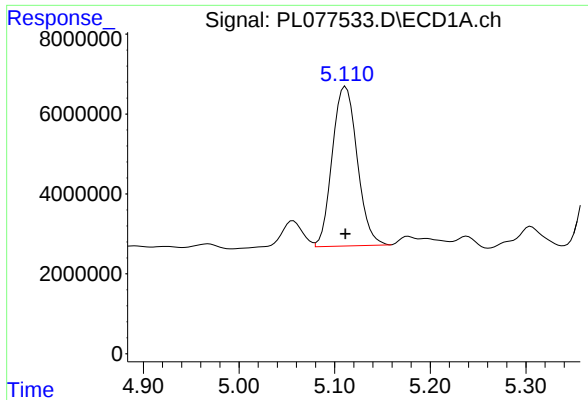

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 72376499
Conc: 964.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

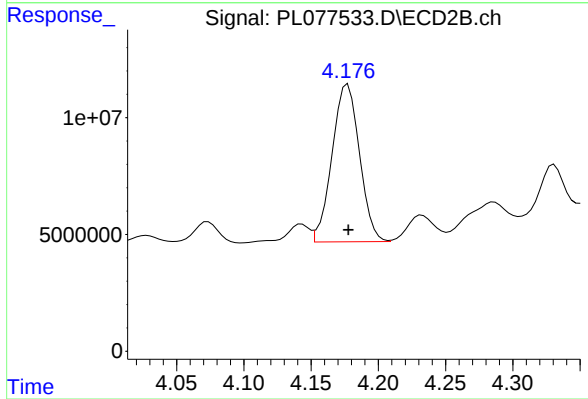


#24 Chlordane-2

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 95303462
Conc: 961.33 ng/ml

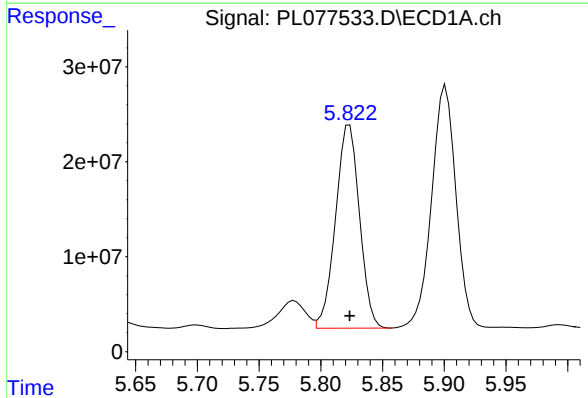


#25 Chlordane-3

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 289180216
Conc: 1028.51 ng/ml

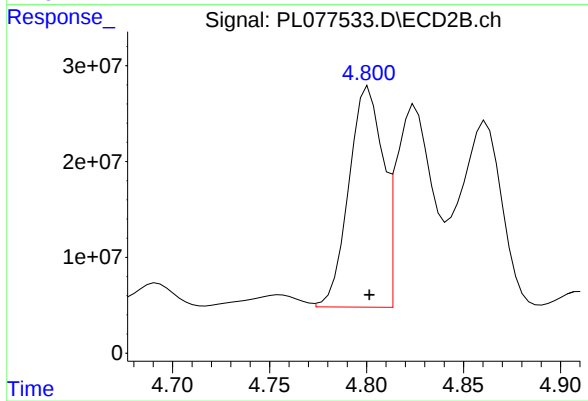

#25 Chlordane-3


R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 278654499
Conc: 973.05 ng/ml

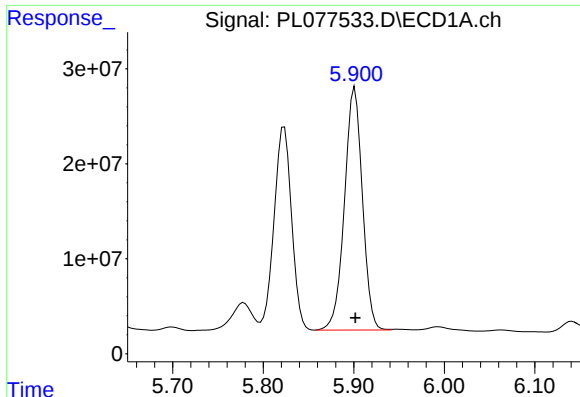

#26 Chlordane-4


R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 352224175
Conc: 1013.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

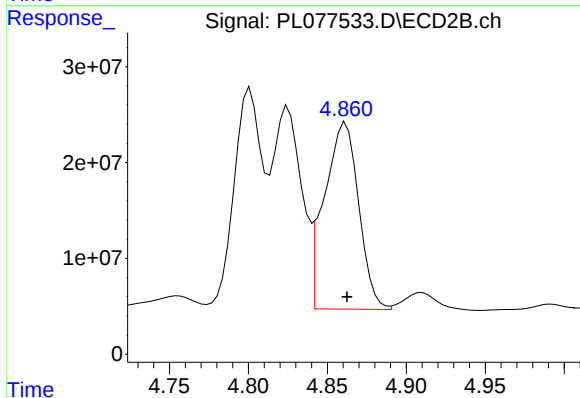


#26 Chlordane-4

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 294027429
Conc: 978.15 ng/ml

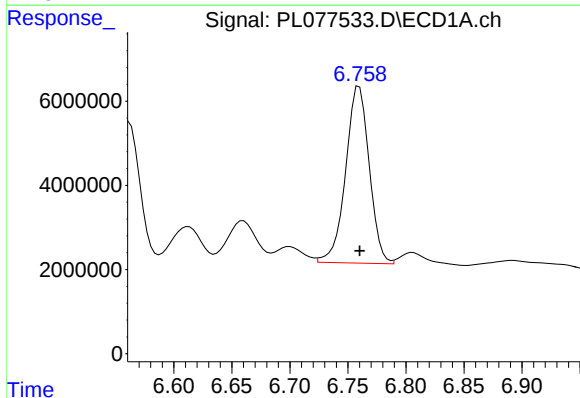


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 59508806
Conc: 975.56 ng/ml

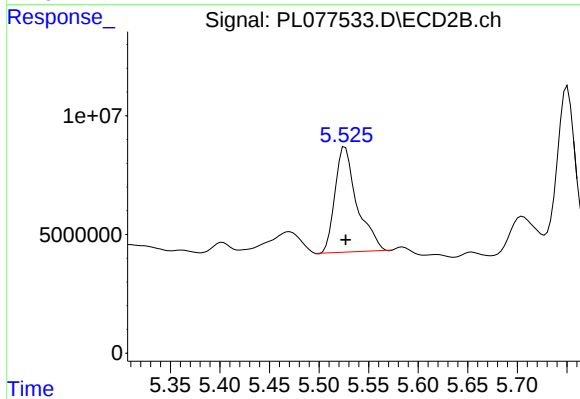

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 68475768
Conc: 974.44 ng/ml

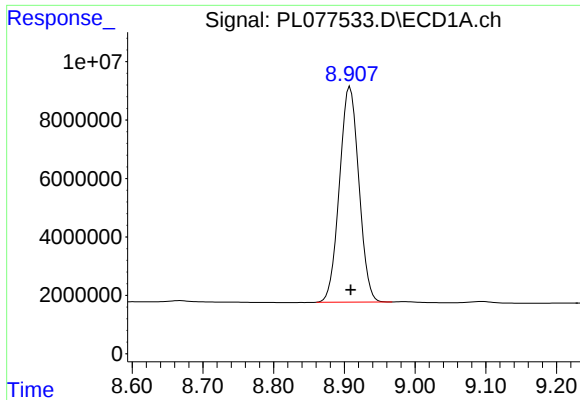

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: -0.001 min
Response: 140752167
Conc: 94.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

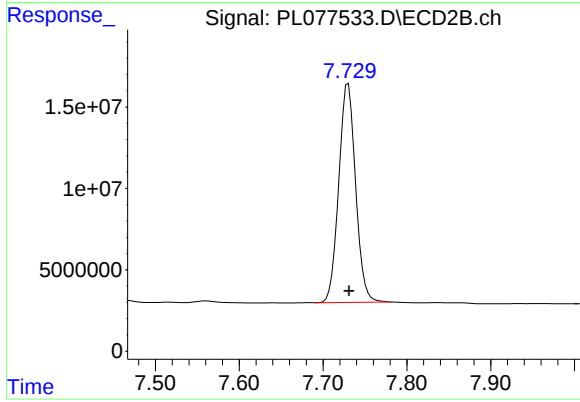

#28 Decachlorobiphenyl

R.T.: 7.730 min
Delta R.T.: -0.001 min
Response: 187643162
Conc: 95.82 ng/ml